
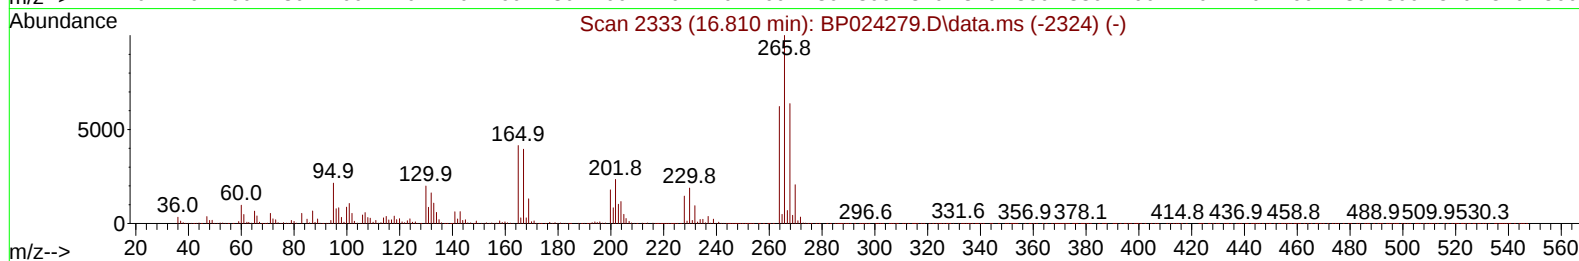
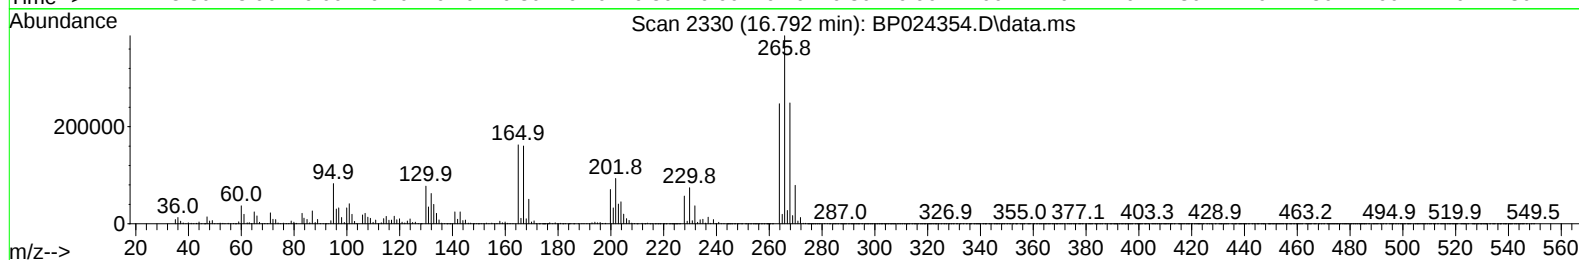


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042125\
Data File : BP024354.D
Acq On : 21 Apr 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 11:41:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

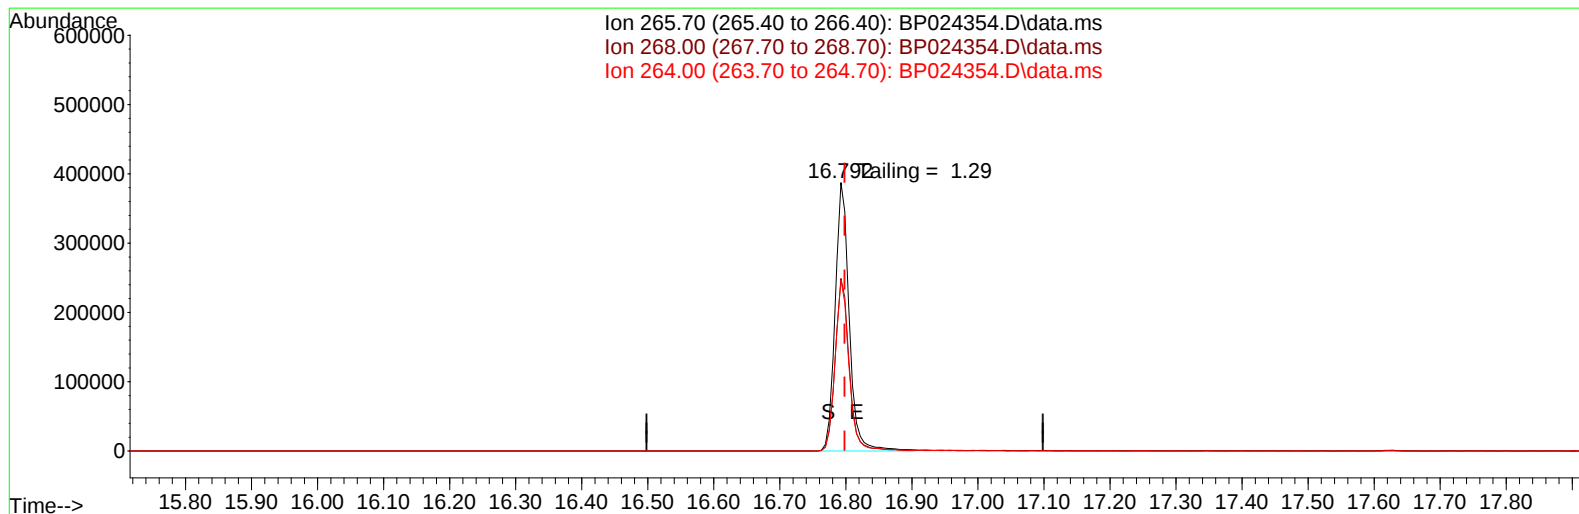

TIC: BP024354.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.006) 1511600.00 ng

response 575596

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.28
264.00	62.20	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042125\
Data File : BP024354.D
Acq On : 21 Apr 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 11:41:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

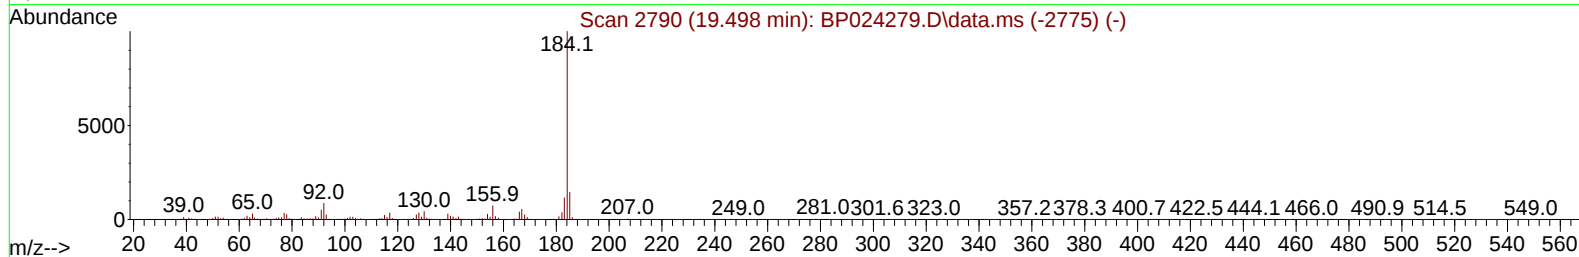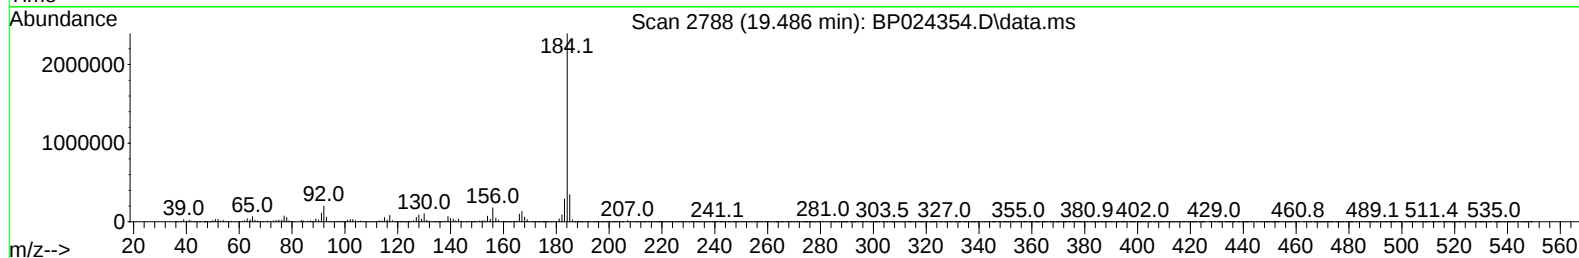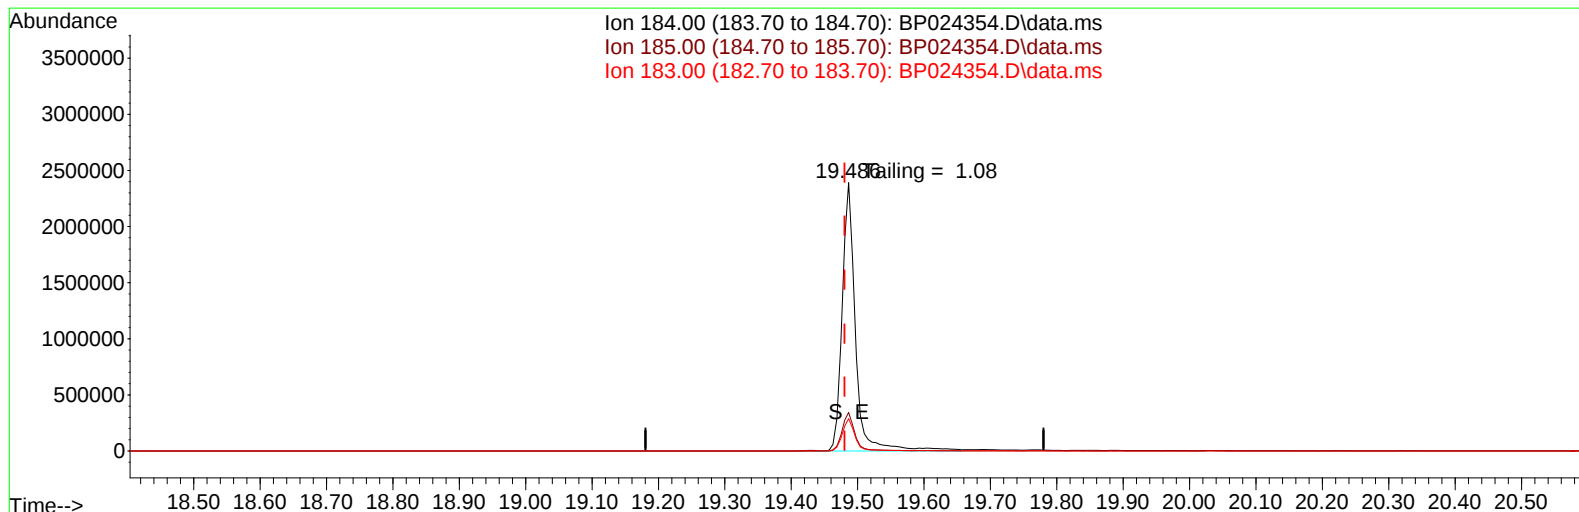

TIC: BP024354.D\data.ms

(77) Benzidine

19.486min (+ 0.006) 1881751.69 ng

response 3267833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.37
183.00	11.50	12.06
0.00	0.00	0.00