
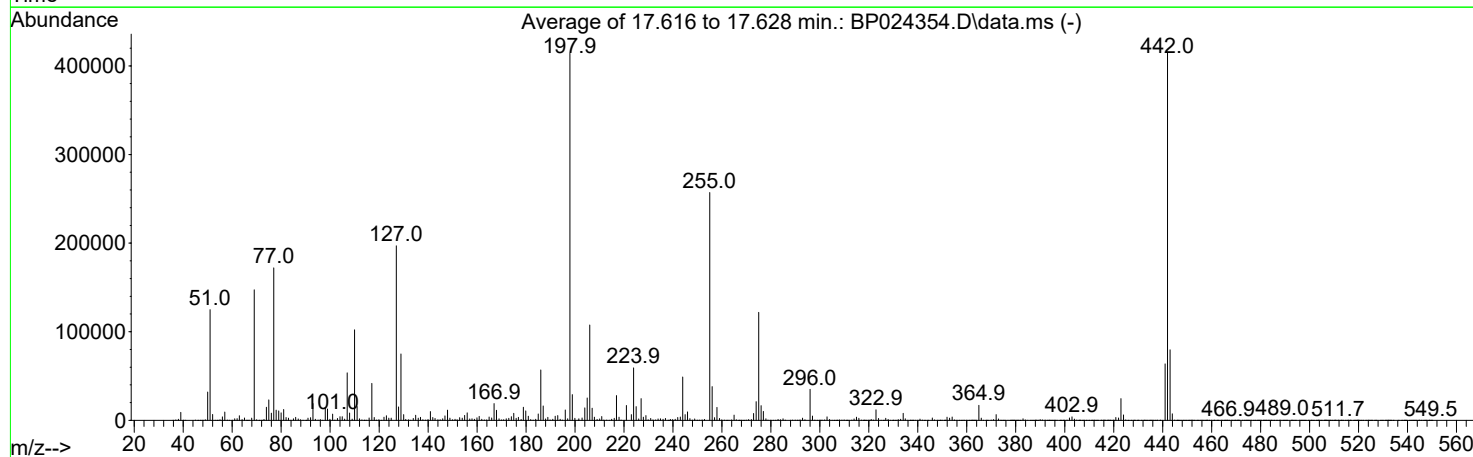


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042125\
Data File : BP024354.D
Acq On : 21 Apr 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

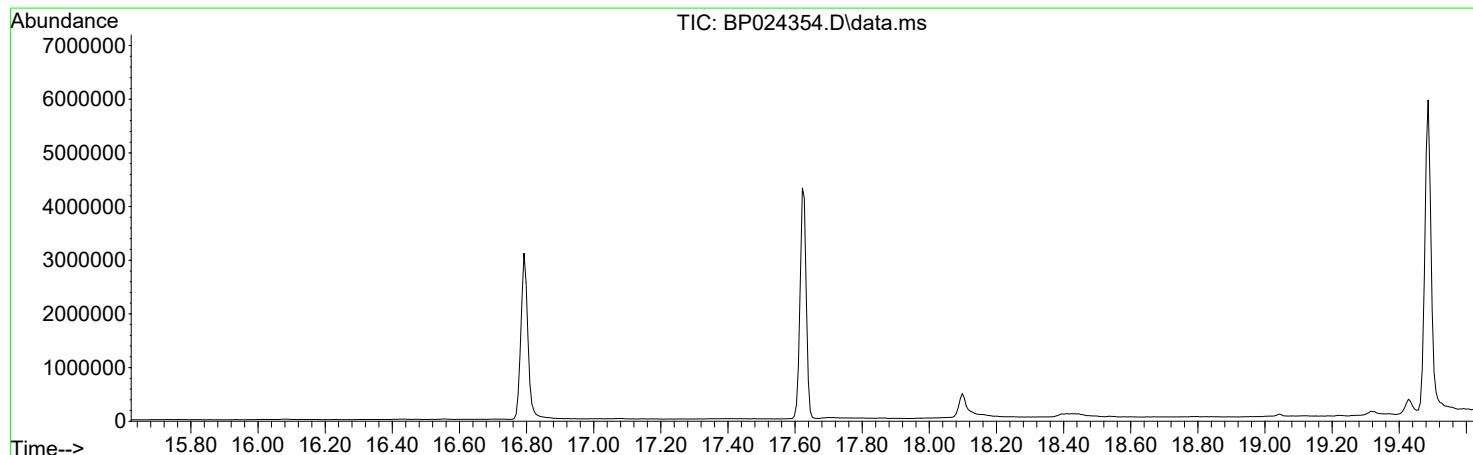

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	125021	PASS
68	69	0.00	2	1.7	2516	PASS
69	198	0.00	100	35.6	147343	PASS
70	69	0.00	2	0.5	710	PASS
127	198	10	80	47.6	196953	PASS
197	198	0.00	2	0.4	1736	PASS
198	198	100	100	100.0	414174	PASS
199	198	5	9	7.0	28999	PASS
275	198	10	60	29.4	121867	PASS
365	198	1	100	4.1	16982	PASS
441	198	0.01	100	15.4	63705	PASS
442	442	100	100	100.0	415125	PASS
443	442	15	24	19.2	79619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/21/2025	BNA_P	<u>BP024354.D</u>
Compound Name	Response	Retention Time
DDT	1579325	20.769
DDD	33647	20.322
DDE	2900	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36547	1615872	2.26

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042125\
Data File : BP024354.D
Acq On : 21 Apr 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 21 11:41:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

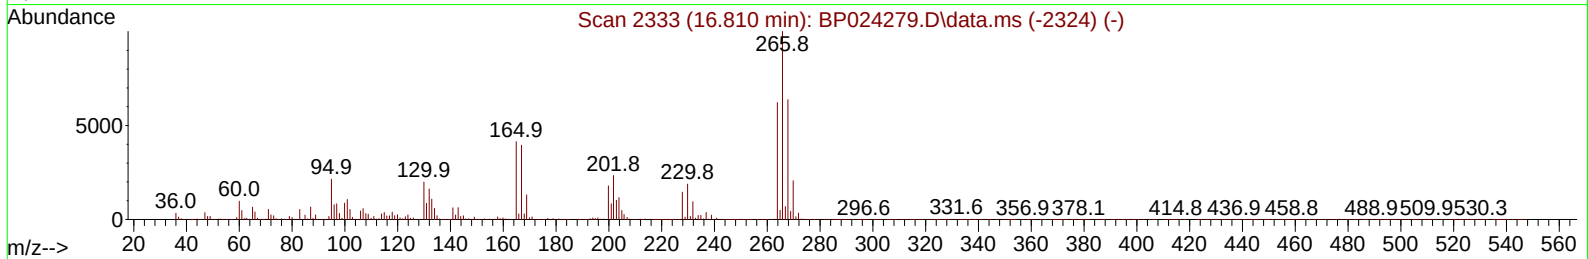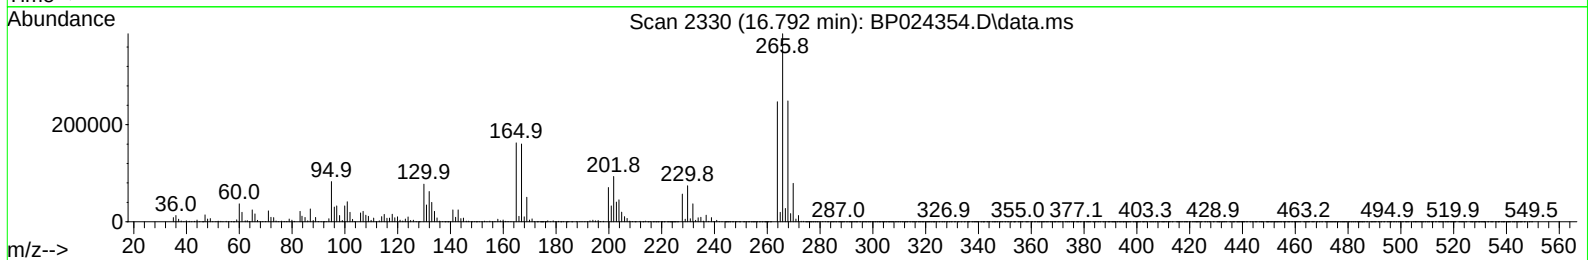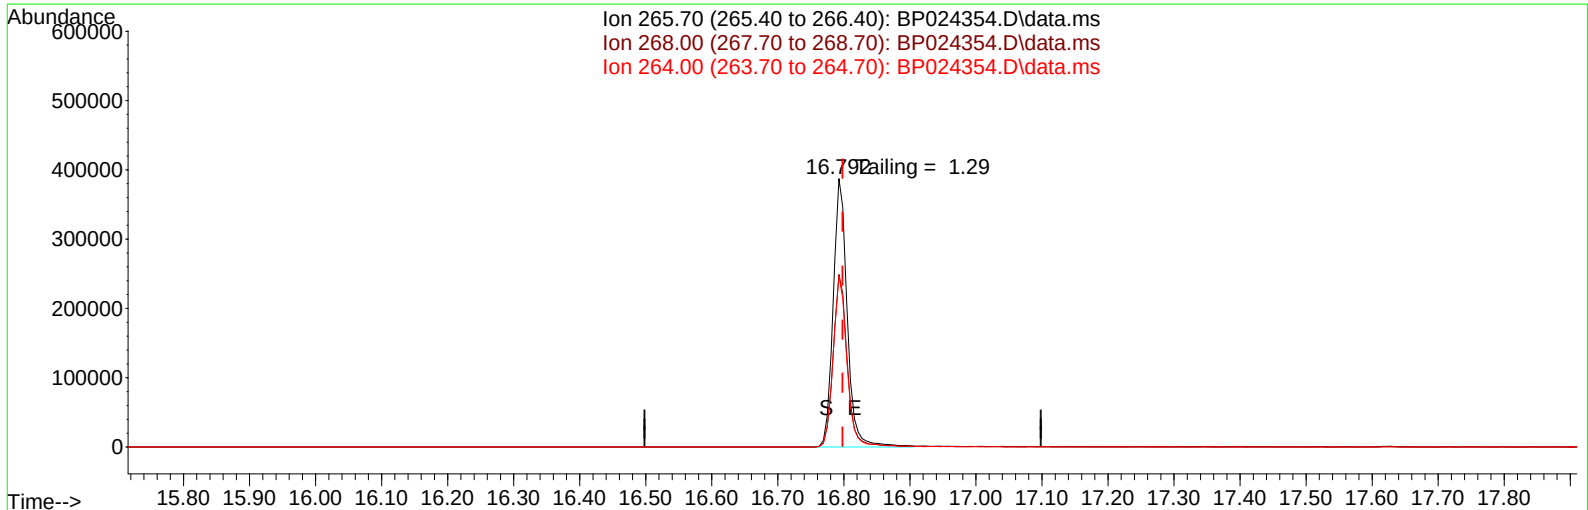

TIC: BP024354.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.006) 1511600.00 ng




response 575596

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.28
264.00	62.20	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042125\
Data File : BP024354.D
Acq On : 21 Apr 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 21 11:41:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

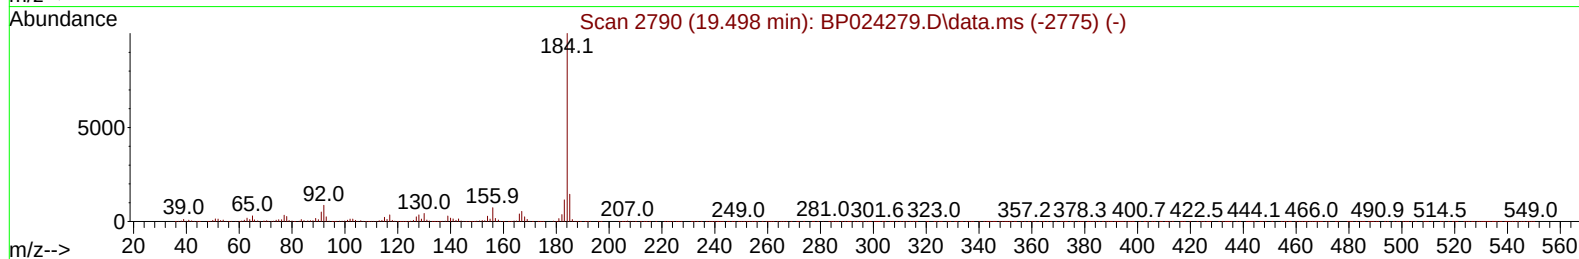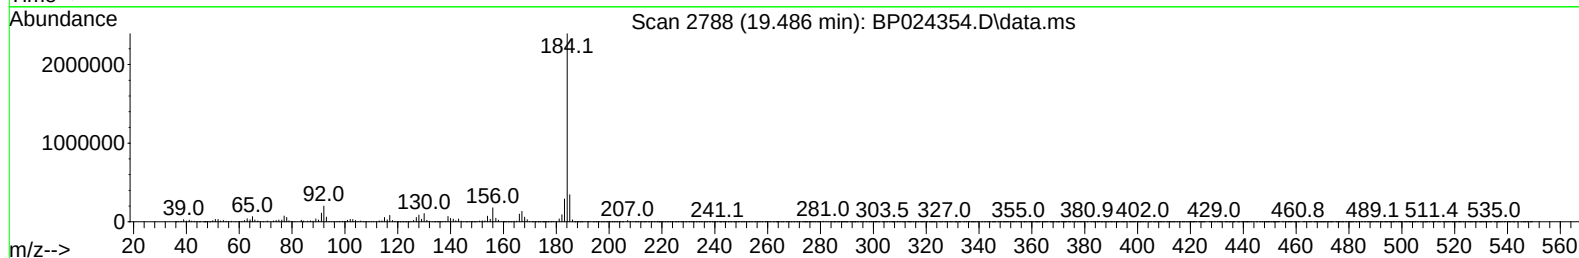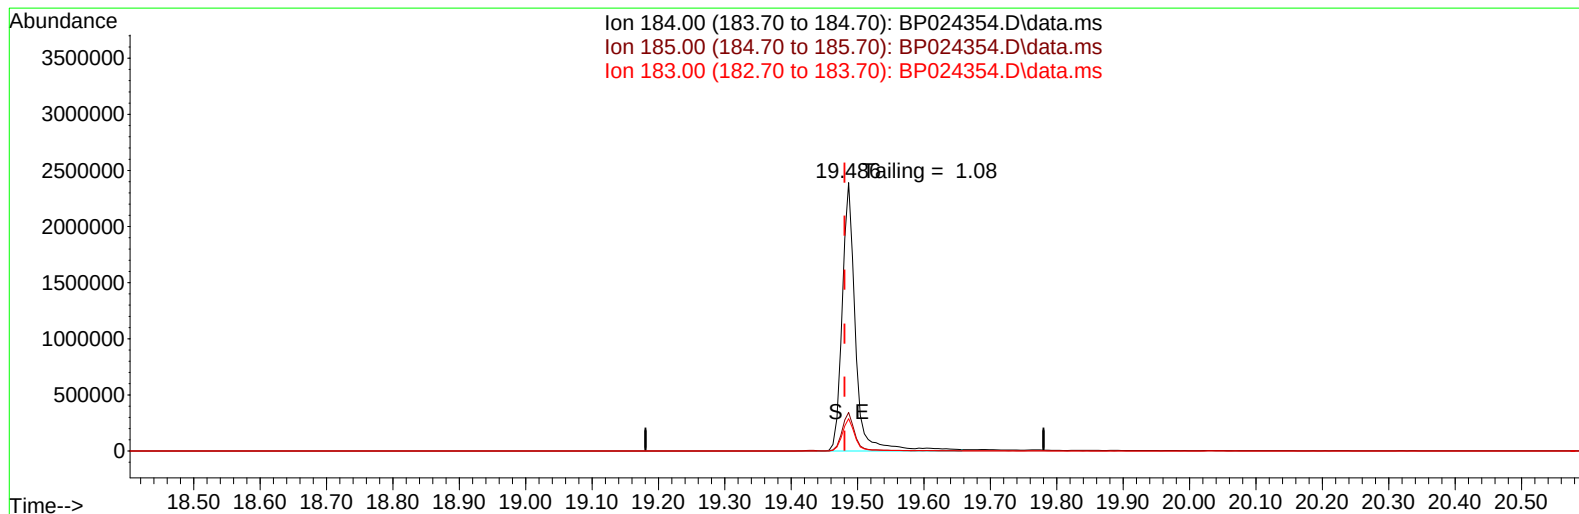

TIC: BP024354.D\data.ms

(77) Benzidine

19.486min (+ 0.006) 1881751.69 ng

response 3267833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.37
183.00	11.50	12.06
0.00	0.00	0.00