




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020076.D
Acq On : 22 Apr 2024 14:28
Operator : MA/JU
Sample : P2104-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:35:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

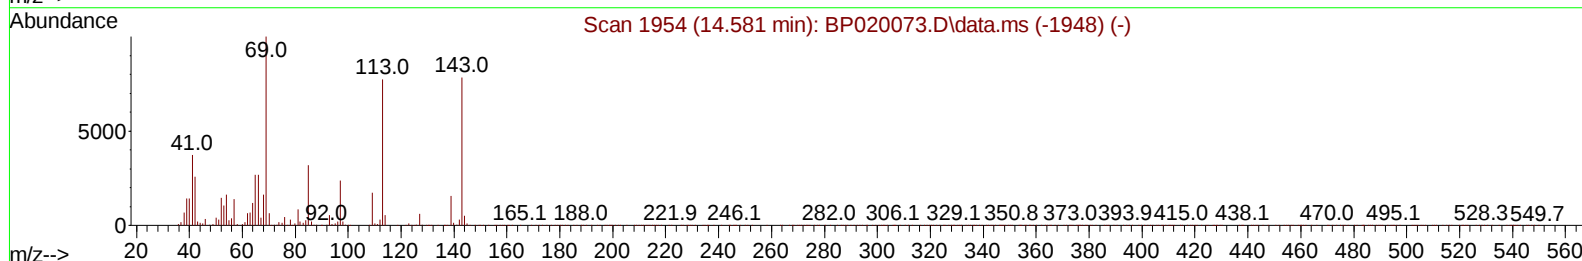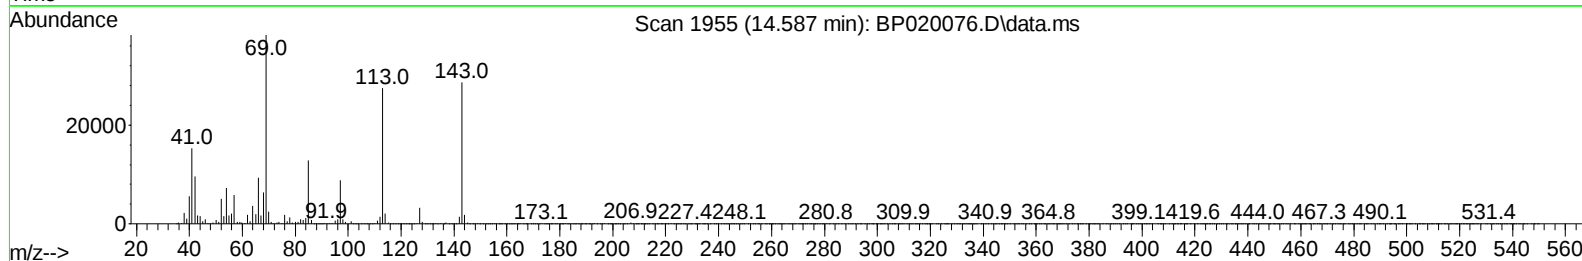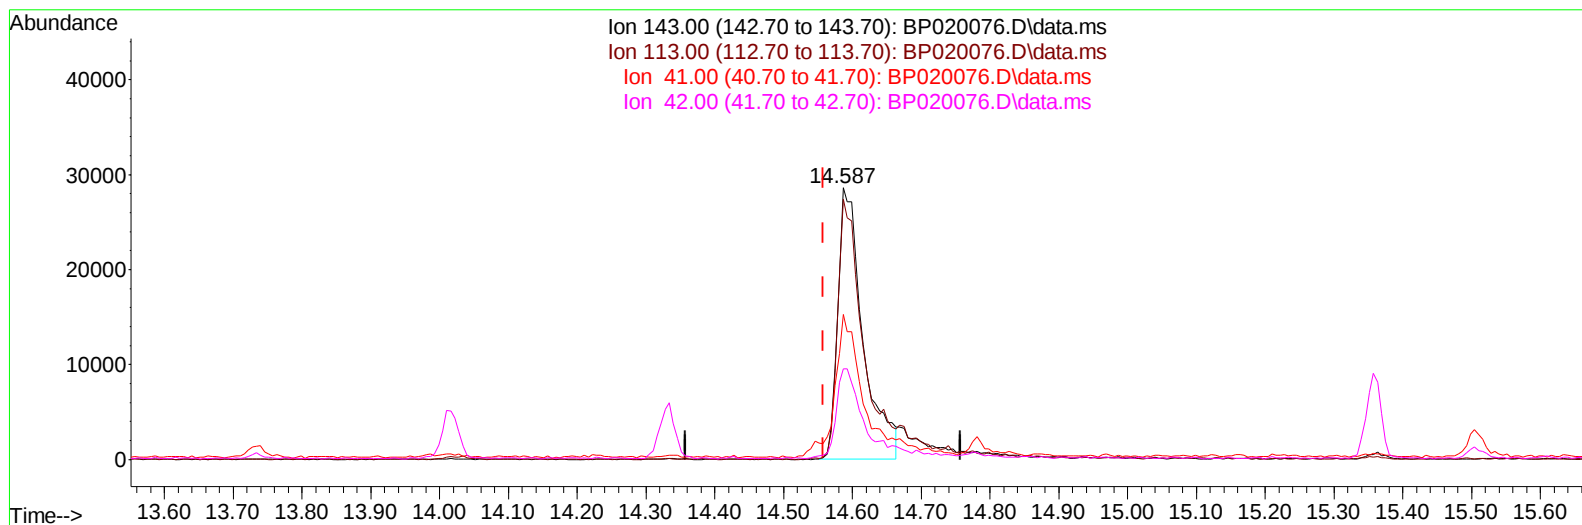

TIC: BP020076.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.029) 26.57 ng/u1

response 73126

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	95.95
41.00	50.70	53.36
42.00	34.00	33.42




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020076.D
Acq On : 22 Apr 2024 14:28
Operator : MA/JU
Sample : P2104-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:35:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

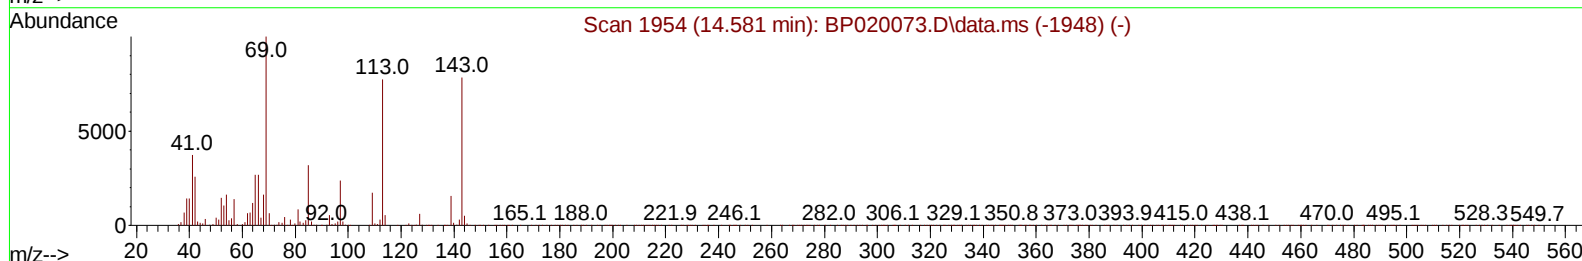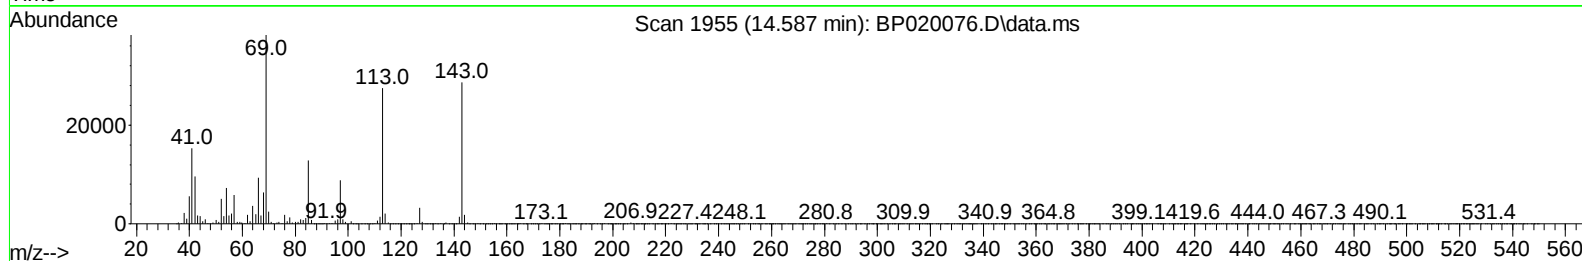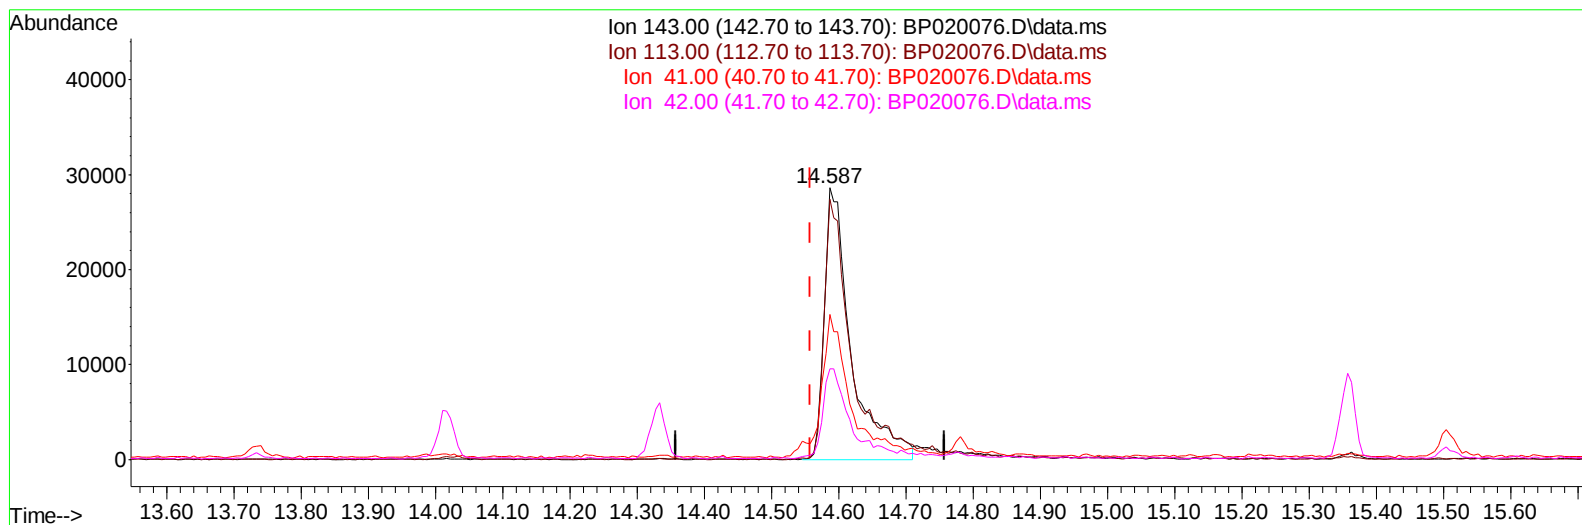

TIC: BP020076.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.029) 28.94 ng/ul m

response 79629

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	95.95
41.00	50.70	53.36
42.00	34.00	33.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020076.D
 Acq On : 22 Apr 2024 14:28
 Operator : MA/JU
 Sample : P2104-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 23 01:50:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	96369	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	385950	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.334	164	264525	20.000	ng/ul	0.02
64) Phenanthrene-d10	17.169	188	596475	20.000	ng/ul	0.01
79) Chrysene-d12	21.674	240	555127	20.000	ng/ul	0.02
88) Perylene-d12	25.080	264	601216	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	9874	4.198	ng/uL	0.00
4) Pyridine-d5	3.634	84	103699	14.979	ng/ul	0.00
7) Phenol-d5	6.822	99	202882	24.155	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	133883	22.806	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	143420	25.009	ng/ul	0.00
15) 4-Methylphenol-d8	8.352	113	159651	24.334	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	73343	26.418	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	87275	29.083	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	156380	26.268	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	204476	25.729	ng/ul	0.00
46) Dimethylphthalate-d6	13.734	166	519777	28.752	ng/ul	0.00
49) Acenaphthylene-d8	14.016	160	587904	27.285	ng/ul	0.02
54) 4-Nitrophenol-d4	14.587	143	79629m	28.935	ng/ul	0.03
60) Fluorene-d10	15.357	176	459295	28.541	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.504	200	51625	14.815	ng/ul	0.02
73) Anthracene-d10	17.281	188	747258	27.964	ng/ul	0.02
81) Pyrene-d10	19.675	212	928315	31.117	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.845	264	855414	29.126	ng/ul	0.04

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020076.D
Acq On : 22 Apr 2024 14:28
Operator : MA/JU
Sample : P2104-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:50:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

