




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

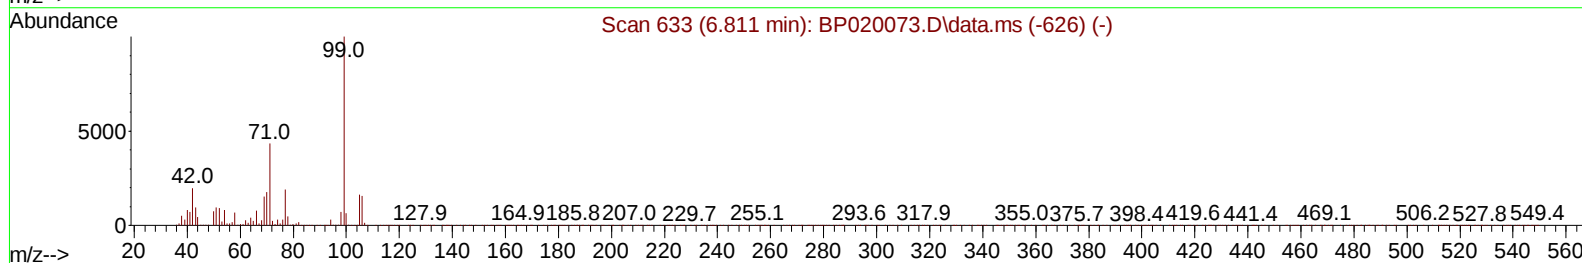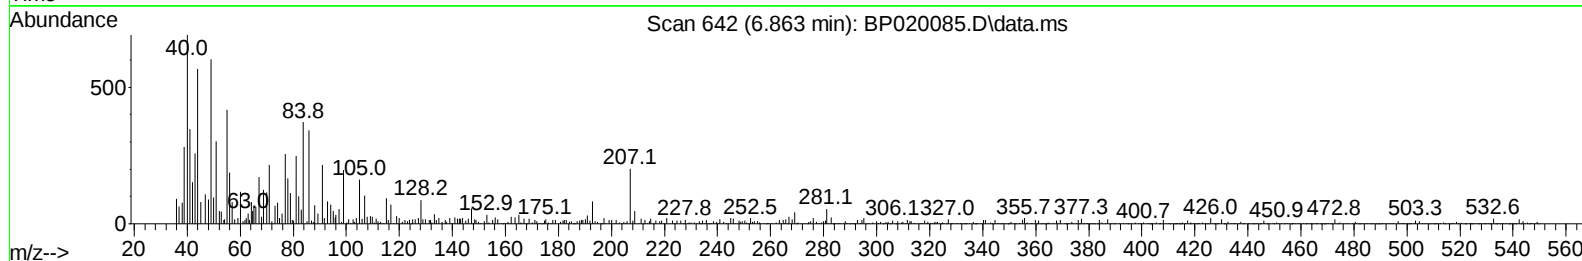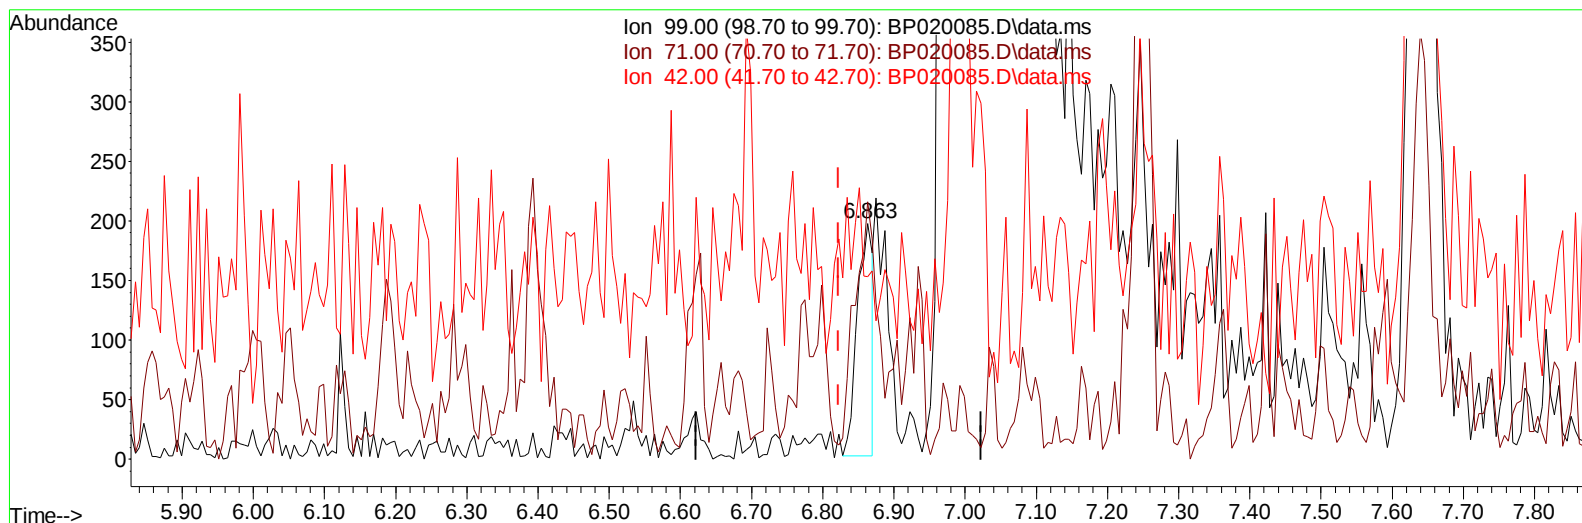

TIC: BP020085.D\data.ms

(7) Phenol-d5 (S)

6.863min (+ 0.041) 0.02 ng/u1

response 292

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	45.80	109.09#
42.00	22.40	77.27#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

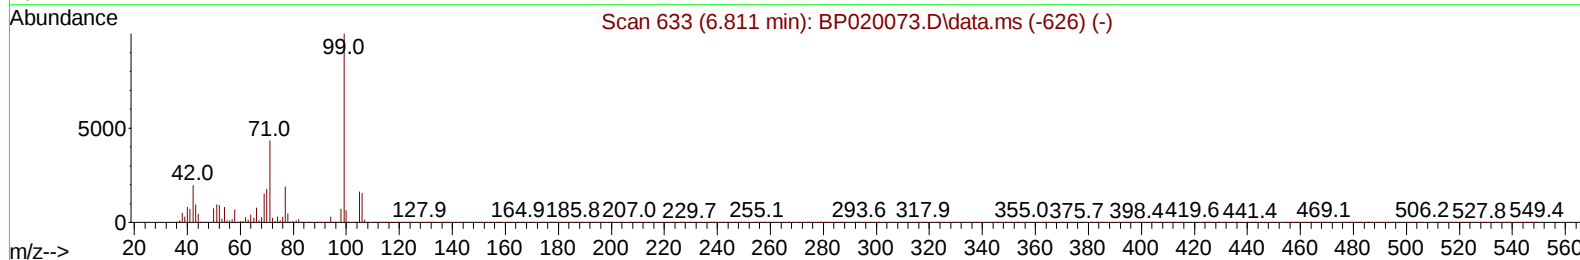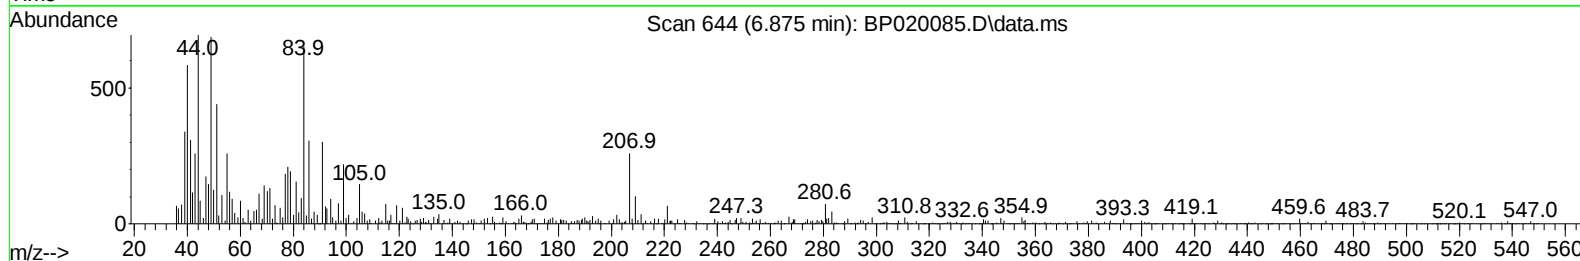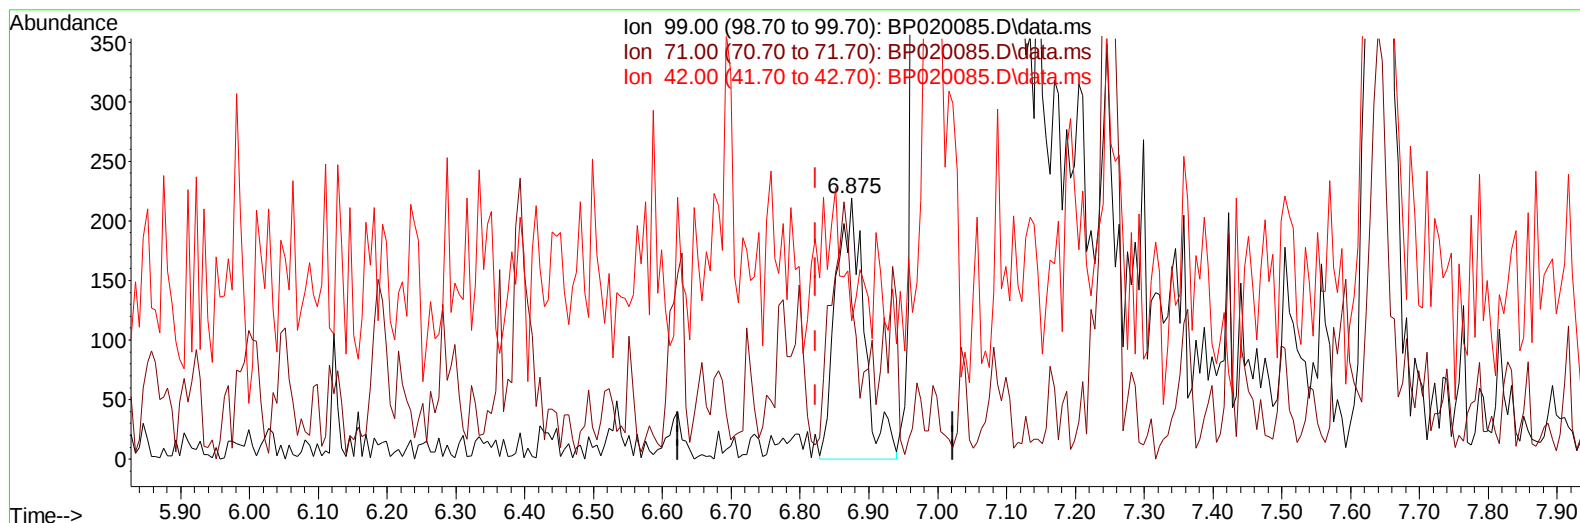

TIC: BP020085.D\data.ms

(7) Phenol-d5 (S)

6.875min (+ 0.053) 0.04 ng/u1 m

response 621

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	45.80	59.82#
42.00	22.40	52.97#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

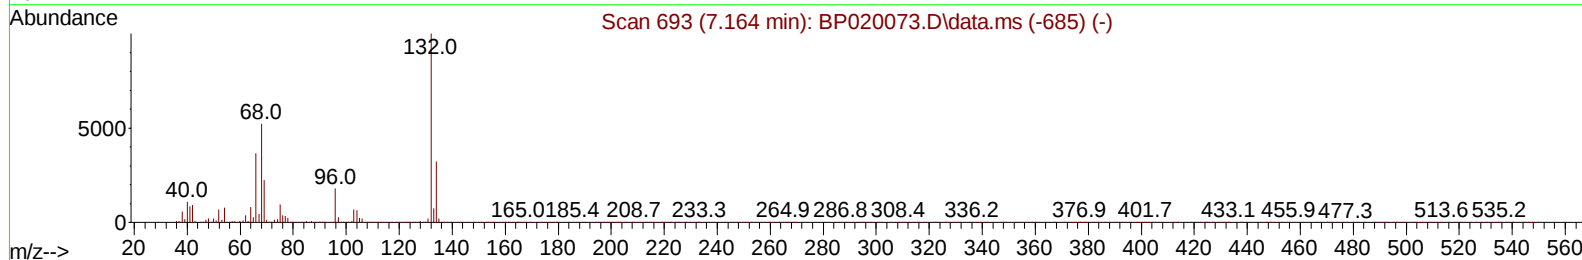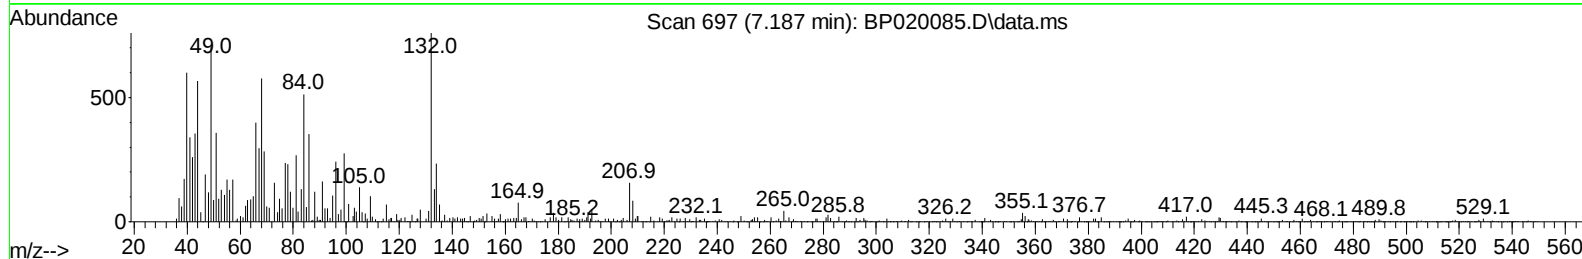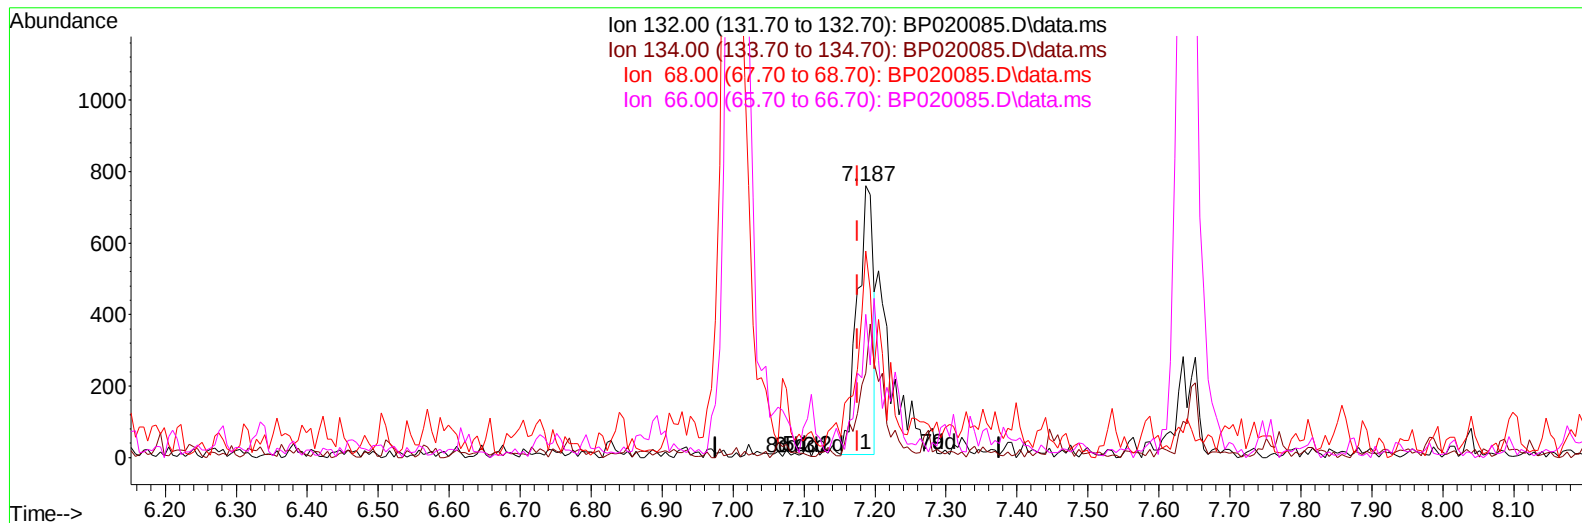

TIC: BP020085.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.187min (+ 0.012) 0.10 ng/u1

response 1168

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.90	30.92
68.00	55.50	76.05#
66.00	40.30	52.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

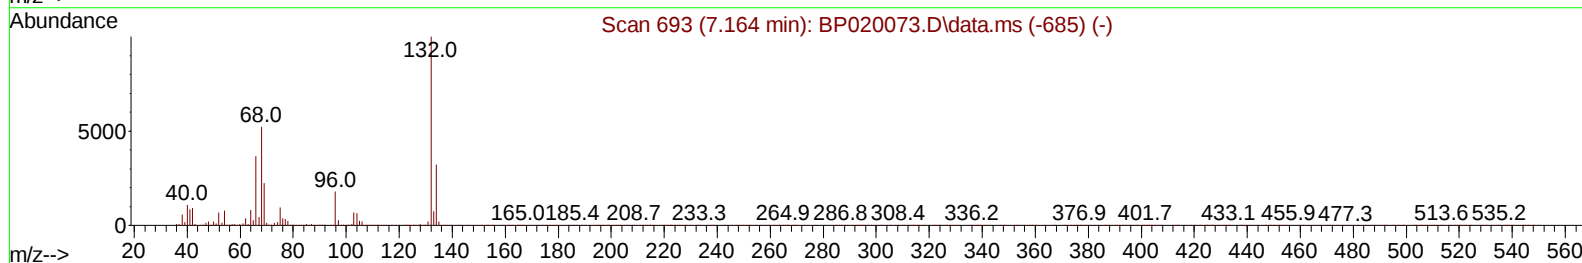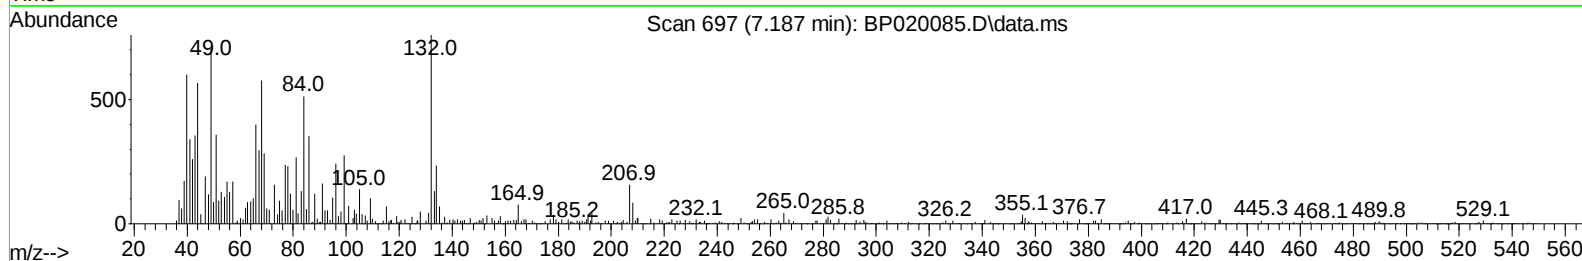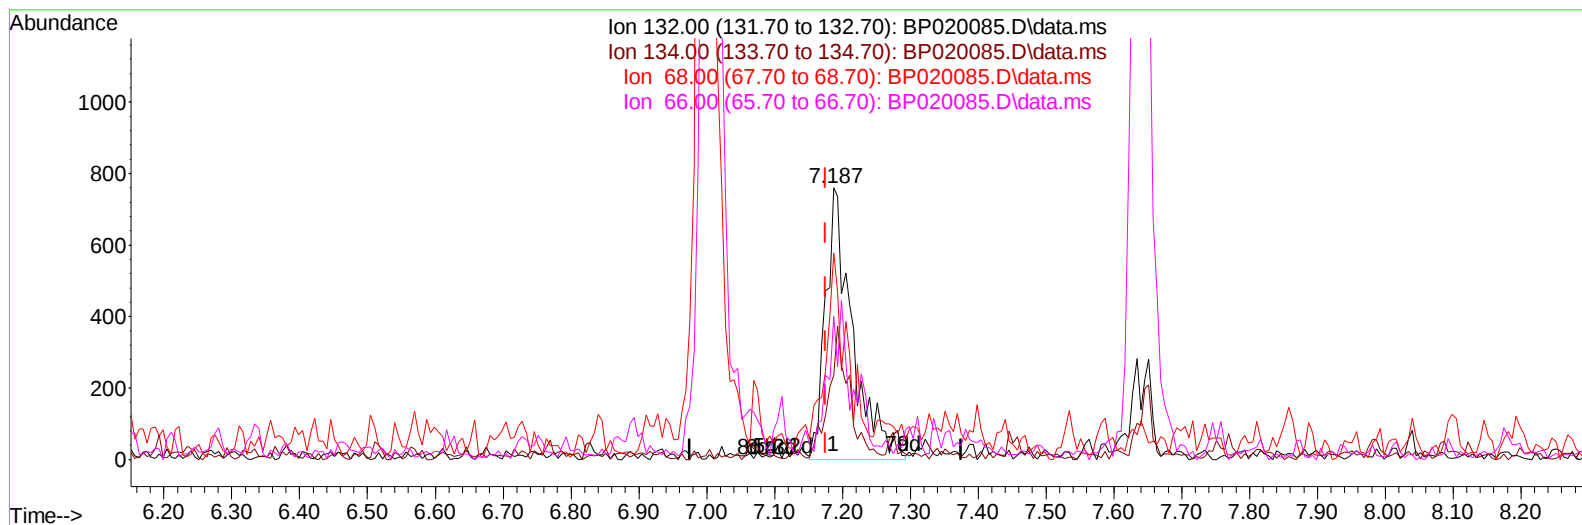

TIC: BP020085.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.187min (+ 0.012) 0.18 ng/ul m

response 2099

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.90	30.92
68.00	55.50	76.05#
66.00	40.30	52.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

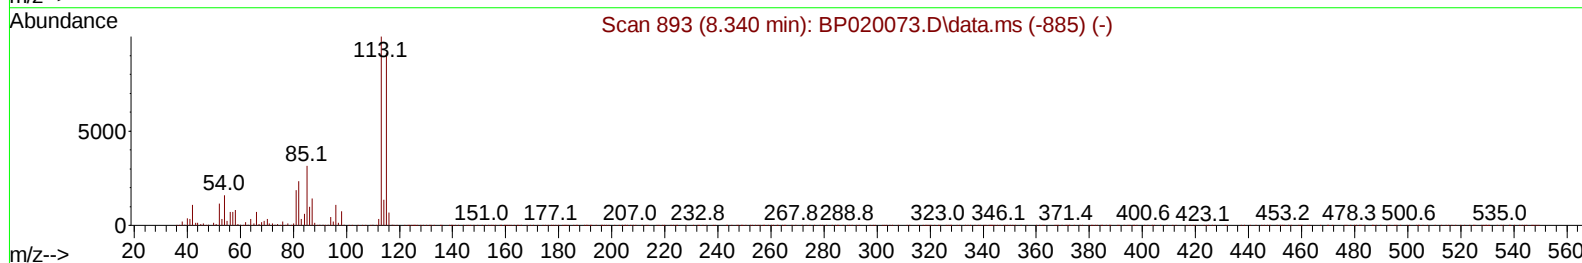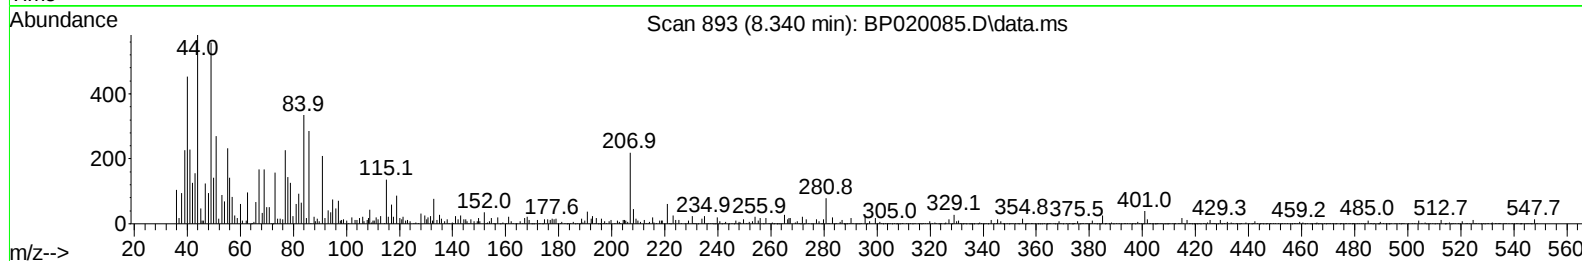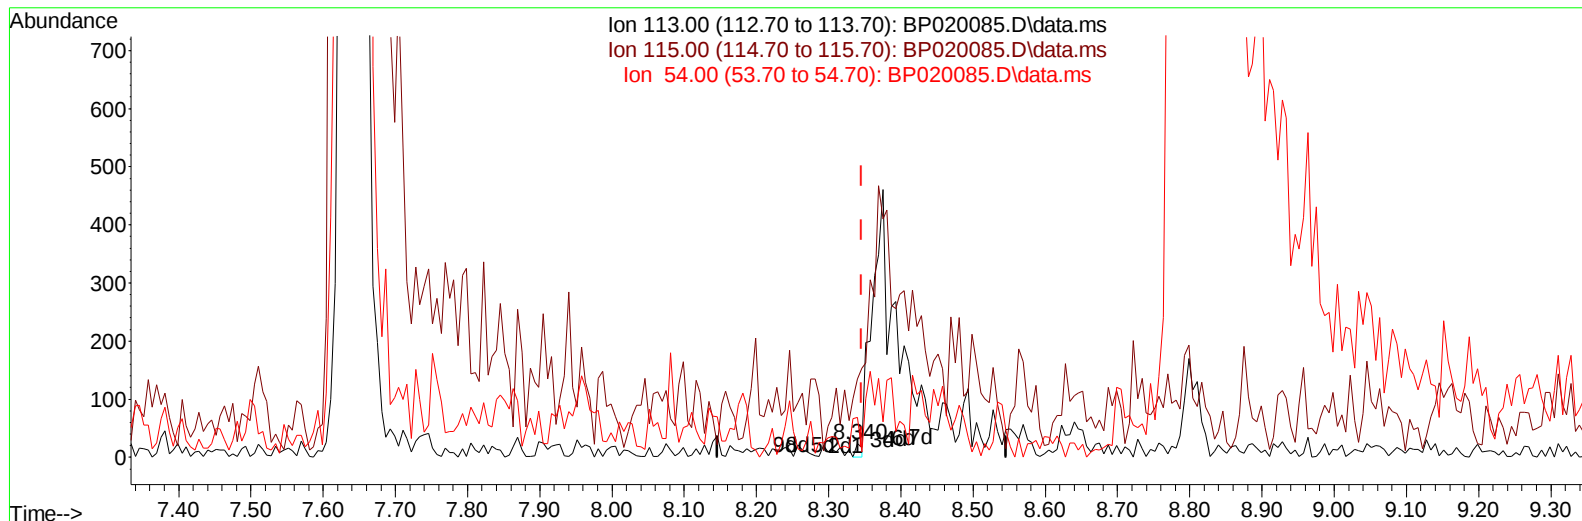

TIC: BP020085.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.340min (-0.006) 0.00 ng/u1

response 14

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	94.50	678.26#
54.00	18.50	300.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

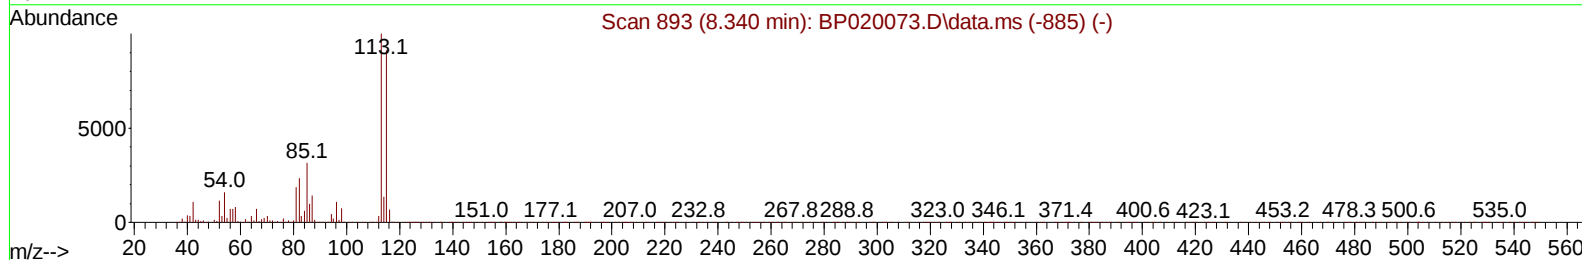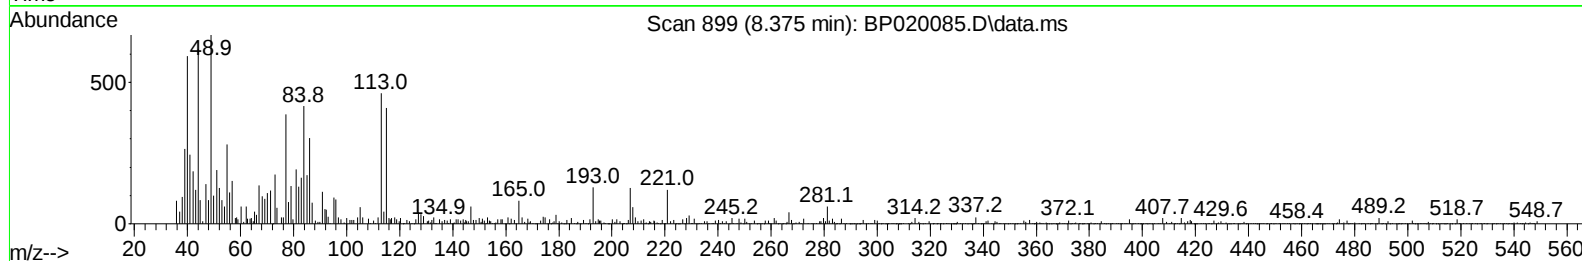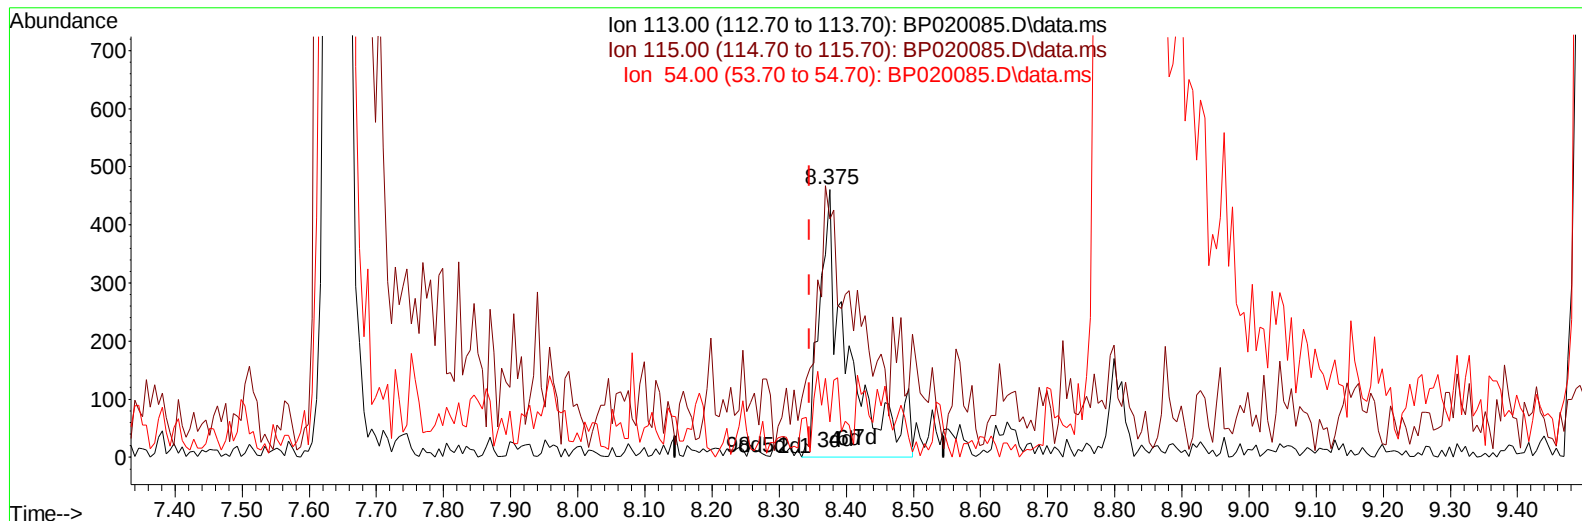

TIC: BP020085.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.375min (+ 0.029) 0.11 ng/ul m

response 1369

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	94.50	88.94
54.00	18.50	13.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

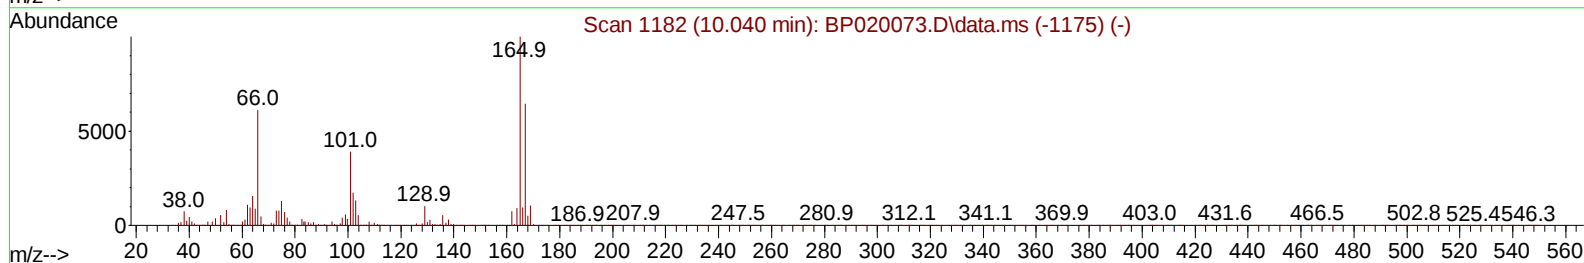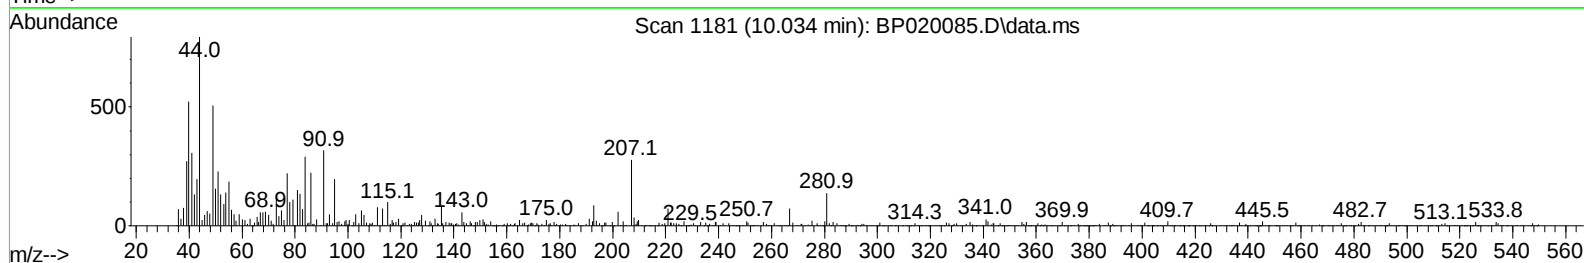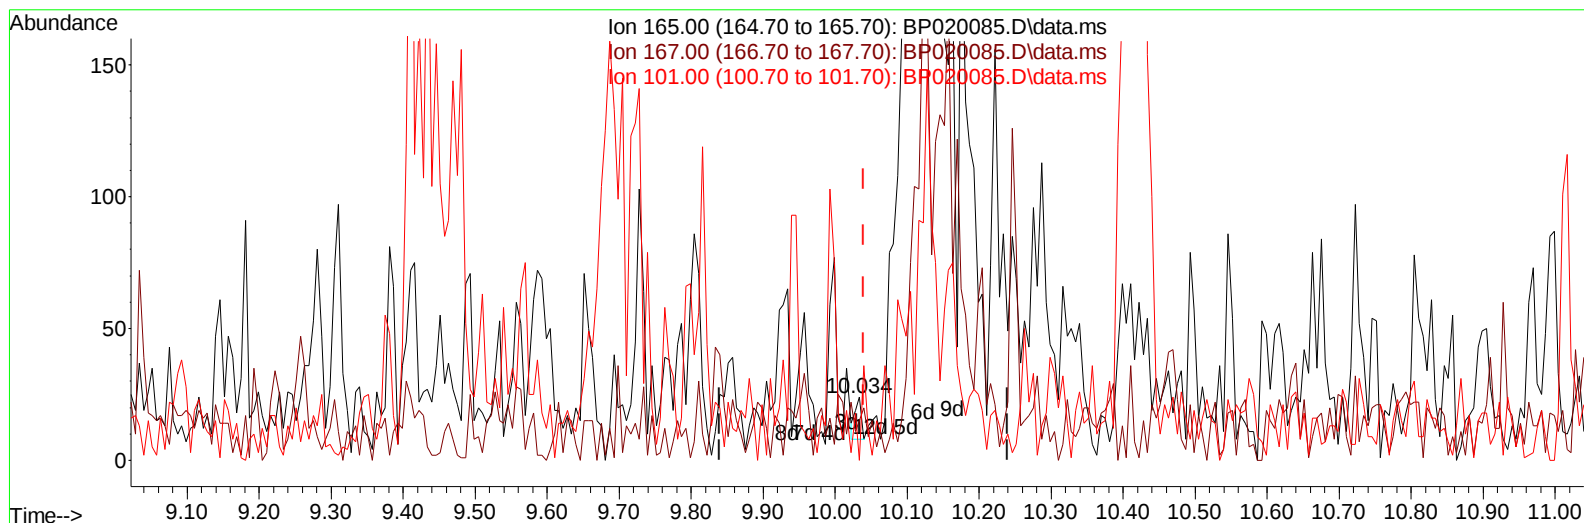

TIC: BP020085.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.034min (-0.006) 0.00 ng/u1

response 10

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	62.50
101.00	40.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

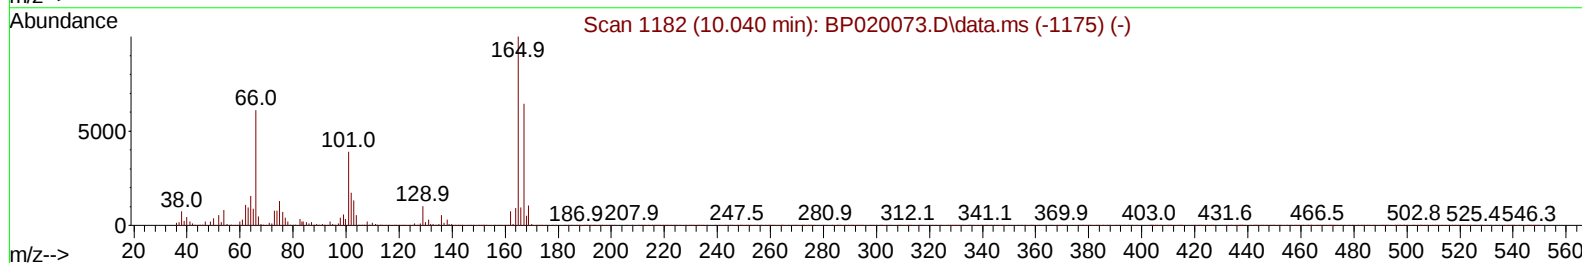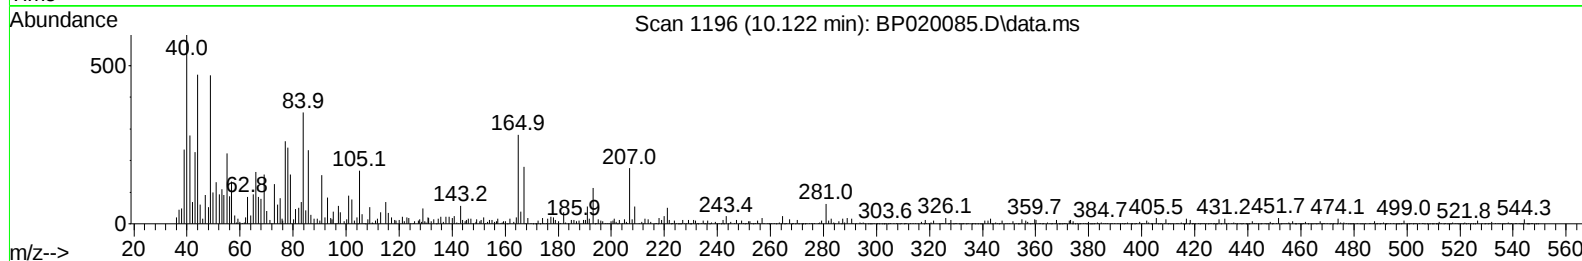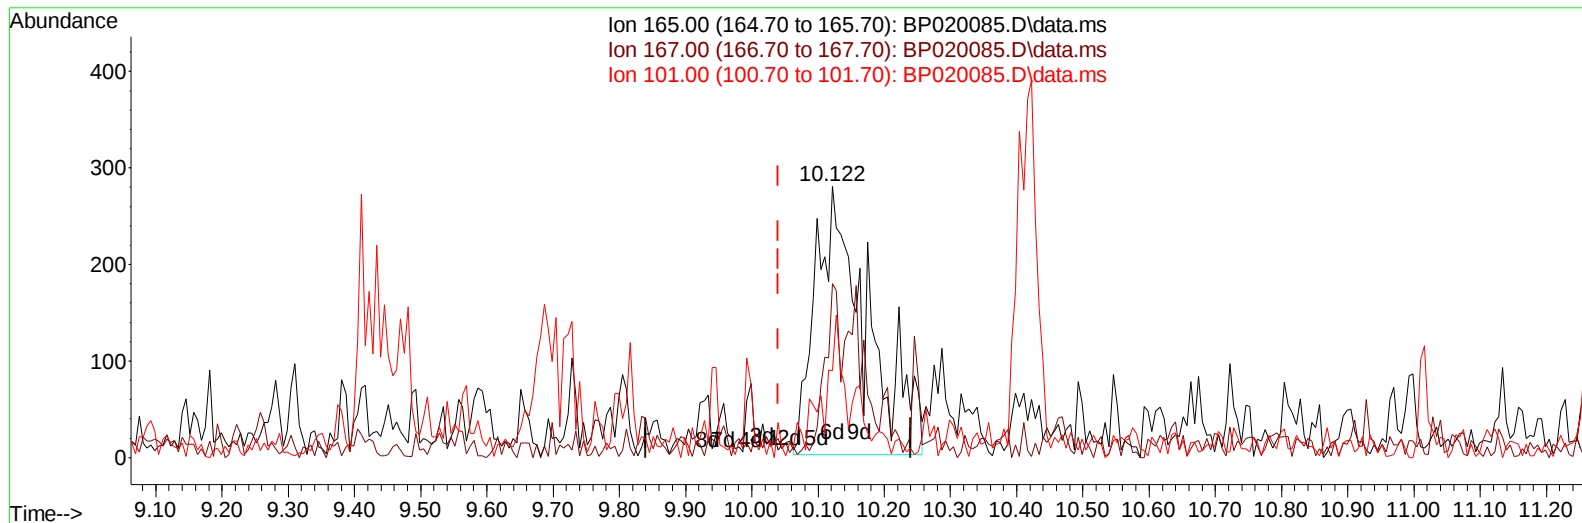

TIC: BP020085.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.122min (+ 0.082) 0.13 ng/ul m

response 1503

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	64.06
101.00	40.90	32.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

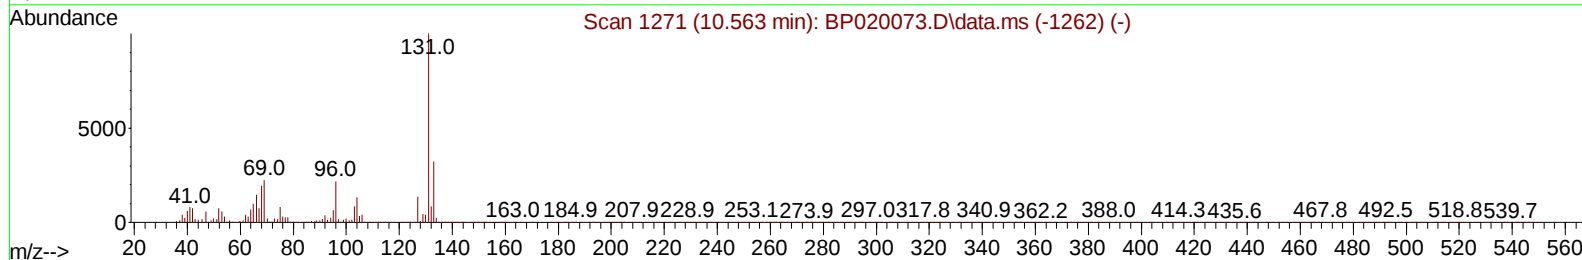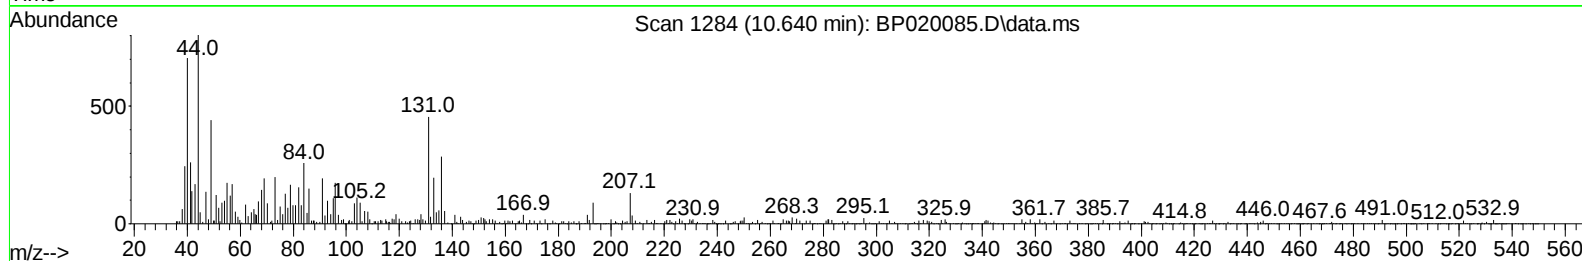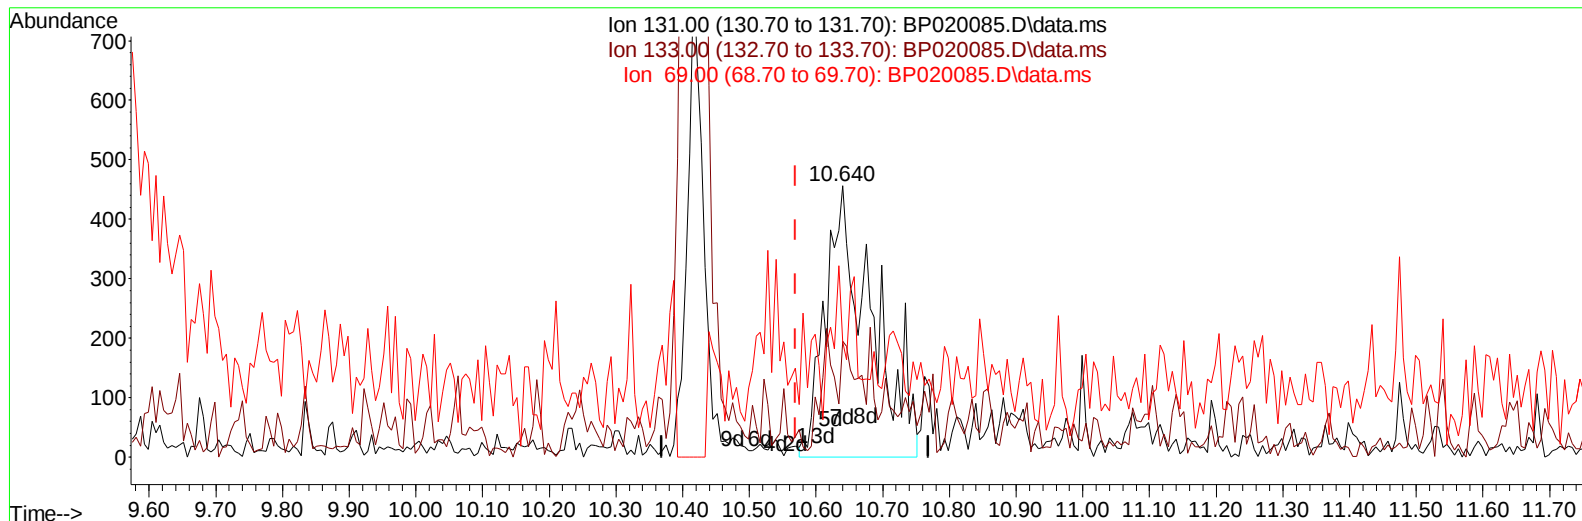

TIC: BP020085.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.640min (+ 0.071) 0.14 ng/ul m

response 2156

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.10	42.76#
69.00	23.50	42.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

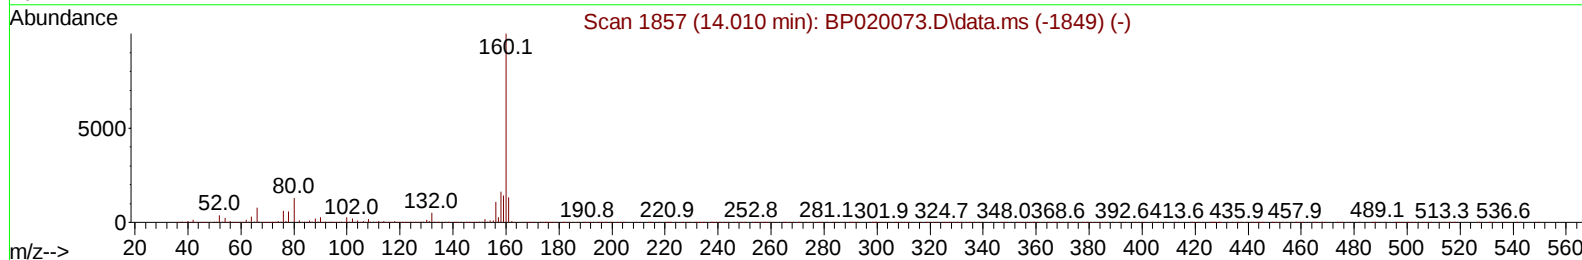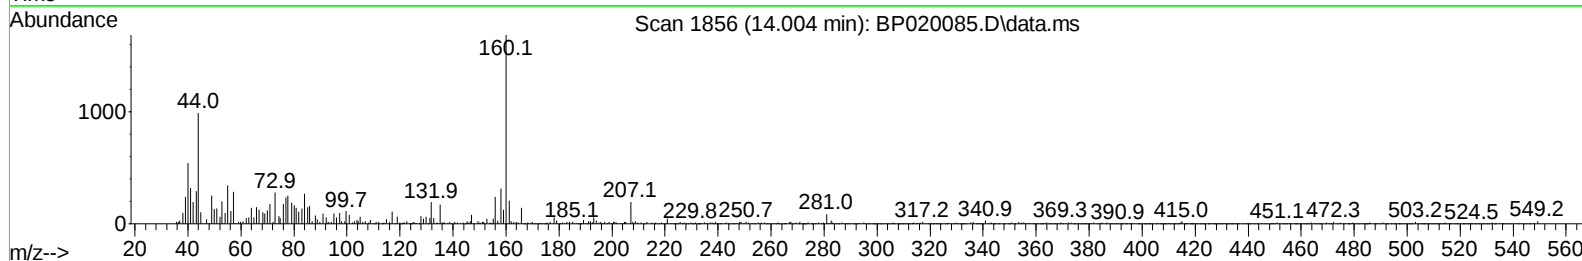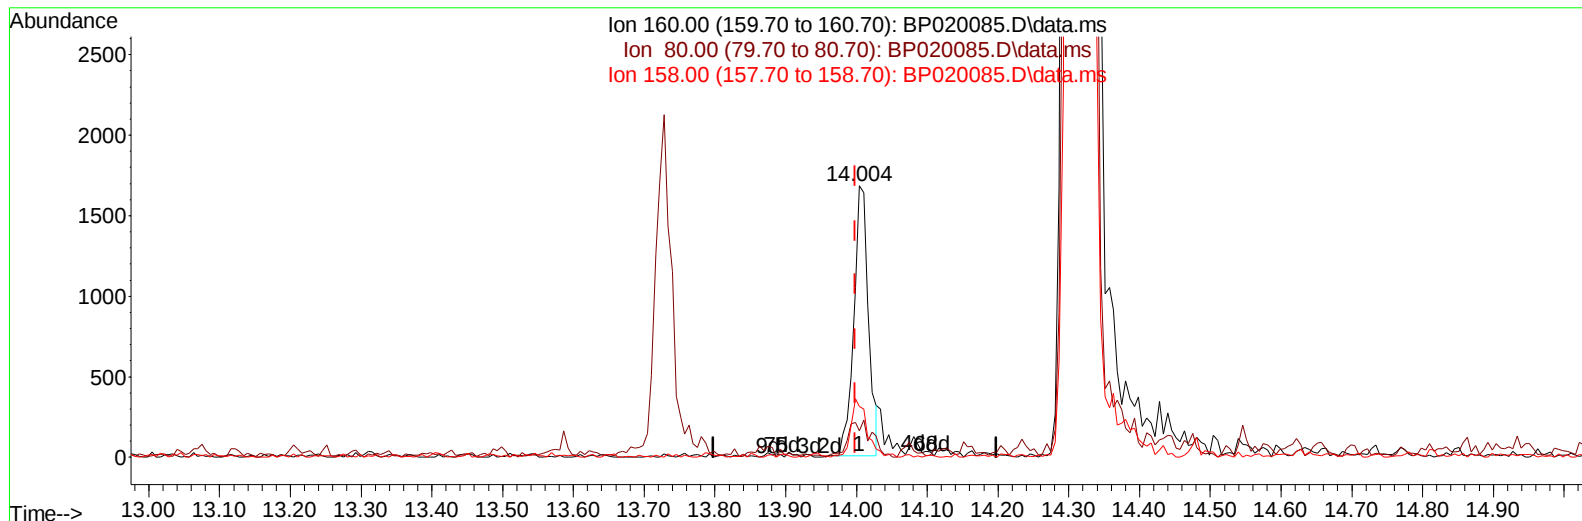

TIC: BP020085.D\data.ms

(49) Acenaphthylene-d8 (S)

14.004min (+ 0.006) 0.07 ng/u1

response 2412

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	12.00	9.67
158.00	15.60	18.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

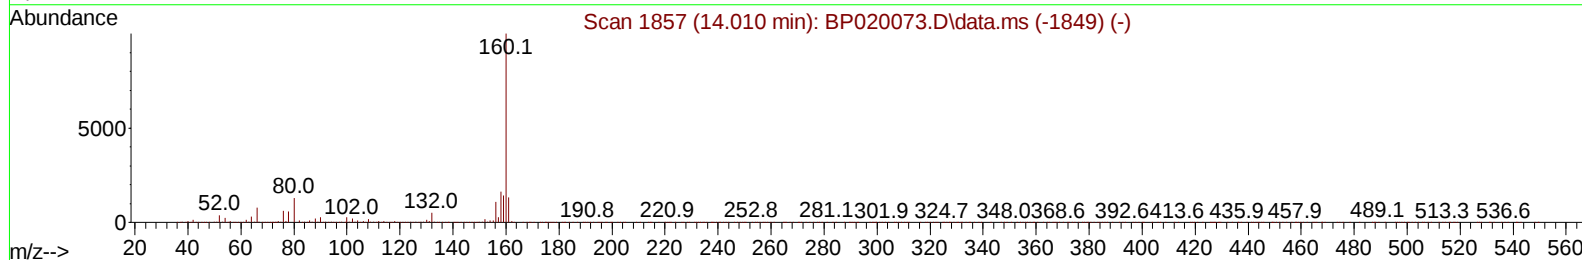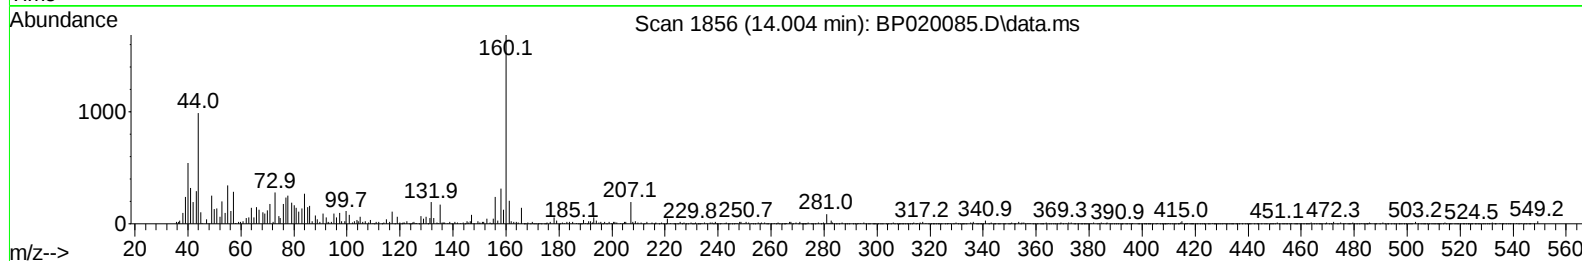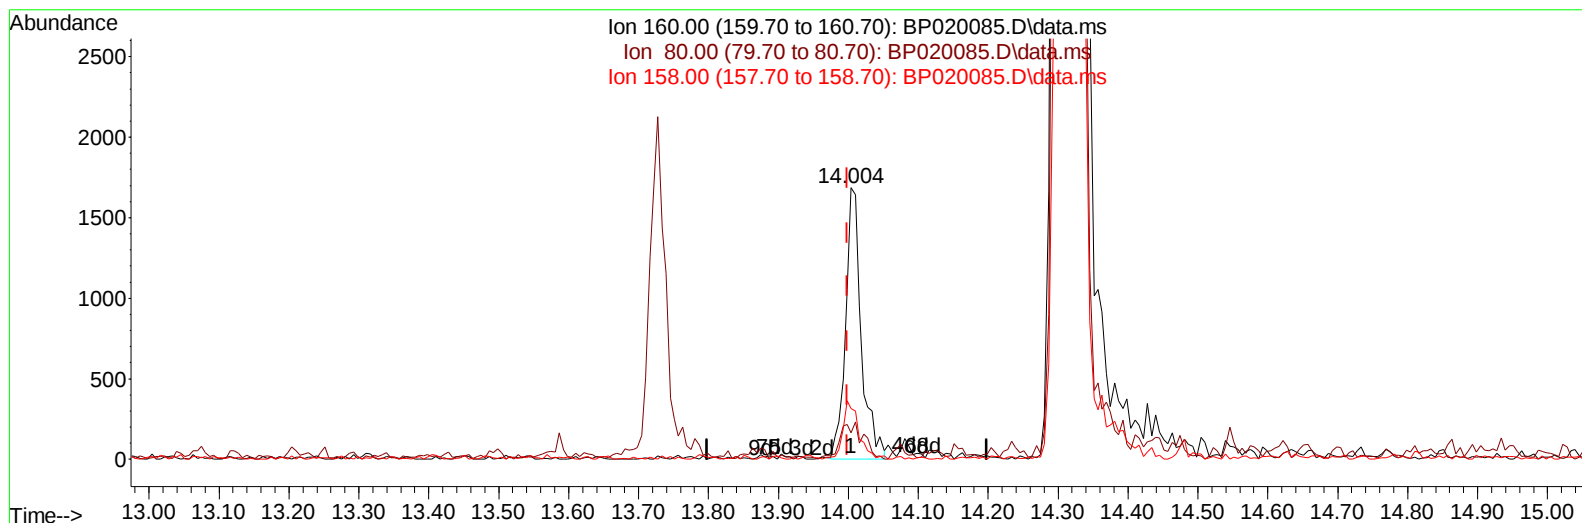

TIC: BP020085.D\data.ms

(49) Acenaphthylene-d8 (S)

14.004min (+ 0.006) 0.08 ng/ul m

response 2645

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	12.00	9.67
158.00	15.60	18.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

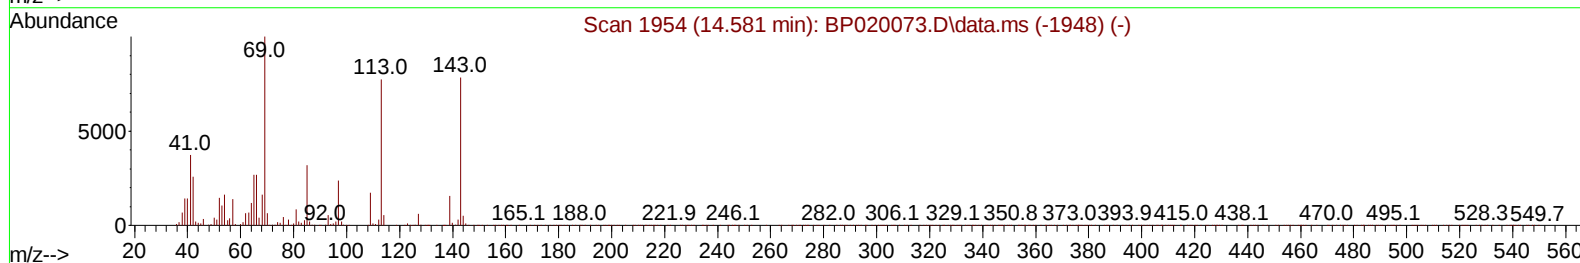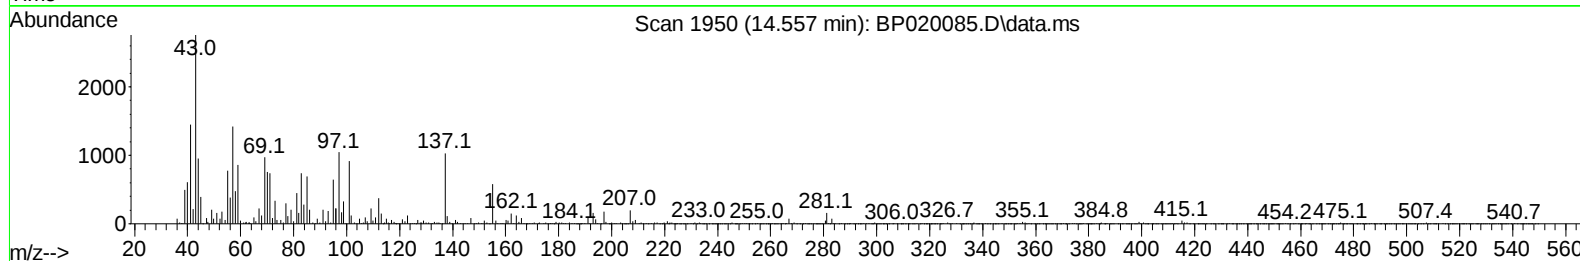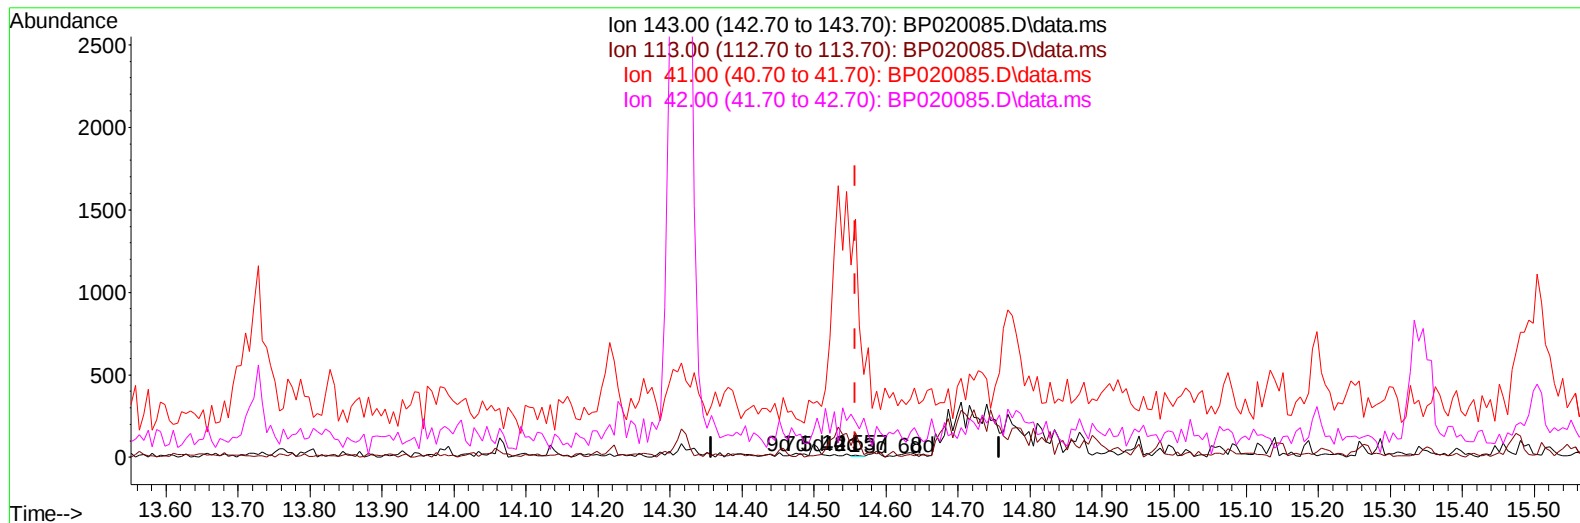

TIC: BP020085.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.000) 0.00 ng/u1

response 6

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	1057.14#
41.00	50.70	10328.57#
42.00	34.00	1542.86#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

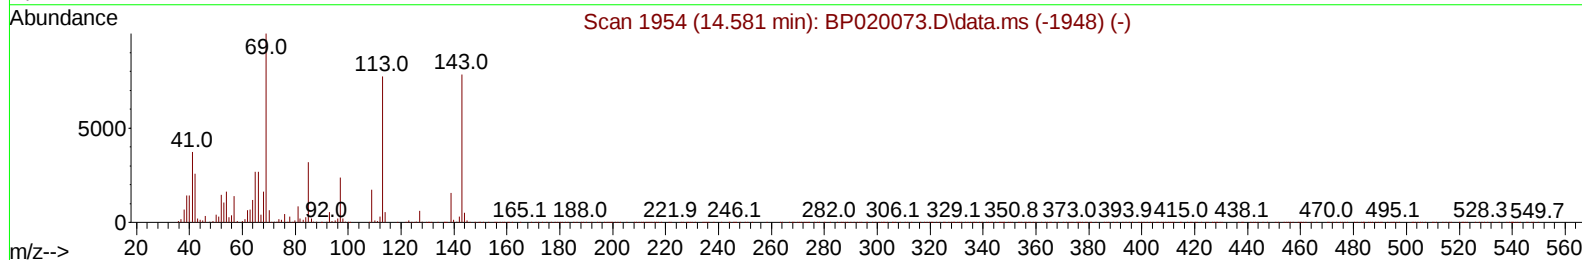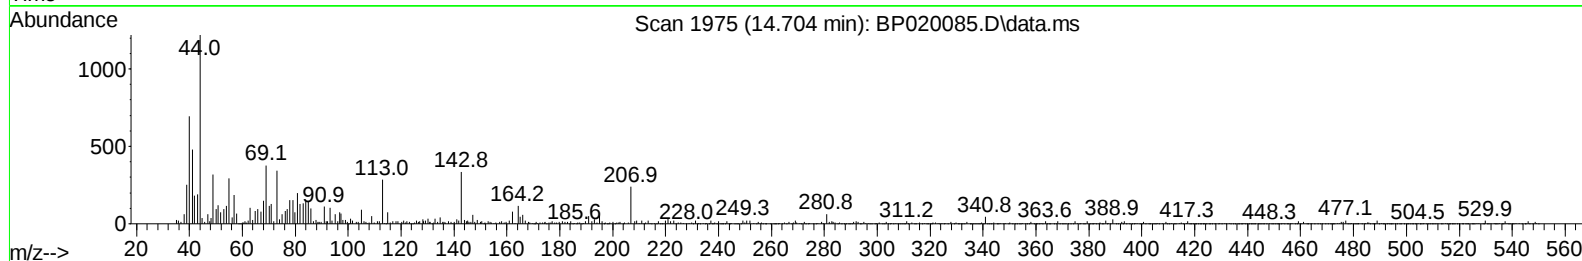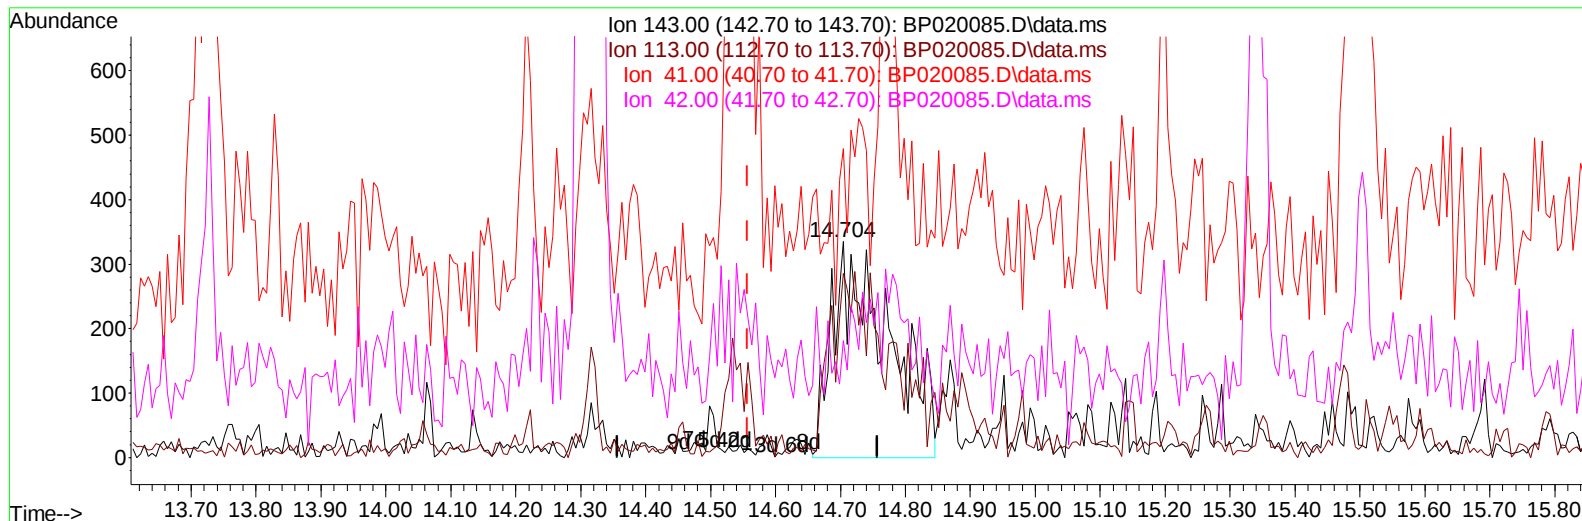

TIC: BP020085.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.704min (+ 0.147) 0.46 ng/ul m

response 2017

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	85.37
41.00	50.70	142.99#
42.00	34.00	54.03#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020085.D
 Acq On : 22 Apr 2024 21:06
 Operator : MA/JU
 Sample : P2104-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

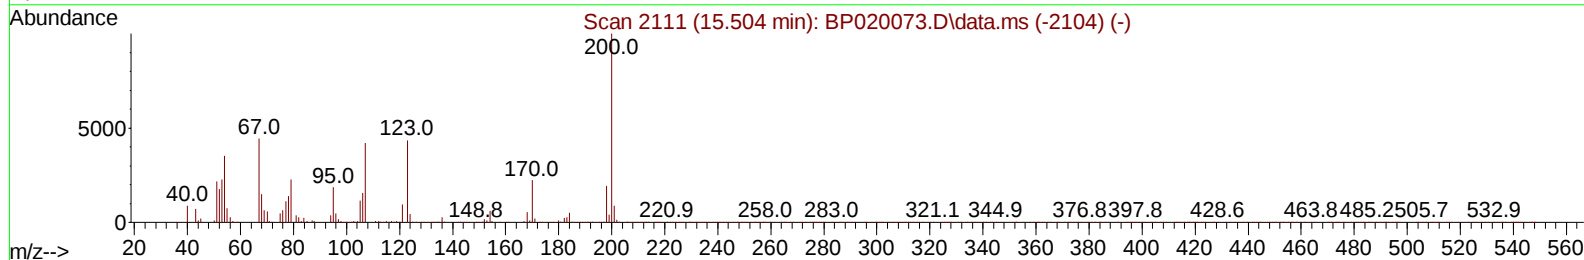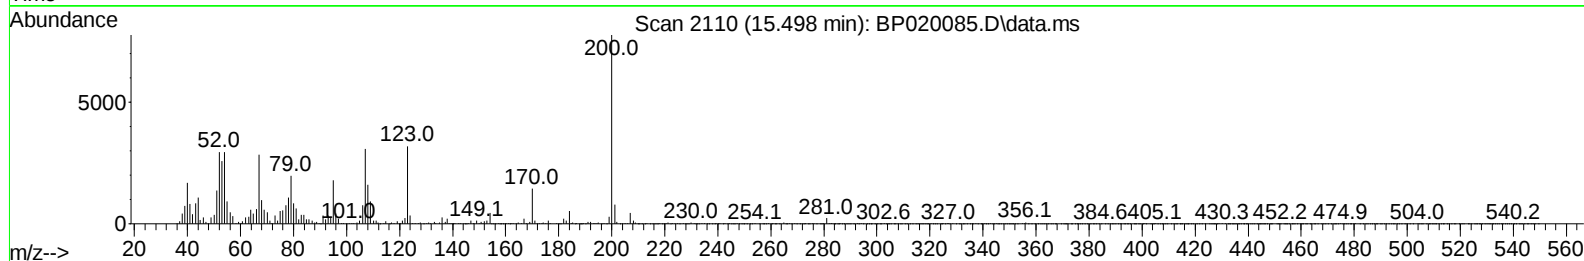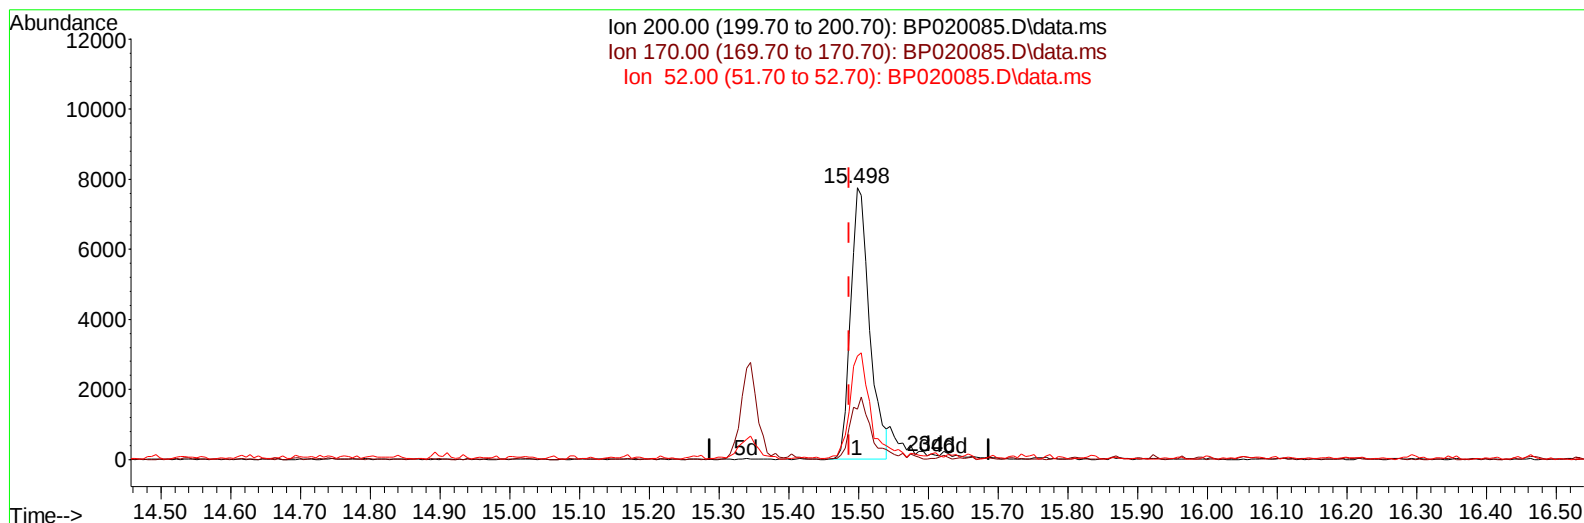

TIC: BP020085.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.498min (+ 0.012) 3.07 ng/u1

response 14620

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	18.59#
52.00	53.50	38.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

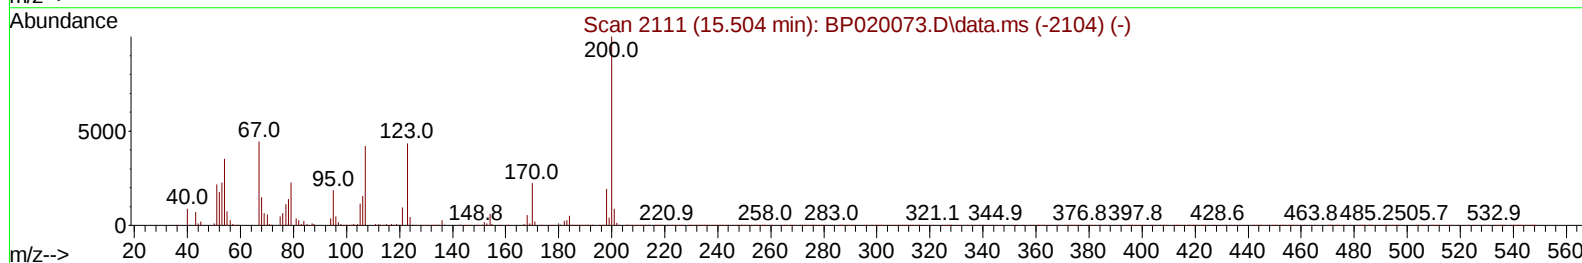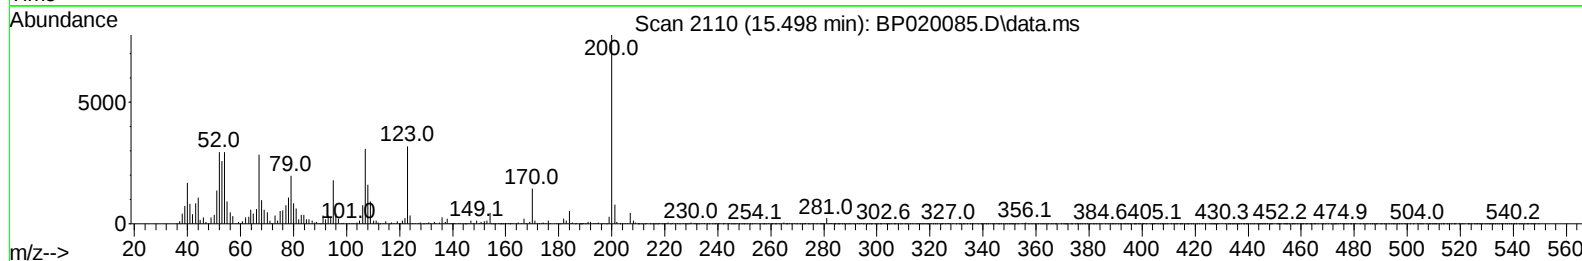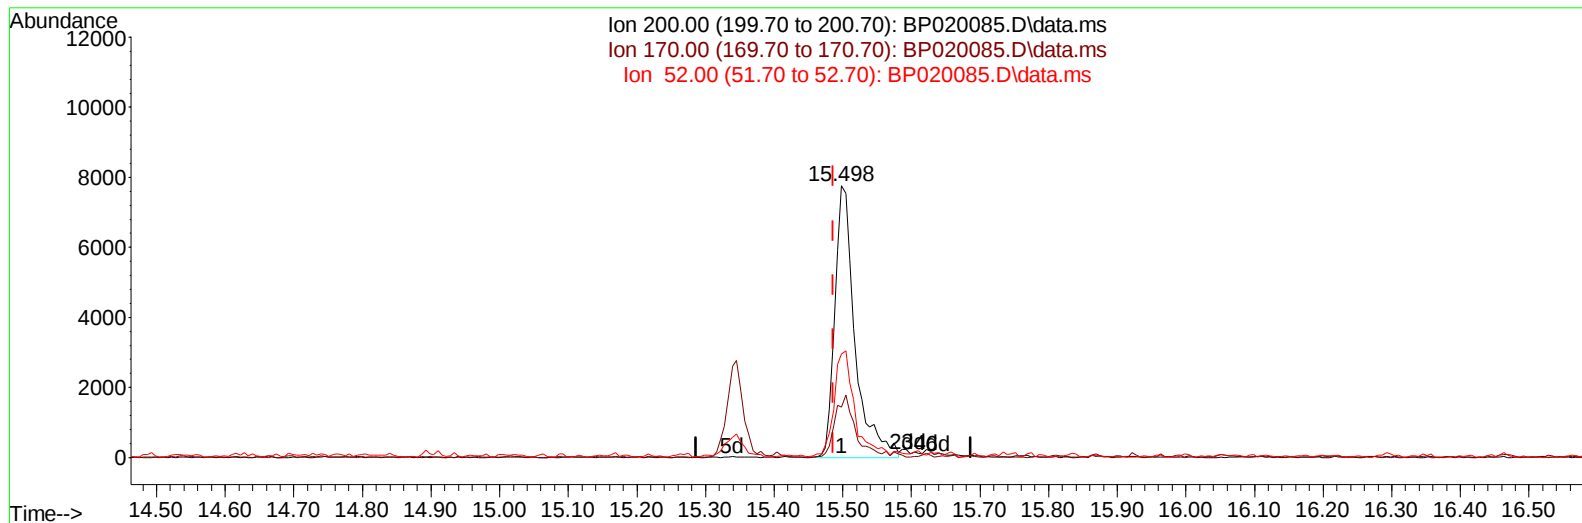

TIC: BP020085.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.498min (+ 0.012) 3.32 ng/ul m

response 15819

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	18.59#
52.00	53.50	38.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

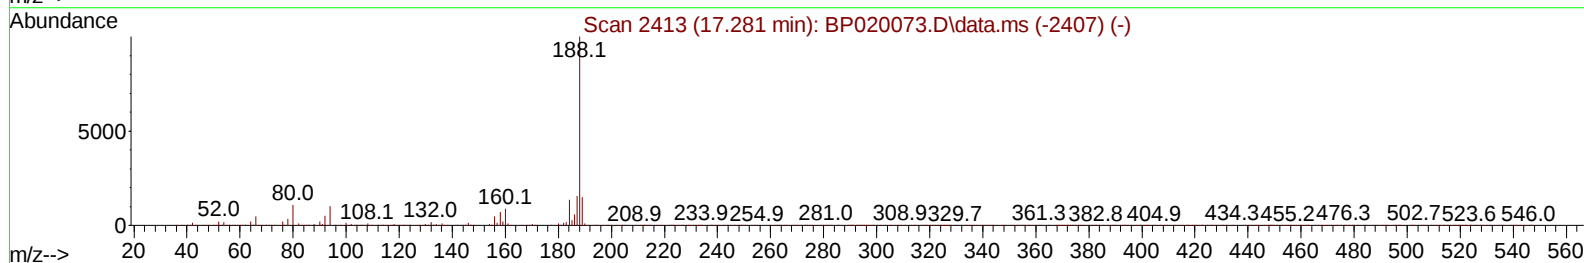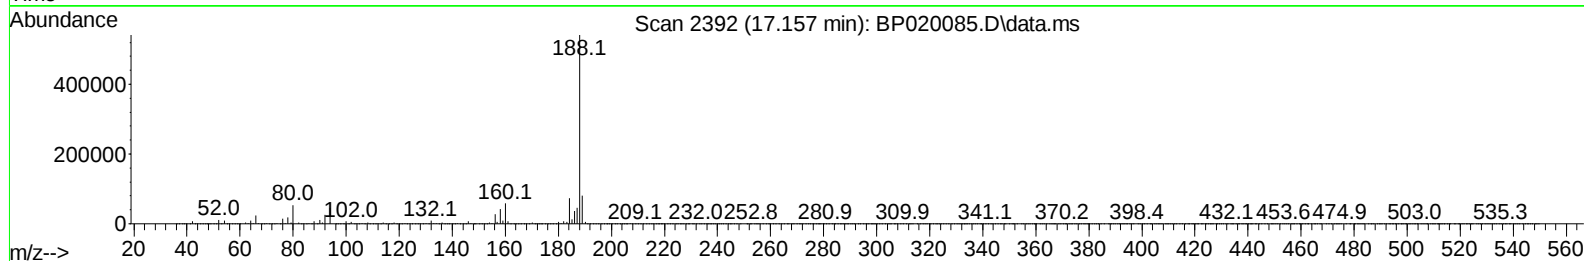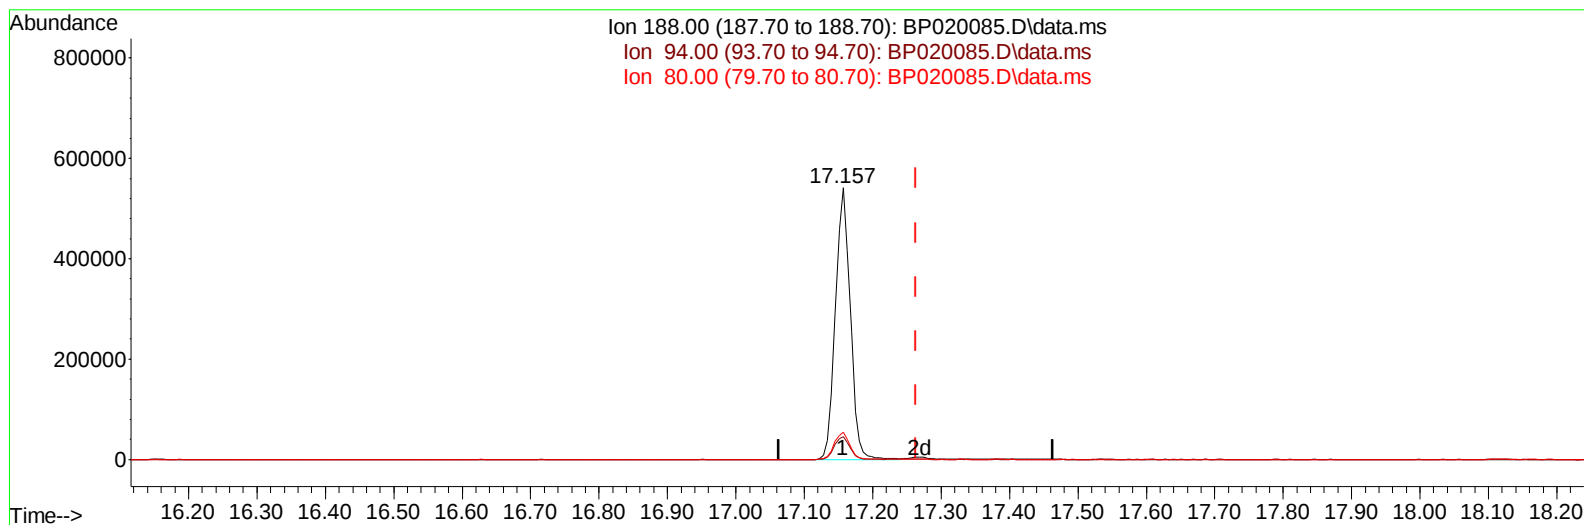

TIC: BP020085.D\data.ms

(73) Anthracene-d10 (S)

17.157min (-0.106) 22.32 ng/u1

response 814940

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.40	8.40
80.00	10.20	9.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

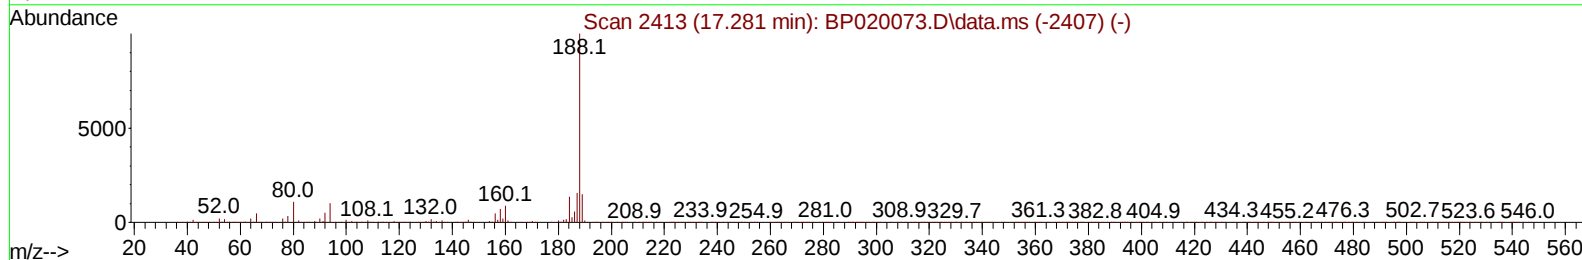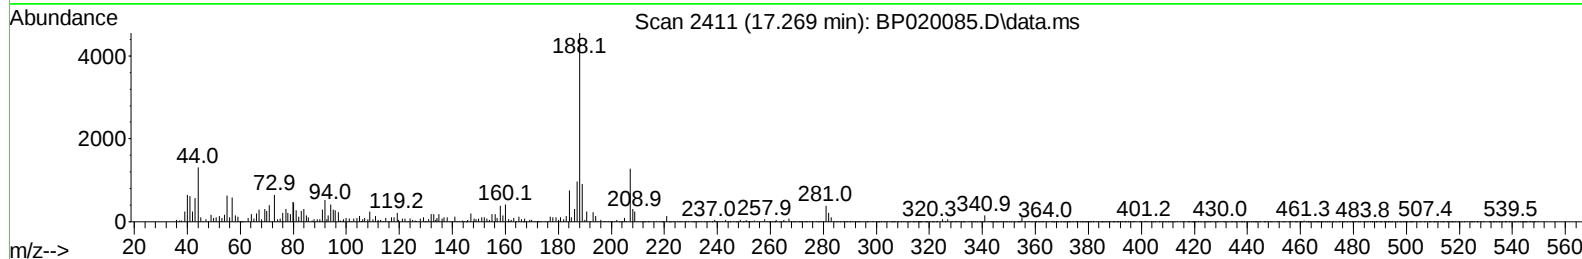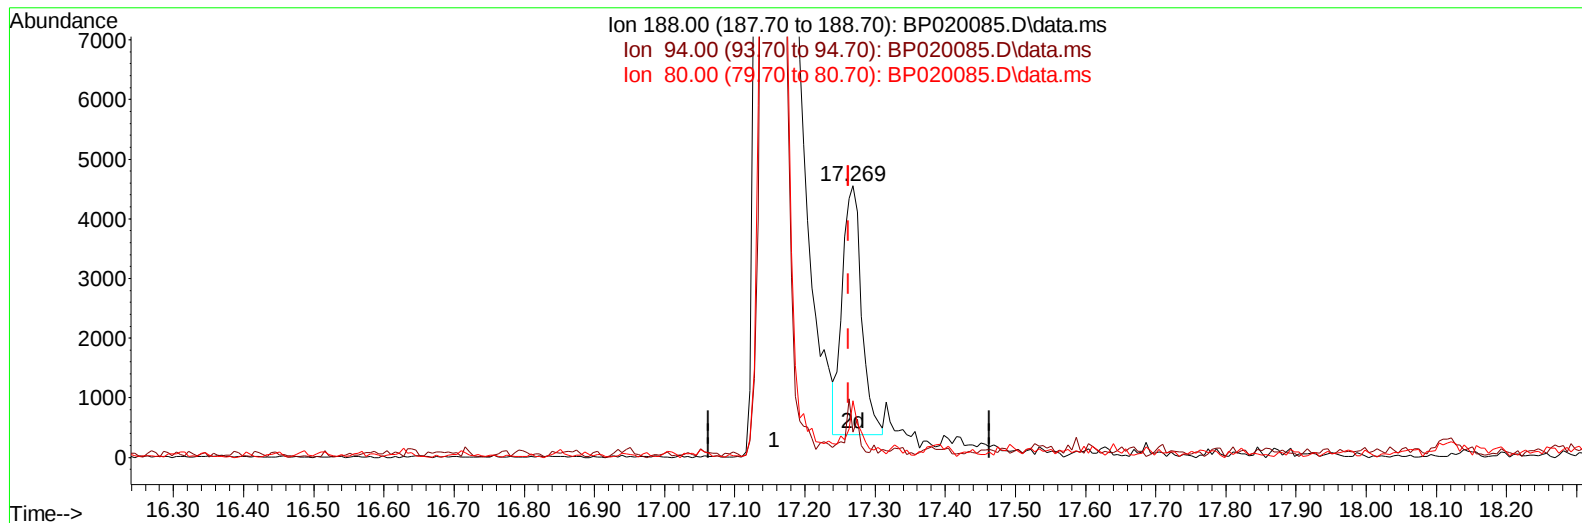

TIC: BP020085.D\data.ms

(73) Anthracene-d10 (S)

17.269min (+ 0.006) 0.22 ng/u1 m

response 7973

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.40	9.23
80.00	10.20	10.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

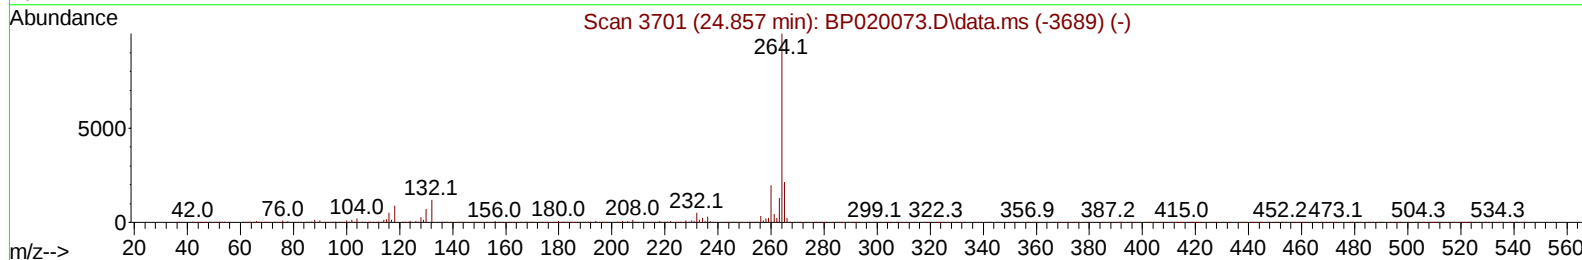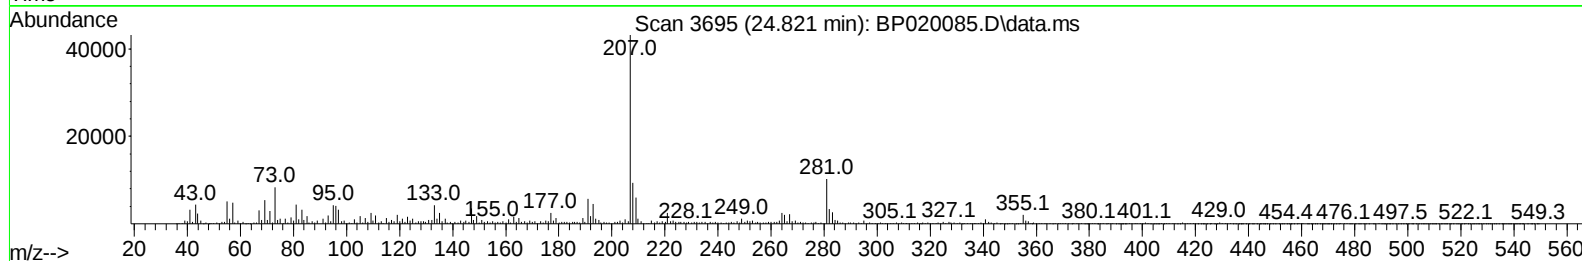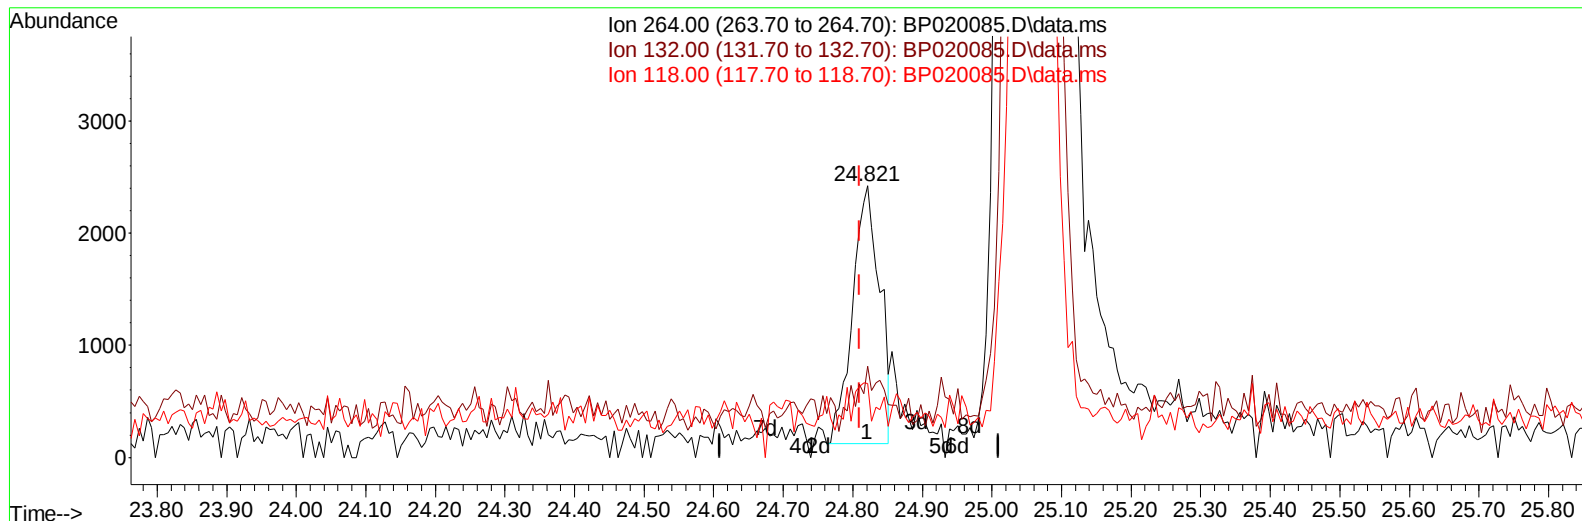

TIC: BP020085.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.821min (+ 0.012) 0.15 ng/u1

response 6190

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	12.10	33.54#
118.00	8.80	27.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 01:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

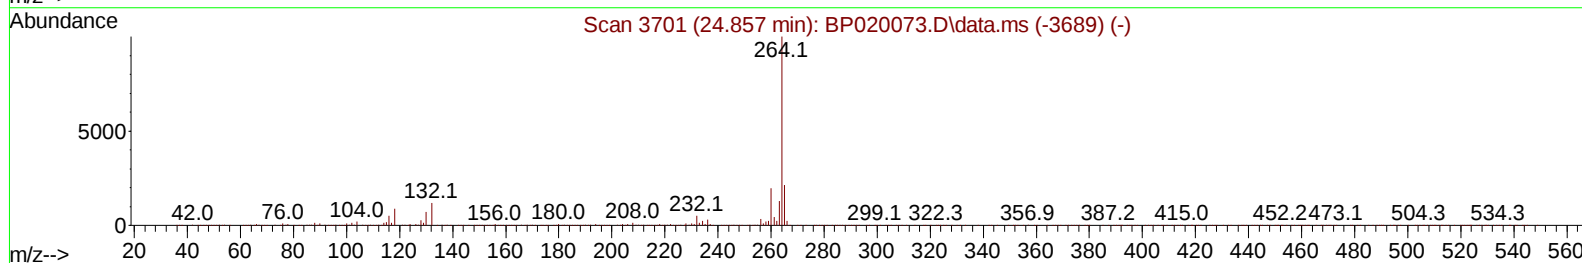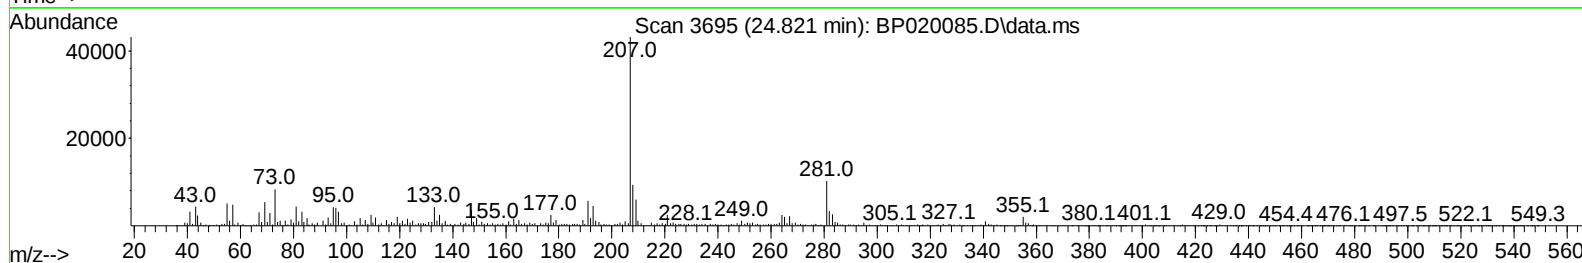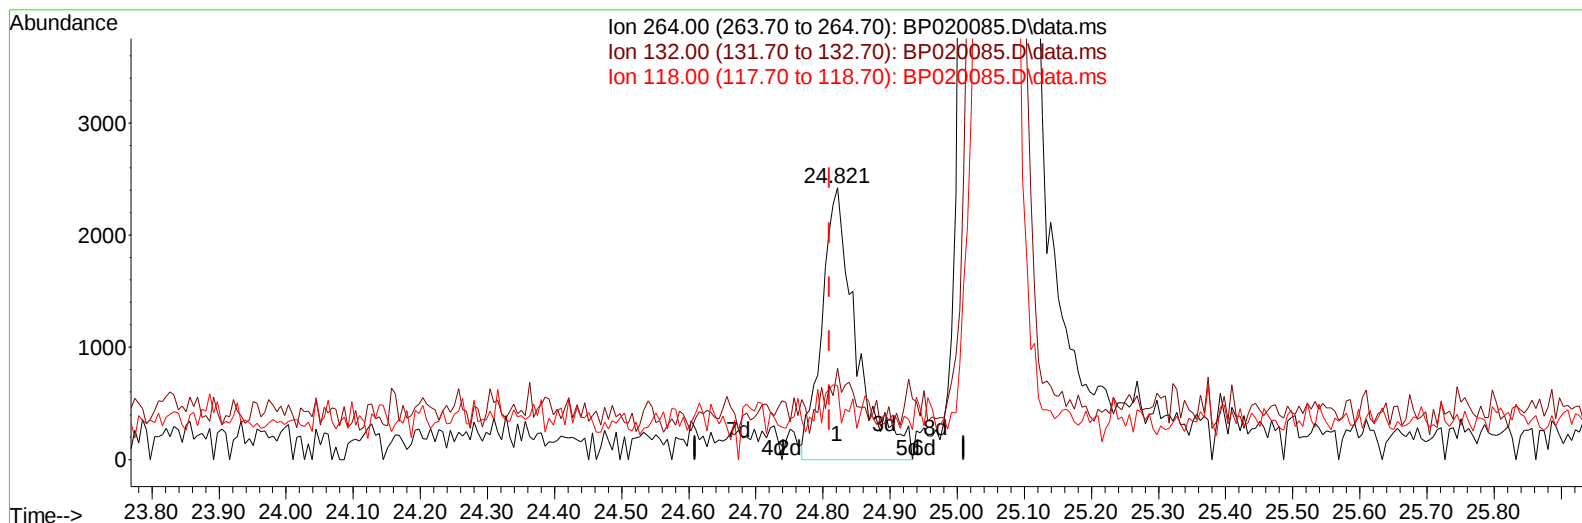

TIC: BP020085.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

24.821min (+ 0.012) 0.21 ng/u1 m

response 8569

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	12.10	33.54#
118.00	8.80	27.26#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020085.D
 Acq On : 22 Apr 2024 21:06
 Operator : MA/JU
 Sample : P2104-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 23 02:19:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	191340	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	753290	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	420036	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	814940	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	770234	20.000	ng/ul	0.00
88) Perylene-d12	25.062	264	849166	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	8233	1.763	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.875	99	621m	0.037	ng/ul	0.05
9) Bis-(2-Chloroethyl)eth...	6.993	67	131734	11.302	ng/ul	0.00
11) 2-Chlorophenol-d4	7.187	132	2099m	0.184	ng/ul	0.01
15) 4-Methylphenol-d8	8.375	113	1369m	0.105	ng/ul	0.03
21) Nitrobenzene-d5	8.799	128	65868	12.156	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	65890	11.250	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	1503m	0.129	ng/ul	0.08
31) 4-Chloroaniline-d4	10.640	131	2156m	0.139	ng/ul	0.07
46) Dimethylphthalate-d6	13.728	166	388747	13.542	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	2645m	0.077	ng/ul	0.00
54) 4-Nitrophenol-d4	14.704	143	2017m	0.462	ng/ul	0.15
60) Fluorene-d10	15.345	176	34487	1.350	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	15819m	3.323	ng/ul	0.01
73) Anthracene-d10	17.269	188	7973m	0.218	ng/ul	0.00
81) Pyrene-d10	19.663	212	6716	0.162	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.821	264	8569m	0.207	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020085.D
Acq On : 22 Apr 2024 21:06
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB0

Manual IntegrationsAPPROVED

Quant Time: Apr 23 02:19:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

