




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020092.D
 Acq On : 23 Apr 2024 02:54
 Operator : MA/JU
 Sample : P2161-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORD7

Manual IntegrationsAPPROVED

Quant Time: Apr 23 04:03:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

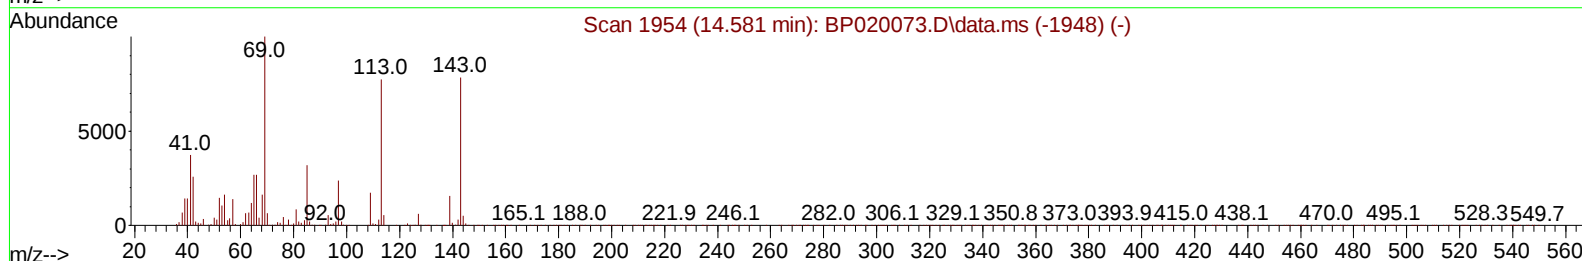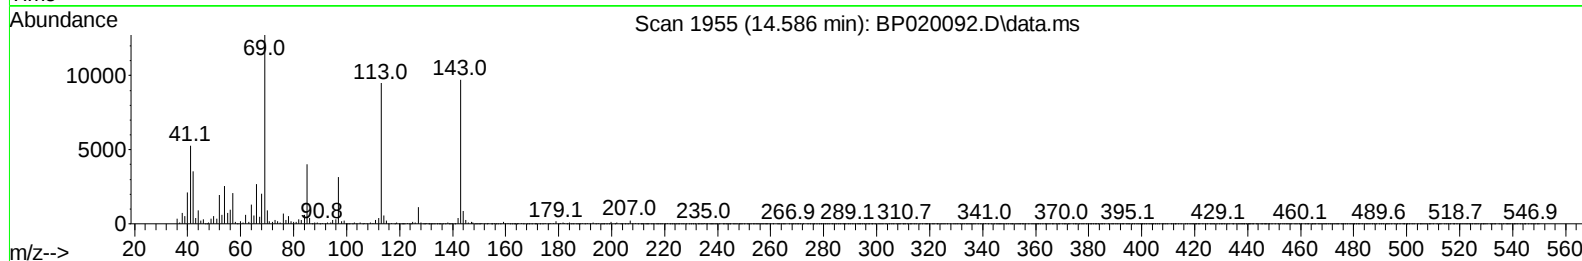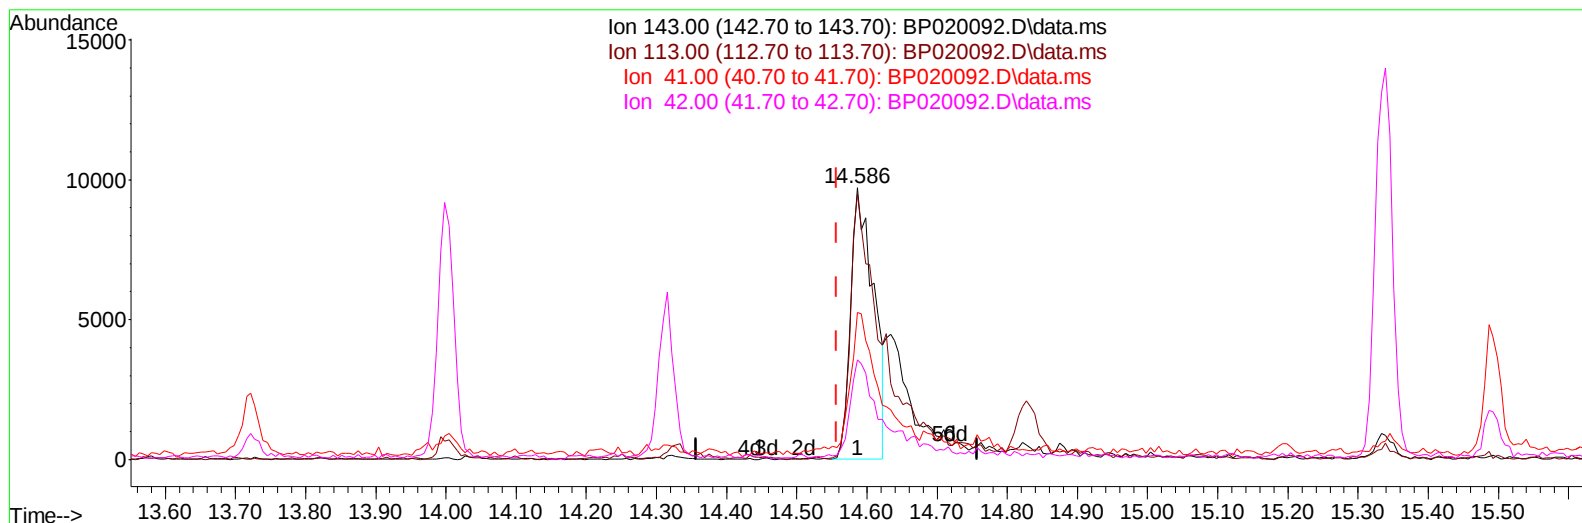

TIC: BP020092.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.029) 8.35 ng/ul

response 22072

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	97.62
41.00	50.70	54.06
42.00	34.00	36.68




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020092.D
 Acq On : 23 Apr 2024 02:54
 Operator : MA/JU
 Sample : P2161-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORD7

Manual IntegrationsAPPROVED

Quant Time: Apr 23 04:03:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

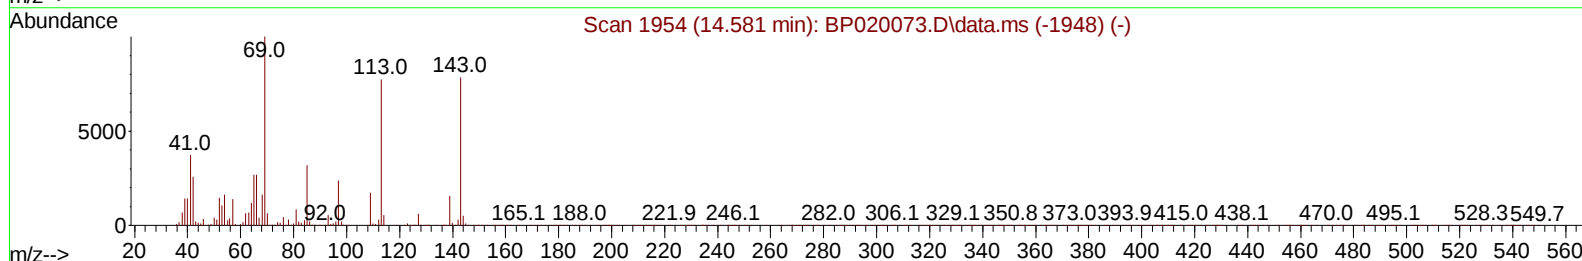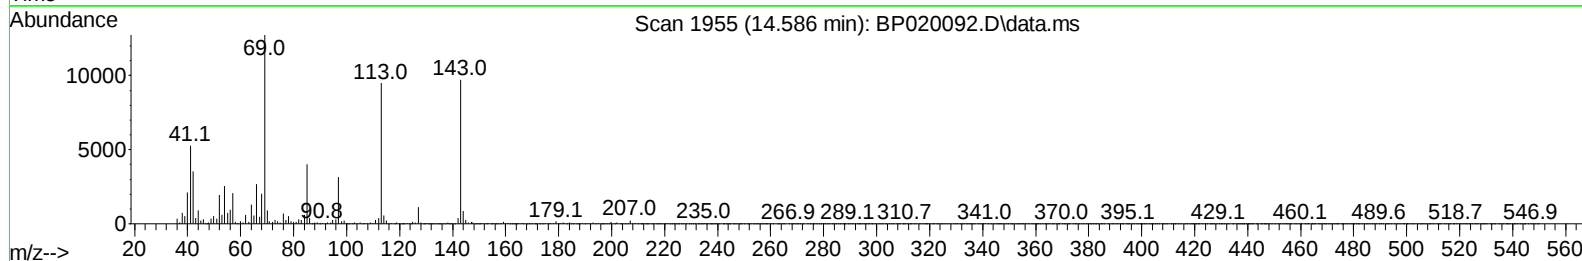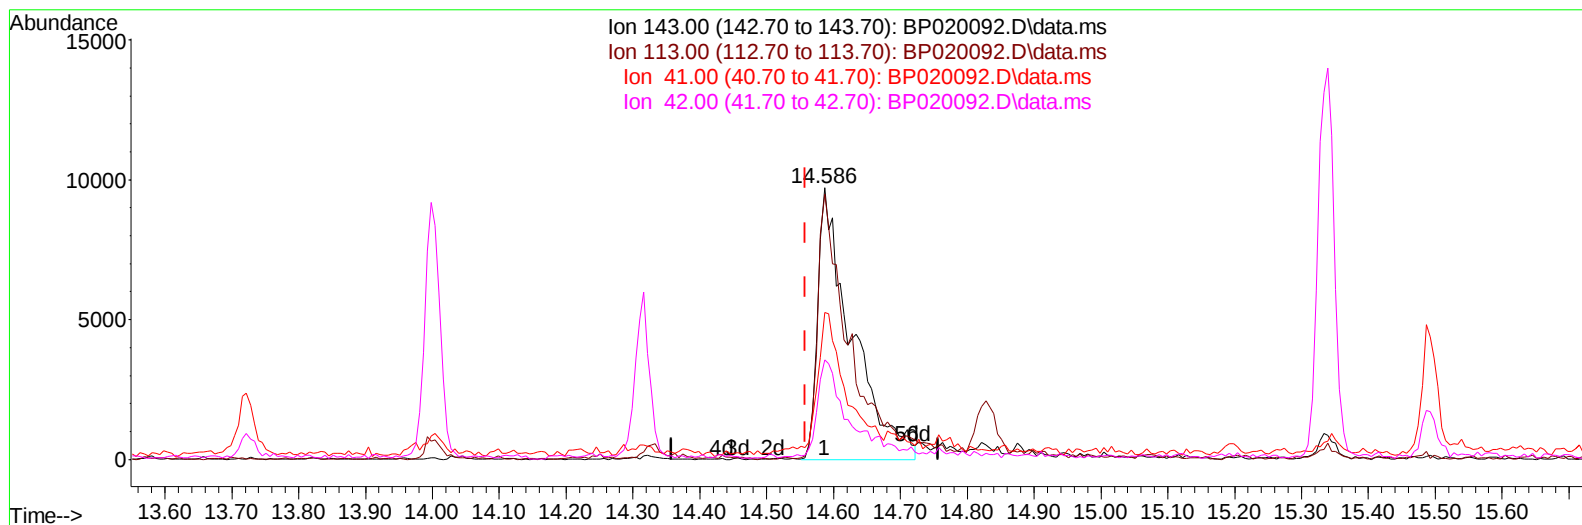

TIC: BP020092.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.029) 12.90 ng/ul m

response 34083

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	97.62
41.00	50.70	54.06
42.00	34.00	36.68

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020092.D
 Acq On : 23 Apr 2024 02:54
 Operator : MA/JU
 Sample : P2161-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORD7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 23 04:04:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	105353	20.000	ng/ul	0.05
20) Naphthalene-d8	10.440	136	392480	20.000	ng/ul	0.03
38) Acenaphthene-d10	14.316	164	253987	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	570477	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	545278	20.000	ng/ul	0.00
88) Perylene-d12	25.045	264	587676	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	16005	6.225	ng/uL	0.00
4) Pyridine-d5	3.640	84	120356	15.903	ng/ul	0.00
7) Phenol-d5	6.828	99	107888	11.750	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.010	67	310432	48.370	ng/ul	0.02
11) 2-Chlorophenol-d4	7.187	132	257799	41.121	ng/ul	0.01
15) 4-Methylphenol-d8	8.357	113	177349	24.727	ng/ul	0.01
21) Nitrobenzene-d5	8.804	128	164783	58.368	ng/ul	0.00
24) 2-Nitrophenol-d4	9.516	143	179311	58.758	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.057	165	297857	49.200	ng/ul	0.02
31) 4-Chloroaniline-d4	10.581	131	353553	43.747	ng/ul	0.01
46) Dimethylphthalate-d6	13.722	166	909295	52.385	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	1097126	53.030	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	34083m	12.899	ng/ul	0.03
60) Fluorene-d10	15.339	176	836339	54.127	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	81102	24.335	ng/ul	0.00
73) Anthracene-d10	17.263	188	1380480	54.014	ng/ul	0.00
81) Pyrene-d10	19.657	212	1686258	57.544	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.821	264	1597232	55.637	ng/ul	0.01
Target Compounds						
						Qvalue
30) Naphthalene	10.481	128	35093	1.724	ng/ul	97
39) 1,2,4,5-Tetrachloroben...	12.463	216	712036	86.022	ng/ul#	94
75) 1,2,3,4-Tetrachloroben...	13.086	216	1347568	148.996	ng/uL	97
76) Pentachlorobenzene	14.639	250	18920	2.223	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020092.D
Acq On : 23 Apr 2024 02:54
Operator : MA/JU
Sample : P2161-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0RD7

Manual IntegrationsAPPROVED

Quant Time: Apr 23 04:04:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

