




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020093.D
Acq On : 23 Apr 2024 03:37
Operator : MA/JU
Sample : P2184-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R94

Manual IntegrationsAPPROVED

Quant Time: Apr 23 04:06:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

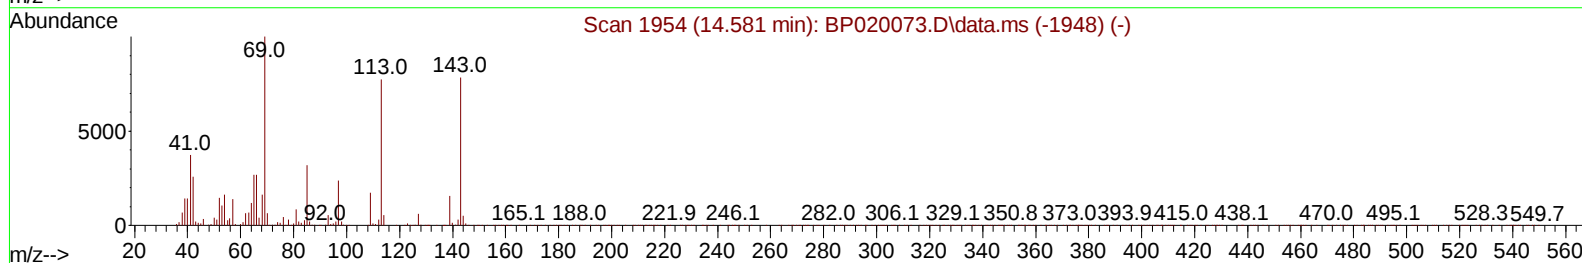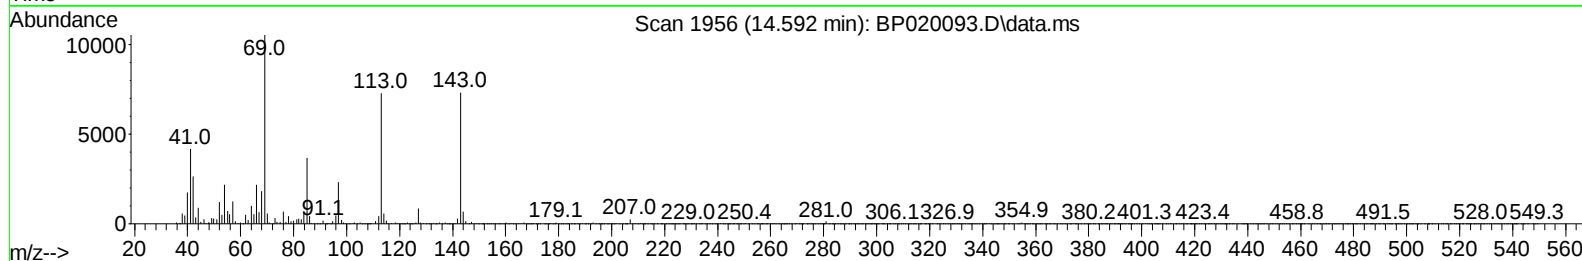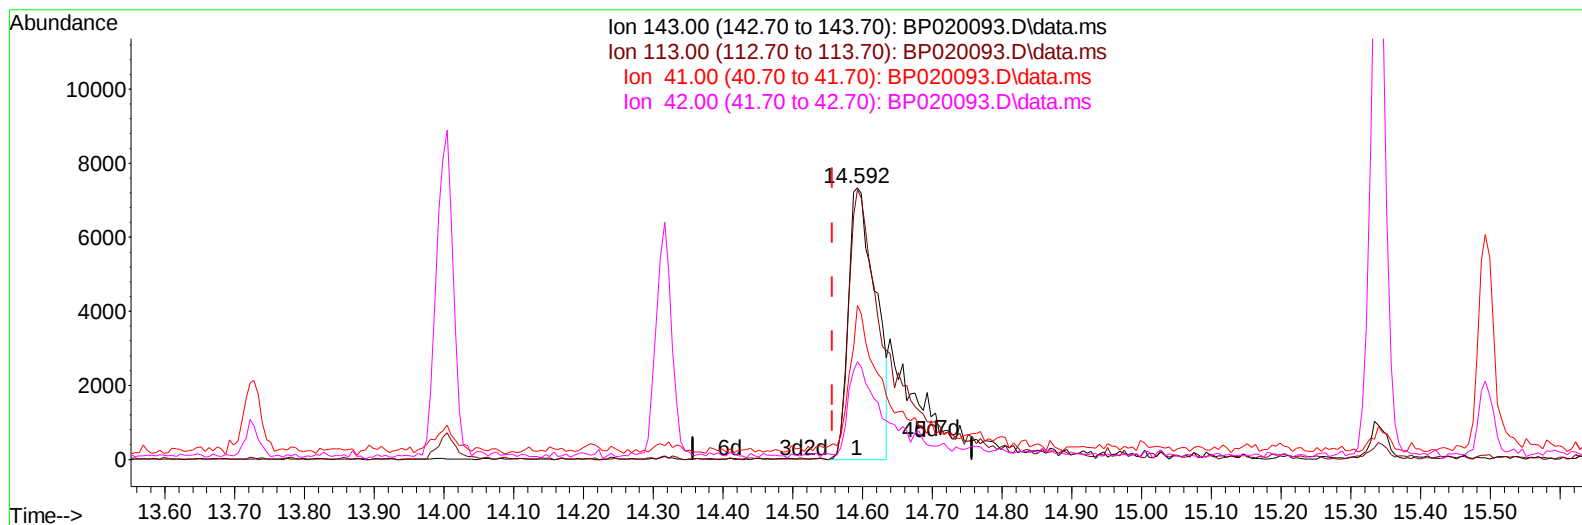

TIC: BP020093.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.592min (+ 0.035) 6.54 ng/u1

response 19796

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	99.36
41.00	50.70	56.81
42.00	34.00	35.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020093.D
Acq On : 23 Apr 2024 03:37
Operator : MA/JU
Sample : P2184-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R94

Manual IntegrationsAPPROVED

Quant Time: Apr 23 04:06:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

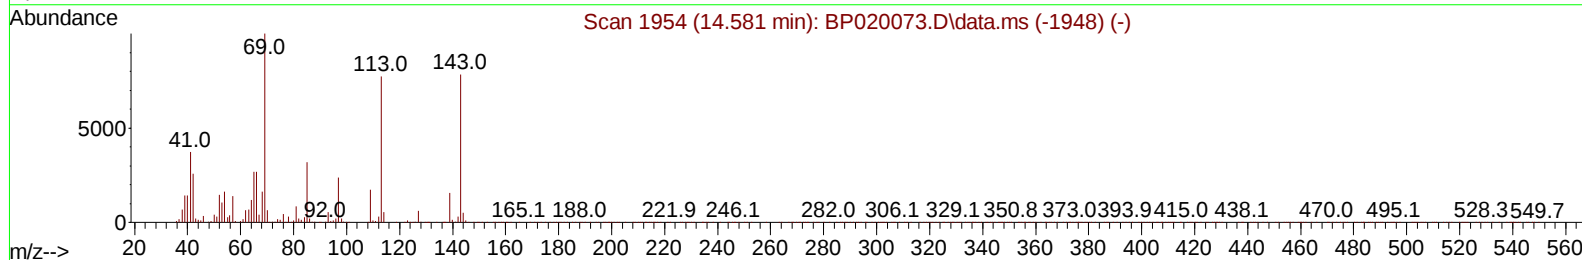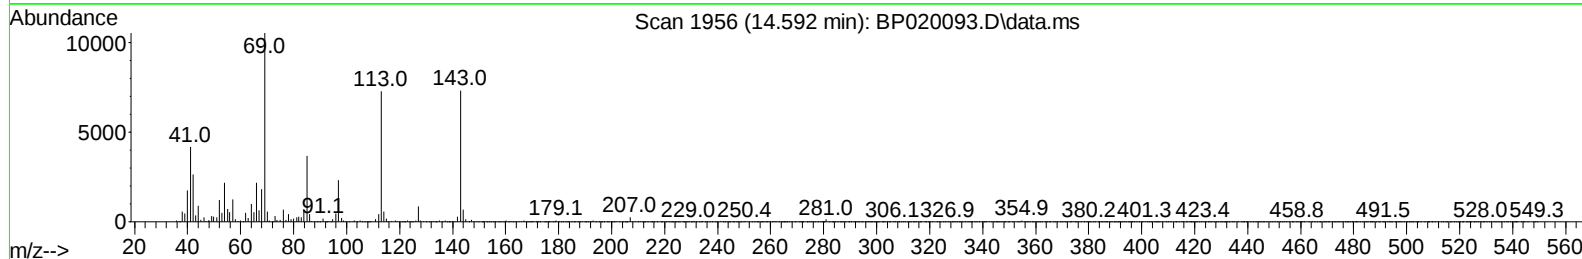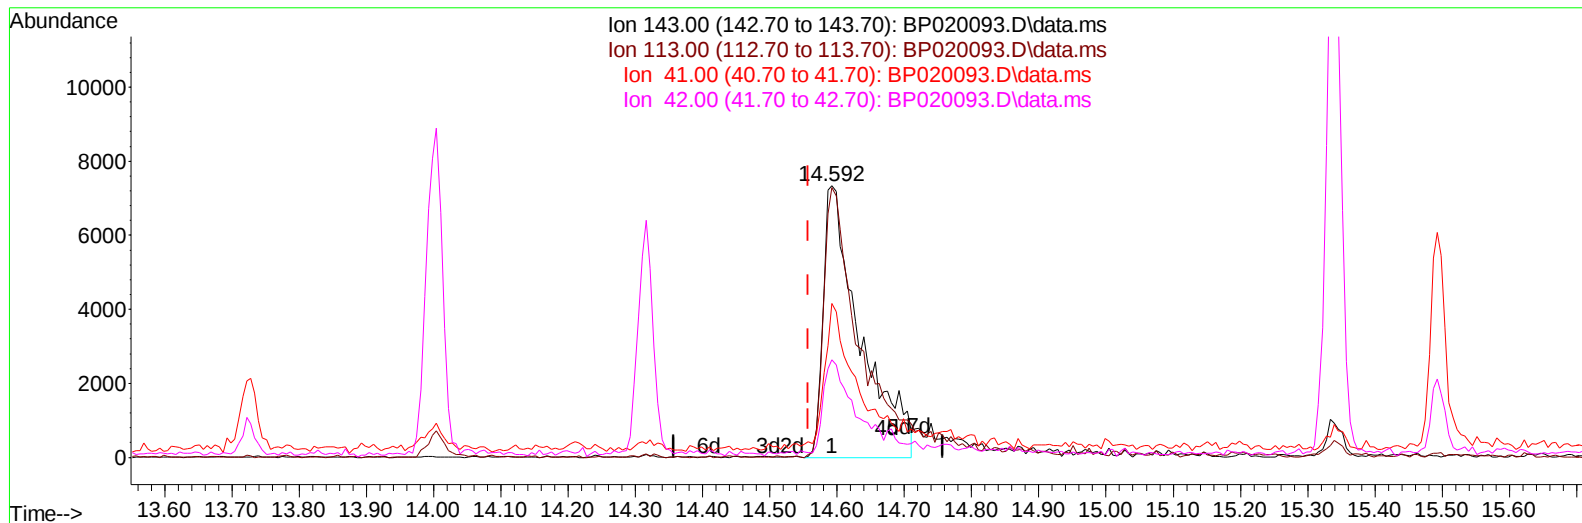

TIC: BP020093.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.592min (+ 0.035) 9.27 ng/ul m

response 28071

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	97.80	99.36
41.00	50.70	56.81
42.00	34.00	35.95

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020093.D
 Acq On : 23 Apr 2024 03:37
 Operator : MA/JU
 Sample : P2184-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R94

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 23 04:07:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	146145	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	541838	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	291041	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	645420	20.000	ng/ul	0.00
79) Chrysene-d12	21.657	240	618928	20.000	ng/ul	0.00
88) Perylene-d12	25.063	264	681374	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	16758	4.698	ng/uL	0.00
4) Pyridine-d5	3.634	84	92160	8.778	ng/ul	0.00
7) Phenol-d5	6.828	99	110137	8.647	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	335707	37.708	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	281506	32.370	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	193510	19.449	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	183030	46.960	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	192286	45.641	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	322911	38.635	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	300508	26.934	ng/ul	0.00
46) Dimethylphthalate-d6	13.728	166	924596	46.485	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	1070943	45.174	ng/ul	0.00
54) 4-Nitrophenol-d4	14.592	143	28071m	9.271	ng/ul	0.04
60) Fluorene-d10	15.340	176	827362	46.729	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	99064	26.273	ng/ul	0.01
73) Anthracene-d10	17.257	188	1349073	46.656	ng/ul	0.00
81) Pyrene-d10	19.663	212	1704464	51.244	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.821	264	1607424	48.293	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020093.D
Acq On : 23 Apr 2024 03:37
Operator : MA/JU
Sample : P2184-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R94

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 23 04:07:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

