

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020095.D
 Acq On : 23 Apr 2024 05:03
 Operator : MA/JU
 Sample : P2161-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0R89

Quant Time: Apr 23 05:36:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 01:17:52 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	115648	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	463292	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	318643	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.151	188	725481	20.000	ng/ul	0.00
79) Chrysene-d12	21.657	240	684050	20.000	ng/ul	0.00
88) Perylene-d12	25.051	264	750684	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	14062	4.982	ng/uL	0.00
4) Pyridine-d5	3.640	84	90587	10.904	ng/ul	0.00
7) Phenol-d5	6.828	99	78518	7.790	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	272558	38.688	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	225208	32.725	ng/ul	0.00
15) 4-Methylphenol-d8	8.345	113	148149	18.817	ng/ul	0.00
21) Nitrobenzene-d5	8.798	128	150627	45.199	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	163747	45.456	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.045	165	281723	39.422	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	369407	38.722	ng/ul	0.00
46) Dimethylphthalate-d6	13.728	166	1030989	47.344	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	1161425	44.747	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	26573	8.016	ng/ul	0.05
60) Fluorene-d10	15.339	176	922797	47.604	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	69270	16.344	ng/ul	0.00
73) Anthracene-d10	17.257	188	1617014	49.751	ng/ul	0.00
81) Pyrene-d10	19.663	212	2034119	55.333	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.821	264	1857262	50.647	ng/ul	0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	11.739	107	16451	1.972	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020095.D
Acq On : 23 Apr 2024 05:03
Operator : MA/JU
Sample : P2161-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0R89

Quant Time: Apr 23 05:36:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 01:17:52 2024
Response via : Initial Calibration

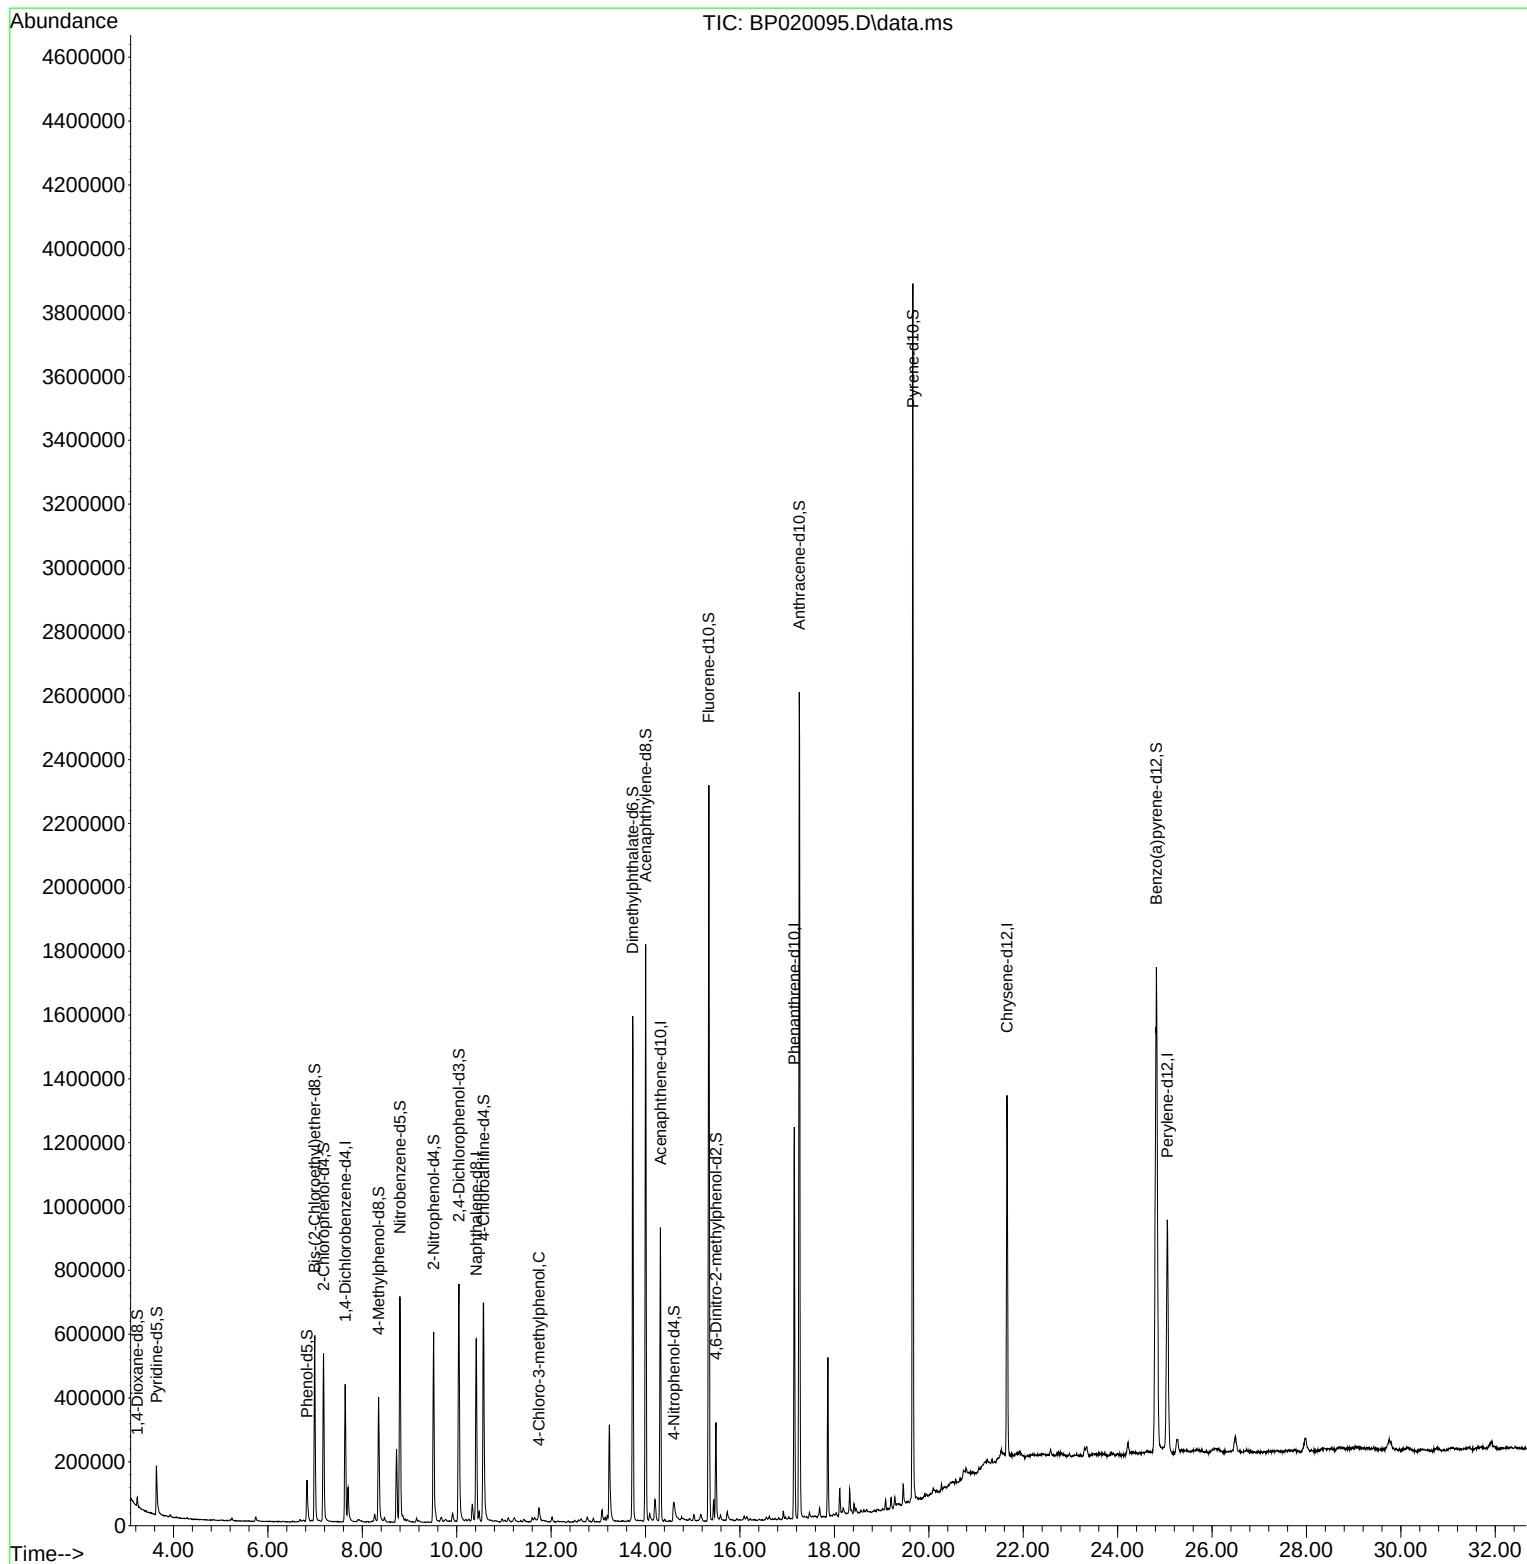

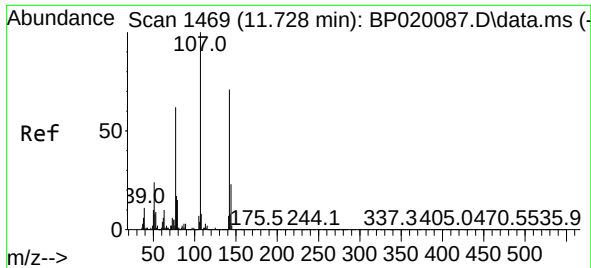

#35
 4-Chloro-3-methylphenol
 Concen: 1.972 ng/ul
 RT: 11.739 min Scan# 14
 Delta R.T. 0.017 min
 Lab File: BP020095.D
 Acq: 23 Apr 2024 05:03

Instrument :
 BNA_P
 ClientSampleId :
 C0R89

Tgt Ion:	107	Resp:	16451
Ion	Ratio	Lower	Upper
107	100		
144	22.9	18.0	27.0
142	69.1	56.3	84.5

