

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020074.D
 Acq On : 22 Apr 2024 13:01
 Operator : MA/JU
 Sample : PB160401BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK401

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	35	rVB	54160	81100	2.17%	0.190%
2	3.628	88	92	118	rBV	657023	1060323	28.37%	2.488%
3	3.934	140	144	149	rVB2	9643	13672	0.37%	0.032%
4	6.822	628	635	655	rBV	885470	1552605	41.54%	3.643%
5	6.993	657	664	682	rVB	712354	1154982	30.90%	2.710%
6	7.175	688	695	710	rBV	860513	1480141	39.60%	3.473%
7	7.640	766	774	787	rBV	612988	1013400	27.11%	2.378%
8	8.346	885	894	910	rBV	1032379	1785001	47.76%	4.188%
9	8.799	963	971	987	rBV	826533	1493049	39.95%	3.503%
10	9.510	1084	1092	1104	rBV	667912	1269519	33.97%	2.979%
11	10.046	1174	1183	1214	rBV	931282	1750391	46.83%	4.107%
12	10.416	1238	1246	1255	rBV	704866	1321397	35.35%	3.101%
13	10.569	1264	1272	1289	rBV	890865	1658790	44.38%	3.892%
14	12.028	1515	1520	1529	rBV2	9653	23379	0.63%	0.055%
15	13.204	1714	1720	1726	rBV2	17278	28040	0.75%	0.066%
16	13.739	1802	1811	1823	rBV	1363947	2089640	55.91%	4.903%
17	14.010	1844	1857	1872	rBV2	1561602	2450989	65.58%	5.751%
18	14.322	1902	1910	1922	rBV	980973	1481394	39.63%	3.476%
19	14.575	1945	1953	1982	rBV	432920	1099160	29.41%	2.579%
20	15.351	2077	2085	2099	rBV	1814381	2885691	77.21%	6.771%
21	15.504	2104	2111	2123	rBV	388517	635803	17.01%	1.492%
22	15.604	2124	2128	2134	rVB3	10233	19086	0.51%	0.045%
23	15.945	2183	2186	2193	rVB9	3293	5643	0.15%	0.013%
24	16.169	2220	2224	2230	rVB6	6373	7996	0.21%	0.019%
25	16.851	2335	2340	2343	rVB6	3126	5346	0.14%	0.013%
26	16.957	2353	2358	2360	rBV5	4326	7472	0.20%	0.018%
27	17.180	2389	2396	2405	rBV	1239731	1740417	46.56%	4.084%
28	17.275	2405	2412	2426	rVV	2033736	3140950	84.04%	7.370%
29	17.504	2443	2451	2462	rBV4	25175	89827	2.40%	0.211%
30	18.133	2553	2558	2564	rBV2	49868	95993	2.57%	0.225%
31	19.222	2738	2743	2750	rBV	32340	51165	1.37%	0.120%
32	19.298	2751	2756	2760	rBV	27679	43335	1.16%	0.102%
33	19.474	2782	2786	2792	rBV6	31794	51642	1.38%	0.121%
34	19.674	2814	2820	2826	rBV	2655608	3737635	100.00%	8.770%
35	21.674	3154	3160	3173	rVB2	1072022	1862076	49.82%	4.369%
36	24.845	3690	3699	3711	rVB	1382740	3632133	97.18%	8.523%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020074.D
Acq On : 22 Apr 2024 13:01
Operator : MA/JU
Sample : PB160401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK401

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Title : SVOA CALIBRATION

37	25.074	3730	3738	3749	rVB	705027	1798031	48.11%	4.219%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 42617213

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020074.D
Acq On : 22 Apr 2024 13:01
Operator : MA/JU
Sample : PB160401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK401

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

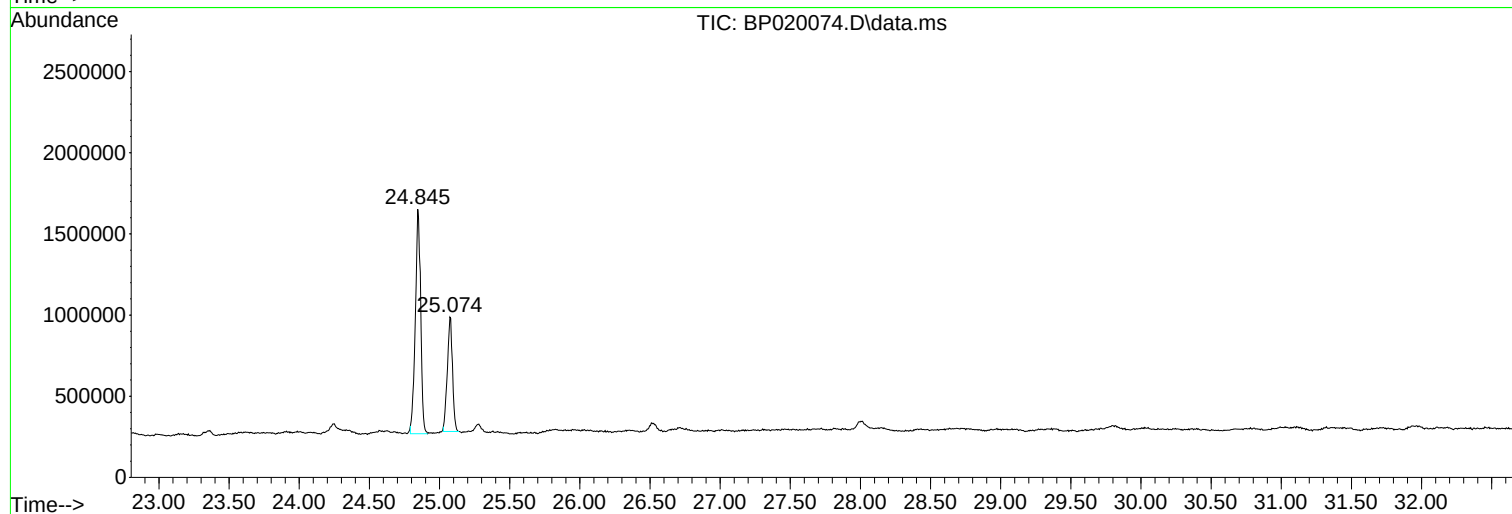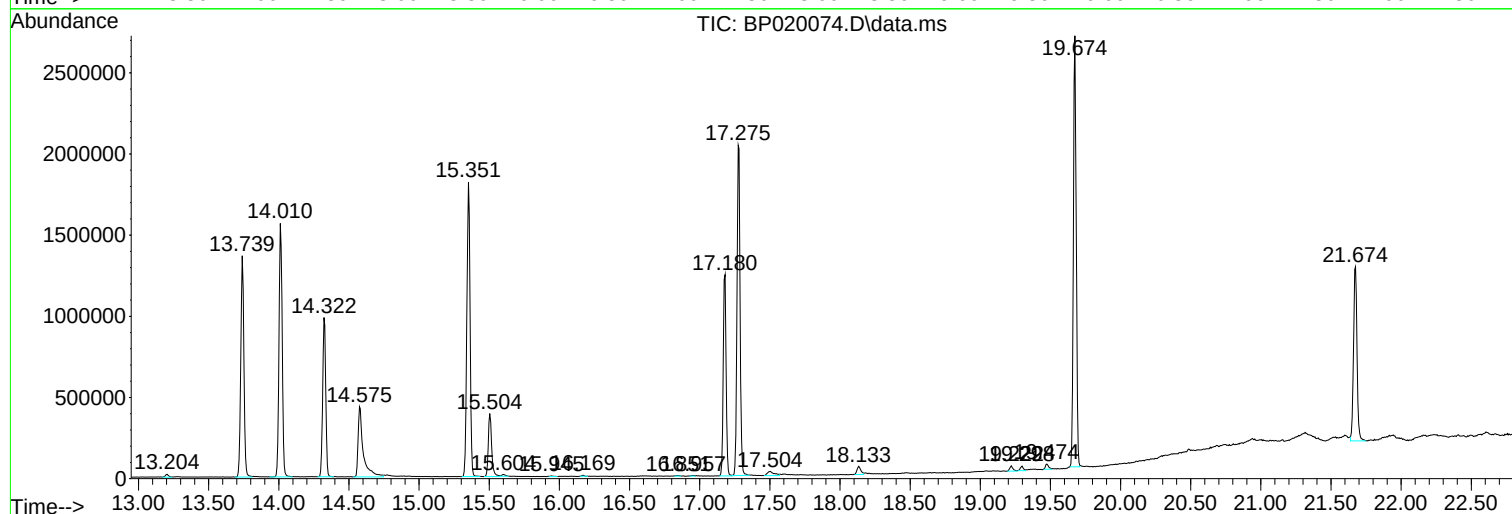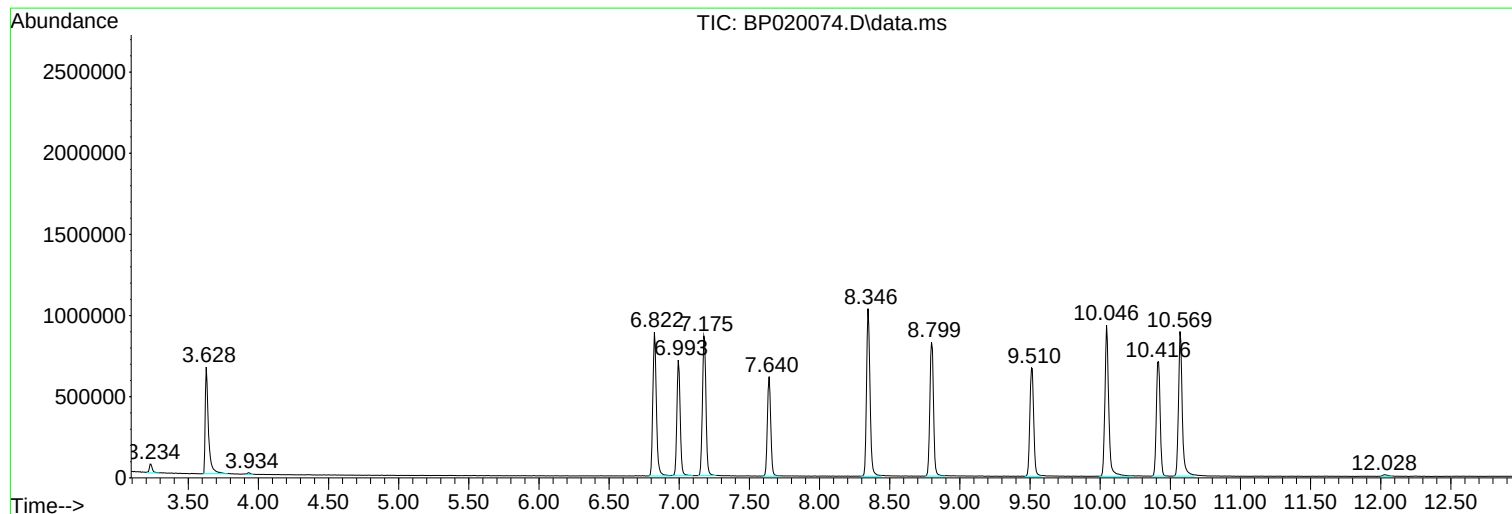

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020074.D
Acq On : 22 Apr 2024 13:01
Operator : MA/JU
Sample : PB160401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK401

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020074.D
Acq On : 22 Apr 2024 13:01
Operator : MA/JU
Sample : PB160401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK401

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc