

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
 Data File : BP020088.D
 Acq On : 23 Apr 2024 00:01
 Operator : MA/JU
 Sample : PB160379BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK379

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	30	rVB	27532	34634	1.19%	0.119%
2	3.634	89	93	113	rBV	230883	410173	14.15%	1.404%
3	3.928	139	143	149	rVB4	5555	9339	0.32%	0.032%
4	6.828	629	636	650	rBV	427040	786861	27.14%	2.693%
5	6.993	658	664	677	rBV	361930	570257	19.67%	1.952%
6	7.181	688	696	714	rBV	424065	764418	26.37%	2.616%
7	7.640	767	774	786	rBV	330526	564120	19.46%	1.931%
8	8.346	887	894	911	rBV	534117	951368	32.82%	3.256%
9	8.799	964	971	986	rBV	447202	809750	27.93%	2.771%
10	9.510	1084	1092	1108	rBV	408793	723241	24.95%	2.475%
11	10.046	1175	1183	1206	rBV	479286	1023386	35.30%	3.503%
12	10.410	1237	1245	1254	rBV	453535	831319	28.68%	2.845%
13	10.569	1263	1272	1301	rBV	386591	802132	27.67%	2.745%
14	12.034	1514	1521	1531	rBV5	6535	14868	0.51%	0.051%
15	13.192	1708	1718	1726	rBV3	13224	21737	0.75%	0.074%
16	13.269	1726	1731	1735	rVB7	1755	3279	0.11%	0.011%
17	13.722	1800	1808	1826	rBV	1025008	1536703	53.01%	5.259%
18	13.998	1847	1855	1872	rBV	1042232	1817641	62.70%	6.221%
19	14.310	1901	1908	1924	rBV	757498	1202242	41.47%	4.115%
20	14.569	1945	1952	1969	rBV	299608	779370	26.89%	2.667%
21	15.339	2076	2083	2096	rBV	1446190	2233258	77.04%	7.644%
22	15.492	2101	2109	2121	rVV	375540	636405	21.95%	2.178%
23	15.586	2121	2125	2134	rVB6	8345	18321	0.63%	0.063%
24	15.934	2180	2184	2187	rVB6	2560	3766	0.13%	0.013%
25	16.151	2217	2221	2228	rVB10	4926	8885	0.31%	0.030%
26	16.816	2327	2334	2341	rBV10	4397	11511	0.40%	0.039%
27	16.933	2350	2354	2356	rBV5	2741	3392	0.12%	0.012%
28	17.151	2383	2391	2401	rBV	1074952	1508231	52.03%	5.162%
29	17.257	2402	2409	2425	rVB2	1528237	2486679	85.78%	8.511%
30	17.486	2444	2448	2450	rBV4	9729	14377	0.50%	0.049%
31	17.863	2508	2512	2519	rVB9	8258	13144	0.45%	0.045%
32	18.110	2550	2554	2560	rBV7	17135	32674	1.13%	0.112%
33	19.204	2736	2740	2744	rVB	22075	28818	0.99%	0.099%
34	19.275	2749	2752	2759	rBV	19799	30308	1.05%	0.104%
35	19.469	2781	2785	2791	rBV7	11595	23708	0.82%	0.081%
36	19.657	2811	2817	2828	rBV	2005195	2898776	100.00%	9.921%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020088.D
Acq On : 23 Apr 2024 00:01
Operator : MA/JU
Sample : PB160379BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Title : SVOA CALIBRATION

37	21.651	3151	3156	3166	rBV2	902841	1477378	50.97%	5.056%
38	24.821	3686	3695	3707	rVB	918034	2612147	90.11%	8.940%
39	25.057	3728	3735	3750	rVB	569835	1519087	52.40%	5.199%




Sum of corrected areas: 29217703

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020088.D
Acq On : 23 Apr 2024 00:01
Operator : MA/JU
Sample : PB160379BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

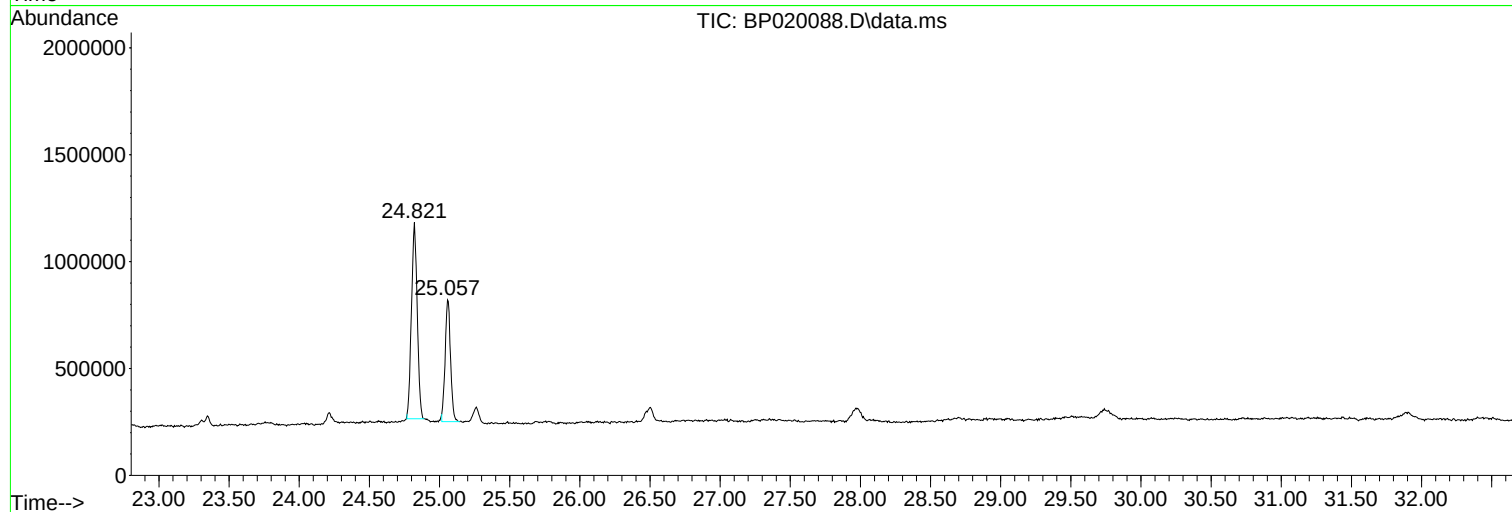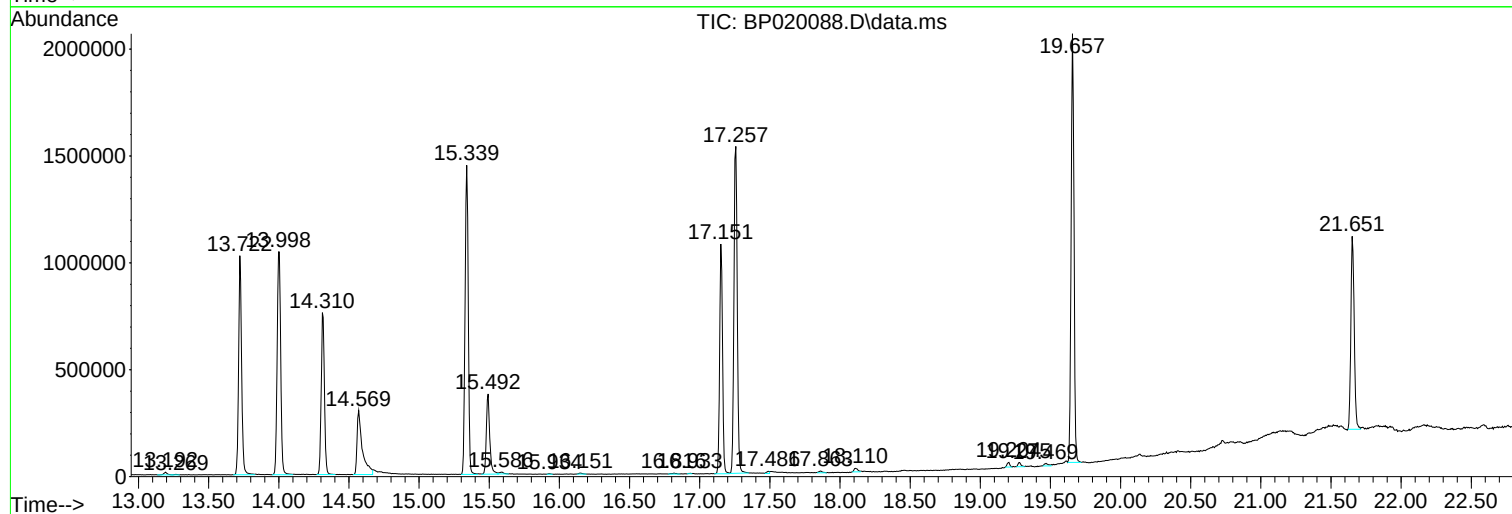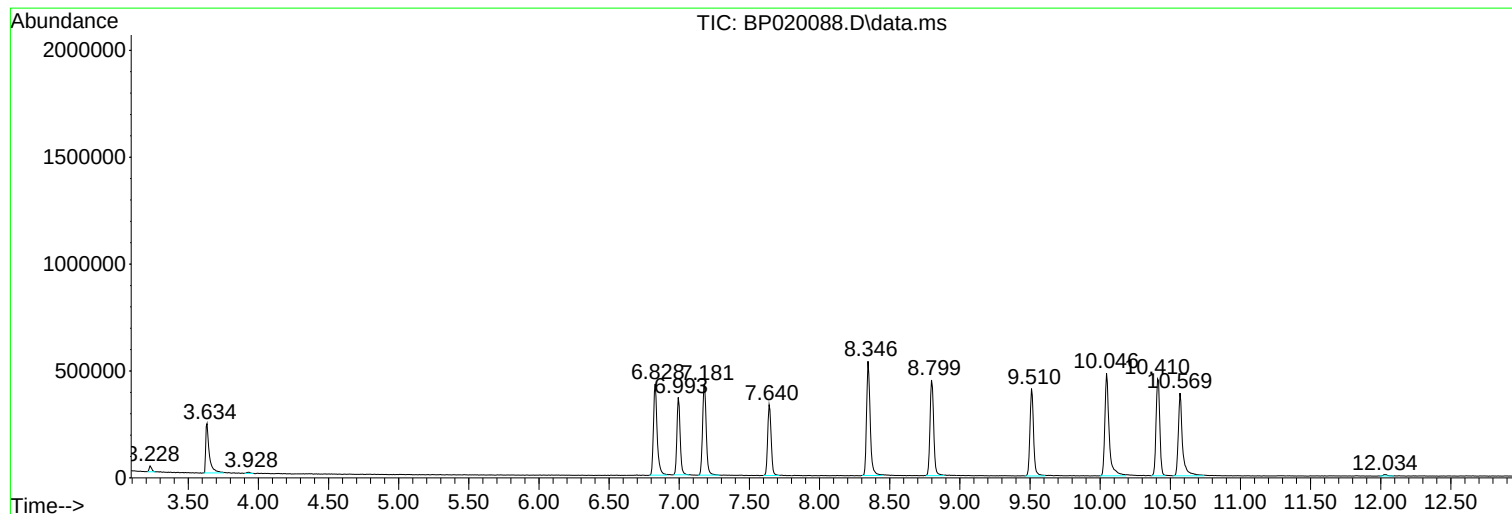

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020088.D
Acq On : 23 Apr 2024 00:01
Operator : MA/JU
Sample : PB160379BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042224\
Data File : BP020088.D
Acq On : 23 Apr 2024 00:01
Operator : MA/JU
Sample : PB160379BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK379

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------