
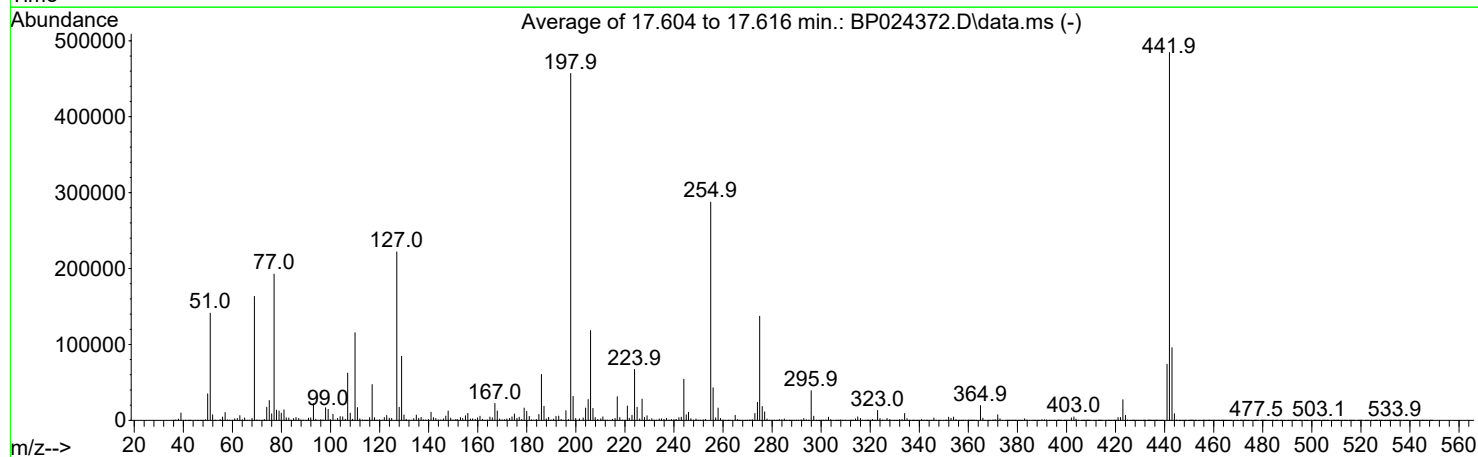


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042225\
Data File : BP024372.D
Acq On : 22 Apr 2025 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

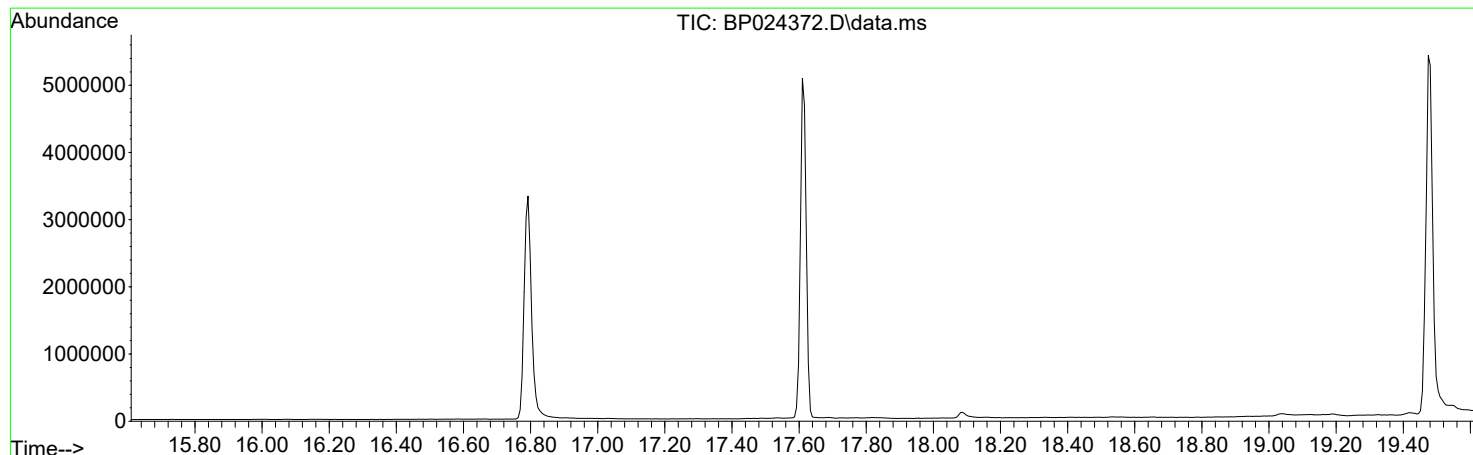

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	141321	PASS
68	69	0.00	2	1.7	2714	PASS
69	198	0.00	100	35.7	163330	PASS
70	69	0.00	2	0.4	692	PASS
127	198	10	80	48.5	221879	PASS
197	198	0.00	2	0.2	1059	PASS
198	198	100	100	100.0	457013	PASS
199	198	5	9	6.9	31670	PASS
275	198	10	60	30.0	137148	PASS
365	198	1	100	4.3	19633	PASS
441	198	0.01	100	16.2	74086	PASS
442	442	100	100	100.0	484548	PASS
443	442	15	24	19.8	95709	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
4/22/2025	BNA_P	<u>BP024372.D</u>
Compound Name	Response	Retention Time
DDT	1460669	20.763
DDD	30758	20.31
DDE	2544	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33302	1493971	2.23

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042225\
Data File : BP024372.D
Acq On : 22 Apr 2025 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 22 12:19:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

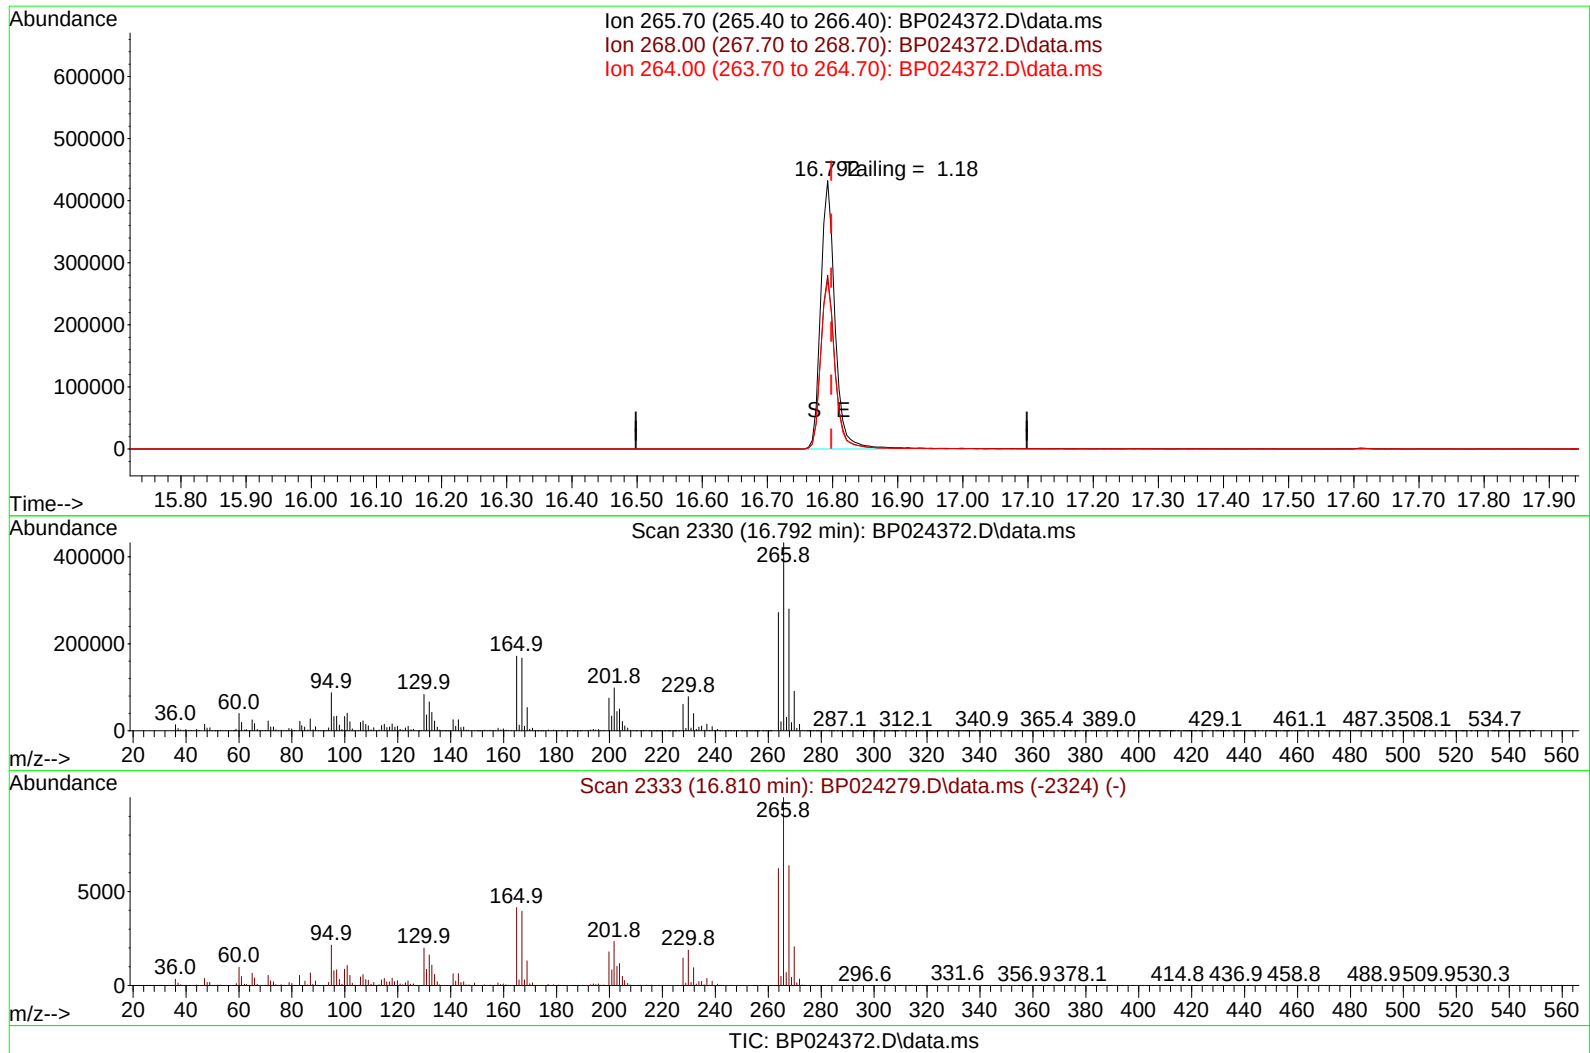

(70) Pentachlorophenol (C)

16.792min (-0.006) 124507.68 ng




response 662622

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.77
264.00	62.20	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042225\
Data File : BP024372.D
Acq On : 22 Apr 2025 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 22 12:19:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

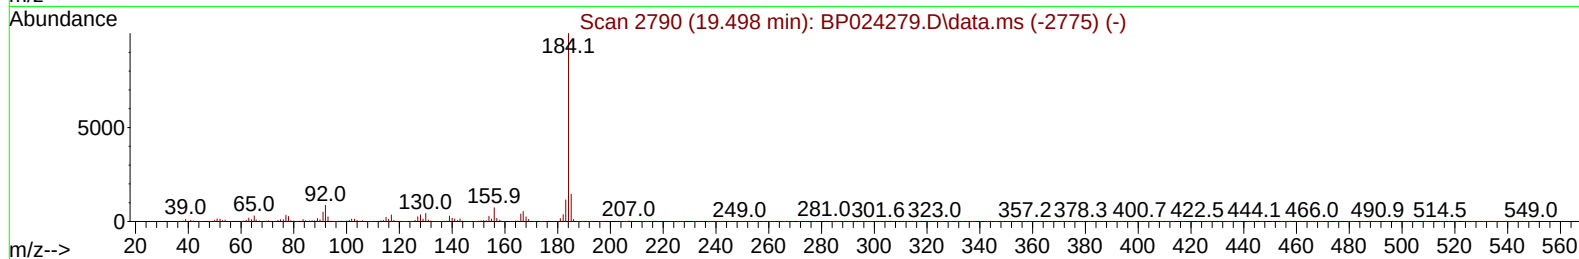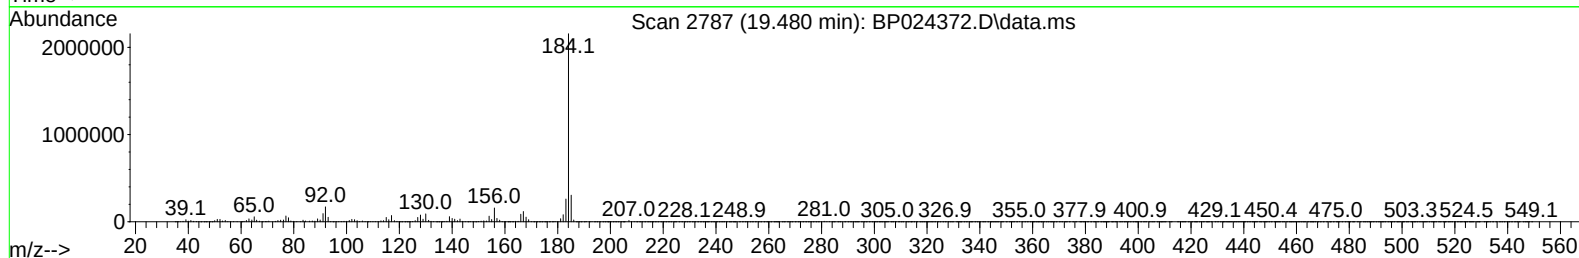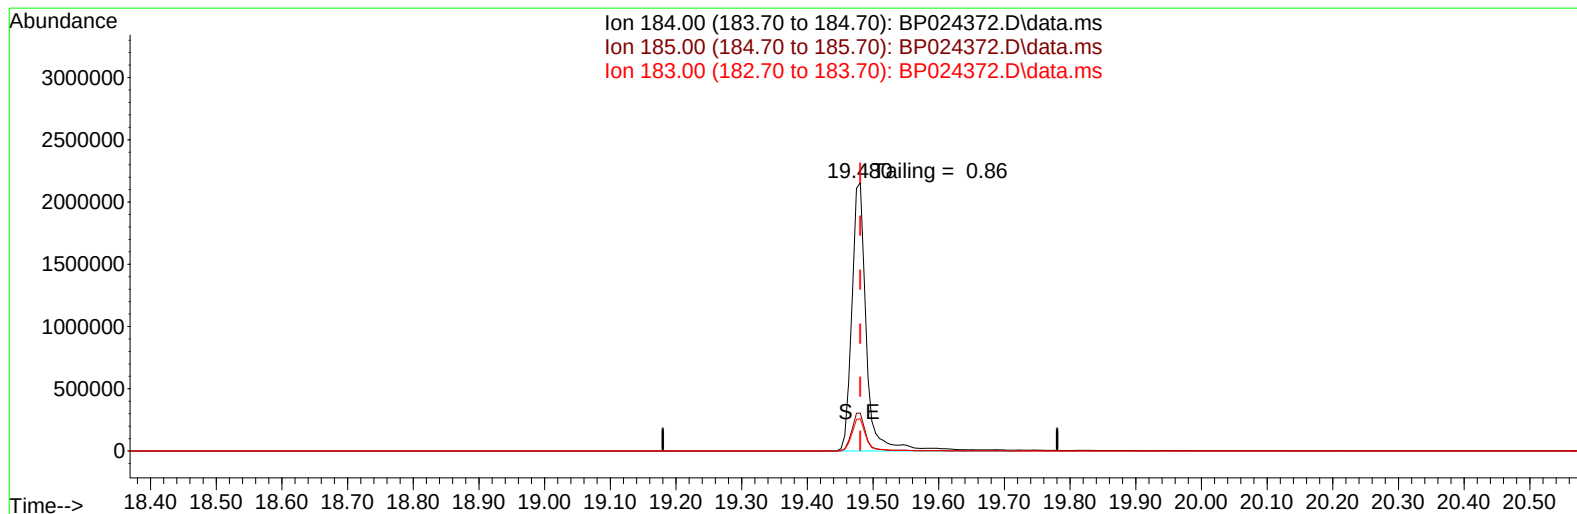

TIC: BP024372.D\data.ms

(77) Benzidine

19.480min (+ 0.000) 121904.37 ng

response 3243461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.16
183.00	11.50	12.05
0.00	0.00	0.00