

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
 Data File : BP005388.D
 Acq On : 23 Apr 2021 11:52
 Operator : CG/JU
 Sample : PB135921BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135921BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	359	365	382	rBV	703533	1032257	42.81%	10.837%
2	6.828	628	636	655	rBV	632925	1023033	42.43%	10.741%
3	7.634	766	773	780	rBV	125523	193298	8.02%	2.029%
4	8.799	963	971	986	rBV	385883	644952	26.75%	6.771%
5	10.428	1239	1248	1261	rBV	129539	231202	9.59%	2.427%
6	12.916	1663	1671	1691	rBV	855173	1224824	50.80%	12.859%
7	14.304	1898	1907	1919	rBV	186749	284089	11.78%	2.983%
8	15.810	2155	2163	2178	rBV	787167	1132817	46.98%	11.893%
9	17.069	2371	2377	2391	rBV	248855	364587	15.12%	3.828%
10	19.651	2810	2816	2829	rBV	2059628	2411054	100.00%	25.313%
11	20.963	3036	3039	3045	rBV2	29209	39559	1.64%	0.415%
12	21.174	3071	3075	3082	rBV	365591	462989	19.20%	4.861%
13	23.433	3454	3459	3468	rVB	263186	480247	19.92%	5.042%




Sum of corrected areas: 9524908

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
Data File : BP005388.D
Acq On : 23 Apr 2021 11:52
Operator : CG/JU
Sample : PB135921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

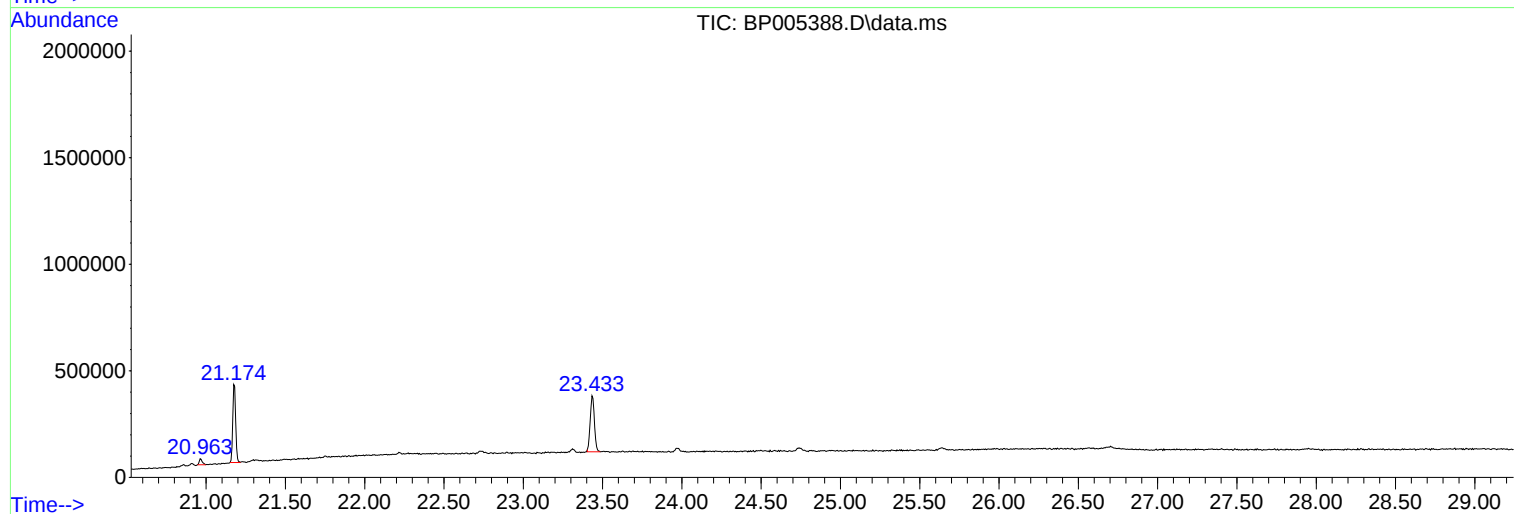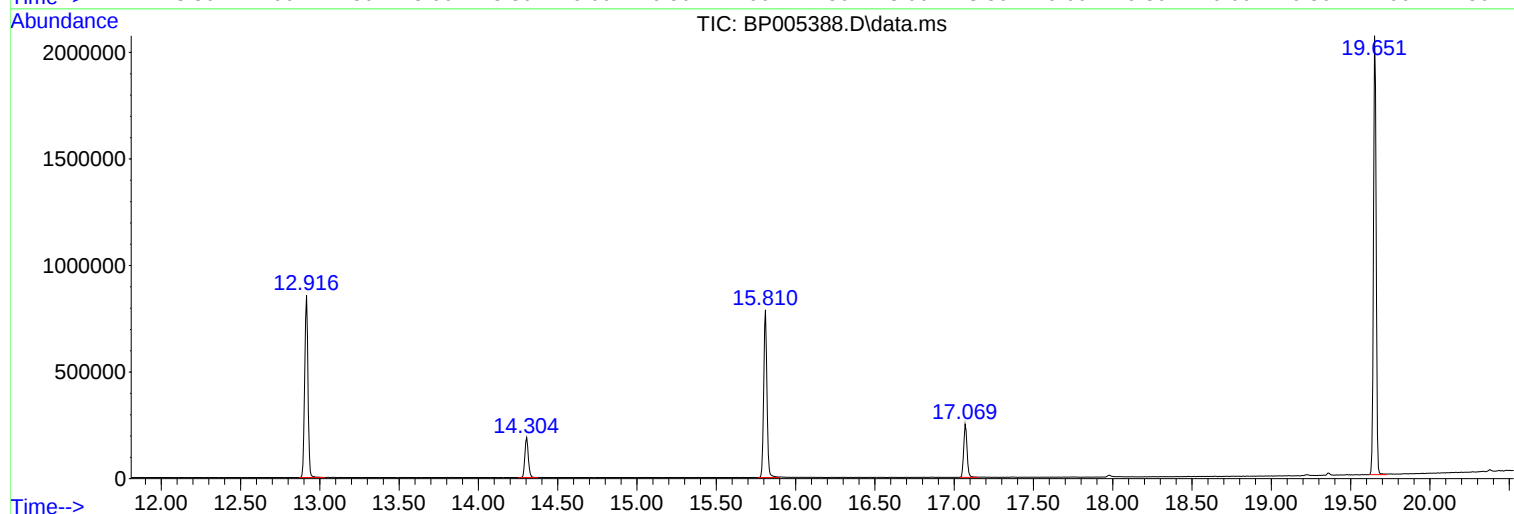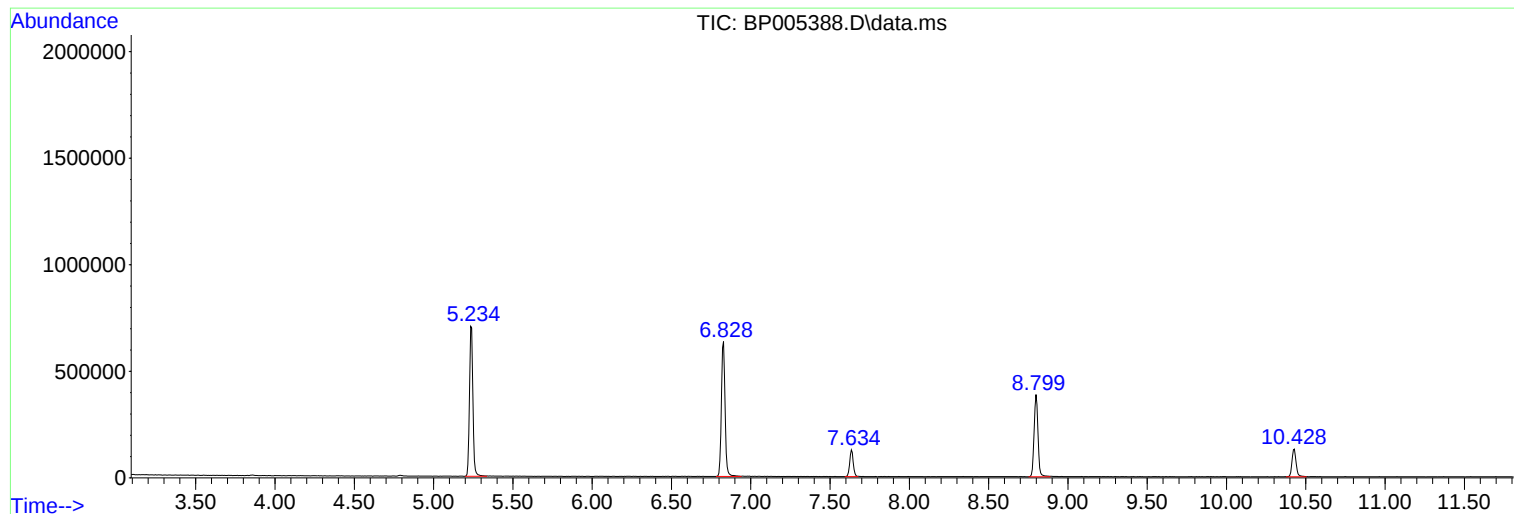

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
Data File : BP005388.D
Acq On : 23 Apr 2021 11:52
Operator : CG/JU
Sample : PB135921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
Data File : BP005388.D
Acq On : 23 Apr 2021 11:52
Operator : CG/JU
Sample : PB135921BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135921BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------