
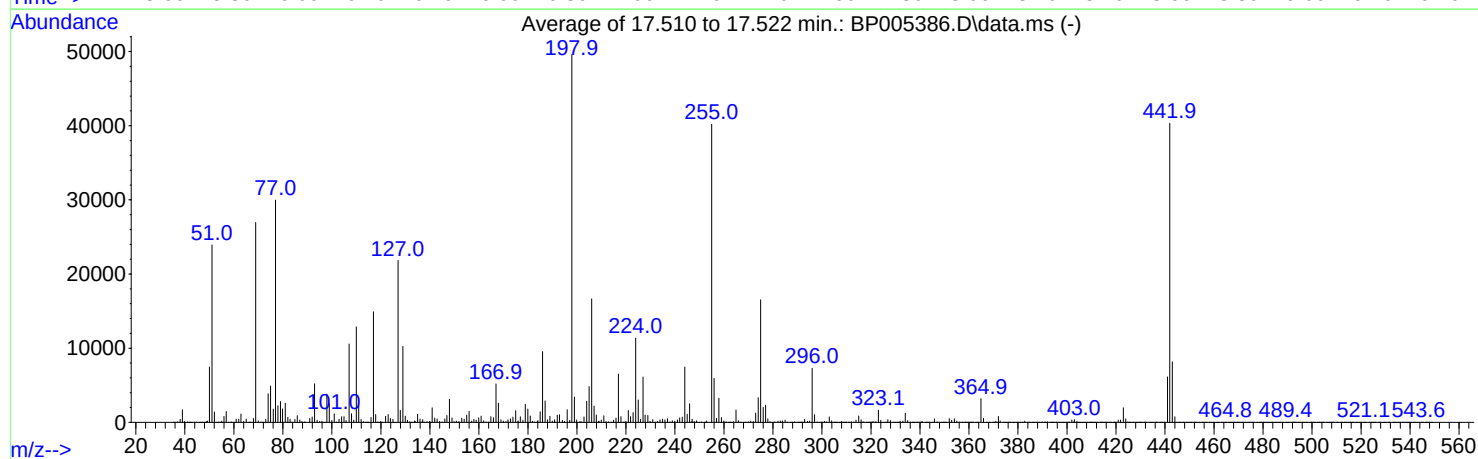


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
 Data File : BP005386.D
 Acq On : 23 Apr 2021 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 21 17:40:15 2021

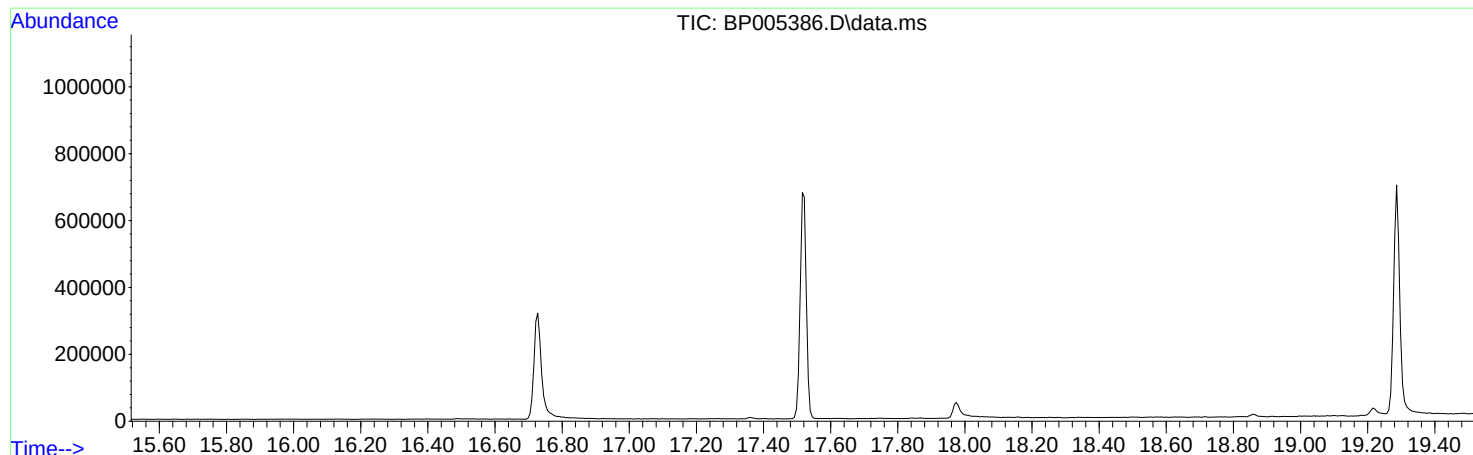




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	23936	PASS
68	69	0.00	2	1.9	521	PASS
69	198	0.00	100	54.3	26938	PASS
70	69	0.00	2	0.8	205	PASS
127	198	10	80	44.0	21825	PASS
197	198	0.00	2	0.5	272	PASS
198	198	100	100	100.0	49601	PASS
199	198	5	9	6.9	3419	PASS
275	198	10	60	33.3	16516	PASS
365	198	1	100	6.4	3193	PASS
441	198	0.01	100	12.4	6133	PASS
442	442	100	100	100.0	40340	PASS
443	442	15	24	20.2	8152	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
Data File : BP005386.D
Acq On : 23 Apr 2021 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 23 11:48:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 17:40:15 2021
Response via : Initial Calibration

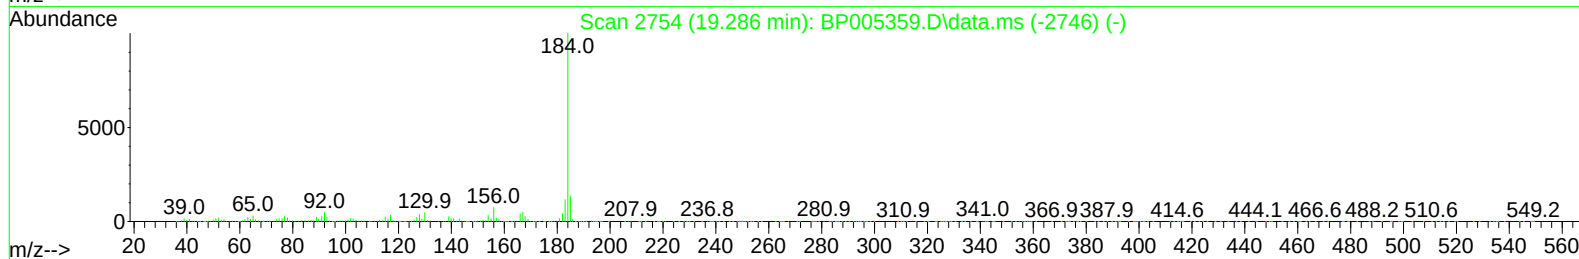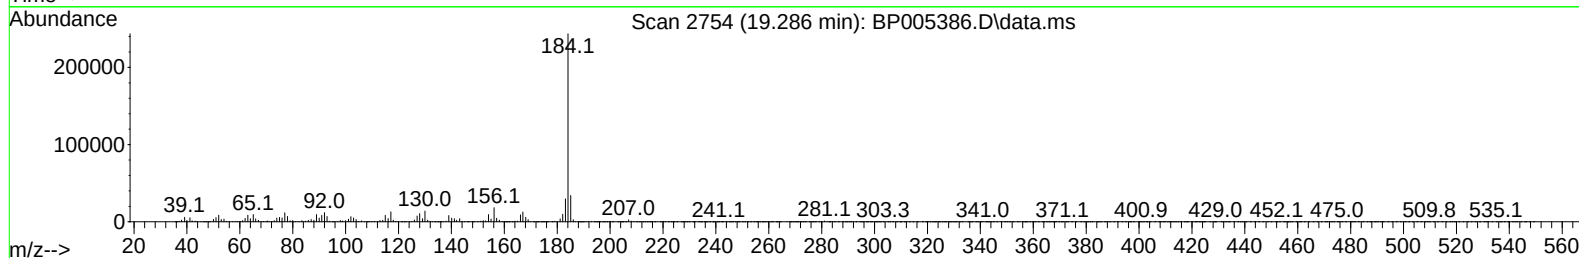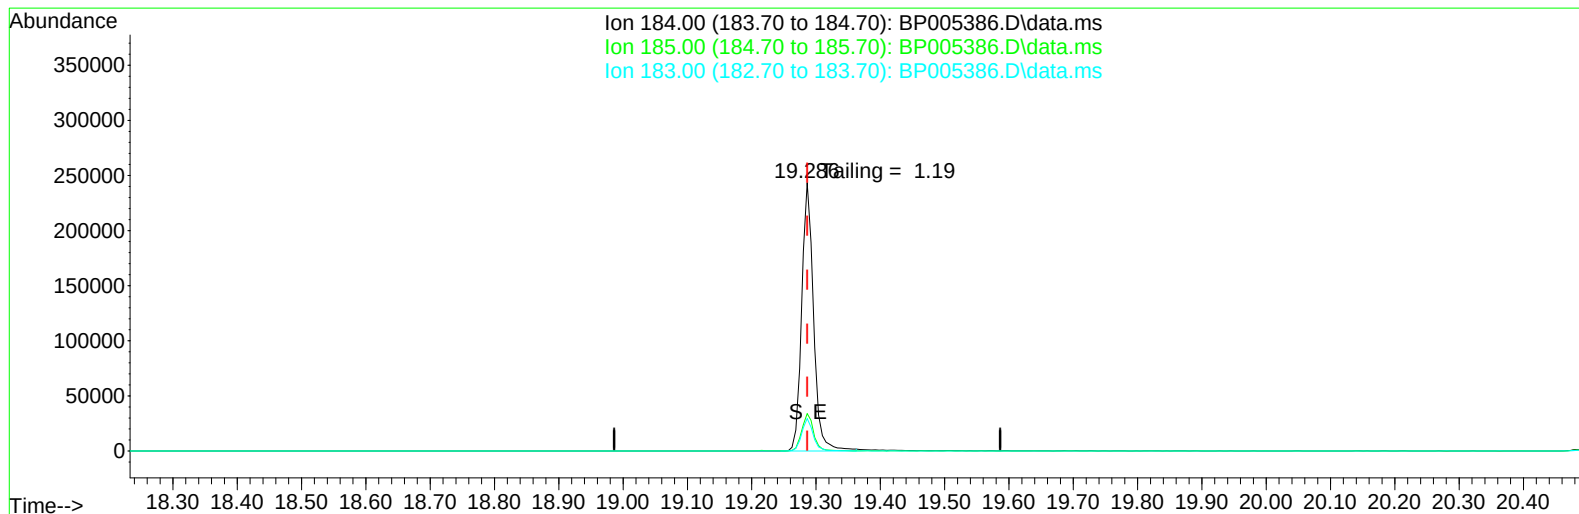

TIC: BP005386.D\data.ms

(77) Benzidine

19.286min (-0.000) 95540.05 ng




response 317017

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.98
183.00	12.30	12.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042321\
Data File : BP005386.D
Acq On : 23 Apr 2021 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 23 11:44:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 17:40:15 2021
Response via : Initial Calibration

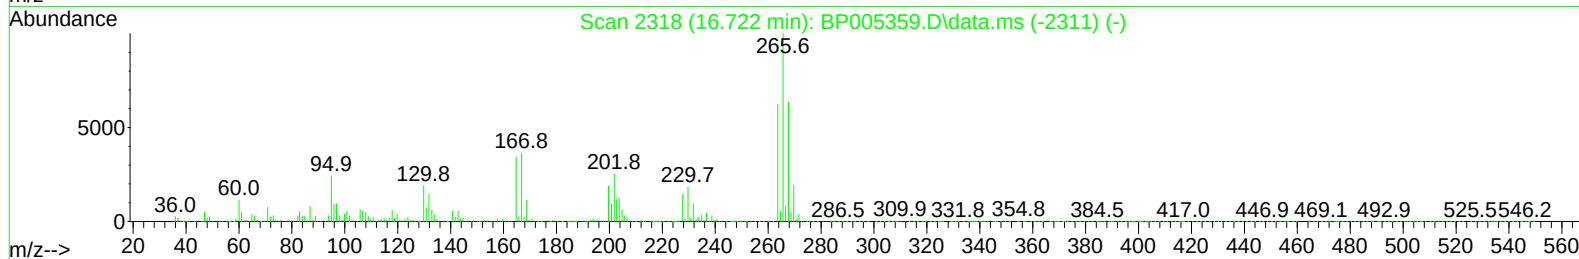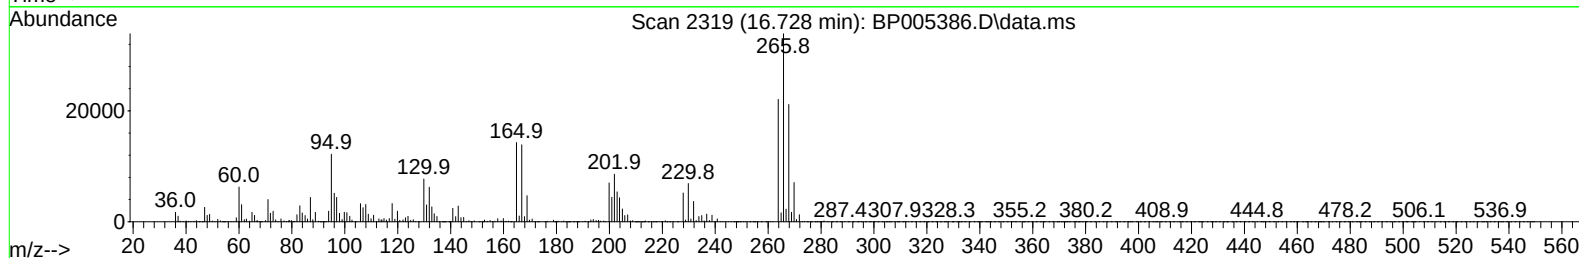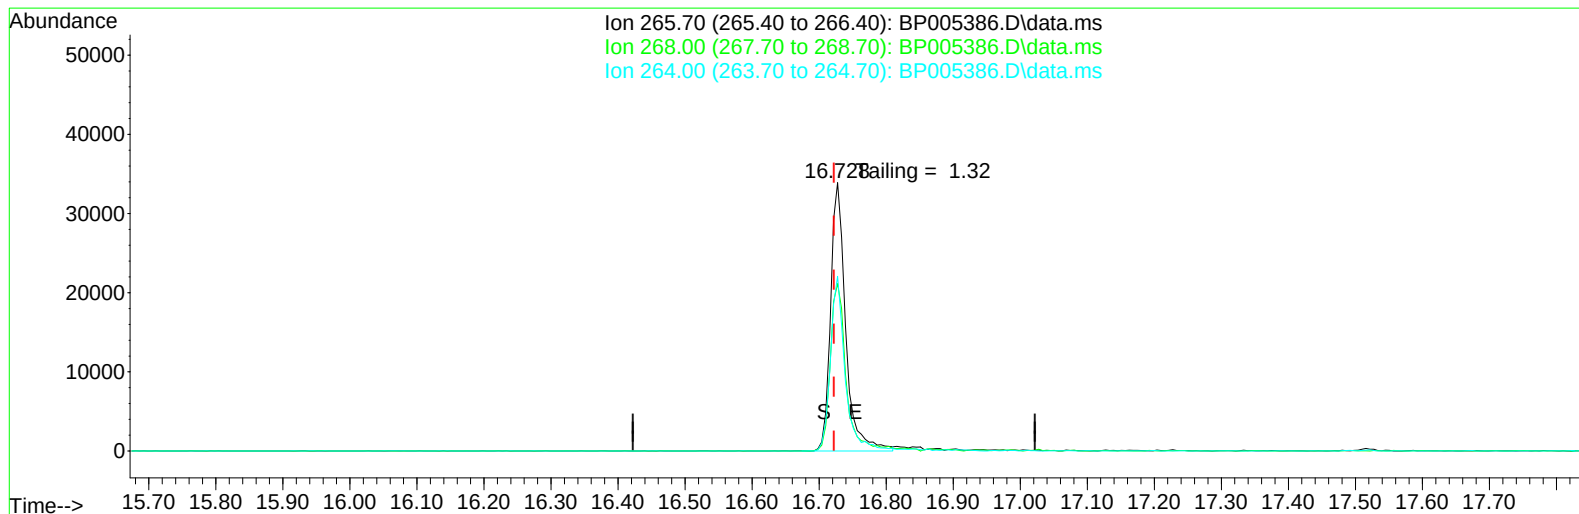

TIC: BP005386.D\data.ms

(70) Pentachlorophenol (C)

16.728min (+ 0.006) 259976.08 ng

response 53757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.39
264.00	67.10	65.10
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/23/2021	BNA_P	BP005386.D
Compound Name	Response	Retention Time
DDT	207195	20.48
DDD	1920	20.05
DDE	466	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2386	209581	1.14

Instrument :
BNA_P
ClientSampleId :
DFTPP