




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020108.D
Acq On : 23 Apr 2024 19:02
Operator : MA/JU
Sample : P2154-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P2154-0623

Manual IntegrationsAPPROVED

Quant Time: Apr 24 01:31:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 24 00:55:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024

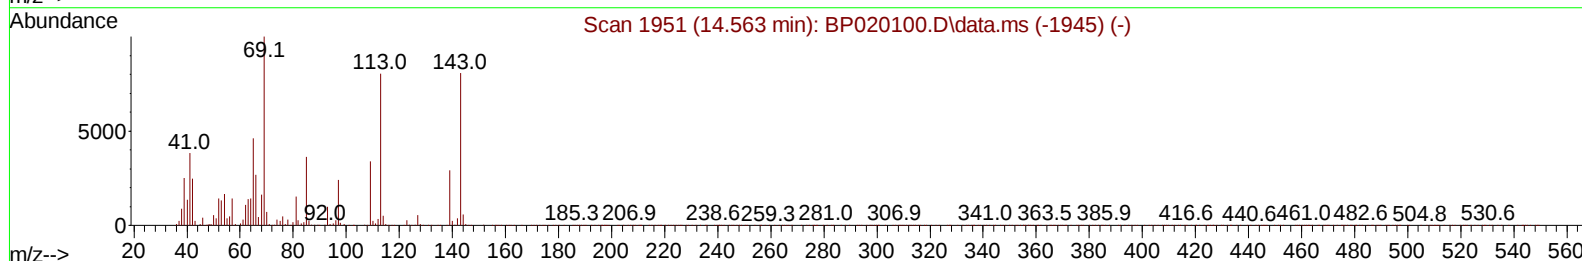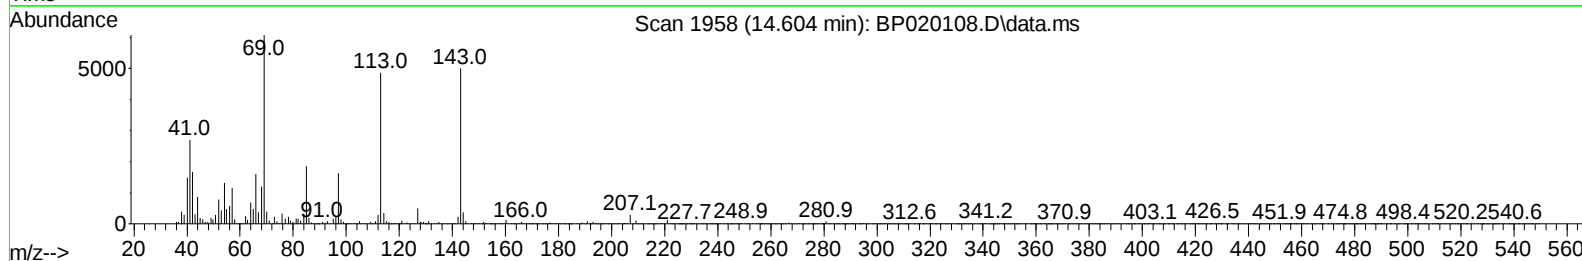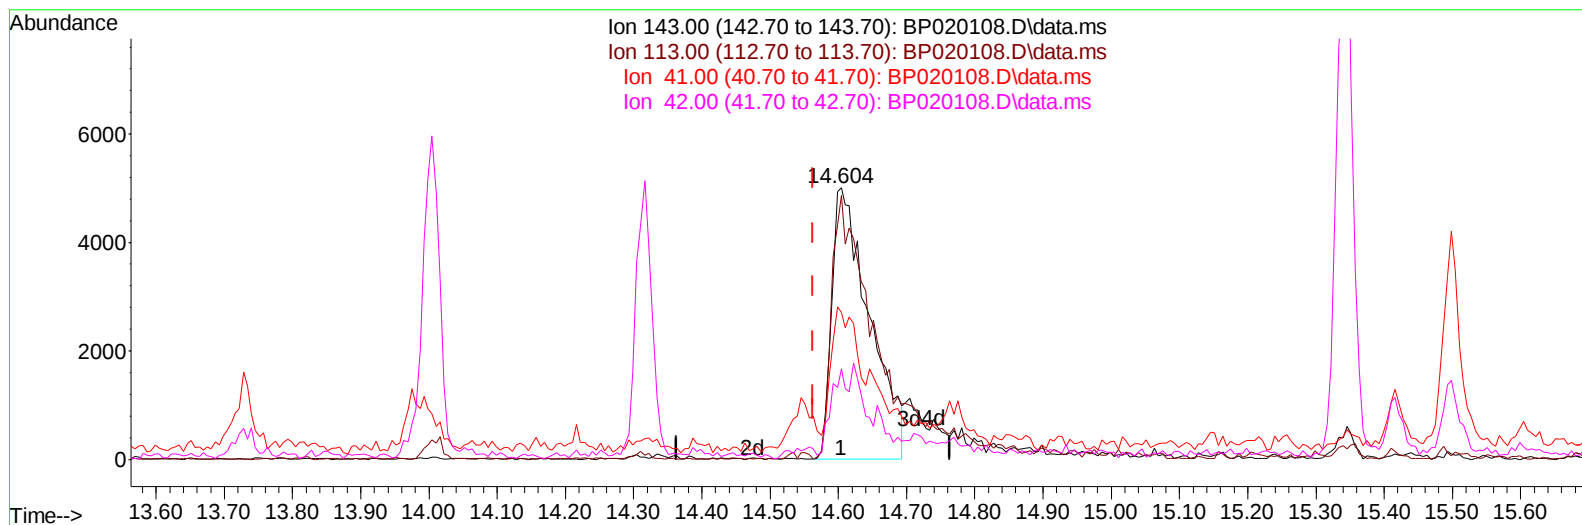

TIC: BP020108.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.604min (+ 0.041) 7.55 ng/u1

response 19196

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	99.60	97.30
41.00	48.00	54.04
42.00	31.00	33.36




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020108.D
Acq On : 23 Apr 2024 19:02
Operator : MA/JU
Sample : P2154-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P2154-0623

Manual IntegrationsAPPROVED

Quant Time: Apr 24 01:31:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 24 00:55:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024

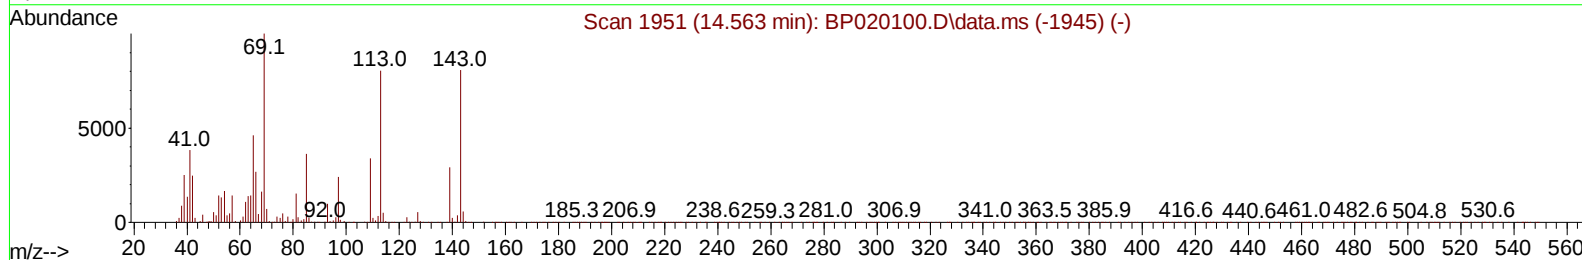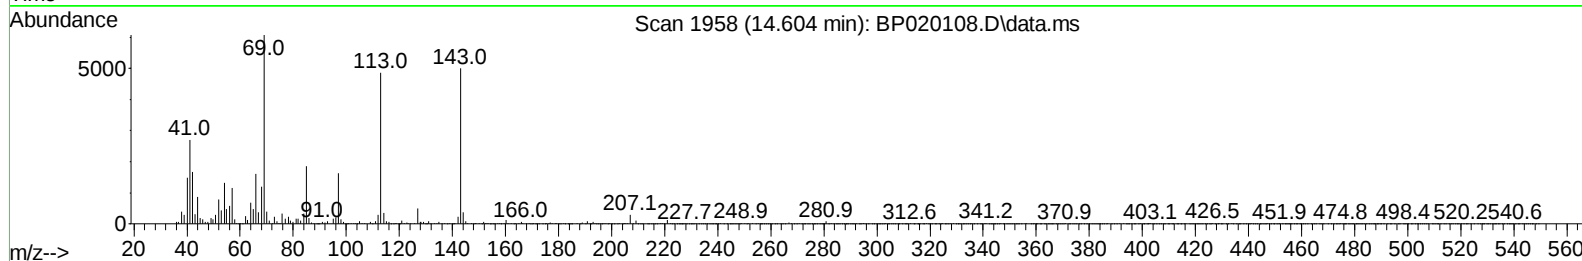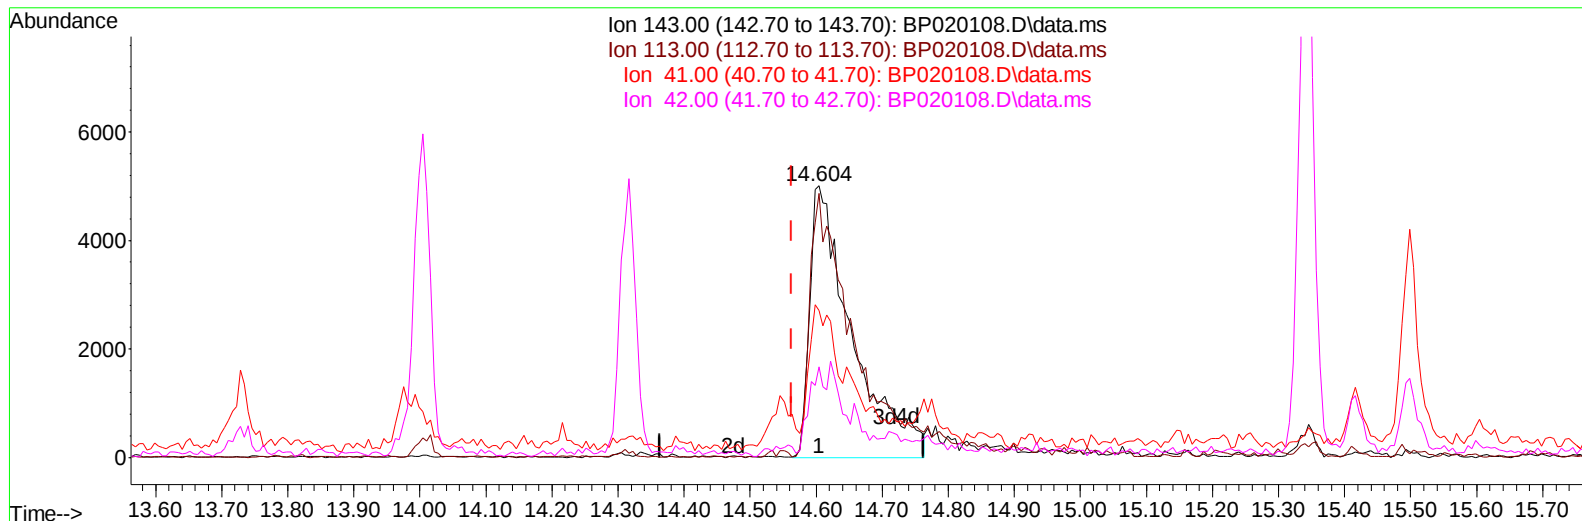

TIC: BP020108.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.604min (+ 0.041) 8.76 ng/ul m

response 22257

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	99.60	97.30
41.00	48.00	54.04
42.00	31.00	33.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
 Data File : BP020108.D
 Acq On : 23 Apr 2024 19:02
 Operator : MA/JU
 Sample : P2154-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P2154-0623

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 04/27/2024

Quant Time: Apr 24 01:35:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 24 00:55:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	89591	20.000	ng/ul	0.00
20) Naphthalene-d8	10.405	136	343416	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	243108	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.169	188	548819	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	524724	20.000	ng/ul	0.00
88) Perylene-d12	25.057	264	571993	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9284	4.708	ng/uL	0.00
4) Pyridine-d5	3.646	84	17616	2.979	ng/ul	0.01
7) Phenol-d5	6.828	99	53796	7.160	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	165242	33.832	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	144652	26.627	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	87931	15.236	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	91180	35.664	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	99551	33.705	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	165030	30.266	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	123748	18.233	ng/ul	0.00
46) Dimethylphthalate-d6	13.728	166	615815	36.251	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	720048	36.115	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	22257m	8.756	ng/ul	0.04
60) Fluorene-d10	15.345	176	574295	39.172	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.498	200	74106	28.146	ng/ul	0.00
73) Anthracene-d10	17.263	188	958252	39.424	ng/ul	0.00
81) Pyrene-d10	19.669	212	1160879	38.878	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.816	264	1077492	38.749	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020108.D
Acq On : 23 Apr 2024 19:02
Operator : MA/JU
Sample : P2154-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P2154-0623

Manual IntegrationsAPPROVED

Quant Time: Apr 24 01:35:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 24 00:55:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024

