

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
 Data File : BP020105.D
 Acq On : 23 Apr 2024 16:49
 Operator : MA/JU
 Sample : PB160399BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK399

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	20	23	29	rVB	28274	37100	1.28%	0.125%
2	3.622	87	91	106	rBV	299209	508893	17.61%	1.716%
3	3.916	138	141	148	rVB5	6424	9483	0.33%	0.032%
4	6.804	626	632	652	rBV	398305	760373	26.31%	2.563%
5	6.975	654	661	672	rVV	316438	544373	18.83%	1.835%
6	7.157	685	692	708	rBV	411147	740677	25.63%	2.497%
7	7.622	764	771	785	rBV	365108	617114	21.35%	2.080%
8	8.334	884	892	915	rBV	495262	919845	31.82%	3.101%
9	8.787	961	969	987	rBV	406506	760381	26.31%	2.563%
10	9.498	1082	1090	1111	rBV	351180	672913	23.28%	2.268%
11	10.040	1173	1182	1205	rBV	439542	969842	33.55%	3.269%
12	10.404	1236	1244	1255	rBV	466731	883655	30.57%	2.979%
13	10.563	1262	1271	1286	rBV	413216	909419	31.46%	3.066%
14	12.028	1511	1520	1532	rBV5	6679	19841	0.69%	0.067%
15	13.186	1713	1717	1724	rVV5	9564	15648	0.54%	0.053%
16	13.269	1724	1731	1735	rVB9	1757	3774	0.13%	0.013%
17	13.728	1801	1809	1827	rBV	885770	1452670	50.26%	4.897%
18	14.004	1848	1856	1875	rBV	1118460	1733328	59.97%	5.843%
19	14.316	1901	1909	1923	rBV	865956	1296240	44.85%	4.370%
20	14.575	1947	1953	1977	rBV	297762	768868	26.60%	2.592%
21	15.345	2077	2084	2100	rBV	1369795	2175438	75.27%	7.333%
22	15.498	2103	2110	2124	rBV	356834	630229	21.80%	2.125%
23	15.592	2124	2126	2132	rVB7	7440	11395	0.39%	0.038%
24	16.157	2219	2222	2227	rVB6	5787	7340	0.25%	0.025%
25	16.833	2332	2337	2342	rBV9	3439	6533	0.23%	0.022%
26	16.951	2352	2357	2362	rVB8	2689	4420	0.15%	0.015%
27	17.163	2384	2393	2404	rBV	1061096	1651695	57.15%	5.568%
28	17.269	2404	2411	2426	rVB2	1543615	2464166	85.26%	8.307%
29	17.521	2448	2454	2458	rBV9	6508	16183	0.56%	0.055%
30	18.127	2551	2557	2560	rBV4	16092	28730	0.99%	0.097%
31	19.210	2737	2741	2747	rVB3	18908	28661	0.99%	0.097%
32	19.286	2750	2754	2759	rBV	17565	25660	0.89%	0.087%
33	19.468	2783	2785	2790	rVB6	8778	12580	0.44%	0.042%
34	19.663	2812	2818	2830	rVB	2125558	2890333	100.00%	9.743%
35	21.662	3151	3158	3172	rBV2	891053	1687689	58.39%	5.689%
36	24.821	3686	3695	3710	rVB	1027333	2726106	94.32%	9.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020105.D
Acq On : 23 Apr 2024 16:49
Operator : MA/JU
Sample : PB160399BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK399

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Title : SVOA CALIBRATION

37	25.056	3726	3735	3749	rVB	566823	1672798	57.88%	5.639%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 29664393

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020105.D
Acq On : 23 Apr 2024 16:49
Operator : MA/JU
Sample : PB160399BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK399

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

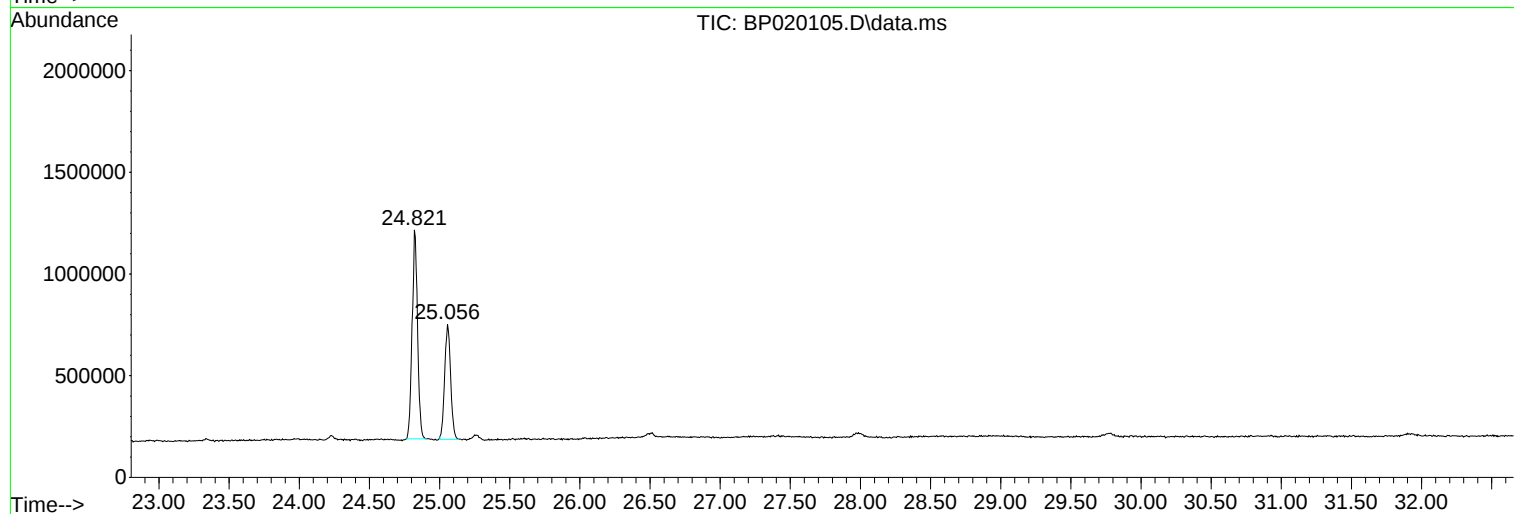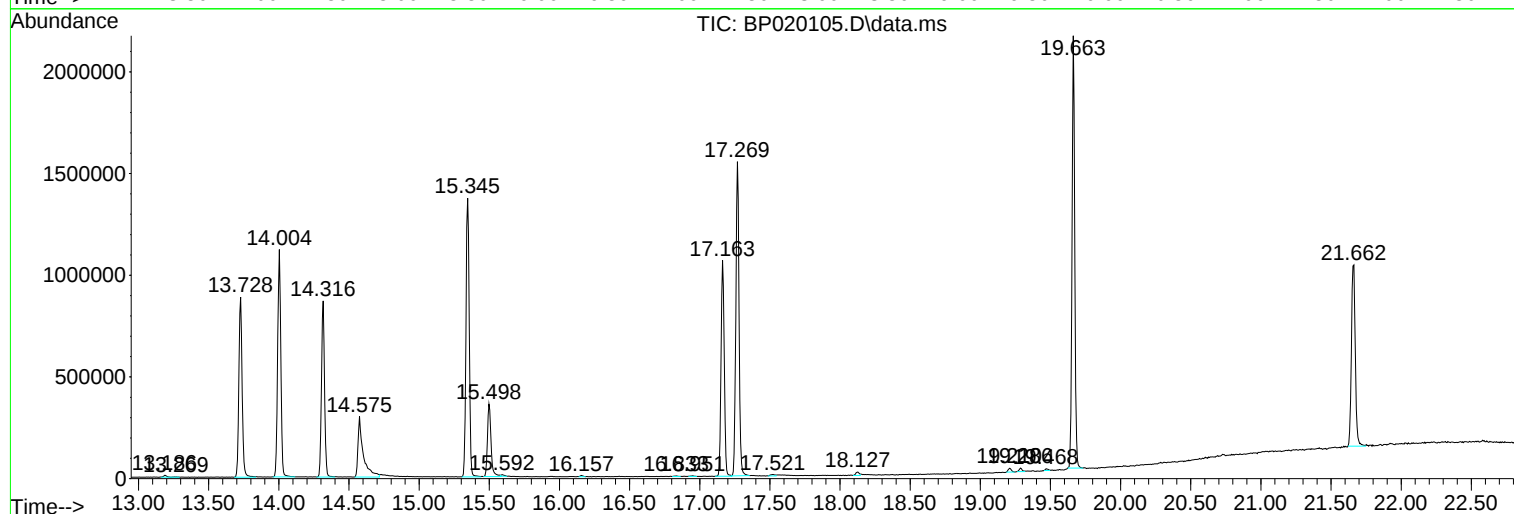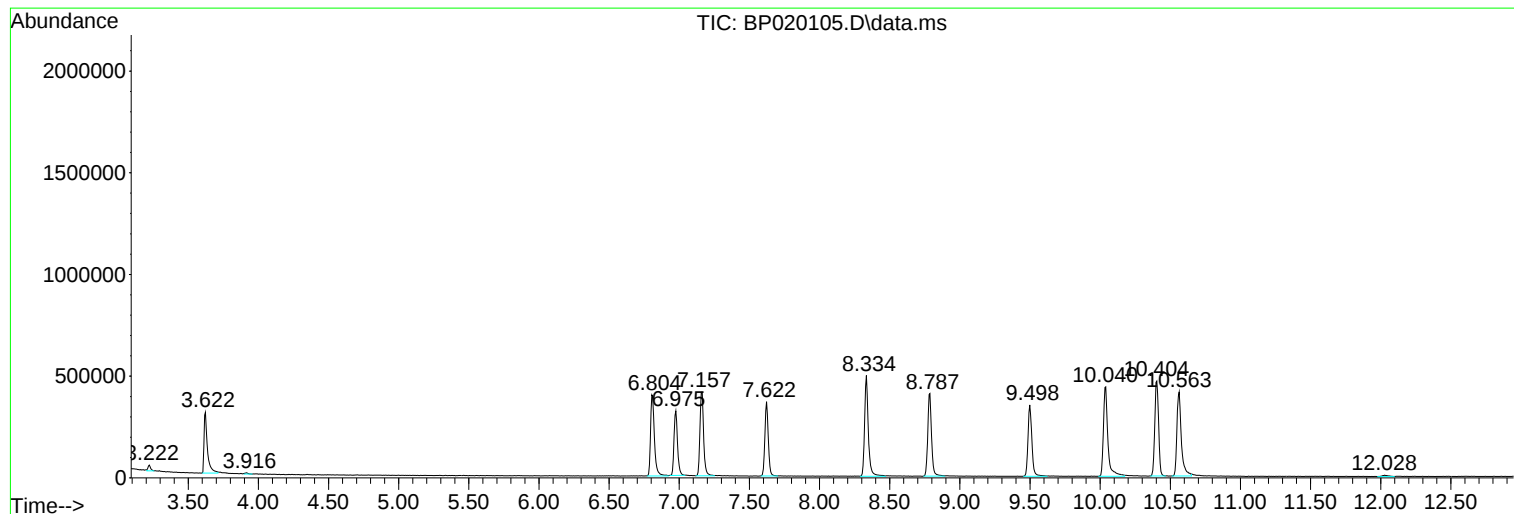

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020105.D
Acq On : 23 Apr 2024 16:49
Operator : MA/JU
Sample : PB160399BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK399

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042324\
Data File : BP020105.D
Acq On : 23 Apr 2024 16:49
Operator : MA/JU
Sample : PB160399BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK399

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc