
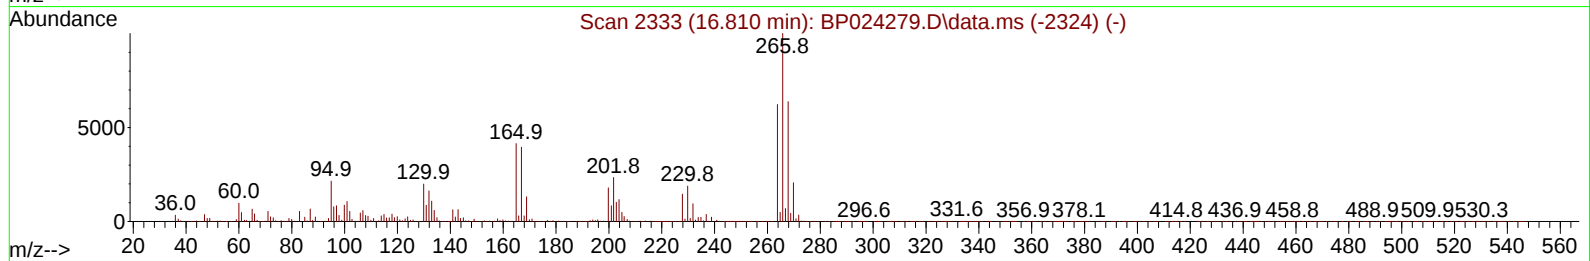
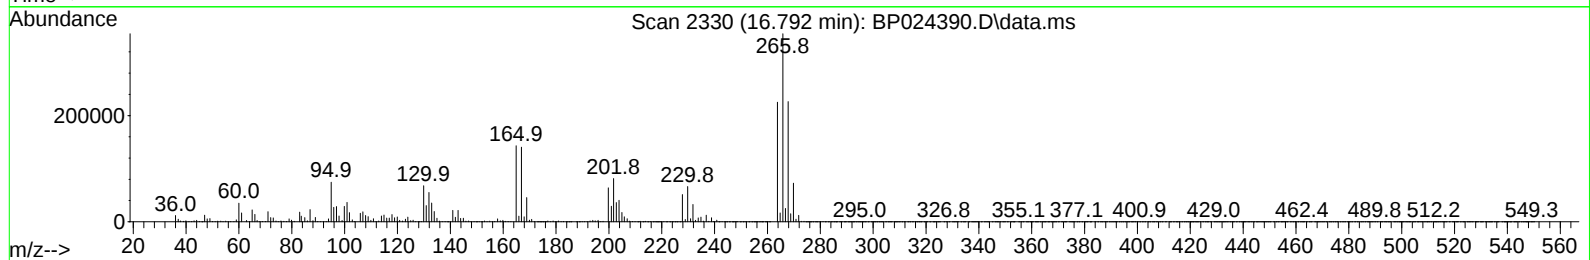


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042325\
Data File : BP024390.D
Acq On : 23 Apr 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 12:11:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

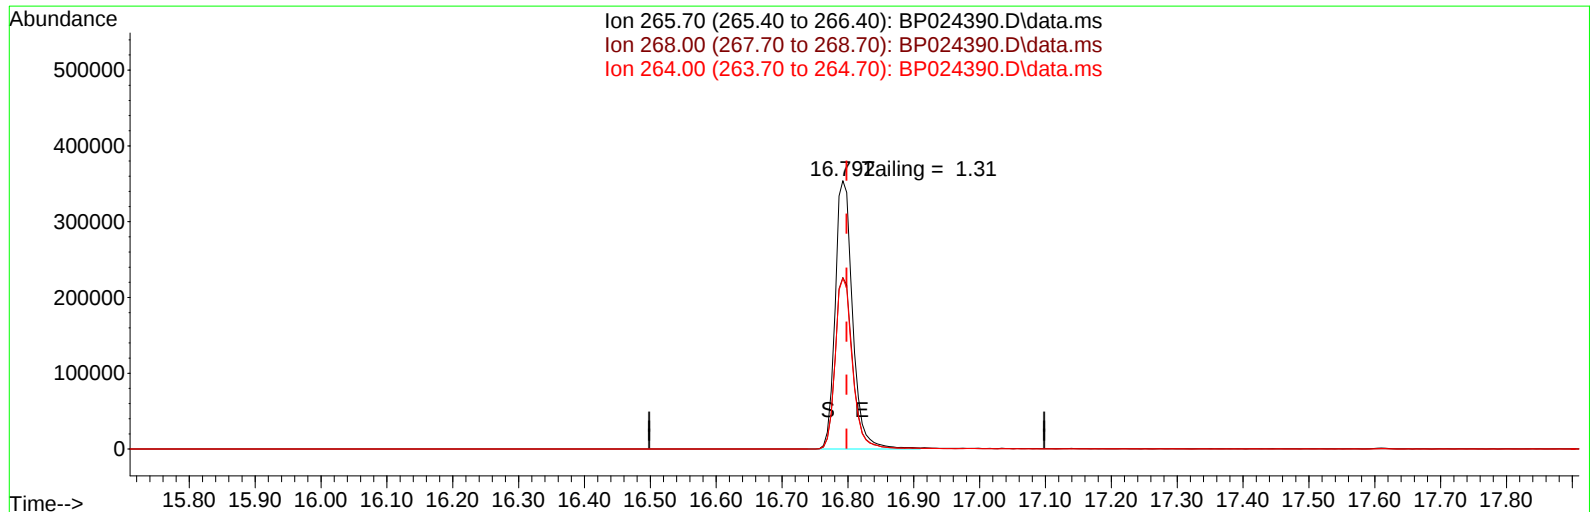

TIC: BP024390.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.006) 1895451.27 ng

response 653022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.90
264.00	62.20	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042325\
Data File : BP024390.D
Acq On : 23 Apr 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 12:11:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

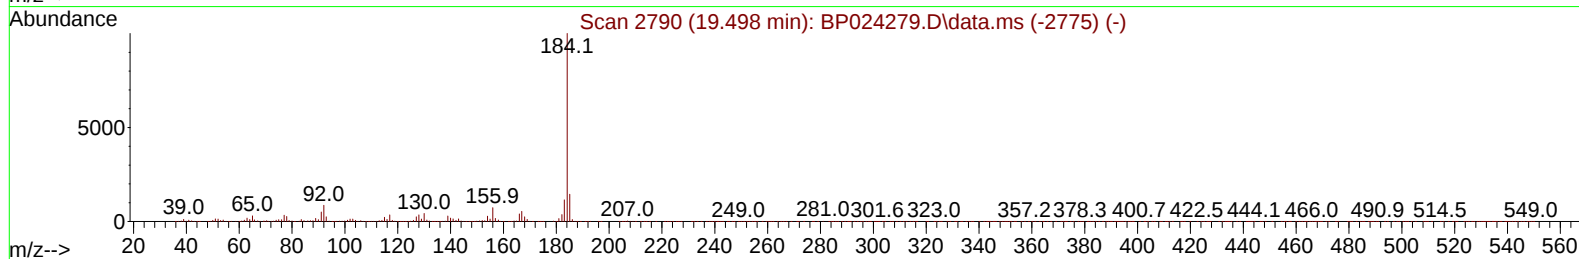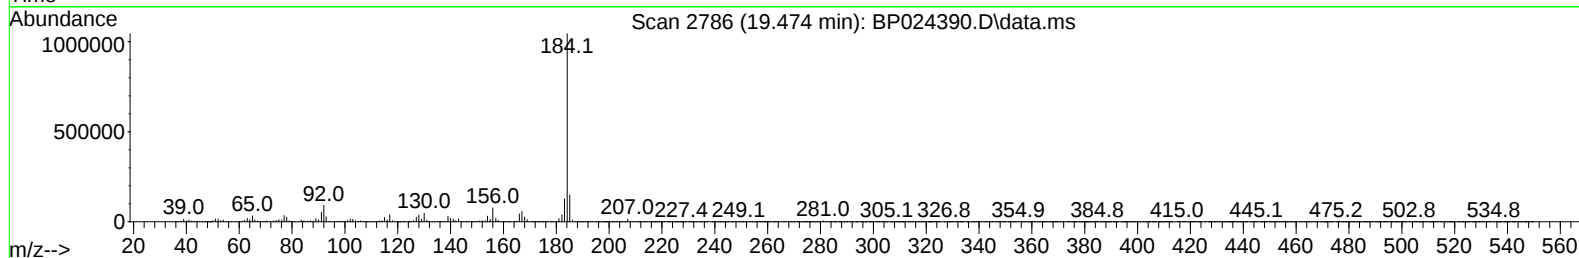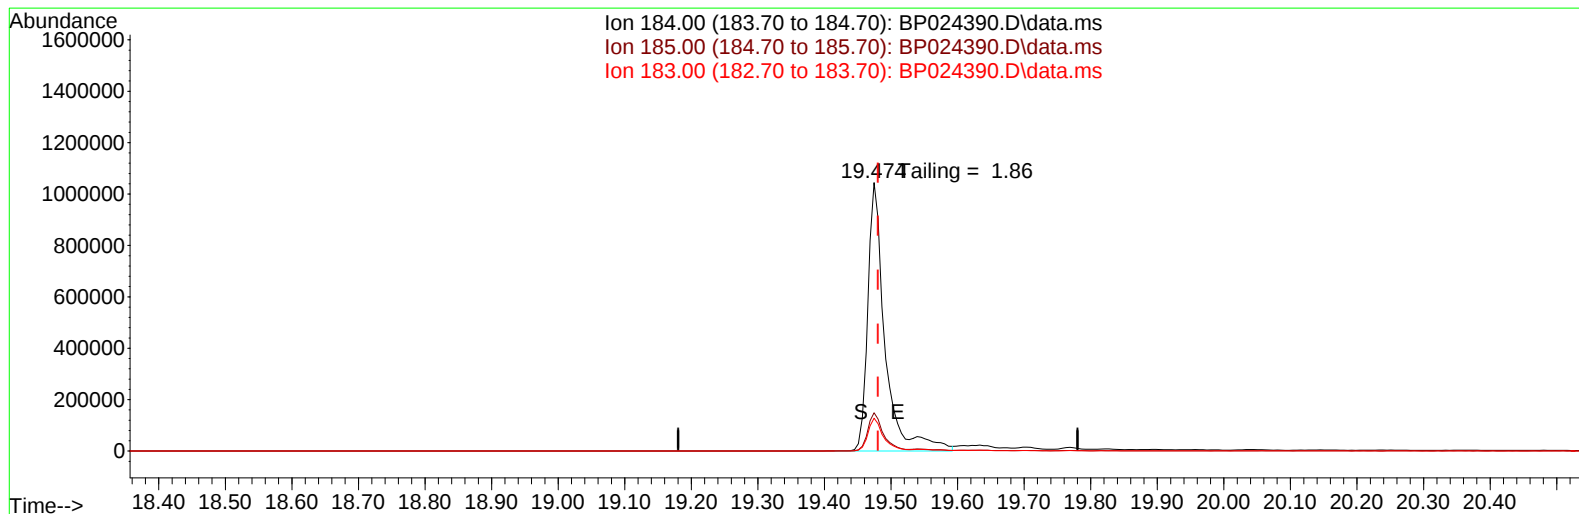

TIC: BP024390.D\data.ms

(77) Benzidine**19.474min (-0.006) 1113291.37 ng****response 1735765**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.29
183.00	11.50	12.23
0.00	0.00	0.00