
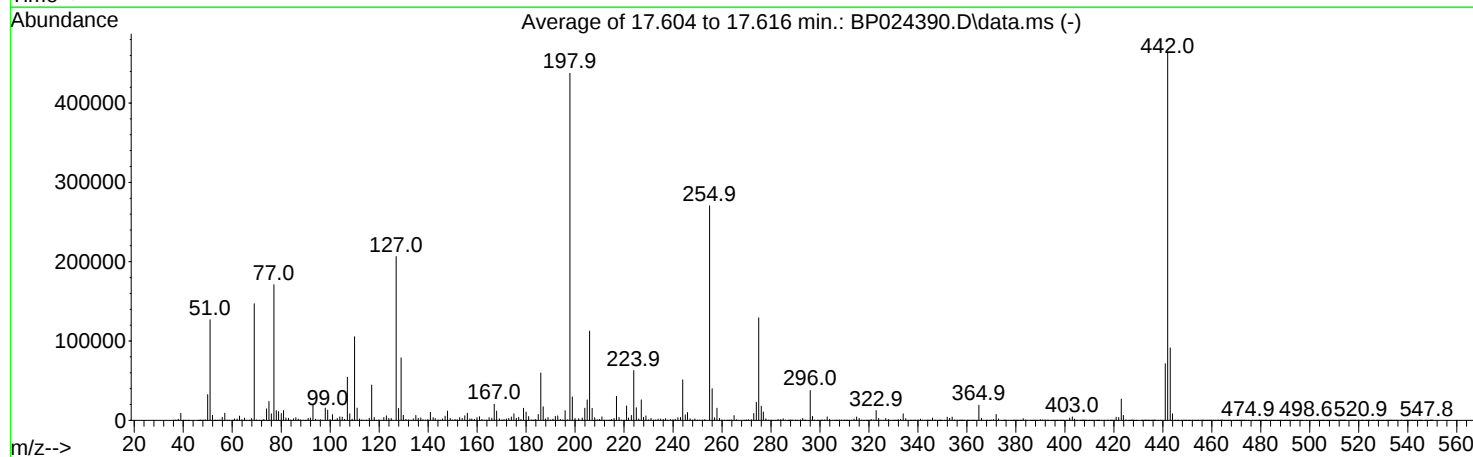


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042325\
Data File : BP024390.D
Acq On : 23 Apr 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

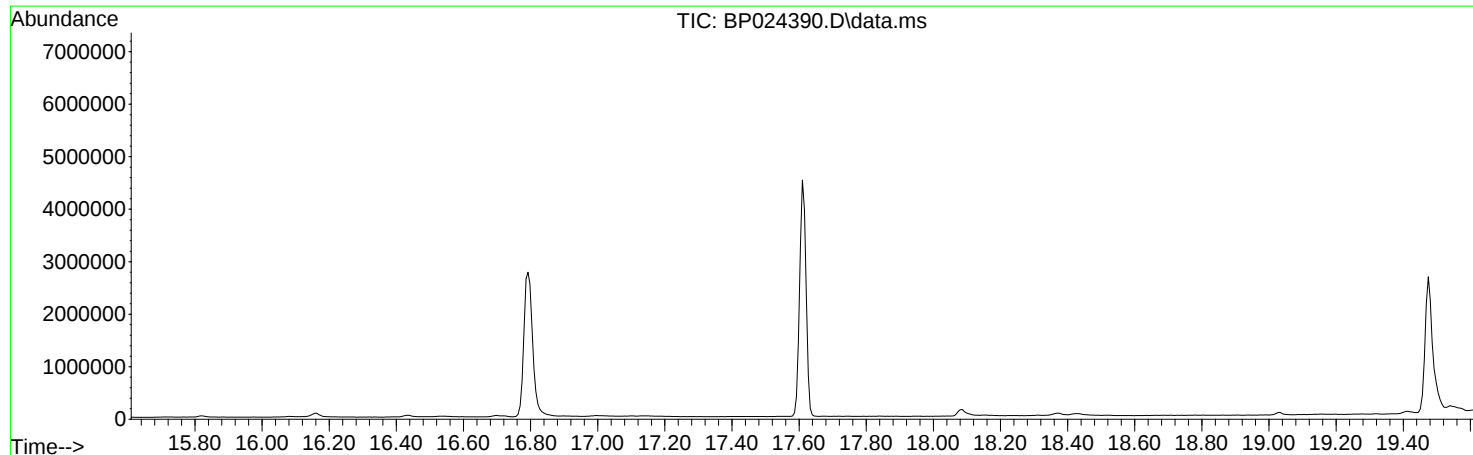

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	126801	PASS
68	69	0.00	2	1.7	2489	PASS
69	198	0.00	100	33.6	147088	PASS
70	69	0.00	2	0.5	684	PASS
127	198	10	80	47.2	206530	PASS
197	198	0.00	2	0.2	773	PASS
198	198	100	100	100.0	437513	PASS
199	198	5	9	6.8	29699	PASS
275	198	10	60	29.6	129335	PASS
365	198	1	100	4.4	19102	PASS
441	198	0.01	100	16.3	71425	PASS
442	442	100	100	100.0	463720	PASS
443	442	15	24	19.7	91357	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/23/2025	BNA_P	<u>BP024390.D</u>
Compound Name	Response	Retention Time
DDT	1648024	20.763
DDD	33472	20.298
DDE	2264	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35736	1683760	2.12

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042325\
Data File : BP024390.D
Acq On : 23 Apr 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 23 12:11:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

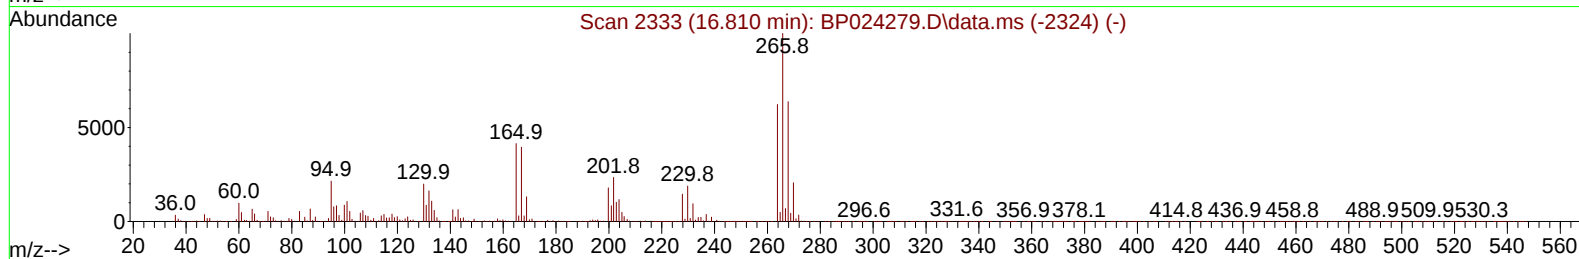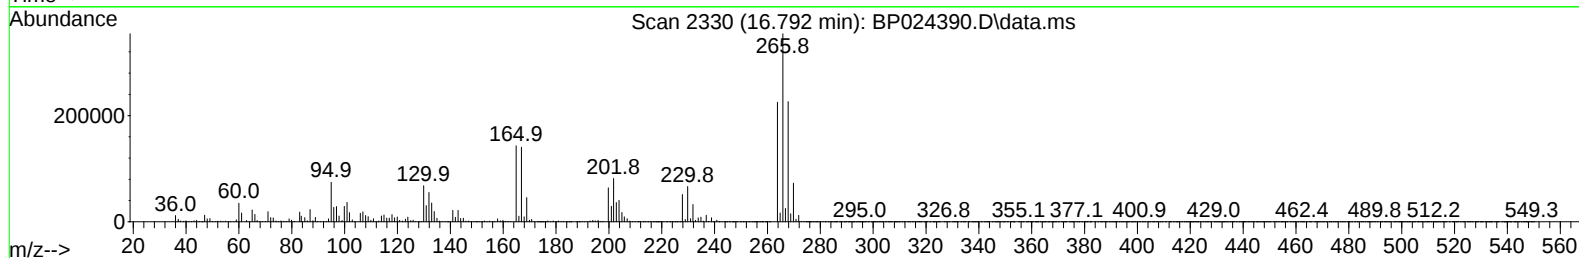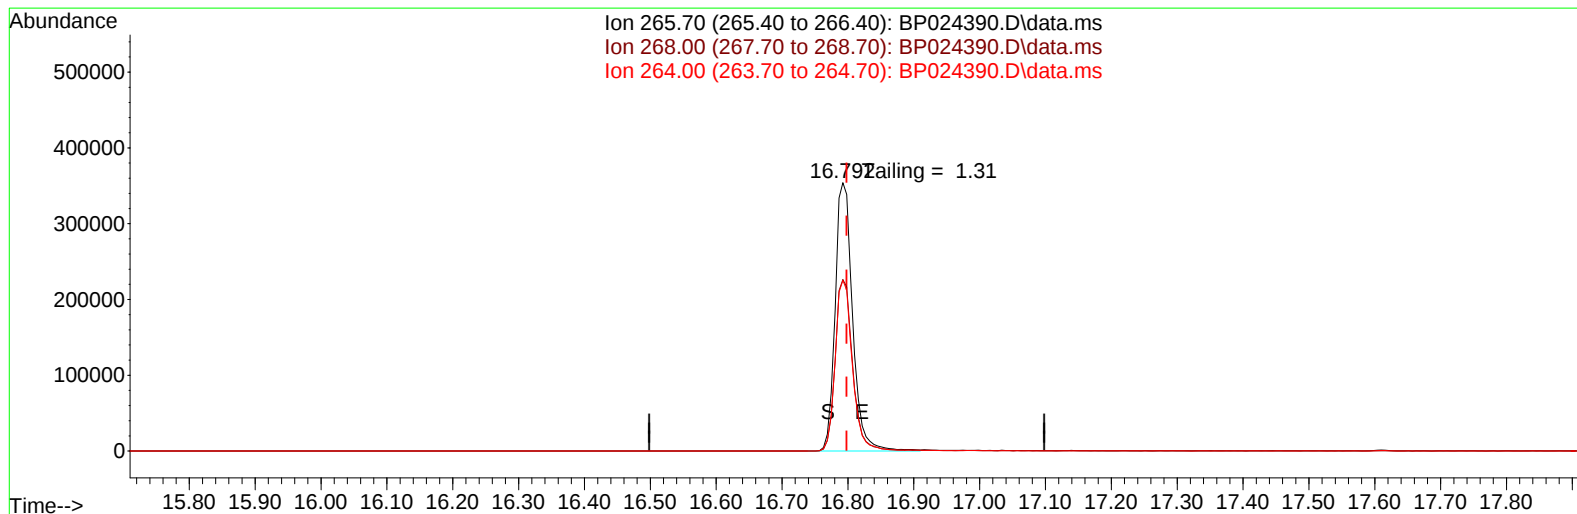

TIC: BP024390.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.006) 1895451.27 ng




response 653022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.90
264.00	62.20	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042325\
Data File : BP024390.D
Acq On : 23 Apr 2025 09:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 23 12:11:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

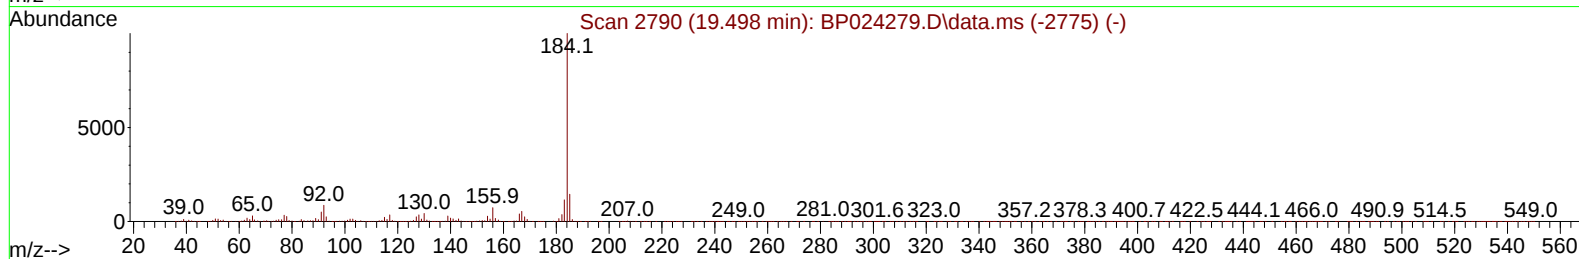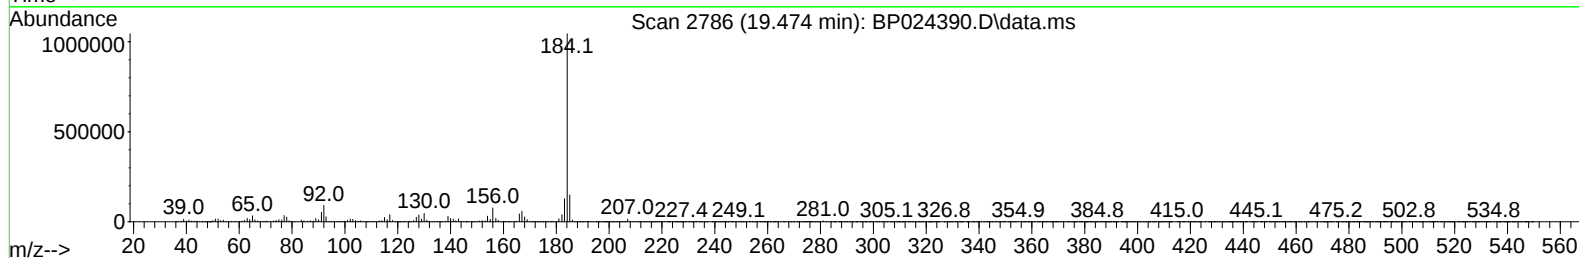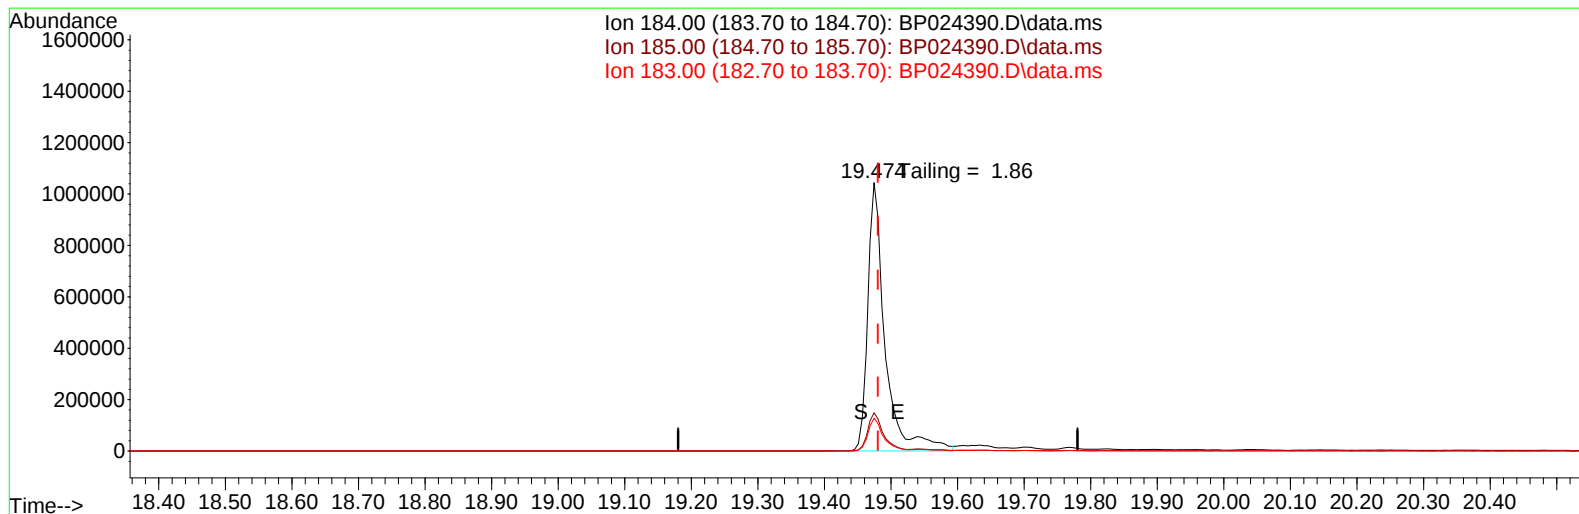

TIC: BP024390.D\data.ms

(77) Benzidine

19.474min (-0.006) 1113291.37 ng

response 1735765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.29
183.00	11.50	12.23
0.00	0.00	0.00