
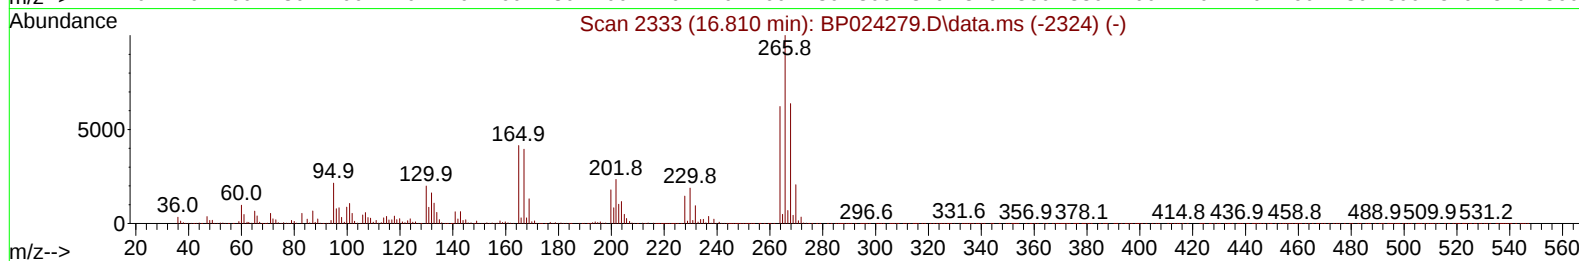
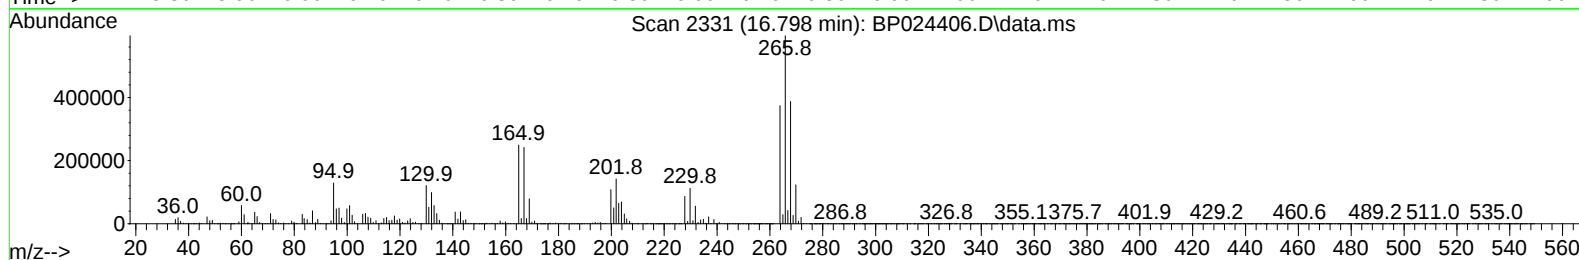


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042425\
Data File : BP024406.D
Acq On : 24 Apr 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 11:48:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

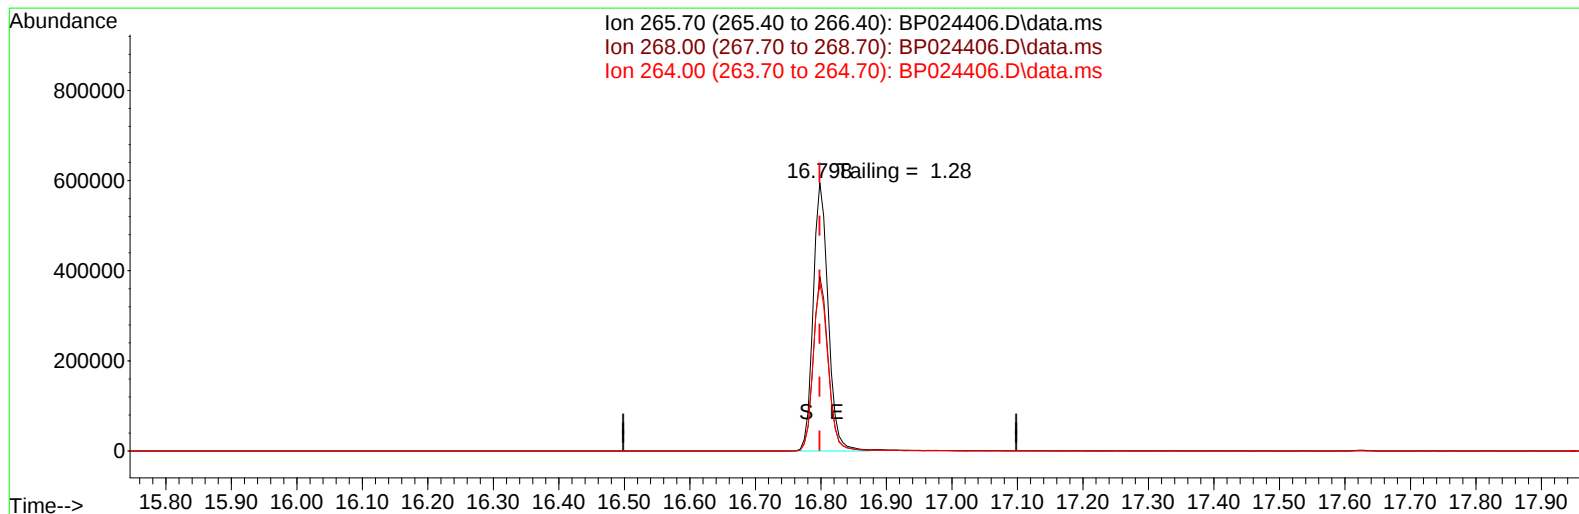

TIC: BP024406.D\data.ms

(70) Pentachlorophenol (C)




16.798min (+ 0.000) 1949769.80 ng

response 954572

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.02
264.00	62.20	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042425\
Data File : BP024406.D
Acq On : 24 Apr 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 11:48:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

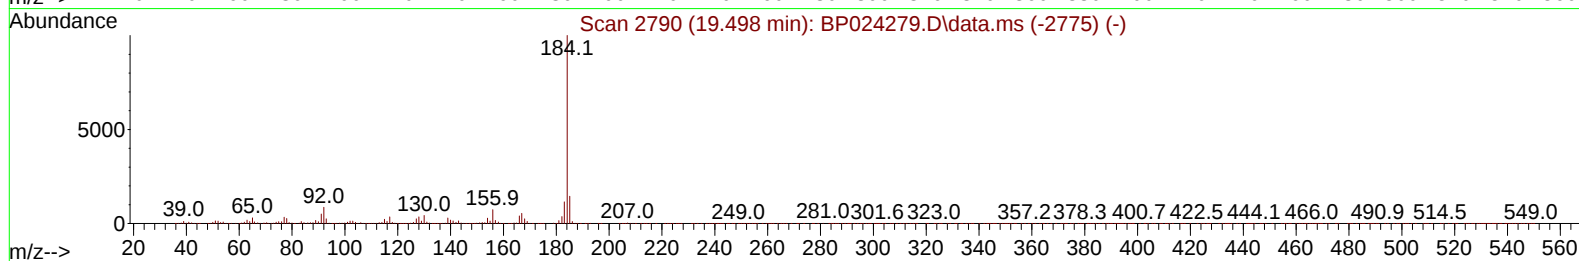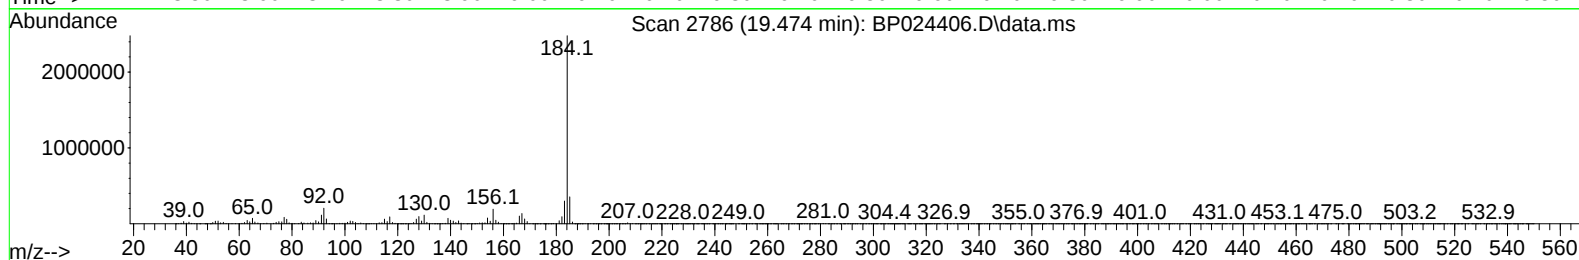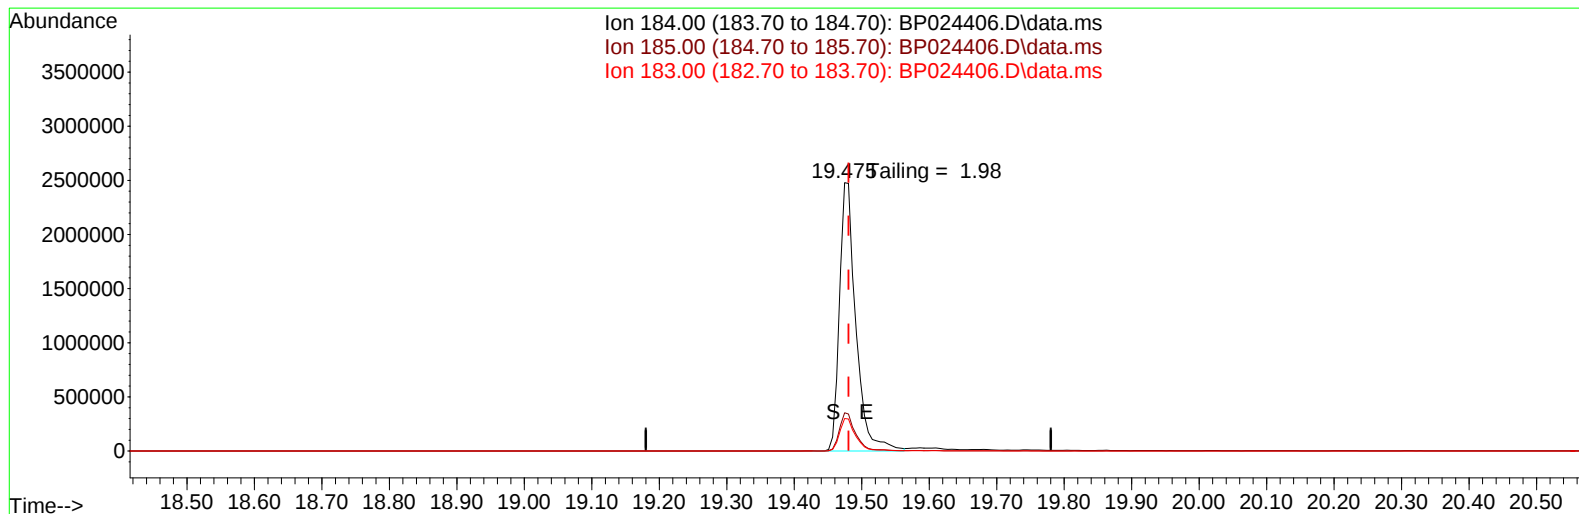

TIC: BP024406.D\data.ms

(77) Benzidine**19.474min (-0.006) 159548.41 ng****response 4190436**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.28
183.00	11.50	12.13
0.00	0.00	0.00