


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP042425\  
Data File : BP024406.D  
Acq On : 24 Apr 2025 11:10  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP041425.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Apr 18 12:04:48 2025

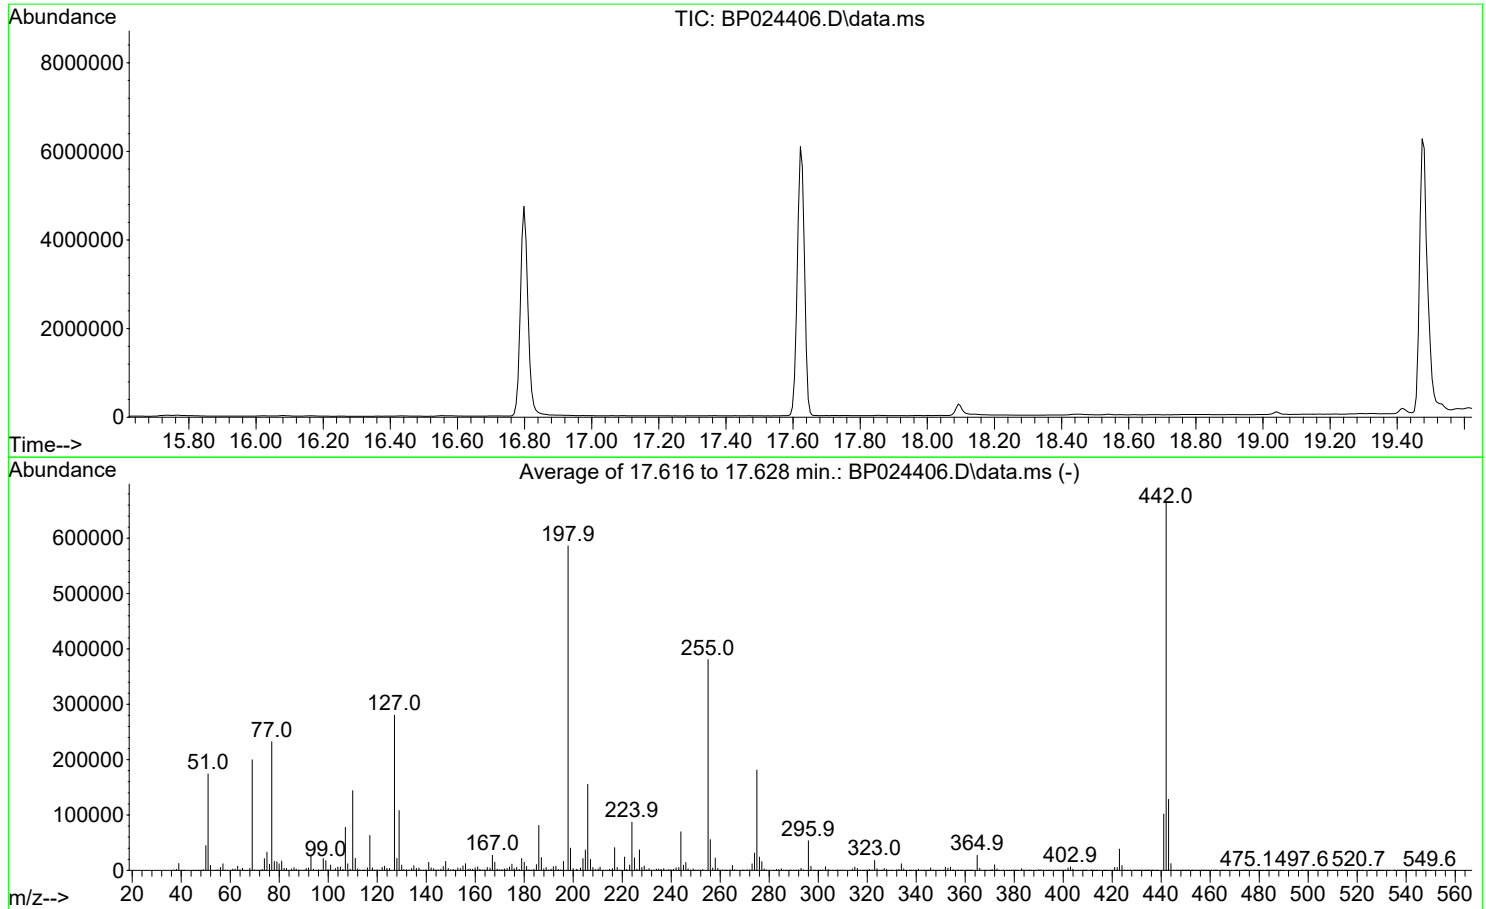

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2460

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.7         | 174345     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 3425       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.1         | 199717     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 989        | PASS                |
| 127            | 198             | 10              | 80              | 47.8         | 280405     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 586148     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 40140      | PASS                |
| 275            | 198             | 10              | 60              | 30.9         | 181200     | PASS                |
| 365            | 198             | 1               | 100             | 4.7          | 27301      | PASS                |
| 441            | 198             | 0.01            | 100             | 17.4         | 101899     | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 664554     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 128227     | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/24/2025     | BNA_P            | <u>BP024406.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2177853          | 20.763             |
| DDD           | 50858            | 20.31              |
| DDE           | 2680             | 19.774             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 53538         | 2231391          | 2.40               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP042425\  
Data File : BP024406.D  
Acq On : 24 Apr 2025 11:10  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Apr 24 11:48:42 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP041425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 18 12:04:48 2025  
Response via : Initial Calibration

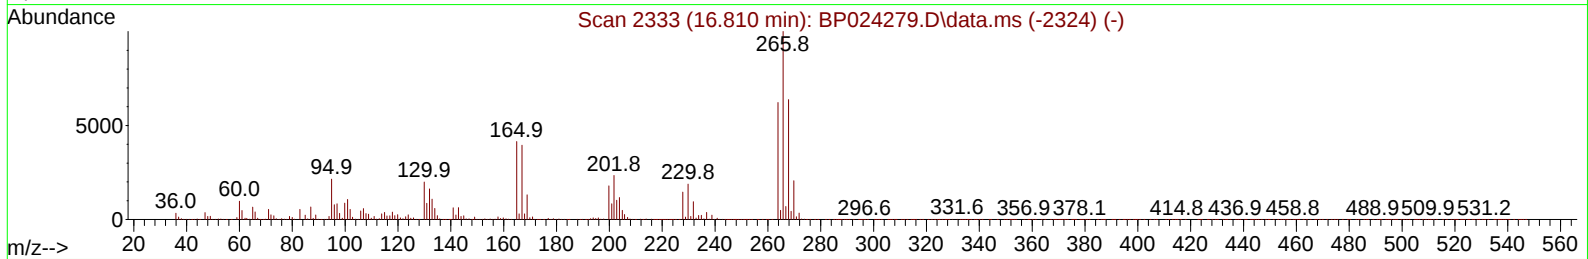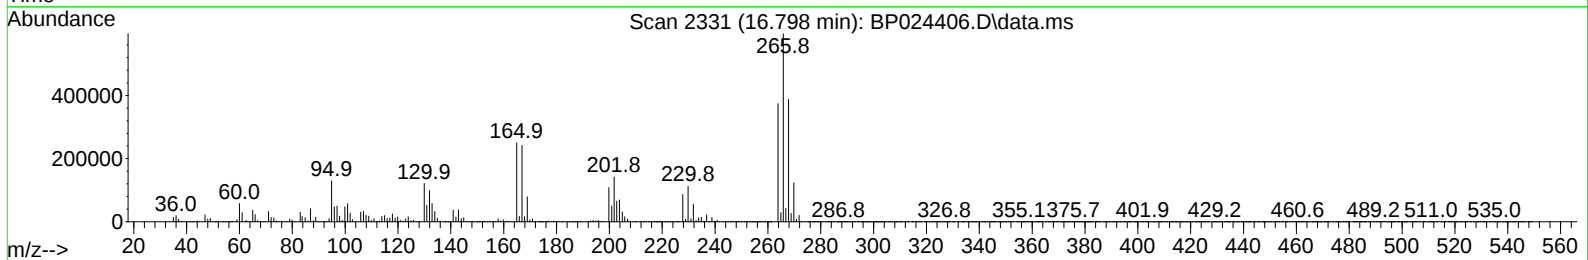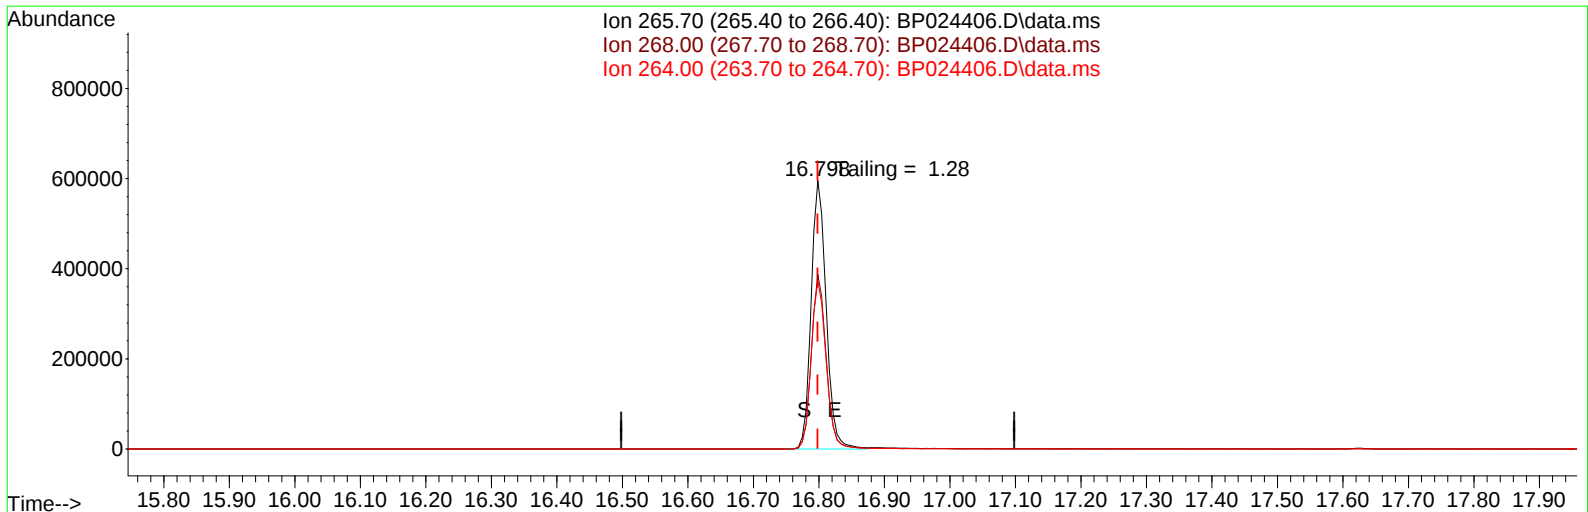

TIC: BP024406.D\data.ms

**(70) Pentachlorophenol (C)**

**16.798min (+ 0.000) 1949769.80 ng**




**response 954572**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 65.02  |
| 264.00 | 62.20  | 62.78  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP042425\  
Data File : BP024406.D  
Acq On : 24 Apr 2025 11:10  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Apr 24 11:48:42 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP041425.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 18 12:04:48 2025  
Response via : Initial Calibration

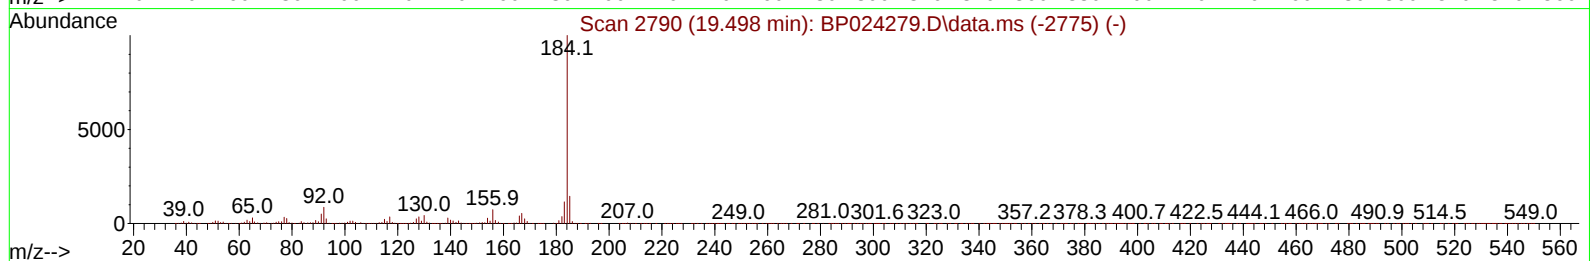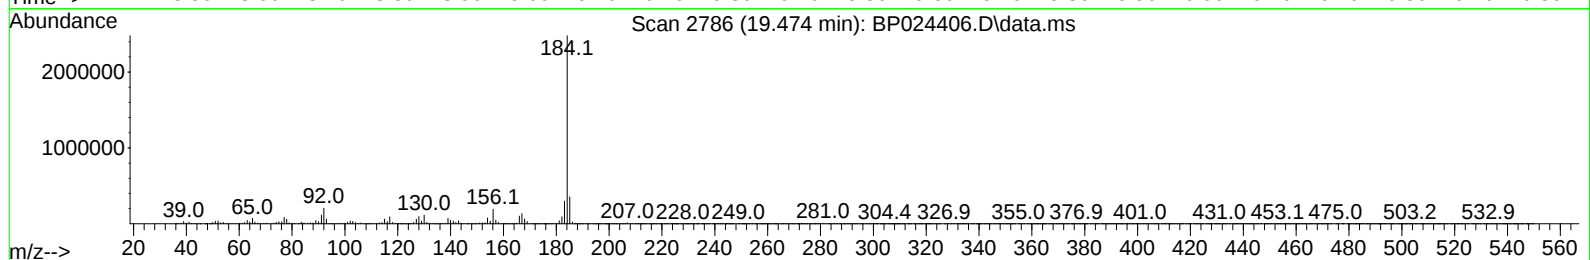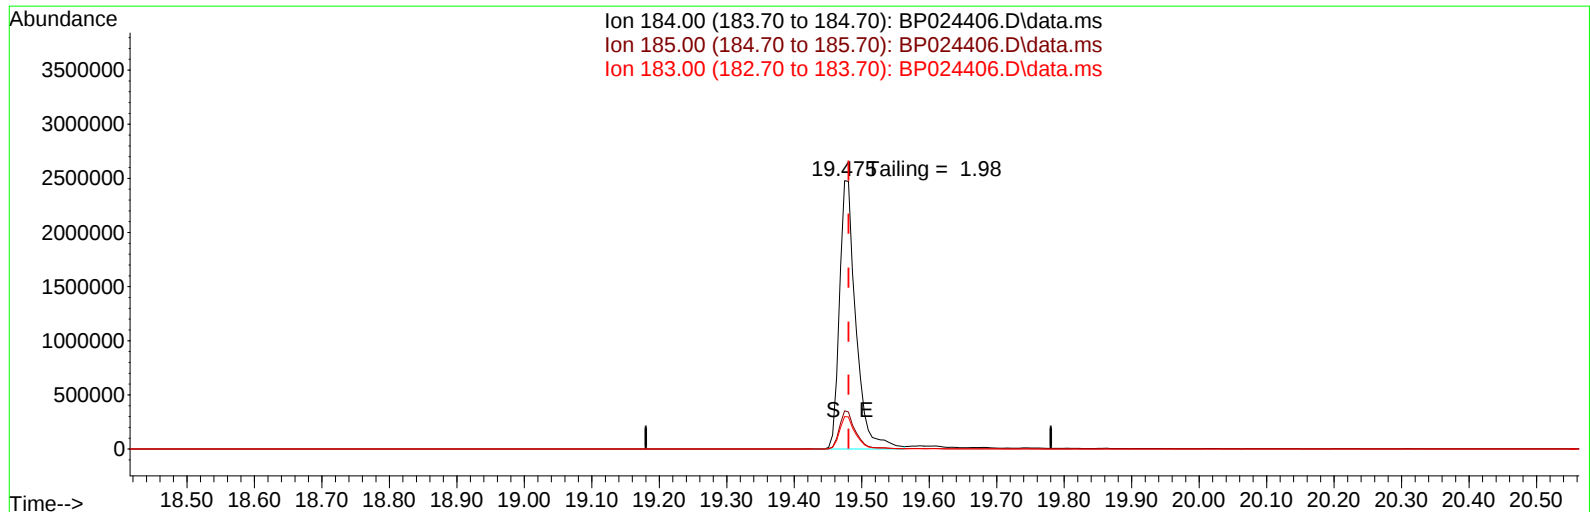

TIC: BP024406.D\data.ms

(77) Benzidine

19.474min (-0.006) 159548.41 ng

response 4190436

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 14.28  |
| 183.00 | 11.50  | 12.13  |
| 0.00   | 0.00   | 0.00   |