




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010080.D
 Acq On : 25 Apr 2022 13:03
 Operator : CG/JU
 Sample : PB144303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK303

Manual IntegrationsAPPROVED

Quant Time: Apr 26 00:58:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

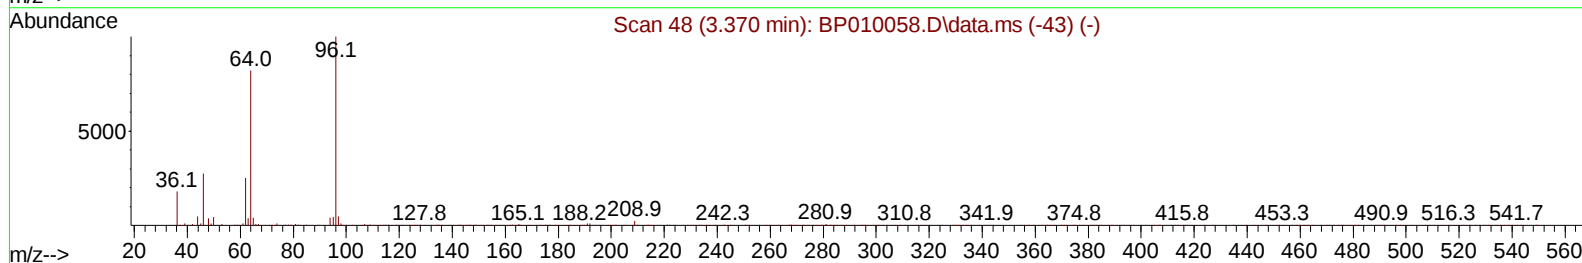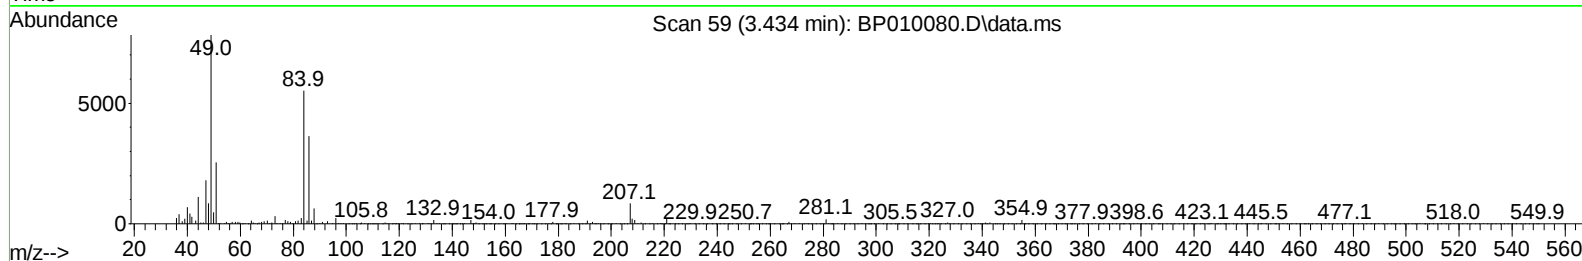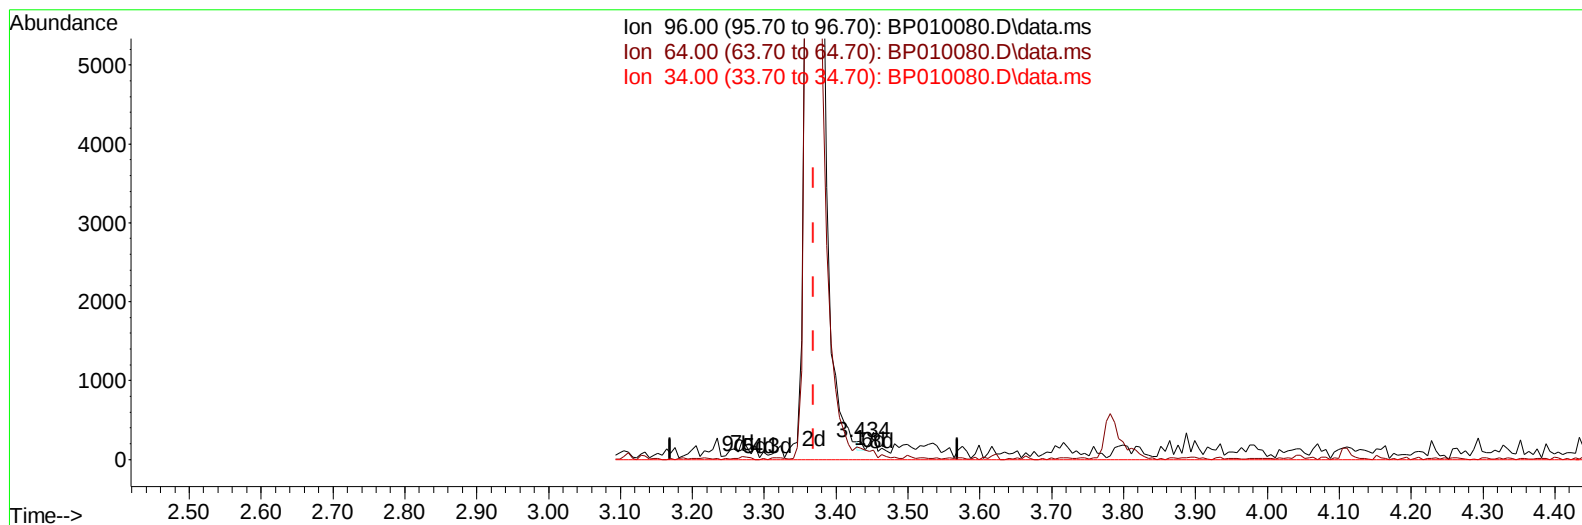

TIC: BP010080.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.434min (+ 0.065) 0.01 ng/uL

response 40

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	60.17
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010080.D
 Acq On : 25 Apr 2022 13:03
 Operator : CG/JU
 Sample : PB144303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK303

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 00:58:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

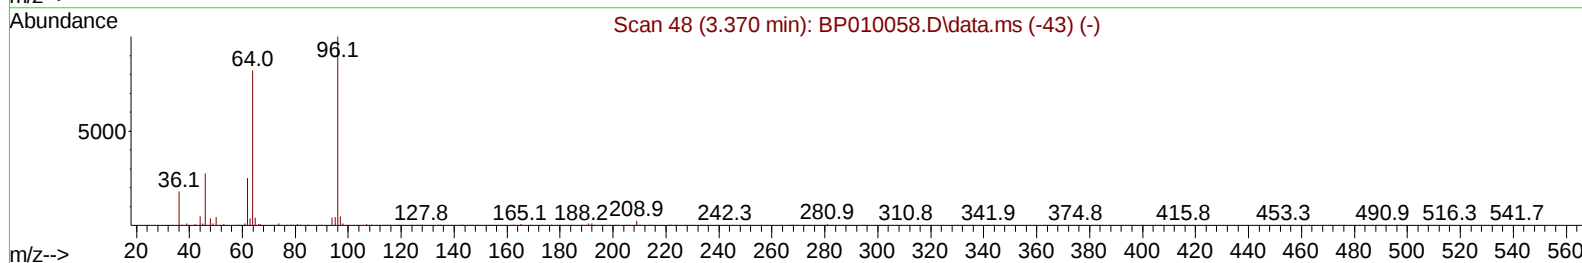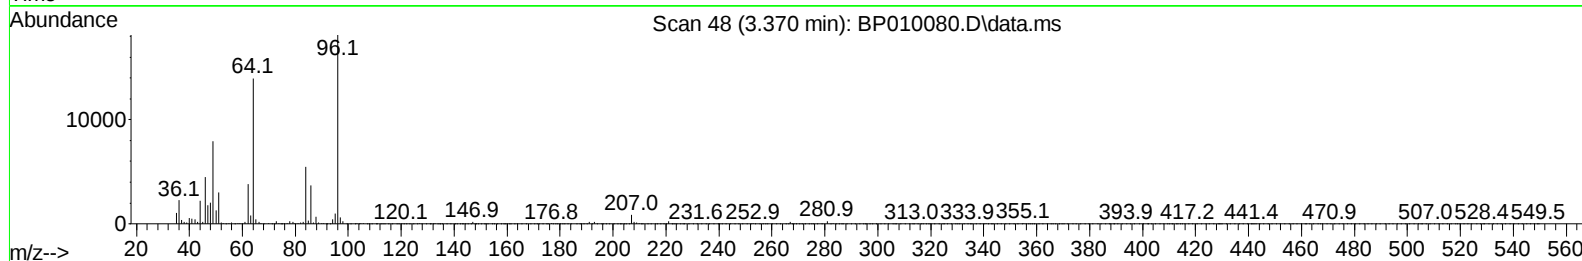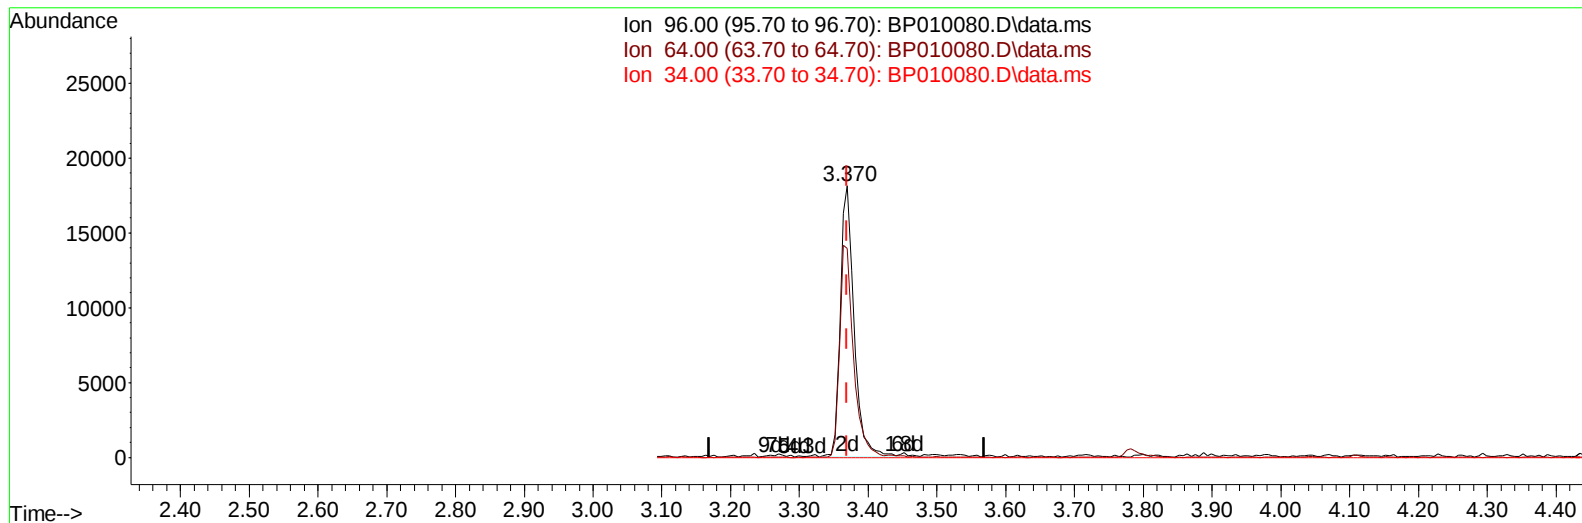

TIC: BP010080.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (+ 0.001) 6.30 ng/uL m

response 25211

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	76.96#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010080.D
 Acq On : 25 Apr 2022 13:03
 Operator : CG/JU
 Sample : PB144303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK303

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 00:58:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	174511	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	759223	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	521712	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	1132286	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	1025733	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	895012	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	25211m	6.300	ng/uL	0.00
4) Pyridine-d5	3.781	84	295176	26.219	ng/ul	0.00
7) Phenol-d5	7.093	99	405999	25.577	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	286576	30.088	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.464	132	336277	28.605	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	346158	26.321	ng/ul	-0.01
21) Nitrobenzene-d5	9.093	128	175965	29.141	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	192736	29.225	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.358	165	322114	25.090	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	484312	26.309	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	1254388	30.909	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1353451	27.556	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	162776	21.787	ng/ul	0.00
60) Fluorene-d10	15.563	176	1030788	29.527	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	179300	25.043	ng/ul	0.00
73) Anthracene-d10	17.422	188	1653372	30.183	ng/ul	0.00
81) Pyrene-d10	19.651	212	1946640	33.371	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	1486909	31.689	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010080.D
Acq On : 25 Apr 2022 13:03
Operator : CG/JU
Sample : PB144303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK303

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 00:58:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

