




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010092.D
Acq On : 25 Apr 2022 20:28
Operator : CG/JU
Sample : N2475-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM8

Manual IntegrationsAPPROVED

Quant Time: Apr 26 01:04:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

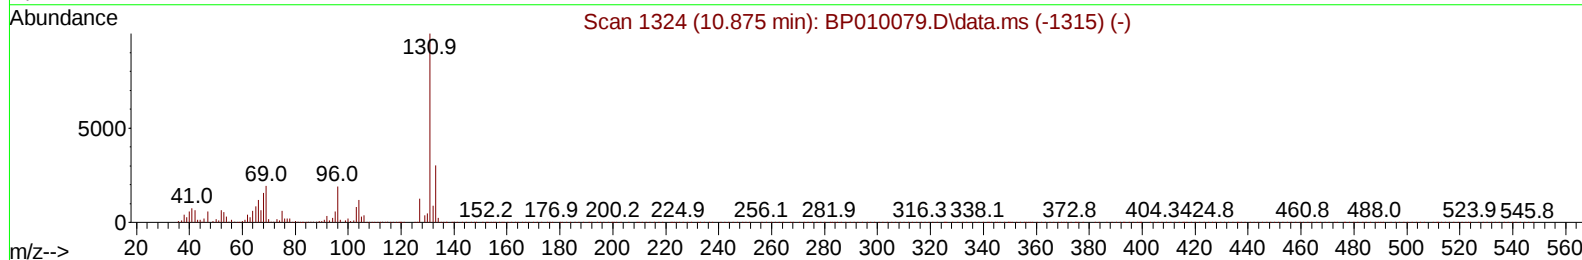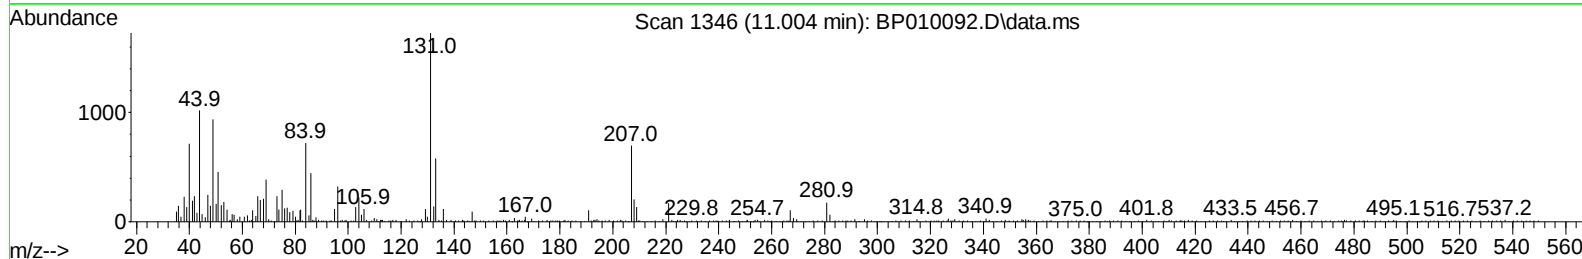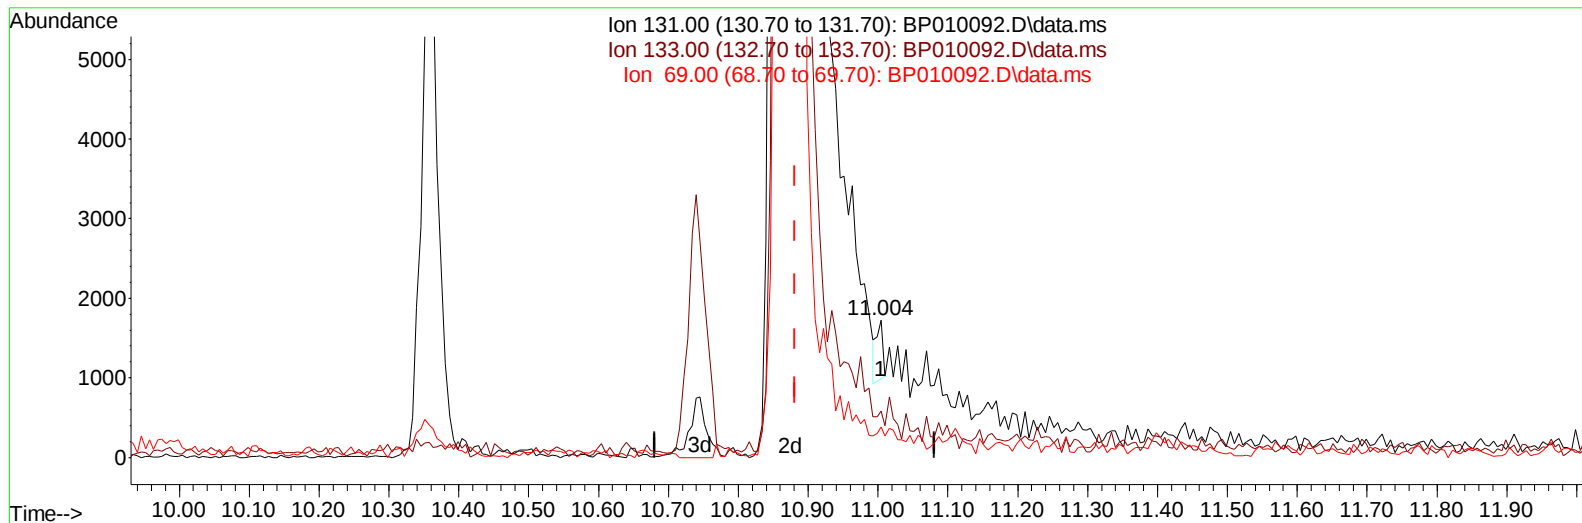

TIC: BP010092.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.004min (+ 0.123) 0.03 ng/u1

response 477

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	33.68
69.00	26.10	22.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010092.D
Acq On : 25 Apr 2022 20:28
Operator : CG/JU
Sample : N2475-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 01:04:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

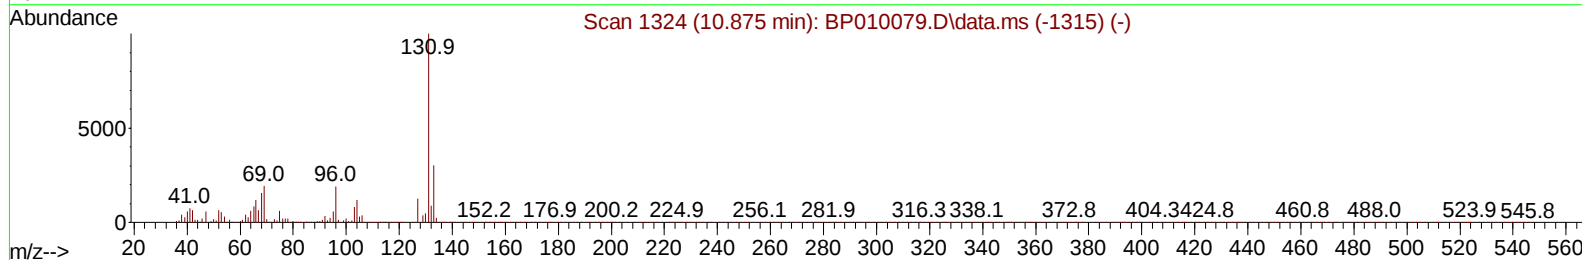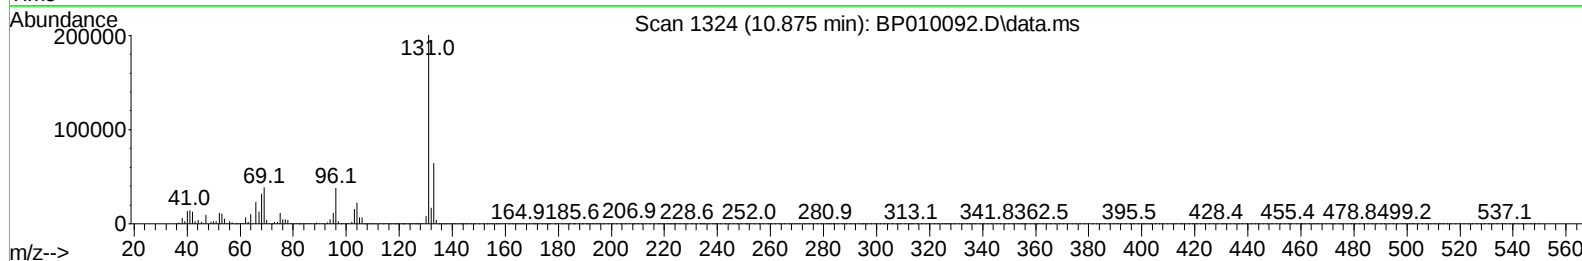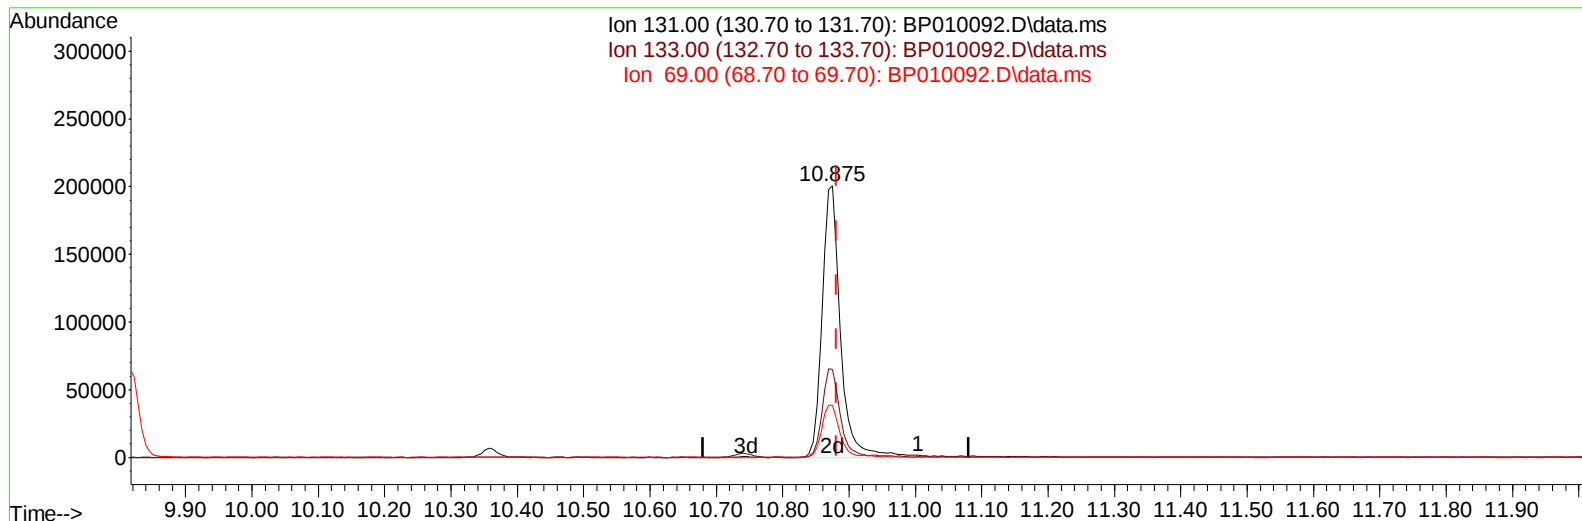

TIC: BP010092.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.875min (-0.006) 23.20 ng/ul m

response 389469

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	32.36
69.00	26.10	19.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010092.D
 Acq On : 25 Apr 2022 20:28
 Operator : CG/JU
 Sample : N2475-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BM8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 01:04:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	164244	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.740	136	692403	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	480720	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188	1010175	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.398	240	821207	20.000	ng/ul	#-0.01
88) Perylene-d12	23.851	264	637739	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	18364	4.876	ng/uL	0.00
4) Pyridine-d5	3.793	84	56243	5.308	ng/ul	0.00
7) Phenol-d5	7.093	99	88934	5.953	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	292539	32.634	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132	266236	24.063	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	185925	15.021	ng/ul	-0.01
21) Nitrobenzene-d5	9.093	128	181436	32.946	ng/ul	0.00
24) 2-Nitrophenol-d4	9.816	143	192326	31.978	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	311212	26.580	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	389469m	23.199	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	1332155	35.624	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1443447	31.894	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	28398	4.125	ng/ul	0.00
60) Fluorene-d10	15.557	176	1133547	35.239	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	195490	30.605	ng/ul	0.00
73) Anthracene-d10	17.416	188	1761716	36.048	ng/ul	0.00
81) Pyrene-d10	19.651	212	1999579	42.815	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	1309075	39.154	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010092.D
Acq On : 25 Apr 2022 20:28
Operator : CG/JU
Sample : N2475-10
Misc :
ALS Vial : 14 Sample Multiplier: 3

Instrument :
BNA_P
ClientSampleId :
A0BM8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 01:04:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

