




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010099.D
 Acq On : 26 Apr 2022 00:23
 Operator : CG/JU
 Sample : N2473-18RX
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9RX

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:48:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

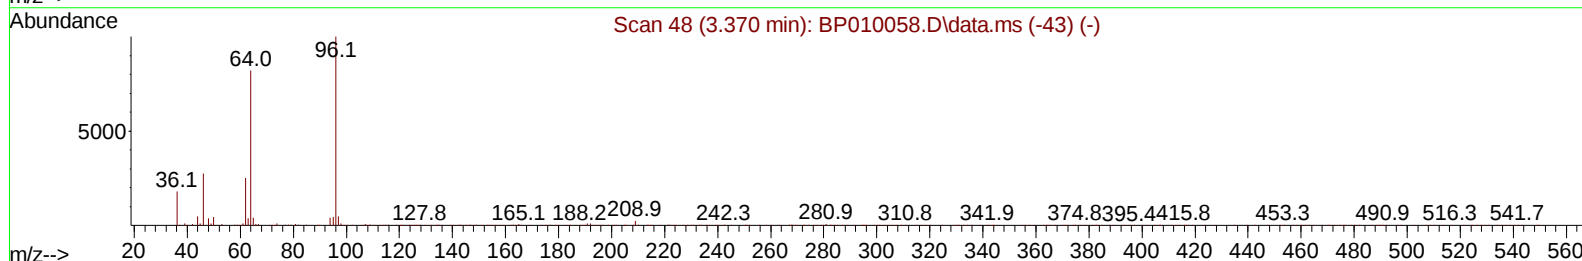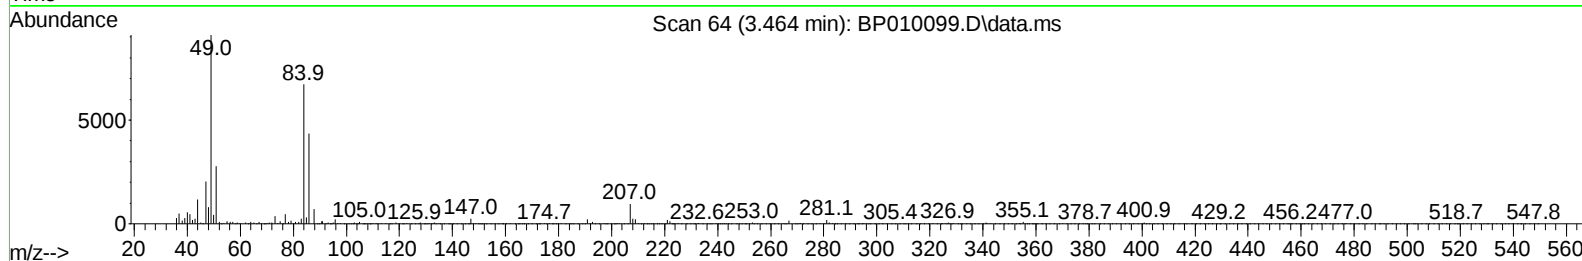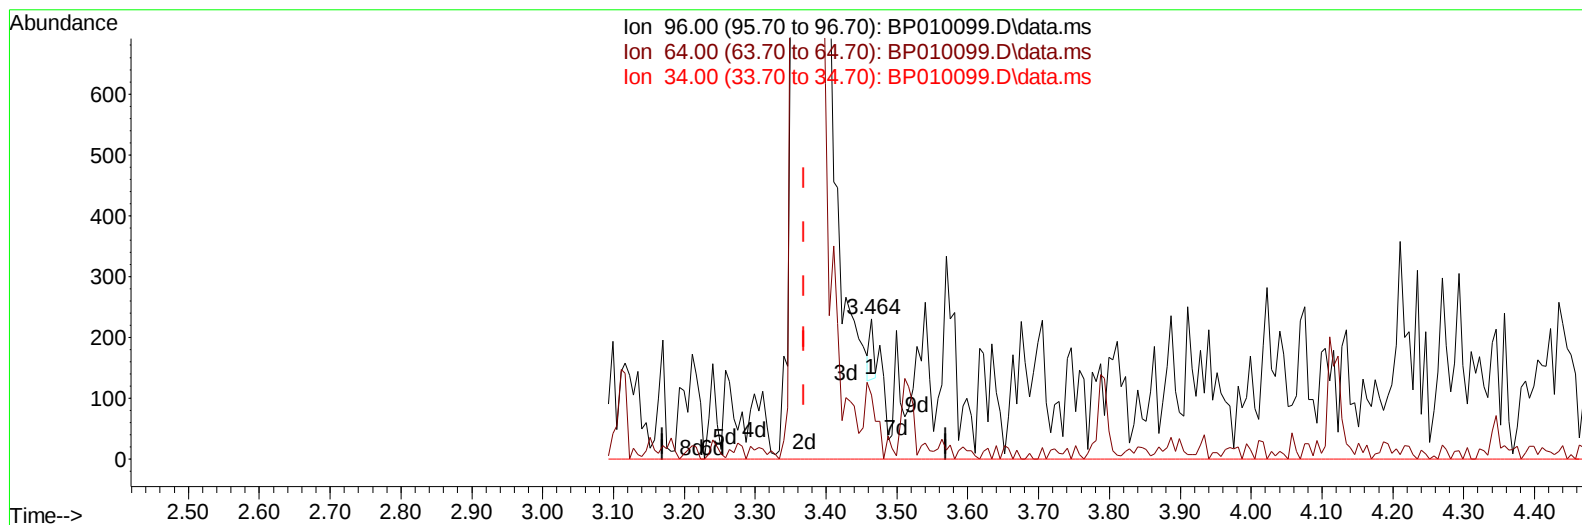

TIC: BP010099.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.464min (+ 0.095) 0.01 ng/uL

response	38	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	45.45
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

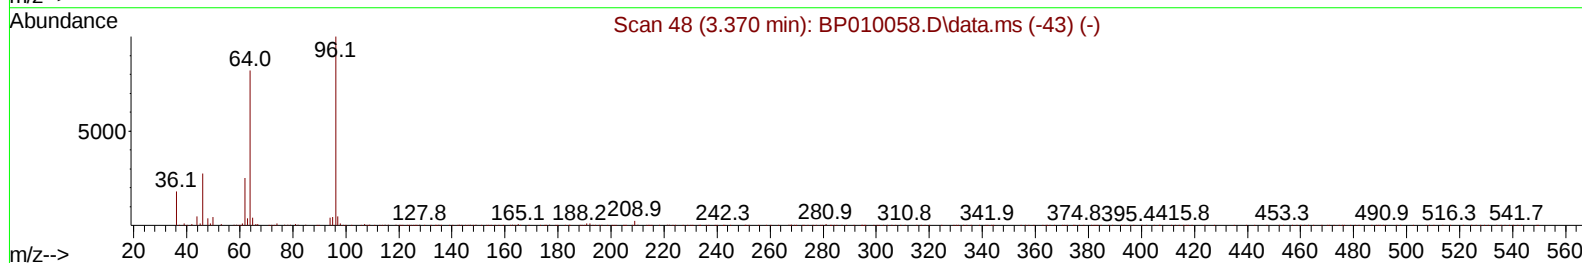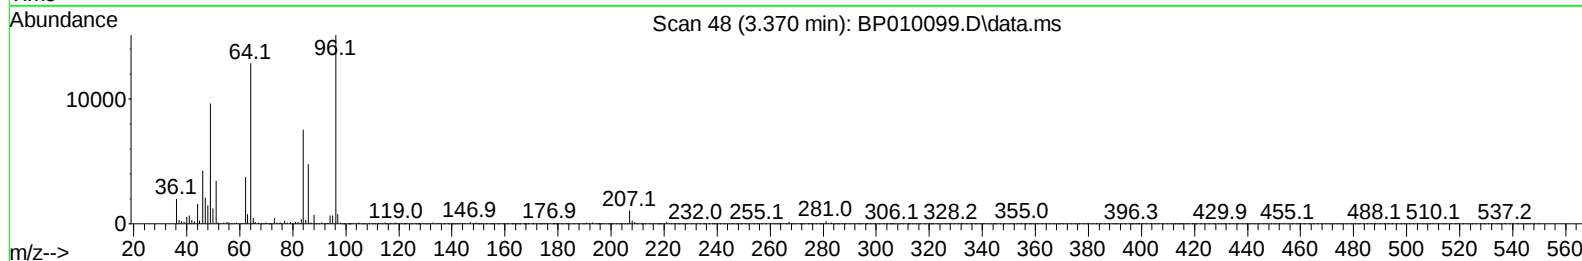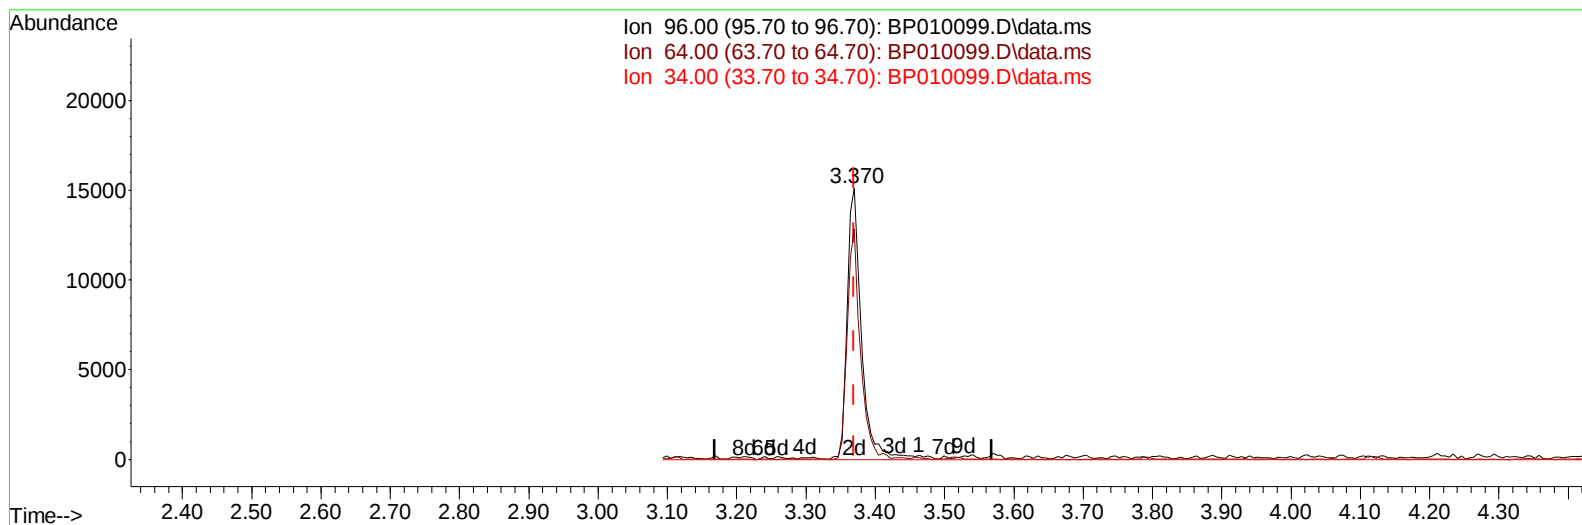

TIC: BP010099.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (+ 0.001) 5.12 ng/uL m

response 21099

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	85.08#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

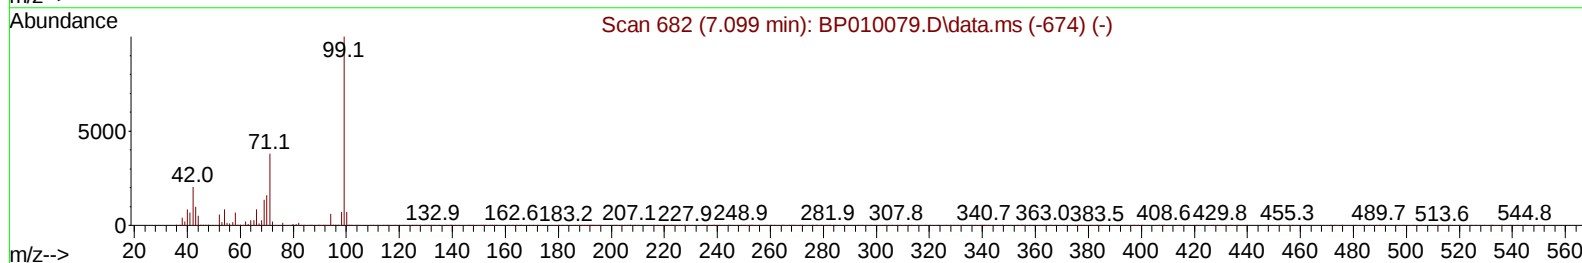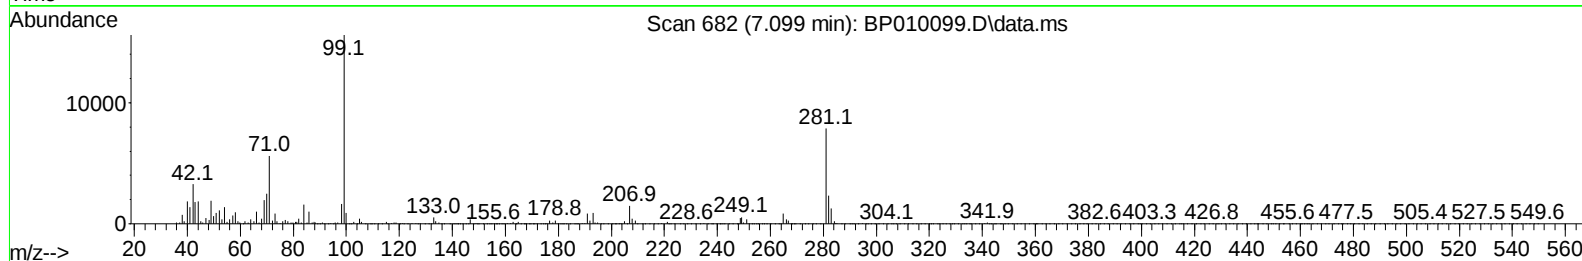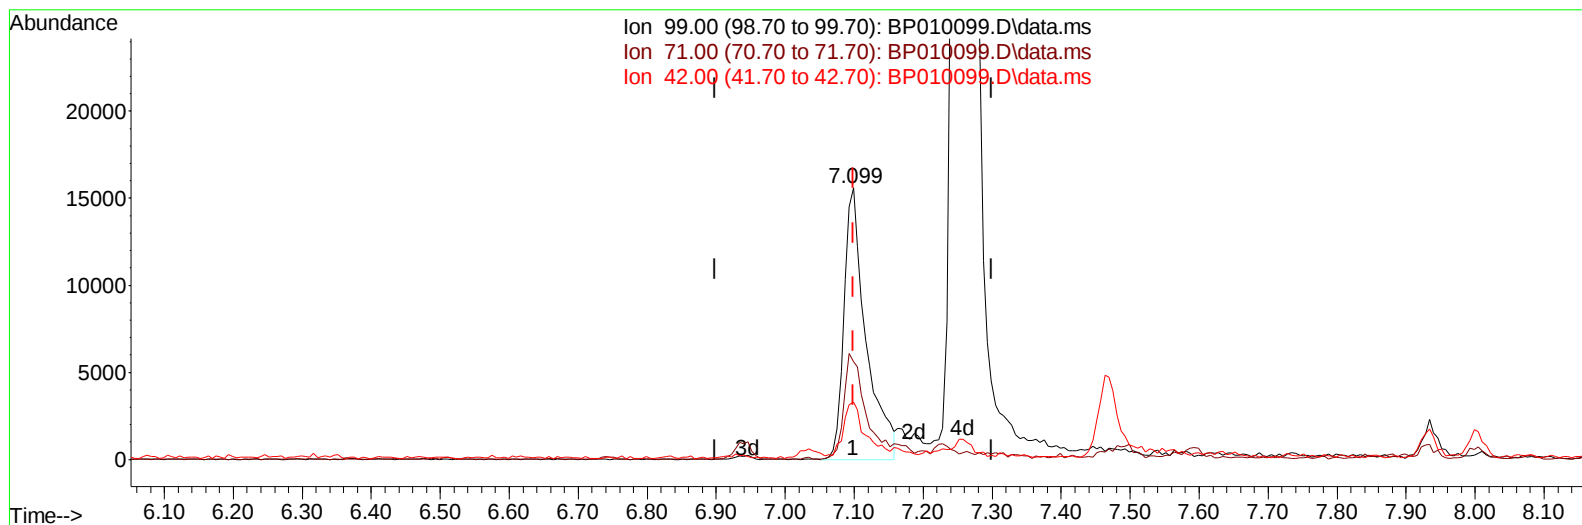

TIC: BP010099.D\data.ms

(7) Phenol-d5 (S)

7.099min (+ 0.000) 2.11 ng/u1

response 34496

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	33.50	35.96
42.00	7.30	21.01#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010099.D
 Acq On : 26 Apr 2022 00:23
 Operator : CG/JU
 Sample : N2473-18RX
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9RX

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:48:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

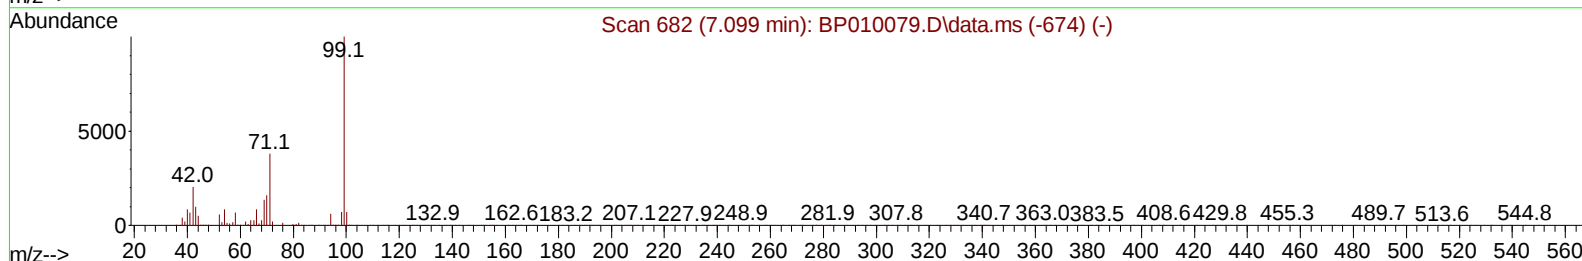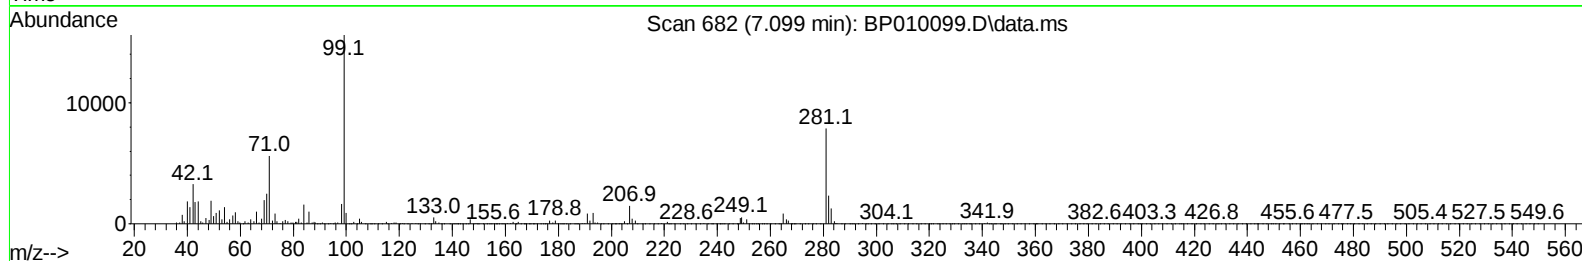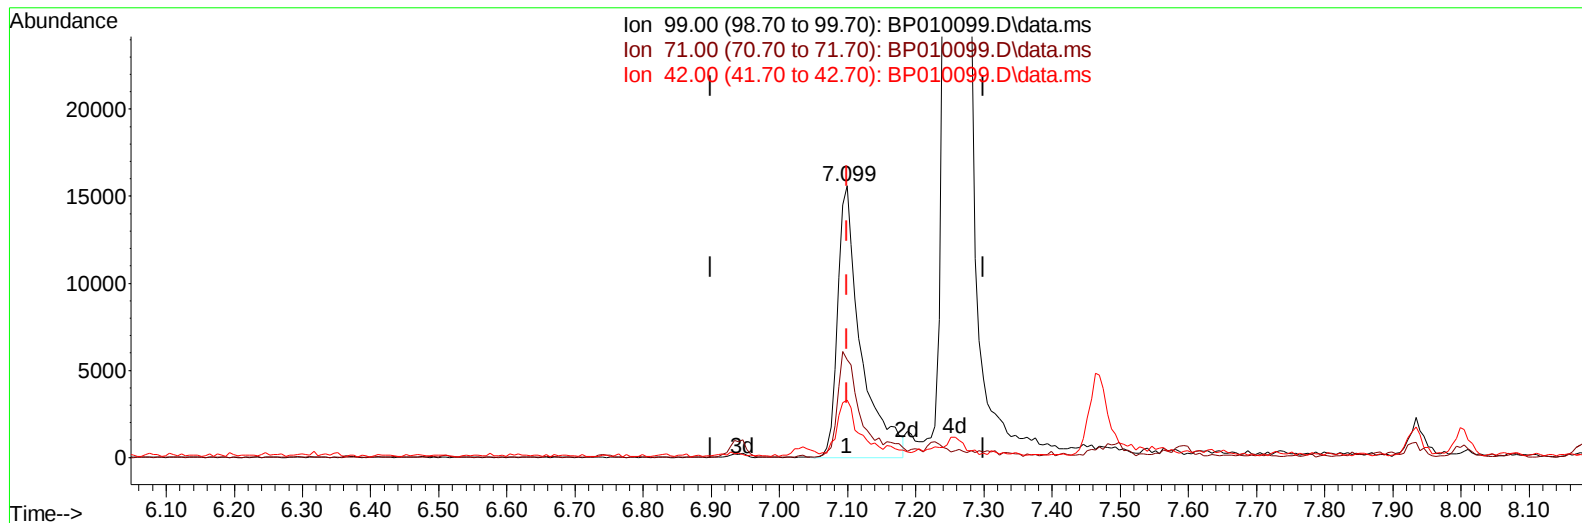

TIC: BP010099.D\data.ms

(7) Phenol-d5 (S)

7.099min (+ 0.000) 2.24 ng/ul m

response 36591

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	33.50	35.96
42.00	7.30	21.01#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

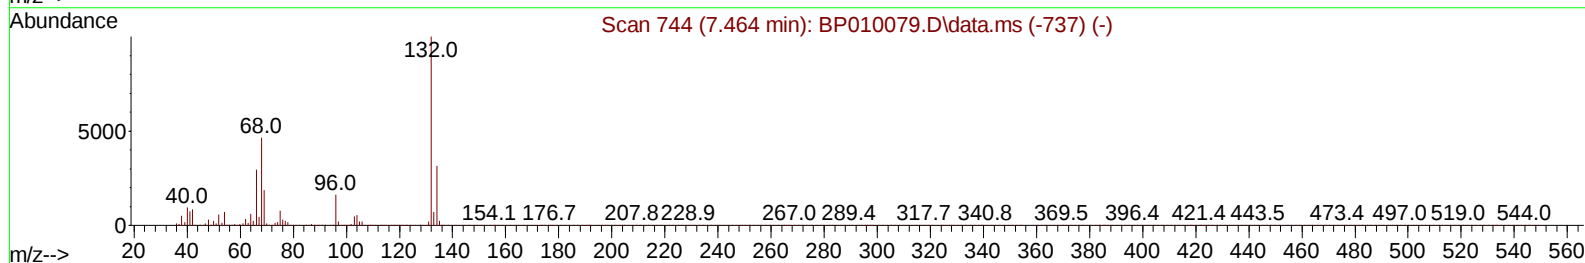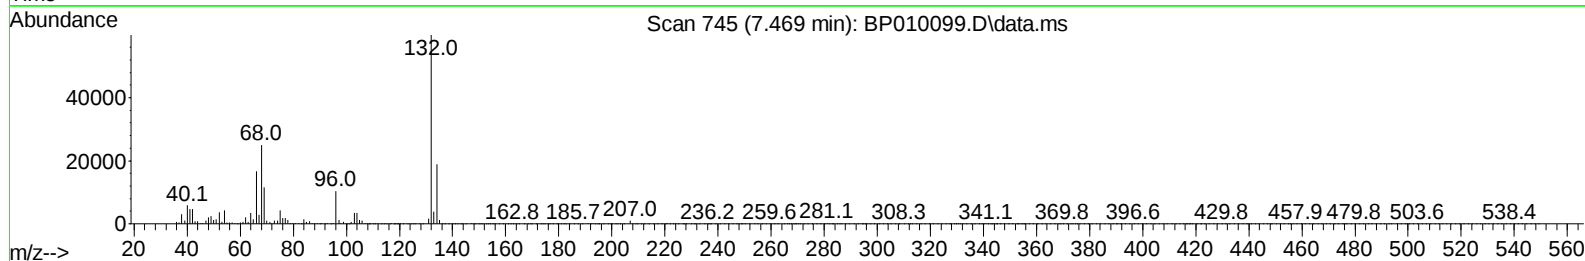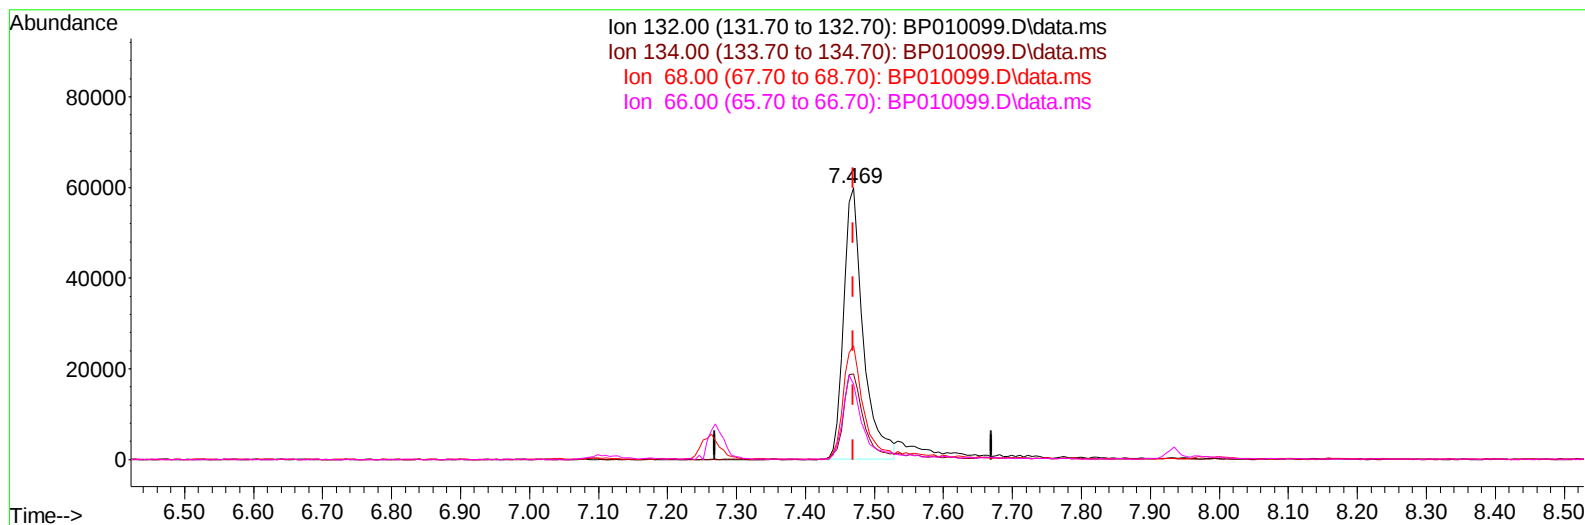

TIC: BP010099.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.469min (+ 0.000) 9.75 ng/u1

response 118102

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	31.52
68.00	51.40	41.84
66.00	26.30	27.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

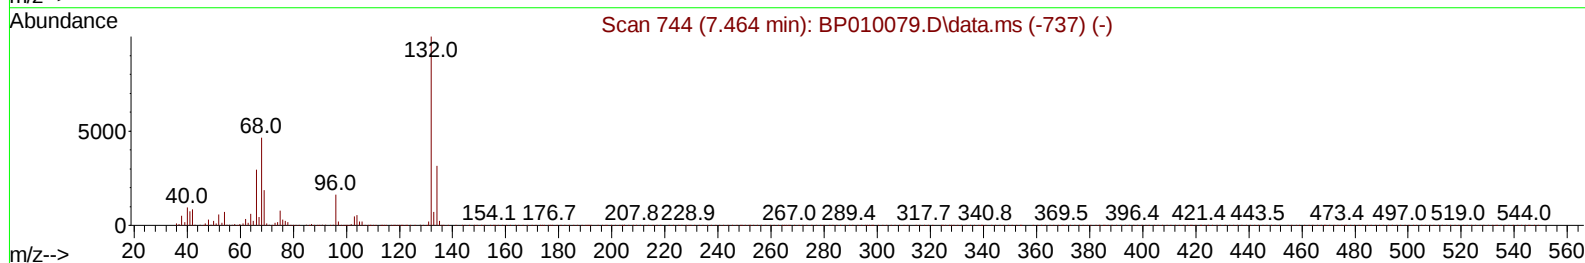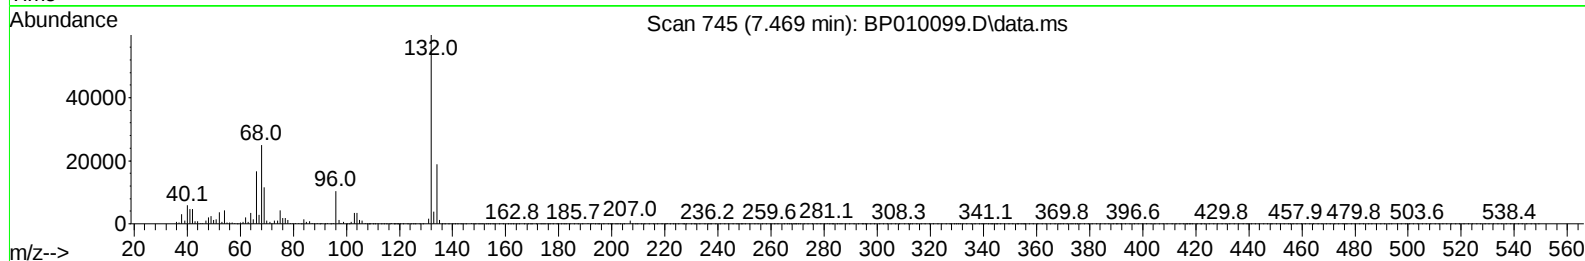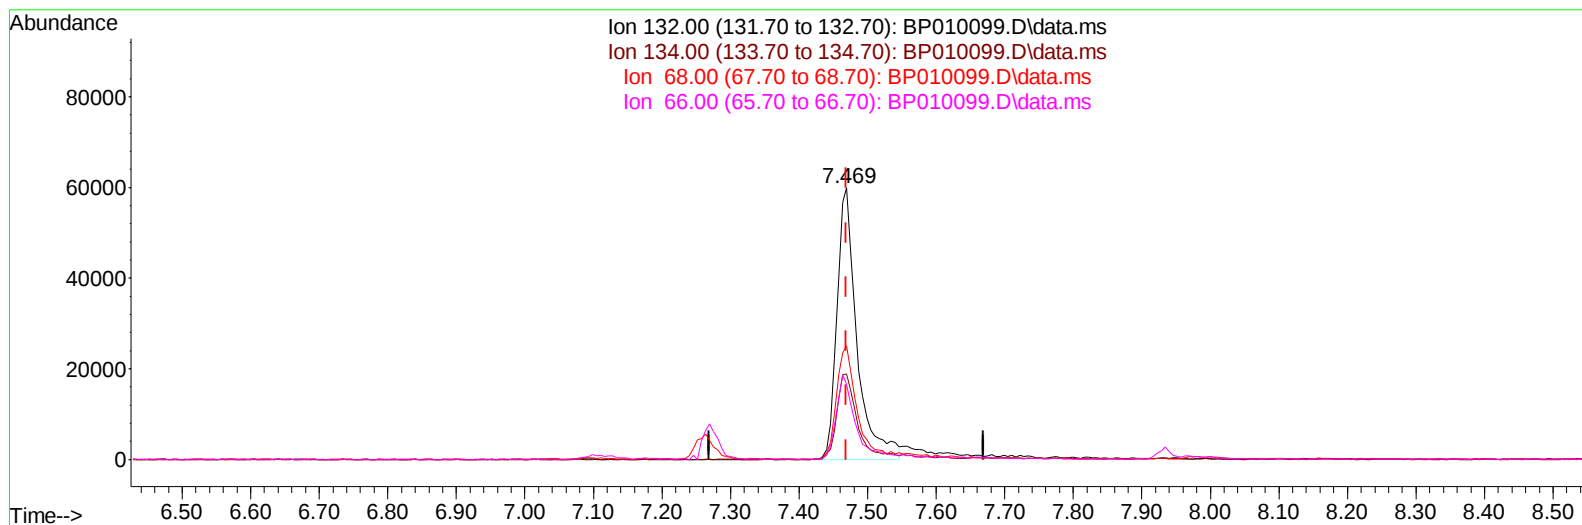

TIC: BP010099.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.469min (+ 0.000) 10.07 ng/ul m

response 121993

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	31.52
68.00	51.40	41.84
66.00	26.30	27.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

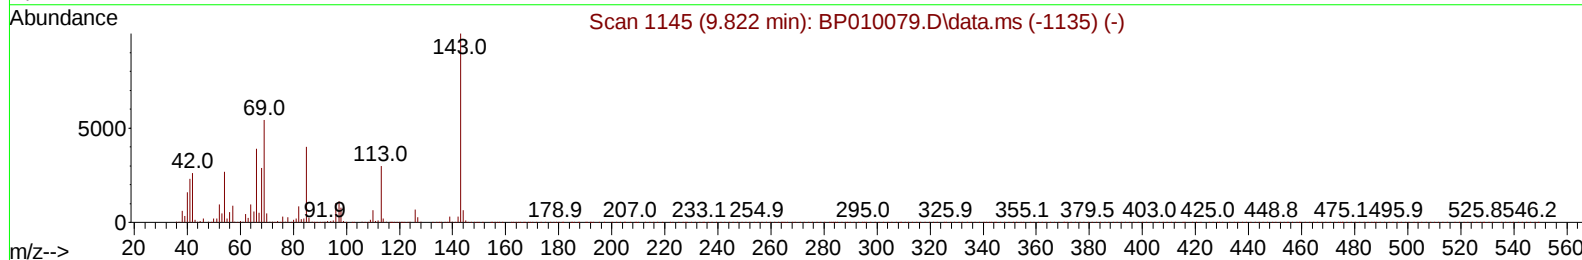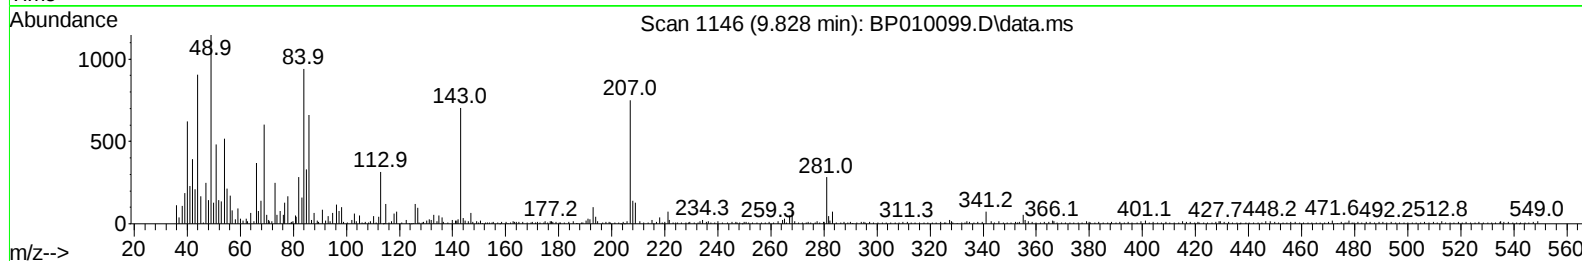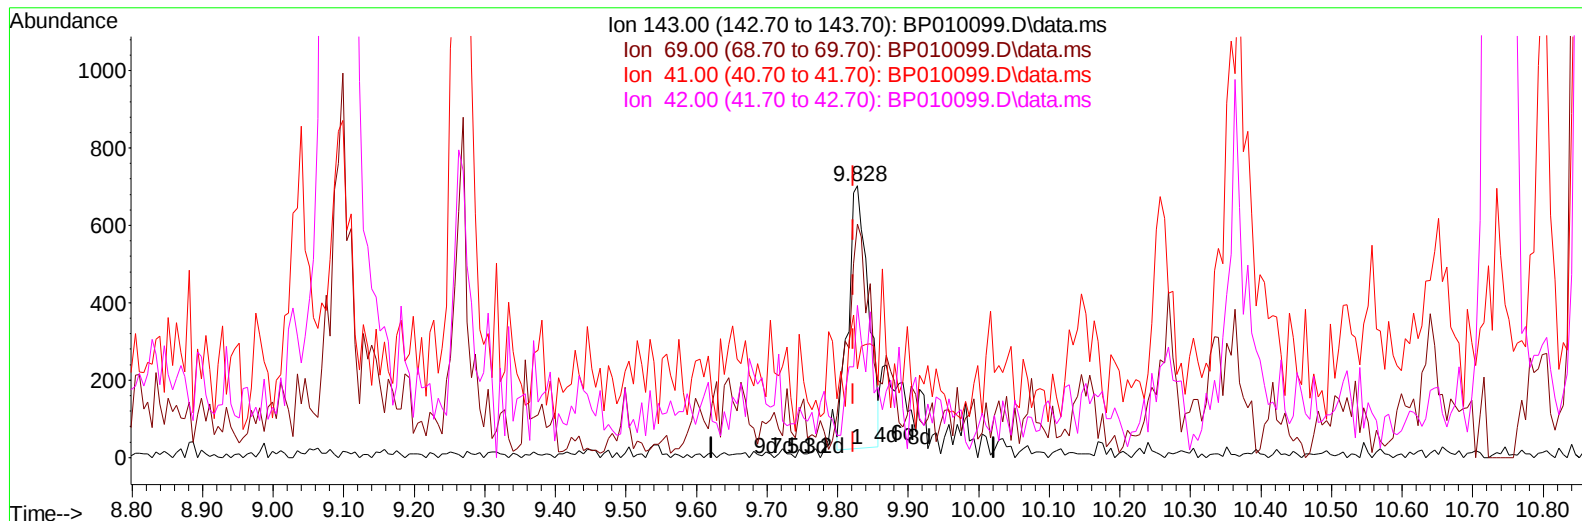

TIC: BP010099.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.828min (+ 0.006) 0.20 ng/u1

response 1364

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	47.10	86.04#
41.00	16.70	32.62#
42.00	20.70	56.13#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

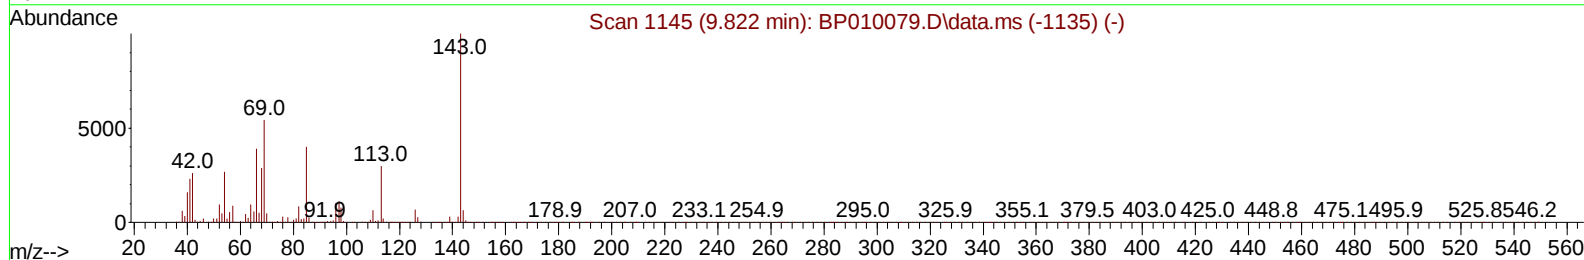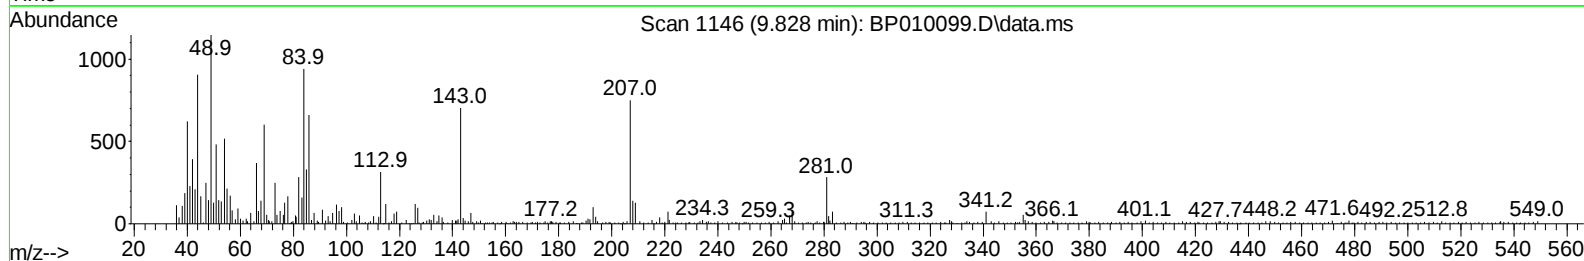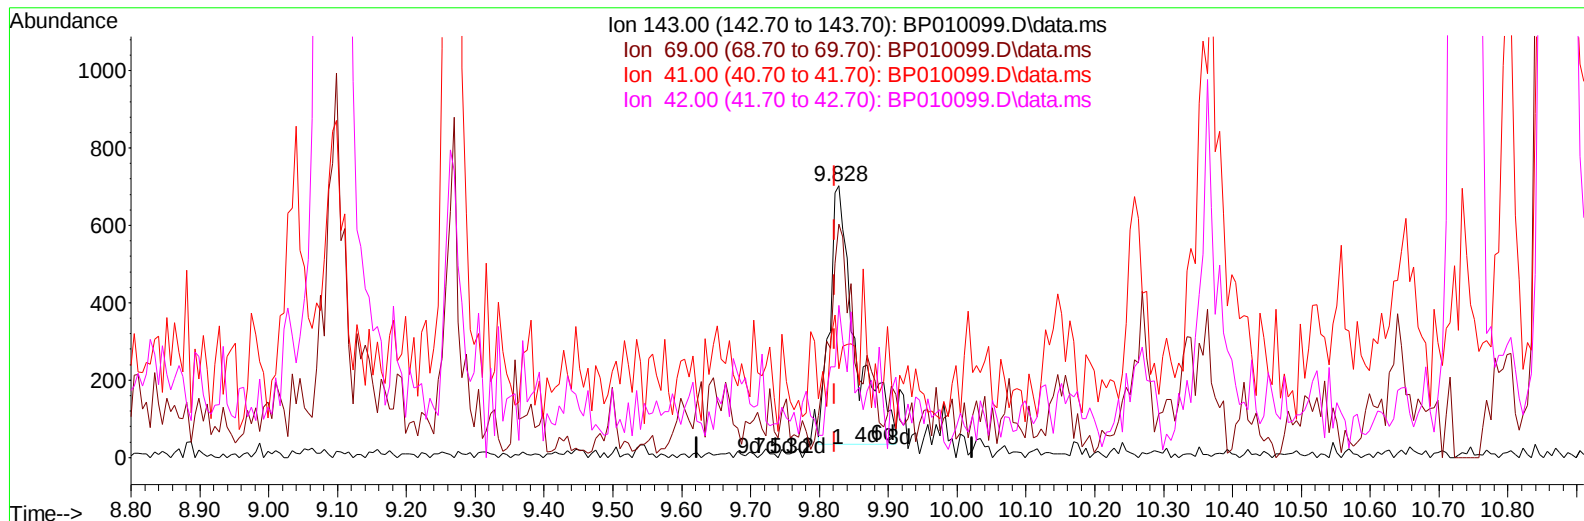

TIC: BP010099.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.828min (+ 0.006) 0.26 ng/ul m

response 1756

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	47.10	86.04#
41.00	16.70	32.62#
42.00	20.70	56.13#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010099.D
 Acq On : 26 Apr 2022 00:23
 Operator : CG/JU
 Sample : N2473-18RX
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ9RX

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/26/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 26 02:48:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	179848	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	778270	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	541009	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.316	188	1148382	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.398	240	925048	20.000	ng/ul	#-0.01
88) Perylene-d12	23.851	264	682544	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	21099m	5.116	ng/uL	0.00
4) Pyridine-d5	3.793	84	64226	5.536	ng/ul	0.00
7) Phenol-d5	7.099	99	36591m	2.237	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	277102	28.230	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.469	132	121993m	10.069	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	68948	5.087	ng/ul	0.00
21) Nitrobenzene-d5	9.093	128	170805	27.594	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	1756m	0.260	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	123573	9.390	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	397751	21.078	ng/ul	-0.01
46) Dimethylphthalate-d6	13.975	166	1164136	27.662	ng/ul	0.00
49) Acenaphthylene-d8	14.257	160	1407829	27.640	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	9	0.001	ng/ul	0.00
60) Fluorene-d10	15.557	176	1141189	31.523	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	8	0.001	ng/ul	0.00
73) Anthracene-d10	17.416	188	1879058	33.822	ng/ul	0.00
81) Pyrene-d10	19.645	212	2133856	40.562	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.692	264	1280866	35.796	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010099.D
Acq On : 26 Apr 2022 00:23
Operator : CG/JU
Sample : N2473-18RX
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ9RX

Manual IntegrationsAPPROVED

Quant Time: Apr 26 02:48:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/26/2022
Supervised By :Yogesh Patel 04/28/2022

