




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010106.D
 Acq On : 26 Apr 2022 09:36
 Operator : CG/JU
 Sample : PB144362BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK362

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/27/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 27 00:43:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

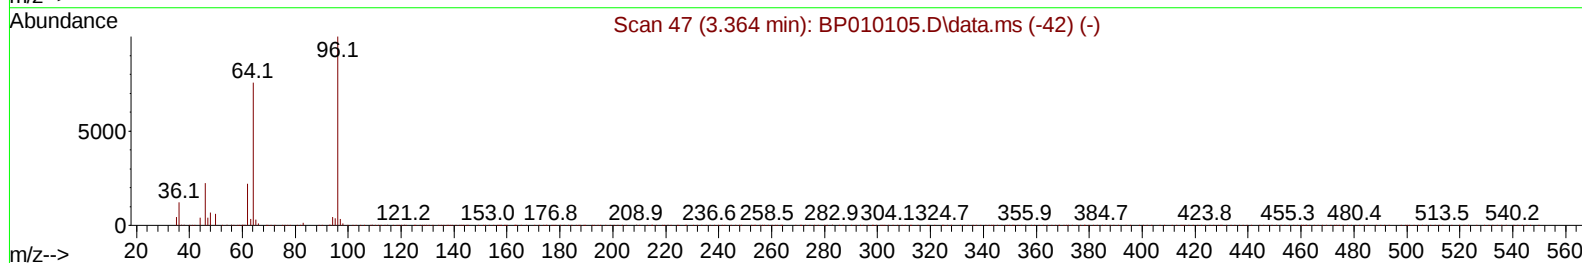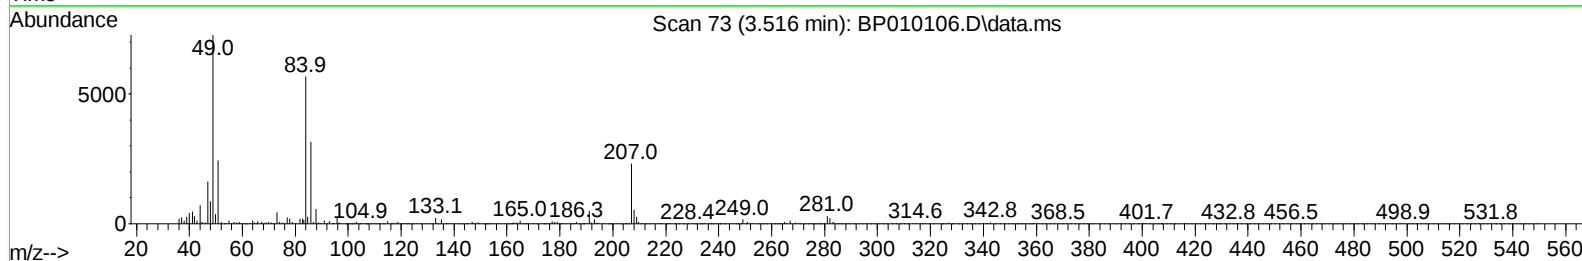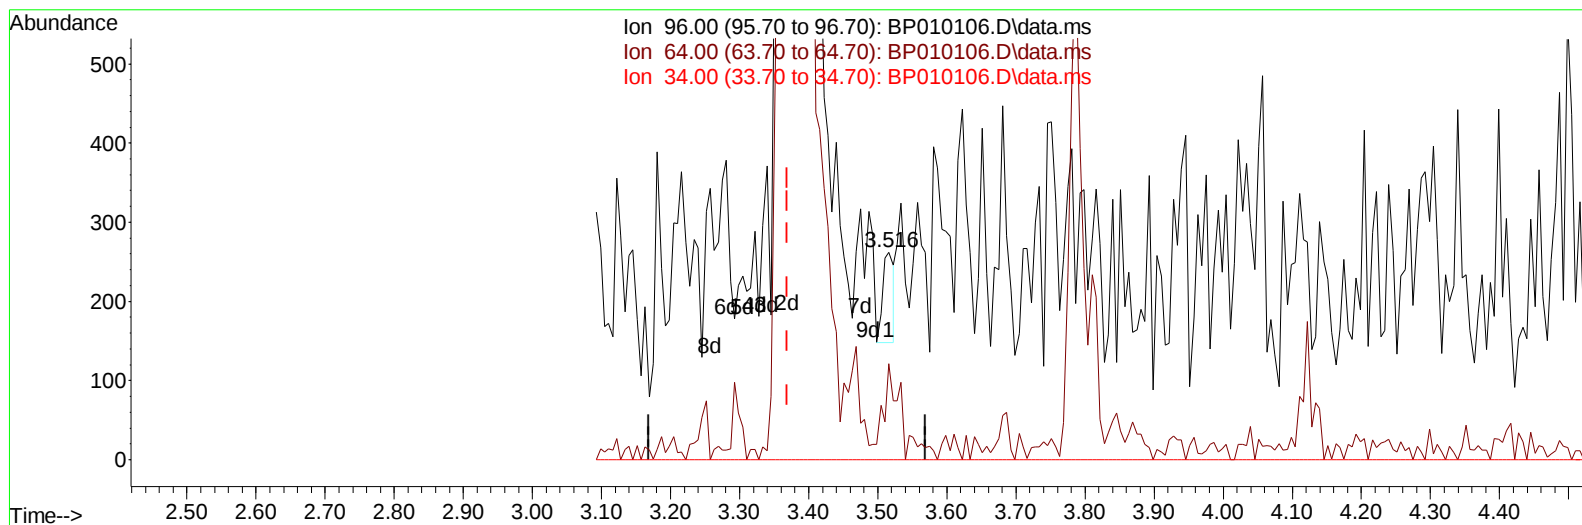

TIC: BP010106.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.516min (+ 0.147) 0.03 ng/uL

response 125

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	62.60
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010106.D
 Acq On : 26 Apr 2022 09:36
 Operator : CG/JU
 Sample : PB144362BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK362

Manual IntegrationsAPPROVED

Quant Time: Apr 27 00:43:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/27/2022
 Supervised By :Yogesh Patel 04/28/2022

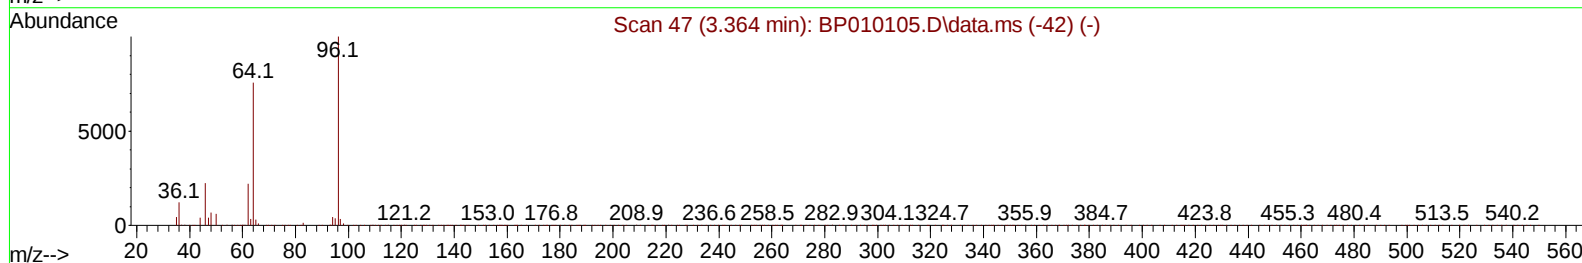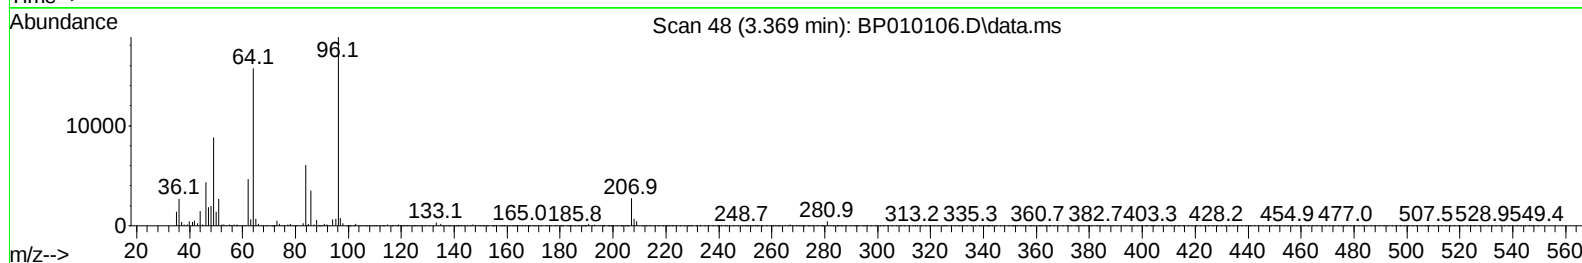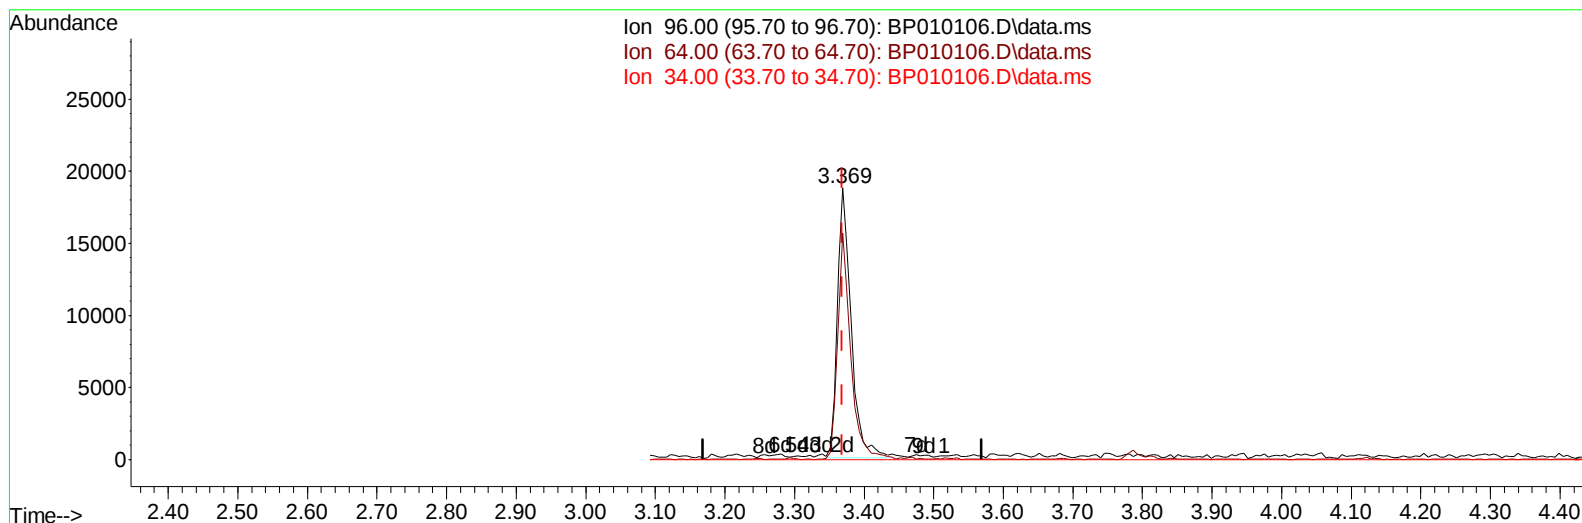

TIC: BP010106.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 6.31 ng/uL m

response 25674

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	83.35#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010106.D
 Acq On : 26 Apr 2022 09:36
 Operator : CG/JU
 Sample : PB144362BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK362

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/27/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 27 00:43:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	177481	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.745	136	748078	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.574	164	503630	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.327	188	1075390	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.409	240	893752	20.000	ng/ul	# 0.00
88) Perylene-d12	23.868	264	668472	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	25674m	6.308	ng/uL	0.00
4) Pyridine-d5	3.787	84	307558	26.861	ng/ul	0.00
7) Phenol-d5	7.098	99	421840	26.131	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	295952	30.552	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	350926	29.352	ng/ul	0.00
15) 4-Methylphenol-d8	8.645	113	362369	27.092	ng/ul	0.00
21) Nitrobenzene-d5	9.098	128	185476	31.173	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	203809	31.365	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	334747	26.462	ng/ul	0.00
31) 4-Chloroaniline-d4	10.880	131	500734	27.607	ng/ul	0.00
46) Dimethylphthalate-d6	13.980	166	1240481	31.664	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	1384819	29.207	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	155064	21.500	ng/ul	0.00
60) Fluorene-d10	15.568	176	1043157	30.954	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	162757	23.935	ng/ul	0.00
73) Anthracene-d10	17.427	188	1591141	30.583	ng/ul	0.00
81) Pyrene-d10	19.662	212	1807435	35.560	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.709	264	1146182	32.706	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010106.D
Acq On : 26 Apr 2022 09:36
Operator : CG/JU
Sample : PB144362BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 27 00:43:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

