

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010108.D
 Acq On : 26 Apr 2022 10:44
 Operator : CG/JU
 Sample : PB144303BS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS303

Quant Time: Apr 27 00:44:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 04/27/2022
 Supervised By :Yogesh Patel 04/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	163712	20.000	ng/u1	0.00
20) Naphthalene-d8	10.739	136	698871	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.569	164	470345	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.316	188	986771	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.404	240	885666	20.000	ng/u1	# 0.00
88) Perylene-d12	23.851	264	673922	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	22956	6.115	ng/uL	0.00
4) Pyridine-d5	3.781	84	301502	28.547	ng/u1	0.00
7) Phenol-d5	7.093	99	442328	29.704	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67	287412	32.166	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.463	132	362196	32.843	ng/u1	0.00
15) 4-Methylphenol-d8	8.645	113	372661	30.205	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	186077	33.476	ng/u1	0.00
24) 2-Nitrophenol-d4	9.816	143	204950	33.761	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	376551	31.863	ng/u1	0.00
31) 4-Chloroaniline-d4	10.869	131	492256	29.050	ng/u1	-0.01
46) Dimethylphthalate-d6	13.975	166	1201531	32.840	ng/u1	0.00
49) Acenaphthylene-d8	14.257	160	1383950	31.254	ng/u1	0.00
54) 4-Nitrophenol-d4	14.763	143	198528	29.474	ng/u1	0.00
60) Fluorene-d10	15.557	176	1014623	32.238	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	206611	33.113	ng/u1	0.00
73) Anthracene-d10	17.421	188	1533776	32.128	ng/u1	0.00
81) Pyrene-d10	19.651	212	1806086	35.858	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.698	264	1215140	34.393	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	46754m	11.984	ng/uL	
5) Pyridine	3.799	79	315257	28.716	ng/u1#	43
6) Benzaldehyde	7.069	77	283045	35.568	ng/u1	95
8) Phenol	7.122	94	463533	30.980	ng/u1#	94
10) Bis(2-Chloroethyl)ether	7.351	93	365606	31.716	ng/u1#	77
12) 2-Chlorophenol	7.498	128	357850	32.169	ng/u1	95
13) 2-Methylphenol	8.375	108	354396	30.884	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.463	45	537892	31.446	ng/u1#	85
16) Acetophenone	8.757	105	581616	30.215	ng/u1#	82
17) N-Nitroso-di-n-propyla...	8.745	70	312181	30.954	ng/u1#	75
18) 4-Methylphenol	8.704	108	378634	29.968	ng/u1	91
19) Hexachloroethane	9.022	117	153170	32.769	ng/u1	85
22) Nitrobenzene	9.134	77	446380	32.777	ng/u1#	85
23) Isophorone	9.663	82	866888	32.228	ng/u1#	97
25) 2-Nitrophenol	9.851	139	216000	33.596	ng/u1#	80
26) 2,4-Dimethylphenol	9.910	107	414590	29.784	ng/u1#	80
27) Bis(2-Chloroethoxy)met...	10.145	93	512721	32.521	ng/u1#	97
29) 2,4-Dichlorophenol	10.387	162	372427	32.783	ng/u1#	83
30) Naphthalene	10.787	128	1186296	32.432	ng/u1	97
32) 4-Chloroaniline	10.898	127	488003	29.225	ng/u1	98
33) Hexachlorobutadiene	11.081	225	263798	32.765	ng/u1	94
34) Caprolactam	11.669	113	126037m	30.843	ng/u1	
35) 4-Chloro-3-methylphenol	12.022	107	425836	31.030	ng/u1#	68
36) 2-Methylnaphthalene	12.392	142	841036	31.703	ng/u1	92

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010108.D
 Acq On : 26 Apr 2022 10:44
 Operator : CG/JU
 Sample : PB144303BS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS303


Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/27/2022
 Supervised By :Yogesh Patel 04/28/2022

Quant Time: Apr 27 00:44:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.616	142	851662	31.618	ng/ul#	94
39) 1,2,4,5-Tetrachloroben...	12.769	216	485360	33.401	ng/ul	94
40) Hexachlorocyclopentadiene	12.751	237	268604	32.800	ng/ul	98
41) 2,4,6-Trichlorophenol	13.004	196	313088	33.300	ng/ul#	82
42) 2,4,5-Trichlorophenol	13.075	196	337179	32.961	ng/ul#	85
43) 1,1'-Biphenyl	13.404	154	1157608	33.370	ng/ul	94
44) 2-Chloronaphthalene	13.445	162	889415	33.130	ng/ul	93
45) 2-Nitroaniline	13.639	65	288410	33.131	ng/ul#	79
47) Dimethylphthalate	14.022	163	1156509	32.524	ng/ul#	92
48) 2,6-Dinitrotoluene	14.139	165	245224	33.605	ng/ul	91
50) Acenaphthylene	14.286	152	1441211	32.858	ng/ul	95
51) 3-Nitroaniline	14.469	138	222886	33.717	ng/ul#	79
52) Acenaphthene	14.628	153	923834	32.392	ng/ul	96
53) 2,4-Dinitrophenol	14.675	184	124204	30.459	ng/ul#	82
55) 4-Nitrophenol	14.775	109	166259	28.411	ng/ul#	48
56) Dibenzofuran	14.963	168	1360901	32.224	ng/ul	99
57) 2,4-Dinitrotoluene	14.928	165	353264	33.138	ng/ul#	87
58) 2,3,4,6-Tetrachlorophenol	15.192	232	297554	32.722	ng/ul#	86
59) Diethylphthalate	15.386	149	1185252	32.771	ng/ul	94
61) Fluorene	15.616	166	1113210	32.104	ng/ul	92
62) 4-Chlorophenyl-phenyle...	15.610	204	584219	32.014	ng/ul	98
63) 4-Nitroaniline	15.627	138	231962m	36.062	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.692	198	200506	33.307	ng/ul#	90
67) N-Nitrosodiphenylamine	15.822	169	951635	33.611	ng/ul	94
68) 4-Bromophenyl-phenylether	16.504	248	361030	34.301	ng/ul	95
69) Hexachlorobenzene	16.627	284	411935	33.718	ng/ul#	91
70) Atrazine	16.774	200	377774	32.819	ng/ul#	89
71) Pentachlorophenol	16.969	266	244327	31.403	ng/ul#	85
72) Phenanthrene	17.363	178	1763015	32.871	ng/ul	98
74) Anthracene	17.451	178	1752659	32.444	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.369	216	511915	35.535	ng/uL#	85
76) Pentachlorobenzene	14.892	250	479958	33.975	ng/uL	89
77) Carbazole	17.721	167	1528275	31.970	ng/ul#	95
78) Di-n-butylphthalate	18.274	149	2004264	34.079	ng/ul#	93
80) Fluoranthene	19.327	202	2092287	36.828	ng/ul	96
82) Pyrene	19.680	202	2098880	35.859	ng/ul#	94
83) Butylbenzylphthalate	20.545	149	900666	37.226	ng/ul#	80
84) 3,3'-Dichlorobenzidine	21.315	252	584776	36.695	ng/ul#	93
85) Benzo(a)anthracene	21.386	228	1871985	33.305	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.310	149	1310373	36.543	ng/ul#	82
87) Chrysene	21.439	228	1828738	33.043	ng/ul	99
89) Di-n-octyl phthalate	22.251	149	2132892	40.711	ng/ul	100
90) Benzo(b)fluoranthene	23.104	252	1656860	36.570	ng/ul	100
91) Benzo(k)fluoranthene	23.156	252	1506725	35.109	ng/ul#	97
93) Benzo(a)pyrene	23.745	252	1447520	34.550	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.415	276	1372783	32.938	ng/ul#	95
95) Dibenzo(a,h)anthracene	26.433	278	1184059	33.202	ng/ul#	94
96) Benzo(g,h,i)perylene	27.203	276	1179054	33.527	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 11.984 ng/uL m
RT: 3.405 min Scan# 54
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion: 88 Resp: 46754
Ion Ratio Lower Upper
88 100
43 32.2 6.8 10.2
58 76.7 28.4 42.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#5
Pyridine
Concen: 28.716 ng/uL
RT: 3.799 min Scan# 121
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion: 79 Resp: 315257
Ion Ratio Lower Upper
79 100
52 89.9 35.5 53.3#
51 42.6 20.2 30.4#

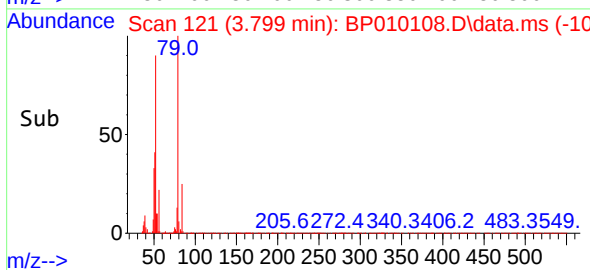



#6
Benzaldehyde
Concen: 35.568 ng/ul
RT: 7.069 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion: 77 Resp: 283045
Ion Ratio Lower Upper
77 100
105 94.6 77.0 115.4
106 88.1 77.0 115.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#8
Phenol
Concen: 30.980 ng/ul
RT: 7.122 min Scan# 686
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion: 94 Resp: 463533
Ion Ratio Lower Upper
94 100
65 31.8 19.0 28.6
66 43.9 34.6 51.8





#10
Bis(2-Chloroethyl)ether
Concen: 31.716 ng/ul
RT: 7.351 min Scan# 71
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion: 93 Resp: 365600
Ion Ratio Lower Upper
93 100
63 82.2 45.0 67.4
95 31.6 26.3 39.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#12
2-Chlorophenol
Concen: 32.169 ng/ul
RT: 7.498 min Scan# 750
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:128 Resp: 357850
Ion Ratio Lower Upper
128 100
64 52.9 45.3 67.9
130 33.1 29.0 43.6





#13
2-Methylphenol
Concen: 30.884 ng/ul
RT: 8.375 min Scan# 899
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:108 Resp: 354390
Ion Ratio Lower Upper
108 100
107 90.2 70.8 106.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#14
2,2'-oxybis(1-Chloropropane)
Concen: 31.446 ng/ul
RT: 8.463 min Scan# 914
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44



Tgt Ion: 45 Resp: 537892
Ion Ratio Lower Upper
45 100
77 13.7 17.1 25.7#
79 10.5 13.2 19.8#









#16
Acetophenone
Concen: 30.215 ng/ul
RT: 8.757 min Scan# 964
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Instrument :
BNA_P
ClientSampleId :
SLCS303

Tgt Ion:105 Resp: 581610
Ion Ratio Lower Upper
105 100
77 79.1 53.4 80.2
51 29.3 13.8 20.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

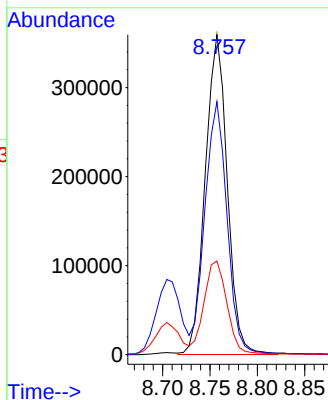

#17
N-Nitroso-di-n-propylamine
Concen: 30.954 ng/ul
RT: 8.745 min Scan# 962
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion: 70 Resp: 312181
Ion Ratio Lower Upper
70 100
42 61.3 31.8 47.8#
101 10.3 15.6 23.4#
130 21.0 13.7 20.5#

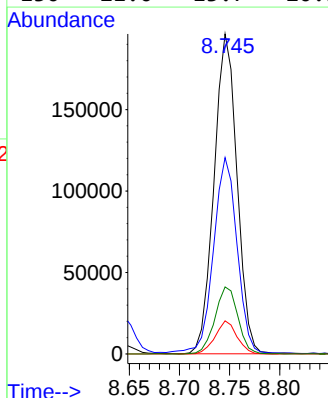



#18
4-Methylphenol
Concen: 29.968 ng/ul
RT: 8.704 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:108 Resp: 378634
Ion Ratio Lower Upper
108 100
107 113.5 83.6 125.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#19
Hexachloroethane
Concen: 32.769 ng/ul
RT: 9.022 min Scan# 1009
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:117 Resp: 153170
Ion Ratio Lower Upper
117 100
201 108.9 106.5 159.7
199 68.5 59.0 88.6





#22
Nitrobenzene
Concen: 32.777 ng/ul
RT: 9.134 min Scan# 1028
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion: 77 Resp: 446380
Ion Ratio Lower Upper
77 100
123 43.0 42.3 63.5
65 15.3 5.8 8.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#23
Isophorone
Concen: 32.228 ng/ul
RT: 9.663 min Scan# 1118
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44



Tgt Ion: 82 Resp: 866888
Ion Ratio Lower Upper
82 100
95 7.4 7.8 11.8#
138 16.7 12.9 19.3









#25
2-Nitrophenol
Concen: 33.596 ng/ul
RT: 9.851 min Scan# 1150
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Instrument :
BNA_P
ClientSampleId :
SLCS303

Tgt Ion:139 Resp: 216000
Ion Ratio Lower Upper
139 100
65 54.6 49.4 74.2
109 32.6 44.7 67.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

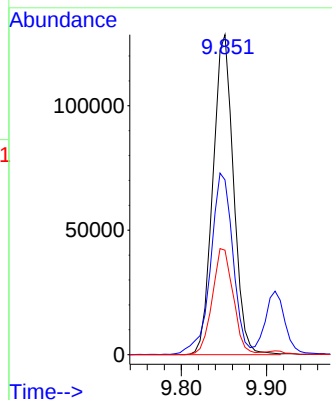

#26
2,4-Dimethylphenol
Concen: 29.784 ng/ul
RT: 9.910 min Scan# 1160
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:107 Resp: 414590
Ion Ratio Lower Upper
107 100
121 47.6 34.1 51.1
122 79.4 46.3 69.5

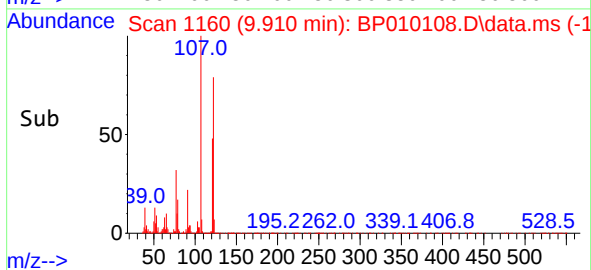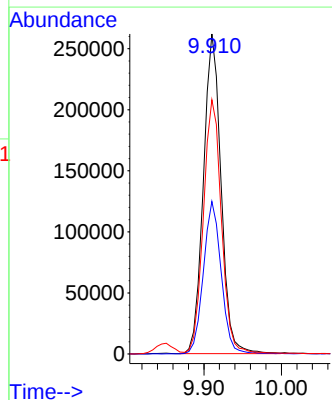



#27
Bis(2-Chloroethoxy)methane
Concen: 32.521 ng/ul
RT: 10.145 min Scan# 1200
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion: 93 Resp: 51272
Ion Ratio Lower Upper
93 100
95 32.1 26.2 39.4
123 11.0 6.2 9.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

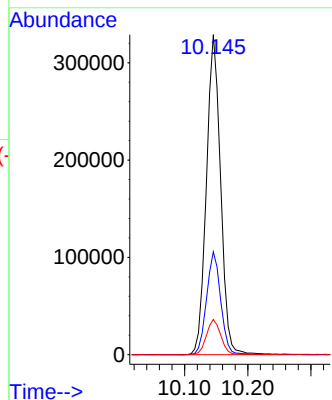


#29
2,4-Dichlorophenol
Concen: 32.783 ng/ul
RT: 10.387 min Scan# 1241
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:162 Resp: 372427
Ion Ratio Lower Upper
162 100
164 66.5 37.0 55.6#
98 37.9 31.0 46.6

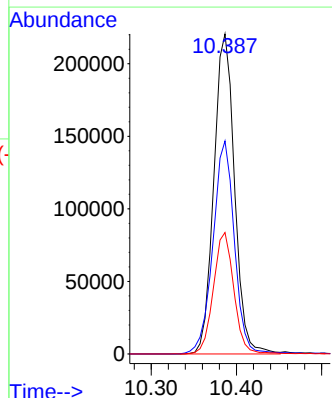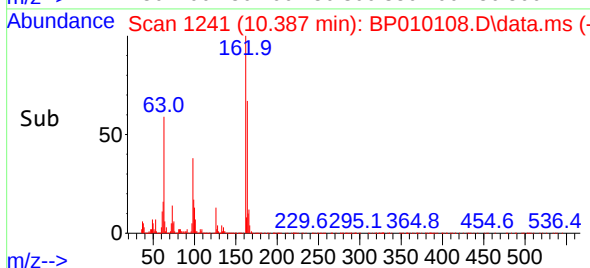



#30
Naphthalene
Concen: 32.432 ng/ul
RT: 10.787 min Scan# 1309
Delta R.T. -0.012 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion:128 Resp: 1186290
Ion Ratio Lower Upper
128 100
129 10.8 8.6 13.0
127 13.0 12.2 18.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#32
4-Chloroaniline
Concen: 29.225 ng/ul
RT: 10.898 min Scan# 1328
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:127 Resp: 488003
Ion Ratio Lower Upper
127 100
129 31.7 24.6 37.0

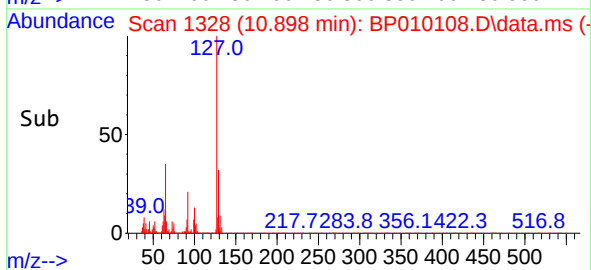



#33
Hexachlorobutadiene
Concen: 32.765 ng/ul
RT: 11.081 min Scan# 1359
Delta R.T. -0.012 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303

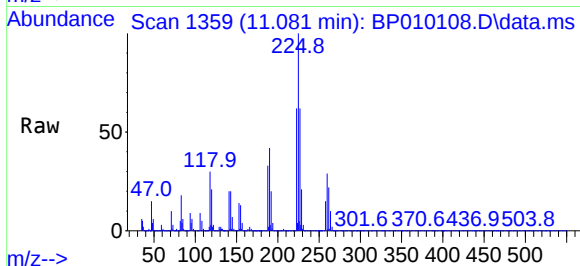


Tgt Ion:225 Resp: 263798
Ion Ratio Lower Upper
225 100
223 61.6 53.4 80.0
227 62.1 53.8 80.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#34
Caprolactam
Concen: 30.843 ng/ul m
RT: 11.669 min Scan# 1459
Delta R.T. 0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

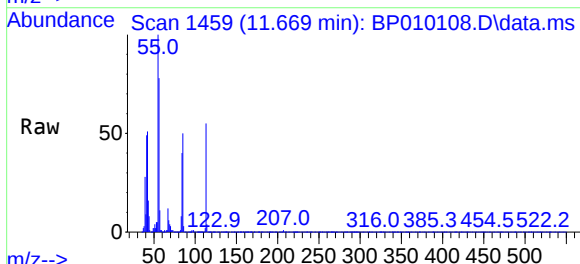

Tgt Ion:113 Resp: 126037
Ion Ratio Lower Upper
113 100
55 181.4 58.2 87.2#
56 142.1 68.6 103.0#









#35
4-Chloro-3-methylphenol
Concen: 31.030 ng/ul
RT: 12.022 min Scan# 1518
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Instrument :
BNA_P
ClientSampleId :
SLCS303

Tgt Ion:107 Resp: 425830
Ion Ratio Lower Upper
107 100
144 24.3 15.8 23.8
142 76.3 38.9 58.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

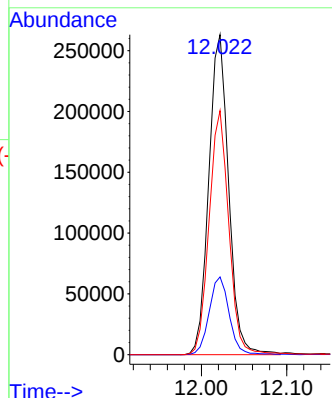

#36
2-Methylnaphthalene
Concen: 31.703 ng/ul
RT: 12.392 min Scan# 1582
Delta R.T. -0.012 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:142 Resp: 841036
Ion Ratio Lower Upper
142 100
141 87.2 64.3 96.5

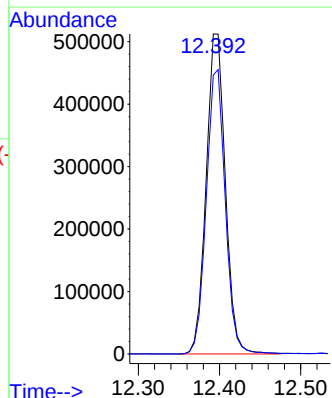



#37
1-Methylnaphthalene
Concen: 31.618 ng/ul
RT: 12.616 min Scan# 1620
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:142 Resp: 851662
Ion Ratio Lower Upper
142 100
141 92.4 69.8 104.8
116 4.0 5.6 8.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

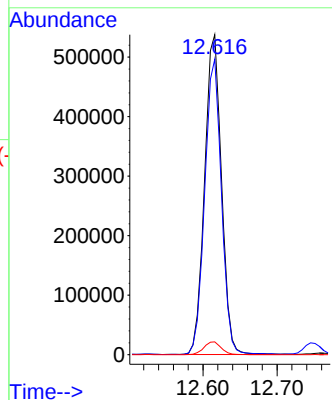


#39
1,2,4,5-Tetrachlorobenzene
Concen: 33.401 ng/ul
RT: 12.769 min Scan# 1646
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:216 Resp: 485360
Ion Ratio Lower Upper
216 100
214 77.8 58.2 87.2
179 20.6 14.2 21.2
108 15.7 15.3 22.9

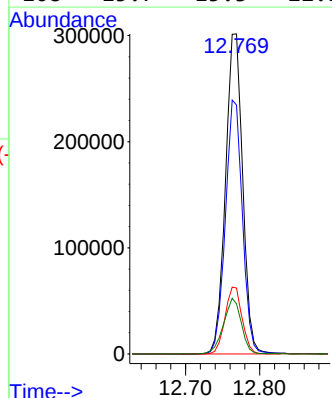



#40
Hexachlorocyclopentadiene
Concen: 32.800 ng/ul
RT: 12.751 min Scan# 1643
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:237 Resp: 268604
Ion Ratio Lower Upper
237 100
235 64.4 53.2 79.8
272 12.9 10.8 16.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#41
2,4,6-Trichlorophenol
Concen: 33.300 ng/ul
RT: 13.004 min Scan# 1686
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:196 Resp: 313088
Ion Ratio Lower Upper
196 100
198 97.7 64.1 96.1#
200 30.0 19.9 29.9#





#42
2,4,5-Trichlorophenol
Concen: 32.961 ng/ul
RT: 13.075 min Scan# 1698
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:196 Resp: 337179
Ion Ratio Lower Upper
196 100
198 98.7 68.6 103.0
200 31.2 32.8 49.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

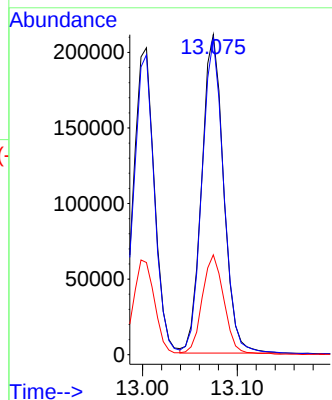


#43
1,1'-Biphenyl
Concen: 33.370 ng/ul
RT: 13.404 min Scan# 1754
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44



Tgt Ion:154 Resp: 1157608
Ion Ratio Lower Upper
154 100
153 40.0 28.6 43.0
76 12.0 8.5 12.7

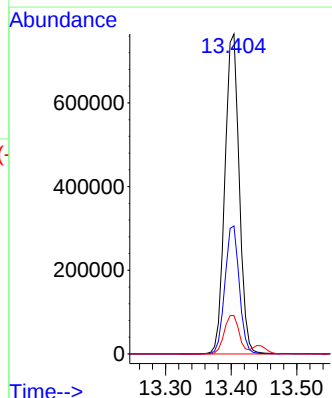







#44
2-Chloronaphthalene
Concen: 33.130 ng/ul
RT: 13.445 min Scan# 1760
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Instrument :
BNA_P
ClientSampleId :
SLCS303

Tgt Ion:162 Resp: 889415
Ion Ratio Lower Upper
162 100
164 32.3 27.5 41.3
127 39.6 37.1 55.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

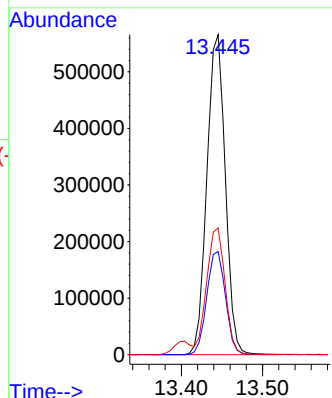

#45
2-Nitroaniline
Concen: 33.131 ng/ul
RT: 13.639 min Scan# 1794
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion: 65 Resp: 288410
Ion Ratio Lower Upper
65 100
92 65.0 77.9 116.9
138 91.6 81.5 122.3

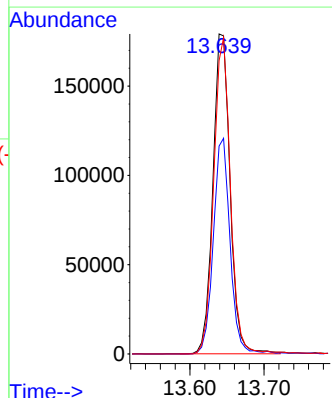



#47
Dimethylphthalate
Concen: 32.524 ng/ul
RT: 14.022 min Scan# 1859
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:163 Resp: 1156509
Ion Ratio Lower Upper
163 100
194 4.5 4.1 6.1
164 10.0 11.3 16.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

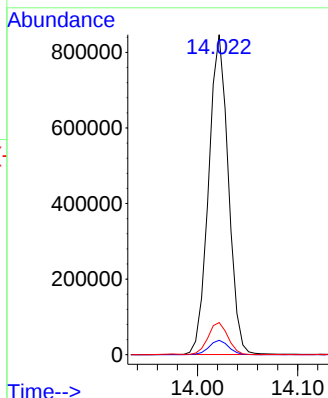


#48
2,6-Dinitrotoluene
Concen: 33.605 ng/ul
RT: 14.139 min Scan# 1879
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44



Tgt Ion:165 Resp: 245224
Ion Ratio Lower Upper
165 100
89 56.7 51.7 77.5
121 20.7 18.3 27.5

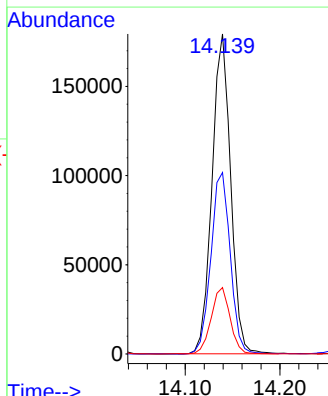







#50
Acenaphthylene
Concen: 32.858 ng/ul
RT: 14.286 min Scan# 1904
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Instrument :
BNA_P
ClientSampleId :
SLCS303

Tgt Ion:152 Resp: 144121
Ion Ratio Lower Upper
152 100
151 19.8 18.3 27.5
153 13.3 11.0 16.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

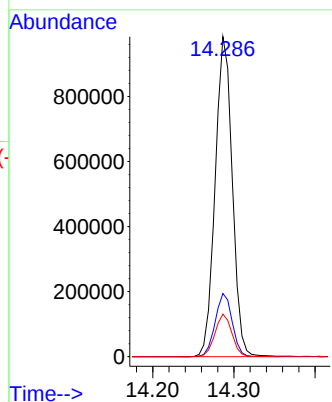

#51
3-Nitroaniline
Concen: 33.717 ng/ul
RT: 14.469 min Scan# 1935
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:138 Resp: 222886
Ion Ratio Lower Upper
138 100
108 11.5 15.8 23.8#
92 120.2 117.1 175.7

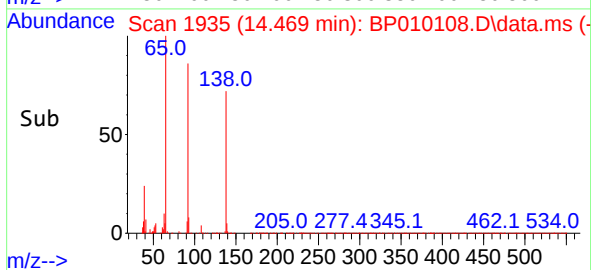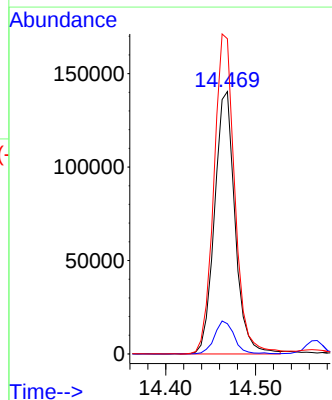



#52
Acenaphthene
Concen: 32.392 ng/ul
RT: 14.628 min Scan# 1962
Delta R.T. -0.012 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:153 Resp: 923834
Ion Ratio Lower Upper
153 100
152 46.3 34.3 51.5
154 90.5 70.0 105.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#53
2,4-Dinitrophenol
Concen: 30.459 ng/ul
RT: 14.675 min Scan# 1970
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:184 Resp: 124204
Ion Ratio Lower Upper
184 100
63 67.9 34.6 52.0#
154 66.7 57.7 86.5

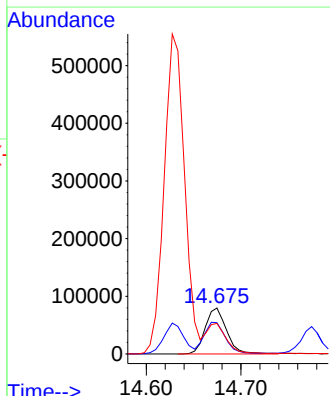



#55
4-Nitrophenol
Concen: 28.411 ng/ul
RT: 14.775 min Scan# 1986
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion:109 Resp: 166259
Ion Ratio Lower Upper
109 100
139 117.9 61.4 92.2
65 132.4 65.3 97.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#56
Dibenzofuran
Concen: 32.224 ng/ul
RT: 14.963 min Scan# 2019
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:168 Resp: 1360901
Ion Ratio Lower Upper
168 100
139 38.1 30.1 45.1





#57
2,4-Dinitrotoluene
Concen: 33.138 ng/ul
RT: 14.928 min Scan# 2012
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303

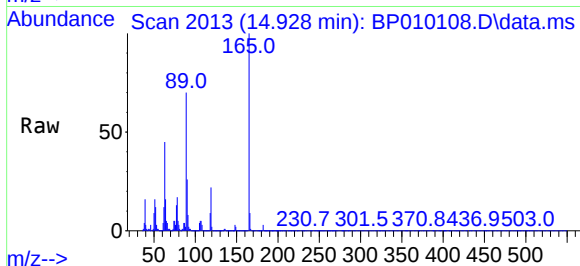


Tgt Ion:165 Resp: 353264
Ion Ratio Lower Upper
165 100
63 45.2 29.5 44.3#
182 3.1 2.8 4.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#58
2,3,4,6-Tetrachlorophenol
Concen: 32.722 ng/ul
RT: 15.192 min Scan# 2058
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

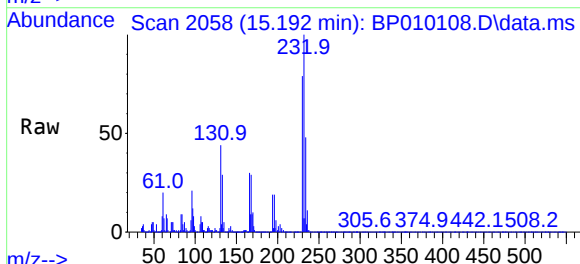


Tgt Ion:232 Resp: 297554
Ion Ratio Lower Upper
232 100
131 43.8 25.4 38.2#
130 2.2 4.2 6.2#
166 30.1 28.1 42.1

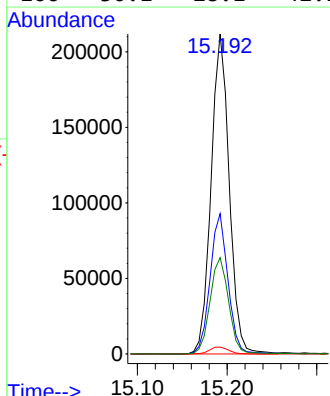



#59
Diethylphthalate
Concen: 32.771 ng/ul
RT: 15.386 min Scan# 2091
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:149 Resp: 118525
Ion Ratio Lower Upper
149 100
177 22.8 22.0 33.0
150 12.8 10.2 15.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#61
Fluorene
Concen: 32.104 ng/ul
RT: 15.616 min Scan# 2130
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:166 Resp: 1113210
Ion Ratio Lower Upper
166 100
165 95.6 70.3 105.5
167 13.3 9.5 14.3





#62
4-Chlorophenyl-phenylether
Concen: 32.014 ng/ul
RT: 15.610 min Scan# 2129
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:204 Resp: 584219
Ion Ratio Lower Upper
204 100
206 33.6 27.6 41.4
141 59.4 46.6 69.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

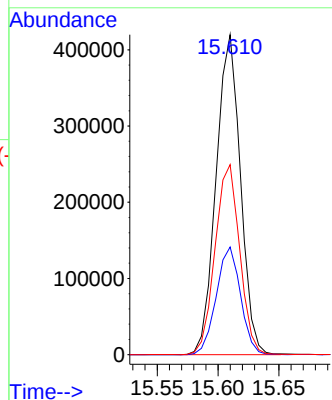


#63
4-Nitroaniline
Concen: 36.062 ng/ul m
RT: 15.627 min Scan# 2132
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:138 Resp: 231962
Ion Ratio Lower Upper
138 100
92 53.3 41.6 62.4
108 83.7 97.6 146.4#

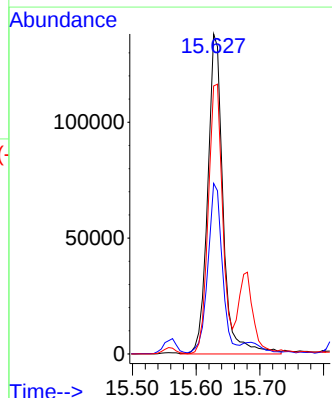



#66
4,6-Dinitro-2-methylphenol
Concen: 33.307 ng/ul
RT: 15.692 min Scan# 2143
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303

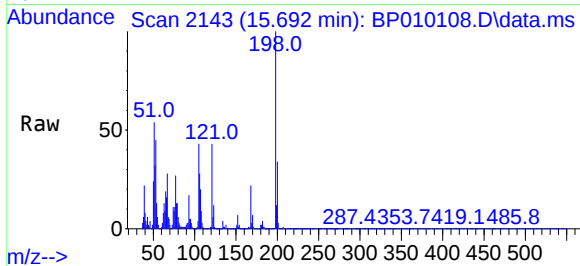


Tgt Ion:198 Resp: 200500
Ion Ratio Lower Upper
198 100
182 4.4 6.0 9.0
77 26.8 17.7 26.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#67
N-Nitrosodiphenylamine
Concen: 33.611 ng/ul
RT: 15.822 min Scan# 2165
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

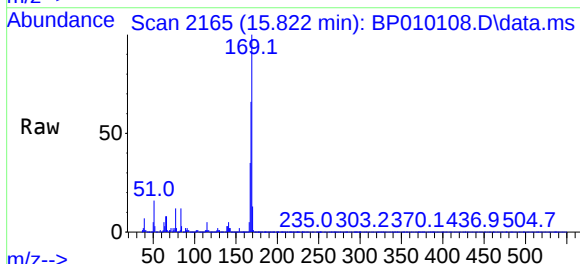


Tgt Ion:169 Resp: 951635
Ion Ratio Lower Upper
169 100
168 66.4 48.3 72.5
167 35.0 29.6 44.4





#68
4-Bromophenyl-phenylether
Concen: 34.301 ng/ul
RT: 16.504 min Scan# 2281
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:248 Resp: 361030
Ion Ratio Lower Upper
248 100
250 100.3 79.4 119.0
141 76.3 67.2 100.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

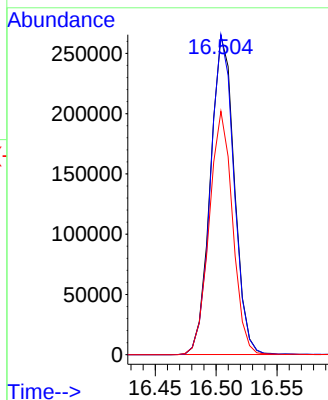


#69
Hexachlorobenzene
Concen: 33.718 ng/ul
RT: 16.627 min Scan# 2302
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:284 Resp: 411935
Ion Ratio Lower Upper
284 100
142 31.6 19.2 28.8#
249 31.5 27.4 41.2

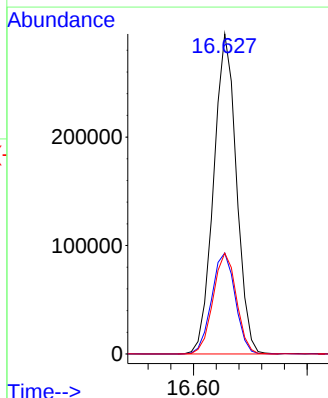



#70
Atrazine
Concen: 32.819 ng/ul
RT: 16.774 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:200 Resp: 377774
Ion Ratio Lower Upper
200 100
173 26.4 19.2 28.8
215 49.2 32.2 48.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#71
Pentachlorophenol
Concen: 31.403 ng/ul
RT: 16.969 min Scan# 2360
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:266 Resp: 244327
Ion Ratio Lower Upper
266 100
264 64.5 57.3 85.9
268 63.5 65.7 98.5

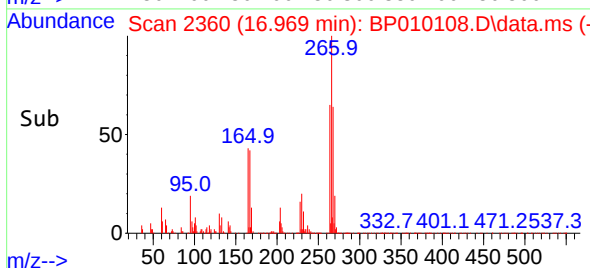



#72
Phenanthrene
Concen: 32.871 ng/u1
RT: 17.363 min Scan# 2427
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion:178 Resp: 1763015
Ion Ratio Lower Upper
178 100
179 15.2 11.7 17.5
176 18.8 14.5 21.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#74
Anthracene
Concen: 32.444 ng/u1
RT: 17.451 min Scan# 2442
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:178 Resp: 1752659
Ion Ratio Lower Upper
178 100
179 15.7 12.3 18.5
176 18.1 13.4 20.2

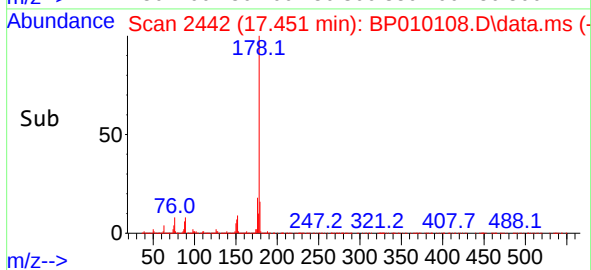



#75
1,2,3,4-Tetrachlorobenzene
Concen: 35.535 ng/uL
RT: 13.369 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:216 Resp: 511915
Ion Ratio Lower Upper
216 100
214 78.3 50.4 75.6
218 49.4 35.2 52.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

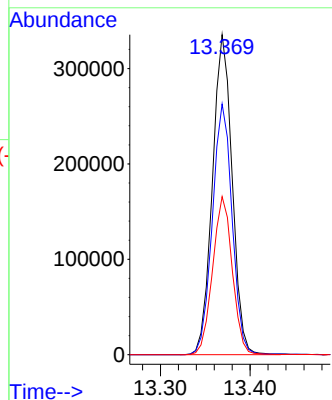


#76
Pentachlorobenzene
Concen: 33.975 ng/uL
RT: 14.892 min Scan# 2007
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:250 Resp: 479958
Ion Ratio Lower Upper
250 100
248 63.9 43.5 65.3
252 64.2 46.5 69.7

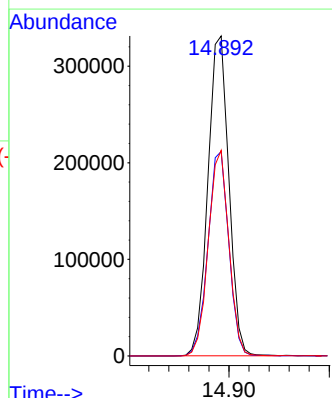



#77
Carbazole
Concen: 31.970 ng/ul
RT: 17.721 min Scan# 2488
Delta R.T. -0.001 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303

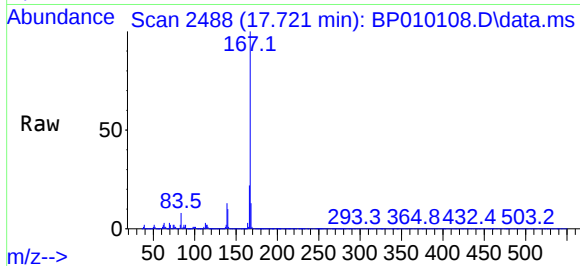


Tgt Ion:167 Resp: 152827
Ion Ratio Lower Upper
167 100
166 21.6 15.8 23.8
139 13.1 8.3 12.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#78
Di-n-butylphthalate
Concen: 34.079 ng/ul
RT: 18.274 min Scan# 2582
Delta R.T. -0.001 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

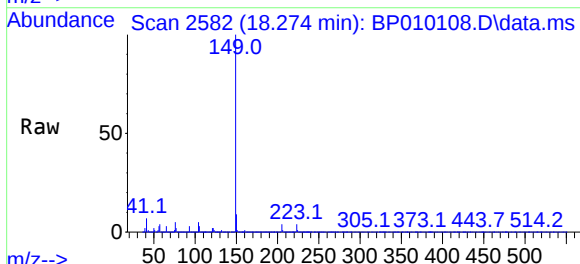


Tgt Ion:149 Resp: 2004264
Ion Ratio Lower Upper
149 100
150 9.2 9.6 14.4#
104 5.4 6.2 9.4#





#80
Fluoranthene
Concen: 36.828 ng/u1
RT: 19.327 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:202 Resp: 209228
Ion Ratio Lower Upper
202 100
101 9.6 9.6 14.4
100 7.4 6.3 9.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

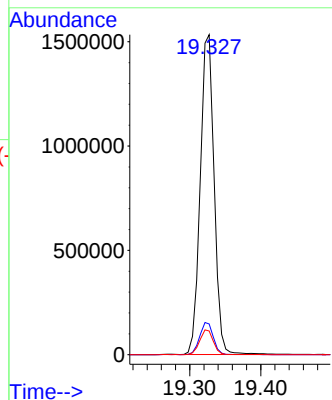


#82
Pyrene
Concen: 35.859 ng/u1
RT: 19.680 min Scan# 2821
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:202 Resp: 2098880
Ion Ratio Lower Upper
202 100
101 11.2 10.6 15.8
100 9.2 9.8 14.6#

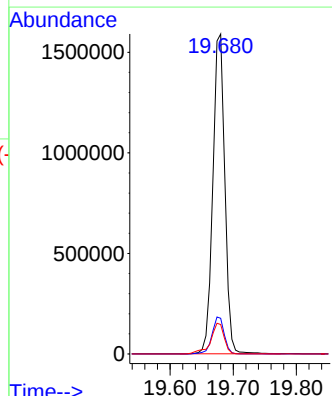



#83
Butylbenzylphthalate
Concen: 37.226 ng/ul
RT: 20.545 min Scan# 2968
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:149 Resp: 900660
Ion Ratio Lower Upper
149 100
91 72.0 71.1 106.7
206 22.0 28.8 43.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#84
3,3'-Dichlorobenzidine
Concen: 36.695 ng/ul
RT: 21.315 min Scan# 3099
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:252 Resp: 584776
Ion Ratio Lower Upper
252 100
254 67.0 49.8 74.6
126 10.1 4.3 6.5





#85
Benzo(a)anthracene
Concen: 33.305 ng/ul
RT: 21.386 min Scan# 3111
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion:228 Resp: 1871985
Ion Ratio Lower Upper
228 100
229 19.9 18.2 27.2
226 26.2 22.8 34.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#86
Bis(2-ethylhexyl)phthalate
Concen: 36.543 ng/ul
RT: 21.310 min Scan# 3098
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:149 Resp: 1310373
Ion Ratio Lower Upper
149 100
167 28.8 32.8 49.2#
279 4.9 5.6 8.4#

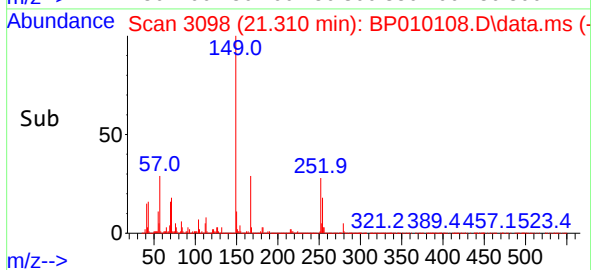



#87
Chrysene
Concen: 33.043 ng/ul
RT: 21.439 min Scan# 3120
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303



Tgt Ion:228 Resp: 1828738
Ion Ratio Lower Upper
228 100
226 29.0 22.7 34.1
229 19.9 15.2 22.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022



#89
Di-n-octyl phthalate
Concen: 40.711 ng/ul
RT: 22.251 min Scan# 3258
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44


Tgt Ion:149 Resp: 2132892

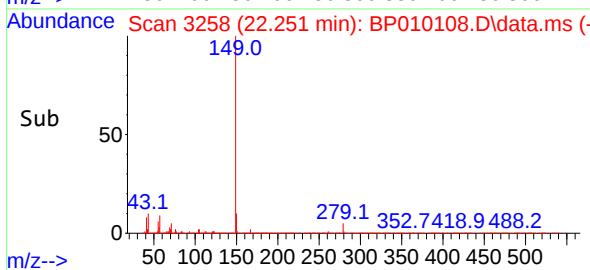



#90
Benzo(b)fluoranthene
Concen: 36.570 ng/u1
RT: 23.104 min Scan# 3403
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:252 Resp: 1656860
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.0
125 8.6 7.3 10.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#91
Benzo(k)fluoranthene
Concen: 35.109 ng/u1
RT: 23.156 min Scan# 3412
Delta R.T. -0.000 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Tgt Ion:252 Resp: 1506725
Ion Ratio Lower Upper
252 100
253 21.2 17.9 26.9
125 8.0 5.1 7.7#





#93
Benzo(a)pyrene
Concen: 34.550 ng/ul
RT: 23.745 min Scan# 3512
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44




Instrument :
BNA_P
ClientSampleId :
SLCS303




Tgt Ion:252 Resp: 1447520
Ion Ratio Lower Upper
252 100
253 21.9 17.5 26.3
125 9.1 6.4 9.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022




#94
Indeno(1,2,3-cd)pyrene
Concen: 32.938 ng/ul
RT: 26.415 min Scan# 3966
Delta R.T. -0.012 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44



Tgt Ion:276 Resp: 1372783
Ion Ratio Lower Upper
276 100
138 19.8 12.3 18.5
277 25.1 19.3 28.9









#95
Dibenzo(a,h)anthracene
Concen: 33.202 ng/ul
RT: 26.433 min Scan# 3968
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Instrument :
BNA_P
ClientSampleId :
SLCS303

Tgt Ion:278 Resp: 1184059
Ion Ratio Lower Upper
278 100
139 14.1 6.6 10.0
279 23.9 18.4 27.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/27/2022
Supervised By :Yogesh Patel 04/28/2022

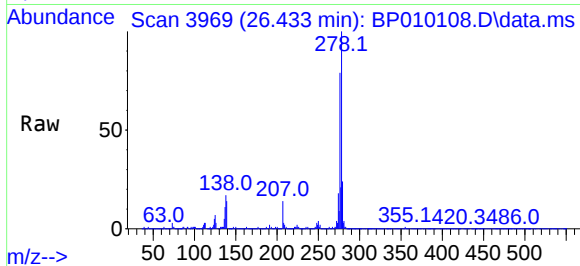

#96
Benzo(g,h,i)perylene
Concen: 33.527 ng/ul
RT: 27.203 min Scan# 4100
Delta R.T. -0.006 min
Lab File: BP010108.D
Acq: 26 Apr 2022 10:44

Tgt Ion:276 Resp: 1179054
Ion Ratio Lower Upper
276 100
138 17.5 11.6 17.4
277 23.7 15.9 23.9

