

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010080.D
 Acq On : 25 Apr 2022 13:03
 Operator : CG/JU
 Sample : PB144303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	56	rVB	50663	71589	1.43%	0.142%
2	3.781	114	118	137	rBV	548579	918572	18.39%	1.820%
3	4.117	171	175	182	rVB4	13541	19729	0.40%	0.039%
4	7.093	672	681	699	rBV	729407	1229182	24.61%	2.436%
5	7.258	703	709	721	rVV	606393	1003280	20.09%	1.988%
6	7.352	722	725	735	rVB8	6041	13180	0.26%	0.026%
7	7.464	737	744	755	rBV	770359	1259170	25.21%	2.495%
8	7.934	817	824	839	rBV	653405	1071169	21.45%	2.123%
9	8.387	893	901	905	rBV7	6429	15131	0.30%	0.030%
10	8.458	908	913	916	rBV6	4348	7936	0.16%	0.016%
11	8.640	935	944	959	rBV	952434	1597612	31.99%	3.166%
12	8.746	961	962	972	rVB4	11411	21107	0.42%	0.042%
13	9.022	1005	1009	1013	rBV7	6074	7990	0.16%	0.016%
14	9.093	1013	1021	1034	rBV	760037	1316567	26.36%	2.609%
15	9.669	1112	1119	1125	rVB3	8211	13817	0.28%	0.027%
16	9.816	1137	1144	1156	rBV	621749	1097392	21.97%	2.175%
17	9.911	1156	1160	1170	rVB7	8712	19157	0.38%	0.038%
18	10.146	1197	1200	1206	rVB4	5990	10183	0.20%	0.020%
19	10.358	1229	1236	1255	rBV	864921	1573892	31.52%	3.119%
20	10.740	1292	1301	1309	rBV	931506	1596164	31.96%	3.163%
21	10.875	1315	1324	1341	rBV	851242	1647040	32.98%	3.264%
22	11.087	1355	1360	1366	rVB7	7698	14262	0.29%	0.028%
23	12.034	1516	1521	1530	rBV7	5976	11035	0.22%	0.022%
24	12.328	1565	1571	1579	rBV2	16399	31664	0.63%	0.063%
25	12.399	1579	1583	1589	rVB3	7769	14874	0.30%	0.029%
26	12.622	1613	1621	1626	rBV2	11388	20896	0.42%	0.041%
27	12.775	1640	1647	1656	rVB6	10235	21923	0.44%	0.043%
28	13.016	1683	1688	1695	rVB10	6009	10640	0.21%	0.021%
29	13.093	1695	1701	1708	rVB9	5492	10611	0.21%	0.021%
30	13.375	1744	1749	1752	rBV4	11863	19494	0.39%	0.039%
31	13.410	1752	1755	1758	rVV3	11720	18749	0.38%	0.037%
32	13.451	1758	1762	1767	rVB3	10818	18436	0.37%	0.037%
33	13.657	1789	1797	1804	rBV3	3959	11365	0.23%	0.023%
34	13.975	1844	1851	1865	rBV	1915504	2755675	55.18%	5.461%
35	14.140	1875	1879	1885	rVB9	7222	12428	0.25%	0.025%
36	14.263	1892	1900	1914	rBV	1866173	2982443	59.72%	5.910%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010080.D
 Acq On : 25 Apr 2022 13:03
 Operator : CG/JU
 Sample : PB144303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.475	1934	1936	1941	rVB6	4299	5403	0.11%	0.011%
38	14.569	1945	1952	1960	rBV	1535794	2247139	45.00%	4.453%
39	14.628	1960	1962	1970	rVB3	17479	28333	0.57%	0.056%
40	14.757	1977	1984	2003	rBV	558927	1131246	22.65%	2.242%
41	14.893	2003	2007	2010	rVV6	20460	38433	0.77%	0.076%
42	14.928	2010	2013	2017	rVV6	11214	22348	0.45%	0.044%
43	14.969	2017	2020	2025	rVB3	13102	22763	0.46%	0.045%
44	15.193	2054	2058	2065	rVB8	8465	15568	0.31%	0.031%
45	15.387	2086	2091	2097	rVB	16872	26515	0.53%	0.053%
46	15.563	2112	2121	2127	rBV	2533290	3793075	75.96%	7.516%
47	15.610	2127	2129	2135	rVV3	49024	80677	1.62%	0.160%
48	15.675	2135	2140	2153	rVV	854411	1283465	25.70%	2.543%
49	15.804	2157	2162	2171	rVB3	32352	74005	1.48%	0.147%
50	16.345	2249	2254	2259	rBV4	10753	17799	0.36%	0.035%
51	16.510	2277	2282	2286	rVB5	12423	18516	0.37%	0.037%
52	16.628	2298	2302	2308	rVB6	14233	19441	0.39%	0.039%
53	16.781	2324	2328	2333	rBV5	10543	17213	0.34%	0.034%
54	16.975	2357	2361	2363	rBV5	5449	7358	0.15%	0.015%
55	16.998	2363	2365	2372	rVB8	6049	8424	0.17%	0.017%
56	17.104	2381	2383	2386	rBV3	4683	5395	0.11%	0.011%
57	17.322	2412	2420	2430	rBV	1833948	2779207	55.65%	5.507%
58	17.422	2430	2437	2460	rVB	2828247	4273117	85.57%	8.468%
59	17.728	2480	2489	2495	rBV3	9406	21585	0.43%	0.043%
60	17.975	2528	2531	2536	rVB6	5240	8199	0.16%	0.016%
61	18.057	2540	2545	2550	rBV8	2395	6618	0.13%	0.013%
62	18.210	2567	2571	2575	rBV7	5751	9638	0.19%	0.019%
63	18.275	2578	2582	2588	rVB	20906	30098	0.60%	0.060%
64	19.228	2740	2744	2749	rVB	36628	48077	0.96%	0.095%
65	19.298	2751	2756	2759	rBV	36411	54529	1.09%	0.108%
66	19.328	2759	2761	2767	rVB	23146	25729	0.52%	0.051%
67	19.651	2809	2816	2830	rBV	3635134	4993827	100.00%	9.896%
68	20.545	2966	2968	2972	rBV2	13710	15381	0.31%	0.030%
69	21.404	3108	3114	3120	rBV	1900594	2694532	53.96%	5.339%
70	23.698	3496	3504	3512	rBV2	1800857	3874501	77.59%	7.678%
71	23.857	3524	3531	3542	rVB2	1068881	2301868	46.09%	4.561%




Sum of corrected areas: 50464376

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010080.D
Acq On : 25 Apr 2022 13:03
Operator : CG/JU
Sample : PB144303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

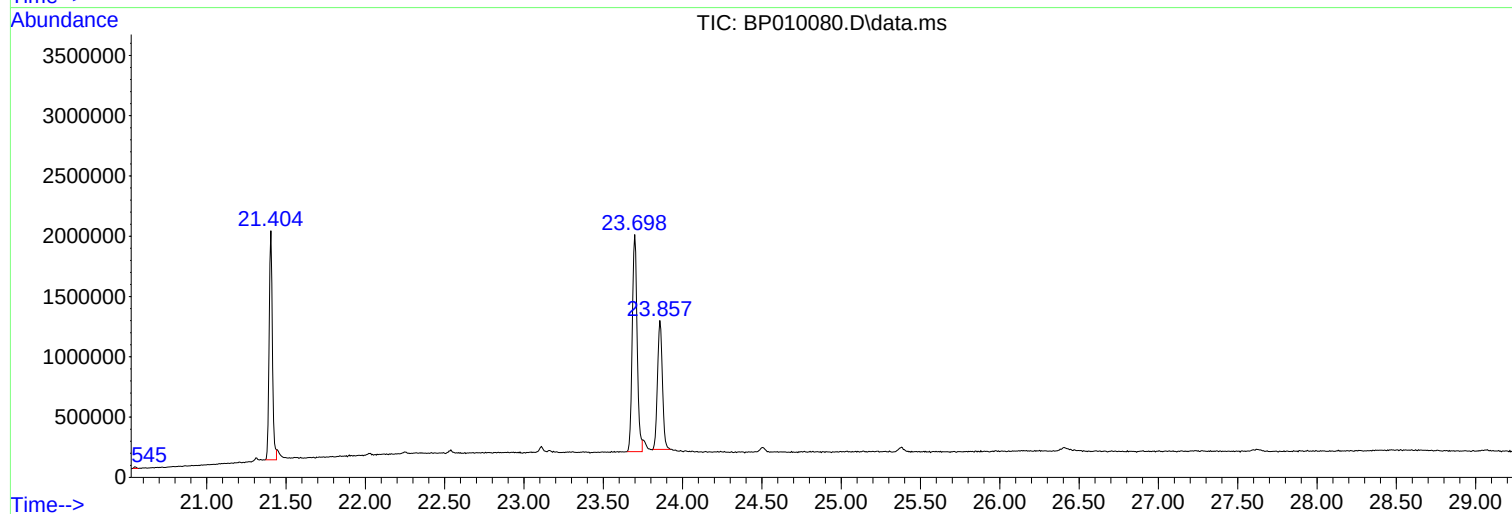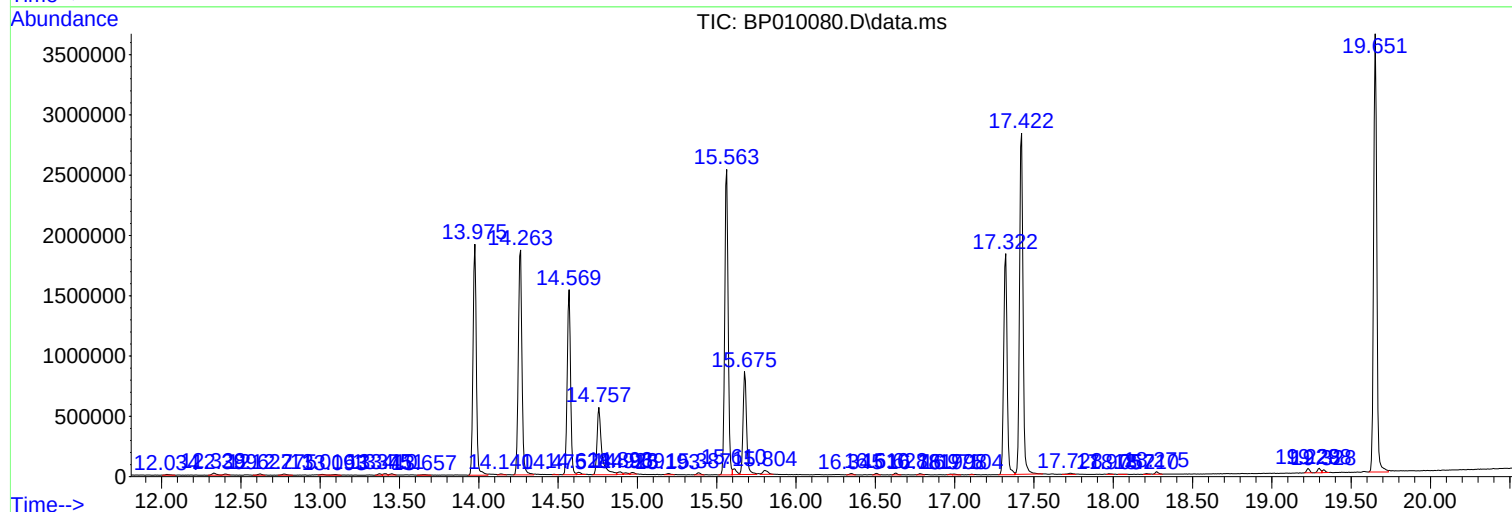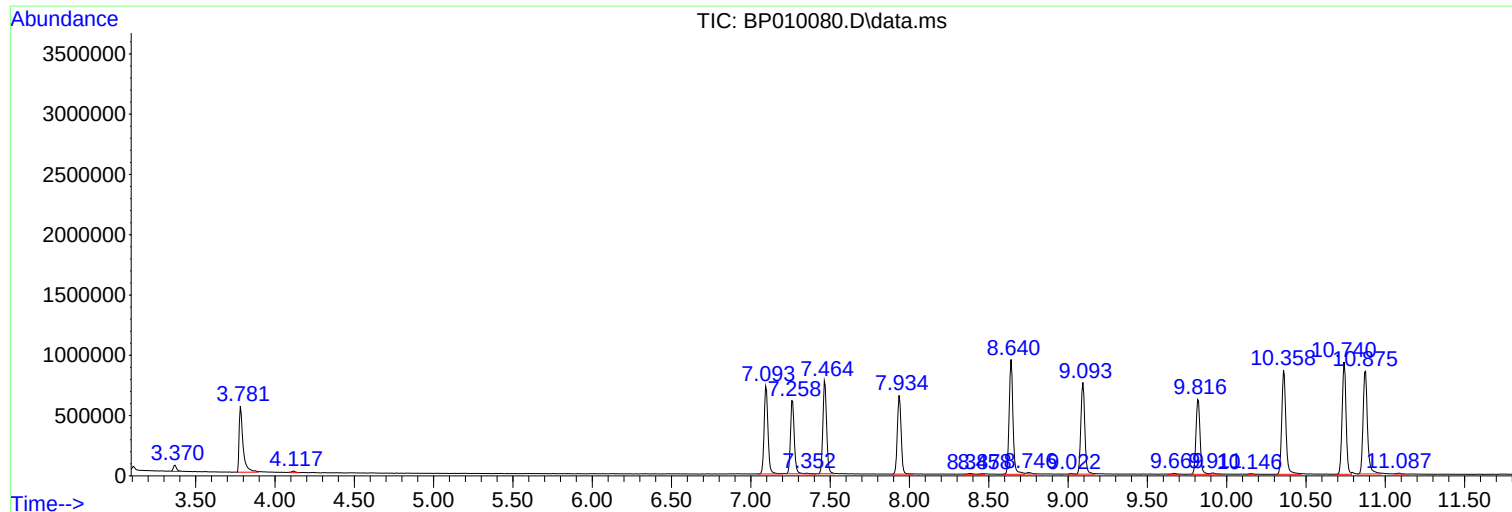

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010080.D
Acq On : 25 Apr 2022 13:03
Operator : CG/JU
Sample : PB144303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010080.D
Acq On : 25 Apr 2022 13:03
Operator : CG/JU
Sample : PB144303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK303

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------