

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010084.D
 Acq On : 25 Apr 2022 15:58
 Operator : CG/JU
 Sample : N2475-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	52	rVB2	23610	27982	0.66%	0.070%
2	3.799	117	121	131	rBV	50386	97907	2.30%	0.245%
3	4.111	172	174	178	rVB3	11773	15847	0.37%	0.040%
4	7.093	672	681	690	rBV	139221	242866	5.72%	0.609%
5	7.263	703	710	723	rBV	554364	929721	21.89%	2.330%
6	7.463	737	744	755	rBV	542820	890658	20.97%	2.232%
7	7.934	817	824	834	rBV	637880	1034358	24.35%	2.592%
8	8.010	834	837	843	rVB6	8066	12489	0.29%	0.031%
9	8.640	937	944	956	rBV	426729	722084	17.00%	1.810%
10	8.763	962	965	969	rVB6	2713	4317	0.10%	0.011%
11	9.093	1009	1021	1036	rBV	712662	1227763	28.90%	3.077%
12	9.552	1092	1099	1105	rVB6	5963	12768	0.30%	0.032%
13	9.816	1137	1144	1156	rBV	547478	941082	22.15%	2.358%
14	10.357	1229	1236	1254	rBV	718902	1297316	30.54%	3.251%
15	10.575	1270	1273	1276	rBV5	2869	4434	0.10%	0.011%
16	10.740	1291	1301	1311	rBV	865263	1511193	35.57%	3.787%
17	10.875	1317	1324	1346	rBV	588091	1140376	26.84%	2.858%
18	12.175	1542	1545	1550	rVB5	4646	7945	0.19%	0.020%
19	12.334	1566	1572	1575	rBV2	14997	29242	0.69%	0.073%
20	12.369	1575	1578	1588	rVB3	14352	34493	0.81%	0.086%
21	13.304	1734	1737	1743	rVB7	2929	4871	0.11%	0.012%
22	13.404	1750	1754	1760	rBV6	11379	18586	0.44%	0.047%
23	13.469	1760	1765	1775	rVB2	50184	84336	1.99%	0.211%
24	13.975	1844	1851	1864	rBV	1763545	2543122	59.86%	6.373%
25	14.257	1892	1899	1917	rBV	1750660	2746039	64.64%	6.882%
26	14.475	1932	1936	1940	rVB6	3067	4593	0.11%	0.012%
27	14.569	1944	1952	1965	rBV	1360613	2057897	48.44%	5.157%
28	14.763	1979	1985	2001	rBV2	58977	159672	3.76%	0.400%
29	15.204	2056	2060	2064	rVB7	4600	4865	0.11%	0.012%
30	15.381	2085	2090	2093	rBV4	5121	7741	0.18%	0.019%
31	15.563	2113	2121	2134	rBV	2310043	3667717	86.34%	9.192%
32	15.675	2134	2140	2154	rVV	786502	1178833	27.75%	2.954%
33	15.804	2156	2162	2168	rVB	28466	55197	1.30%	0.138%
34	16.257	2233	2239	2242	rBV7	2865	6118	0.14%	0.015%
35	16.345	2250	2254	2260	rVB4	9127	14717	0.35%	0.037%
36	17.004	2359	2366	2369	rBV8	5486	11026	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010084.D
 Acq On : 25 Apr 2022 15:58
 Operator : CG/JU
 Sample : N2475-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	17.092	2376	2381	2382	rBV5	3701	4662	0.11%	0.012%
38	17.316	2411	2419	2429	rBV	1531055	2331525	54.88%	5.843%
39	17.416	2430	2436	2454	rVB	2644805	3953213	93.06%	9.907%
40	17.986	2530	2533	2538	rBV7	4395	5059	0.12%	0.013%
41	18.204	2566	2570	2578	rBV4	23028	37665	0.89%	0.094%
42	18.275	2578	2582	2585	rVB	7976	9548	0.22%	0.024%
43	18.763	2662	2665	2669	rBV6	2681	4703	0.11%	0.012%
44	19.227	2740	2744	2748	rBV2	32689	42642	1.00%	0.107%
45	19.298	2751	2756	2765	rBV2	34206	56168	1.32%	0.141%
46	19.651	2809	2816	2832	rBV	3154315	4248145	100.00%	10.646%
47	21.110	3060	3064	3069	rBV	136996	188876	4.45%	0.473%
48	21.404	3108	3114	3120	rBV	1263658	1829204	43.06%	4.584%
49	23.698	3496	3504	3511	rBV2	1294977	2830304	66.62%	7.093%
50	23.851	3523	3530	3545	rVB2	726191	1611365	37.93%	4.038%


Sum of corrected areas: 39903250

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010084.D
Acq On : 25 Apr 2022 15:58
Operator : CG/JU
Sample : N2475-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

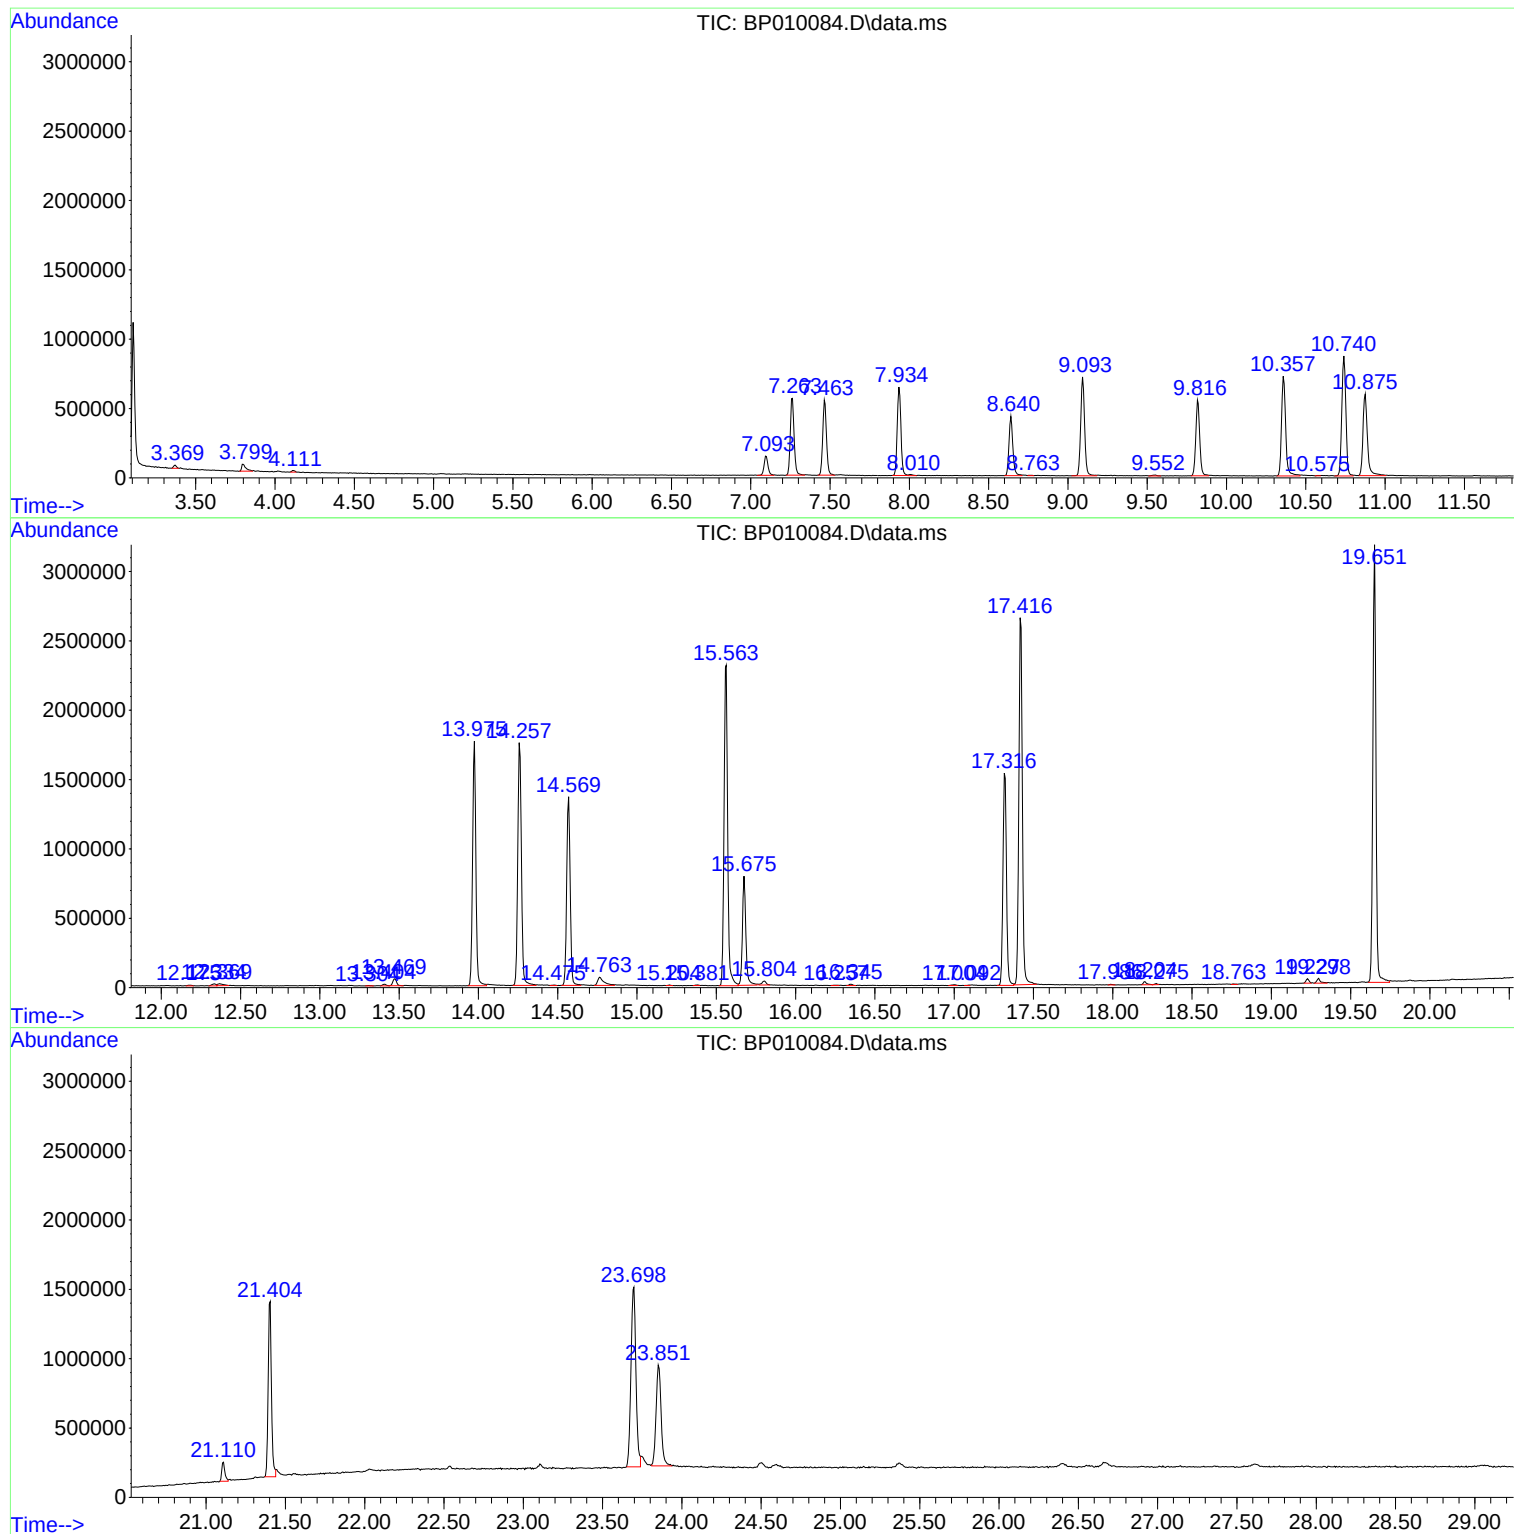

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010084.D
Acq On : 25 Apr 2022 15:58
Operator : CG/JU
Sample : N2475-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.110	2.07 ng/ul	188876	Chrysene-d12	21.404

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Z-5-Nonadecene	266	C19H38	1000131-11-8	98
2			Fumaric acid, 2-chloropropyl tri...	374	C20H35ClO4	1010348-57-1	97
3			1-Heneicosanol	312	C21H44O	015594-90-8	95
4			1-Nonadecene	266	C19H38	018435-45-5	95
5			1-Nonadecene	266	C19H38	018435-45-5	95

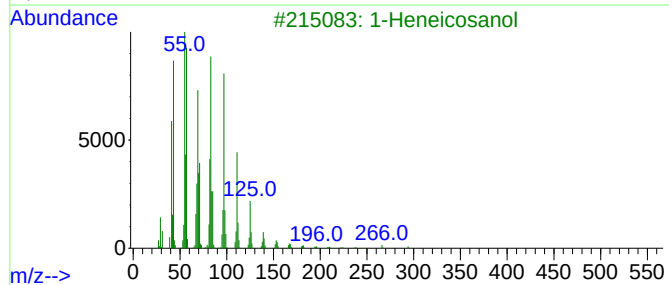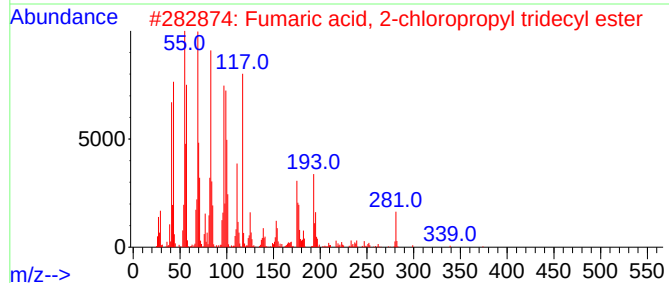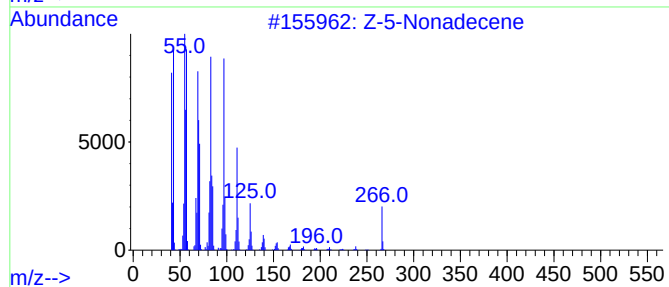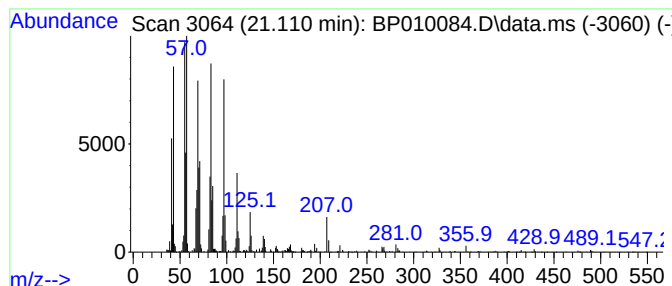

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010084.D
Acq On : 25 Apr 2022 15:58
Operator : CG/JU
Sample : N2475-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.110	2.1	ng/ul	188876	5	21.404	1829200	20.0