

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010087.D
 Acq On : 25 Apr 2022 17:40
 Operator : CG/JU
 Sample : PB144305BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK305

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	44	47	53	rVB	48646	67638	1.37%	0.135%
2	3.781	114	118	138	rBV	579910	950141	19.25%	1.891%
3	4.117	171	175	180	rVB4	12333	19498	0.39%	0.039%
4	7.093	674	681	694	rBV	743304	1218524	24.68%	2.425%
5	7.264	703	710	722	rBV	615566	1023896	20.74%	2.038%
6	7.464	737	744	757	rBV	802243	1296650	26.27%	2.580%
7	7.934	817	824	836	rBV	700733	1127661	22.84%	2.244%
8	8.640	937	944	959	rBV	957139	1597748	32.36%	3.179%
9	9.093	1009	1021	1036	rBV	780311	1353619	27.42%	2.694%
10	9.816	1136	1144	1155	rBV	654040	1118681	22.66%	2.226%
11	10.358	1227	1236	1253	rBV	884285	1591722	32.24%	3.167%
12	10.740	1291	1301	1315	rBV	987108	1675350	33.94%	3.334%
13	10.875	1316	1324	1349	rVV	870494	1689225	34.22%	3.362%
14	12.334	1563	1572	1583	rBV2	15393	36342	0.74%	0.072%
15	13.975	1844	1851	1864	rBV	1894466	2783428	56.38%	5.539%
16	14.257	1891	1899	1916	rBV	1989034	3038385	61.55%	6.046%
17	14.569	1944	1952	1965	rBV	1530671	2345219	47.51%	4.667%
18	14.757	1977	1984	2007	rBV	554599	1126626	22.82%	2.242%
19	15.387	2082	2091	2097	rVB	3696	9059	0.18%	0.018%
20	15.557	2113	2120	2134	rBV	2541275	3900470	79.01%	7.762%
21	15.675	2134	2140	2156	rVV	854441	1299255	26.32%	2.585%
22	15.798	2156	2161	2167	rVB2	32142	54702	1.11%	0.109%
23	16.128	2214	2217	2222	rVB5	3634	5271	0.11%	0.010%
24	16.345	2248	2254	2260	rBV5	11723	17049	0.35%	0.034%
25	16.992	2361	2364	2369	rBV7	4918	7763	0.16%	0.015%
26	17.104	2380	2383	2389	rVB5	4957	6150	0.12%	0.012%
27	17.316	2413	2419	2429	rBV	1969782	2821514	57.15%	5.615%
28	17.416	2429	2436	2456	rVB2	2851361	4266087	86.41%	8.489%
29	18.275	2578	2582	2586	rBV4	3936	6226	0.13%	0.012%
30	19.228	2738	2744	2751	rBV3	38027	61430	1.24%	0.122%
31	19.298	2751	2756	2761	rVV	34655	51712	1.05%	0.103%
32	19.645	2809	2815	2833	rBV	3468973	4936745	100.00%	9.824%
33	21.404	3108	3114	3130	rBV	1777684	2770086	56.11%	5.512%
34	23.698	3496	3504	3521	rBV2	1644732	3689113	74.73%	7.341%
35	23.851	3523	3530	3545	rVB2	1044091	2288808	46.36%	4.555%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010087.D
Acq On : 25 Apr 2022 17:40
Operator : CG/JU
Sample : PB144305BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK305

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION


Sum of corrected areas: 50251793

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010087.D
Acq On : 25 Apr 2022 17:40
Operator : CG/JU
Sample : PB144305BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK305

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

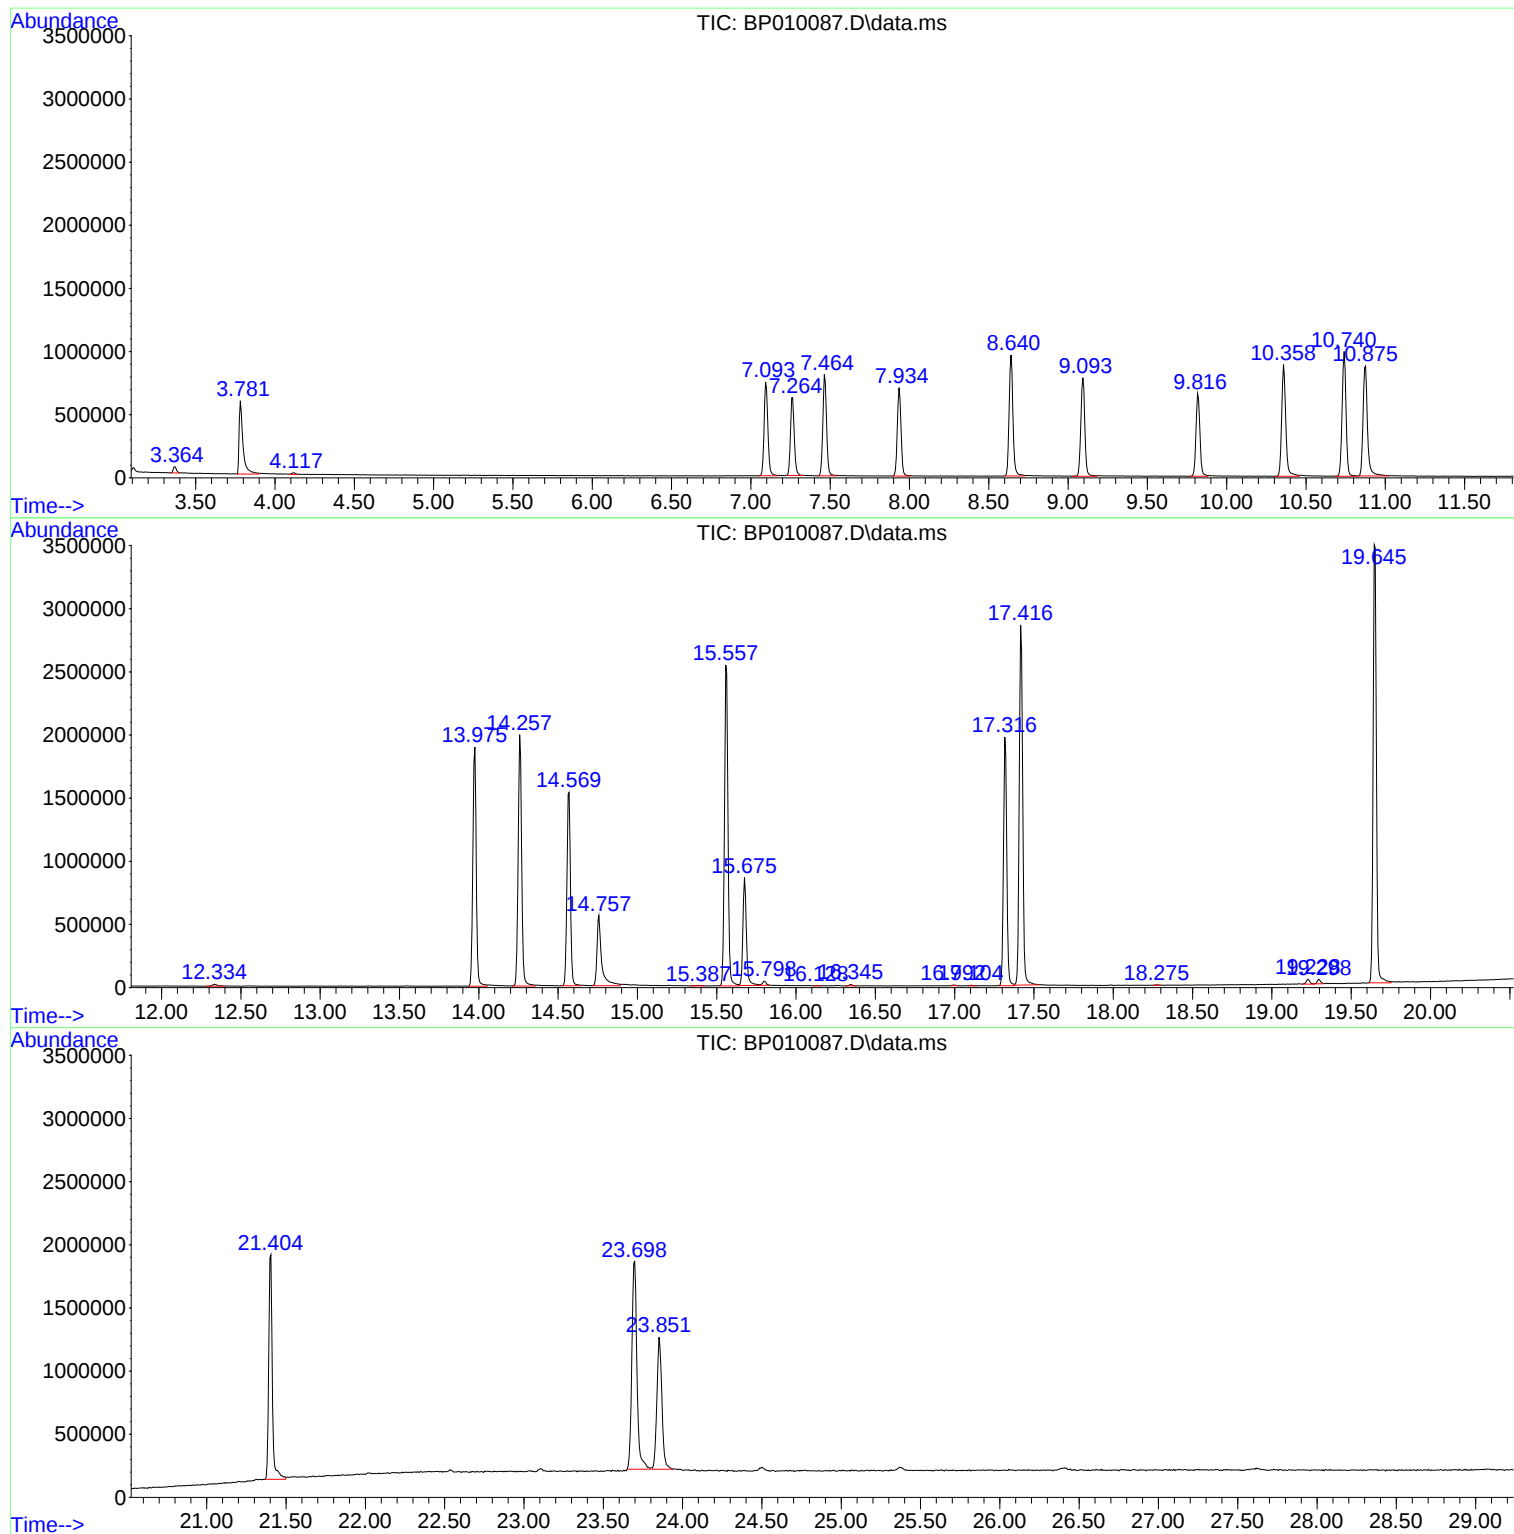

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010087.D
Acq On : 25 Apr 2022 17:40
Operator : CG/JU
Sample : PB144305BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK305

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010087.D
Acq On : 25 Apr 2022 17:40
Operator : CG/JU
Sample : PB144305BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK305

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc