

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010091.D
 Acq On : 25 Apr 2022 19:54
 Operator : CG/JU
 Sample : PB144328BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK328

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	44	47	58	rVB	47292	74677	1.58%	0.156%
2	3.781	114	118	139	rBV	509605	862004	18.19%	1.796%
3	4.116	171	175	182	rVB3	12508	19148	0.40%	0.040%
4	7.093	675	681	698	rBV	668345	1106606	23.35%	2.306%
5	7.263	703	710	725	rBV	557615	934709	19.72%	1.947%
6	7.463	737	744	759	rBV	706448	1157217	24.41%	2.411%
7	7.934	817	824	836	rBV	631907	1026787	21.66%	2.139%
8	8.640	937	944	958	rBV	881222	1472083	31.06%	3.067%
9	9.093	1012	1021	1035	rBV	722128	1241436	26.19%	2.586%
10	9.816	1135	1144	1159	rBV	603338	1031128	21.75%	2.148%
11	10.357	1228	1236	1255	rBV	810236	1465146	30.91%	3.053%
12	10.740	1293	1301	1312	rBV	900159	1540856	32.51%	3.210%
13	10.869	1316	1323	1348	rBV	796568	1575601	33.24%	3.283%
14	12.340	1566	1573	1582	rVB2	12932	27839	0.59%	0.058%
15	13.975	1843	1851	1868	rBV	1812787	2643208	55.77%	5.507%
16	14.257	1892	1899	1917	rBV	1921166	2881745	60.80%	6.004%
17	14.569	1945	1952	1967	rBV	1433720	2219425	46.83%	4.624%
18	14.757	1977	1984	2002	rBV	507108	1032941	21.79%	2.152%
19	15.381	2085	2090	2094	rBV7	3149	6196	0.13%	0.013%
20	15.557	2113	2120	2134	rBV	2418913	3728010	78.65%	7.767%
21	15.675	2134	2140	2157	rVV	824904	1232167	26.00%	2.567%
22	15.798	2157	2161	2169	rVB2	31512	54206	1.14%	0.113%
23	16.345	2250	2254	2259	rVB2	9345	15057	0.32%	0.031%
24	16.998	2361	2365	2371	rVB7	5624	8803	0.19%	0.018%
25	17.316	2413	2419	2429	rVV	1857900	2712266	57.22%	5.651%
26	17.416	2429	2436	2453	rVB	2639495	4050149	85.45%	8.438%
27	18.275	2578	2582	2585	rBV5	3530	5158	0.11%	0.011%
28	19.227	2739	2744	2749	rBV	36037	52215	1.10%	0.109%
29	19.298	2751	2756	2760	rBV	33044	50054	1.06%	0.104%
30	19.651	2809	2816	2830	rBV	3400320	4739810	100.00%	9.875%
31	21.398	3108	3113	3128	rBV	1832016	2805591	59.19%	5.845%
32	23.698	3496	3504	3511	rBV2	1790411	3743625	78.98%	7.800%
33	23.851	3523	3530	3547	rVB2	1096300	2480930	52.34%	5.169%




Sum of corrected areas: 47996793

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010091.D
Acq On : 25 Apr 2022 19:54
Operator : CG/JU
Sample : PB144328BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

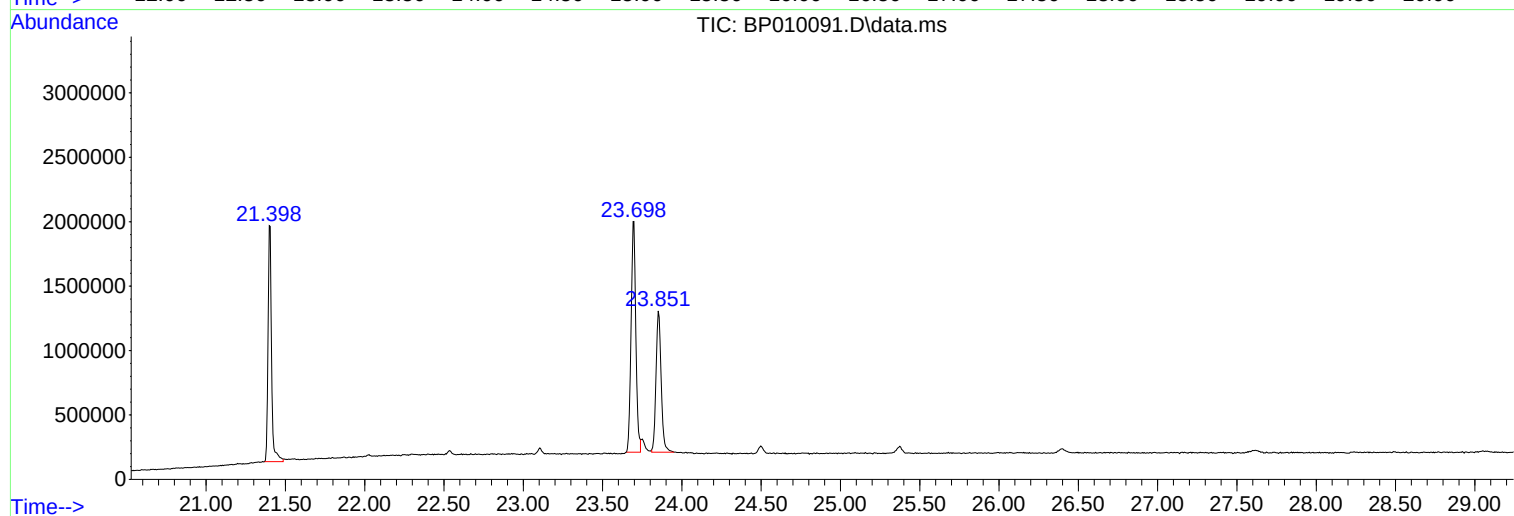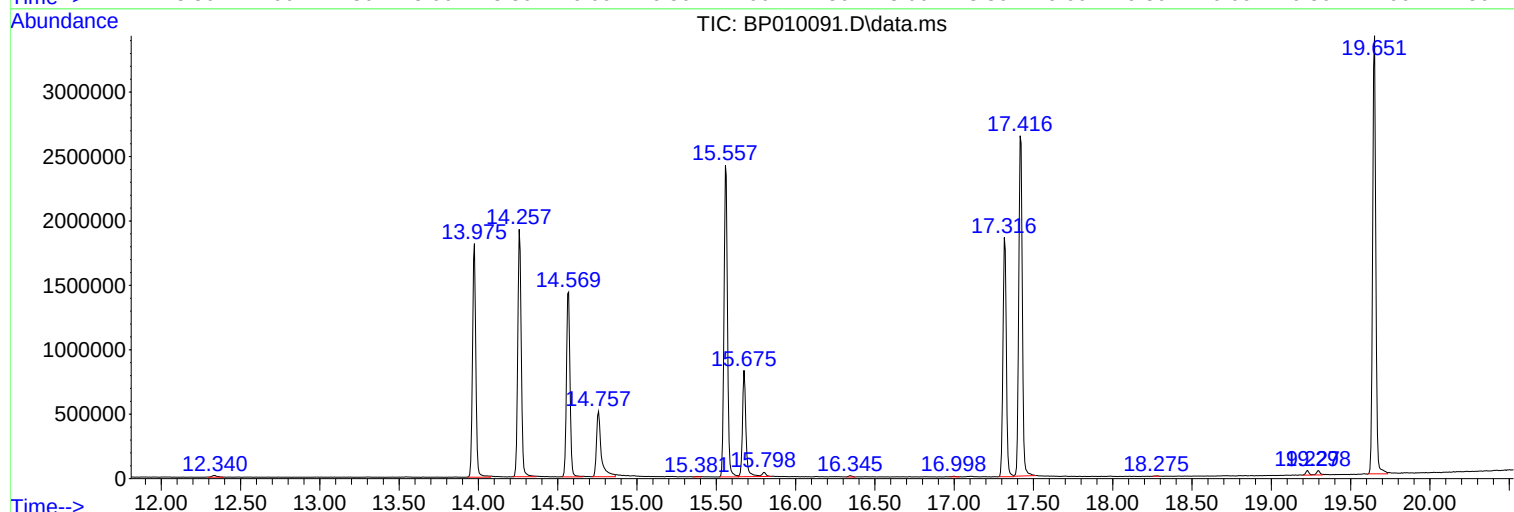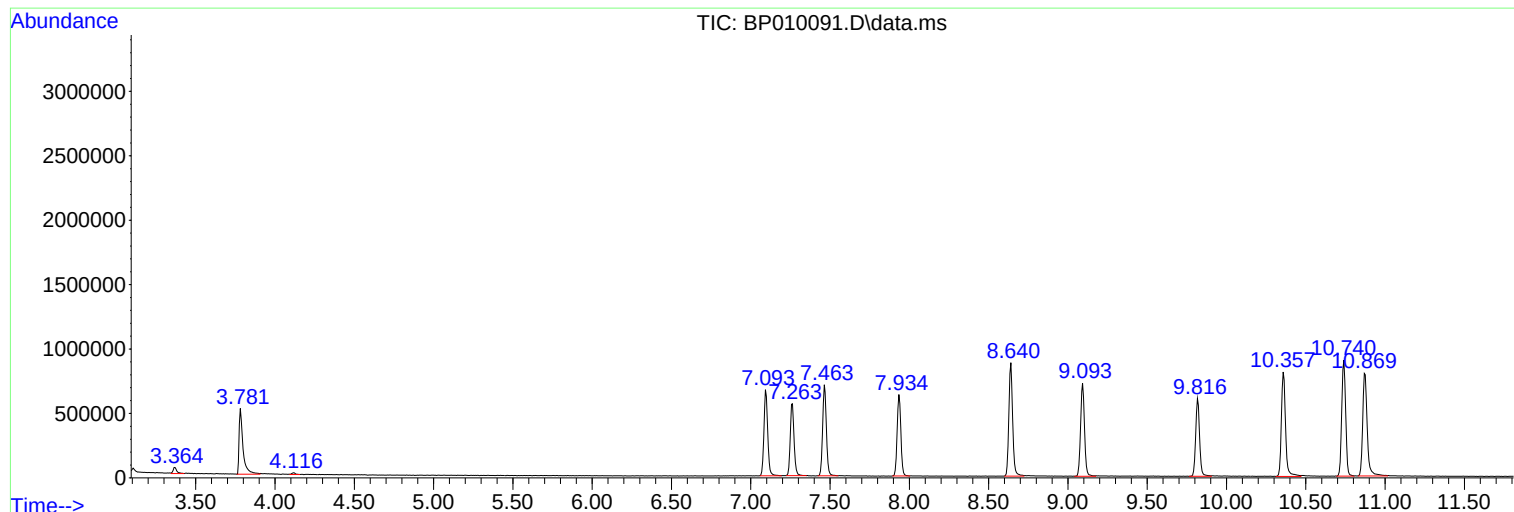

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010091.D
Acq On : 25 Apr 2022 19:54
Operator : CG/JU
Sample : PB144328BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010091.D
Acq On : 25 Apr 2022 19:54
Operator : CG/JU
Sample : PB144328BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK328

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc