

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010092.D
 Acq On : 25 Apr 2022 20:28
 Operator : CG/JU
 Sample : N2475-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BM8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	57	rVB	41847	58827	1.16%	0.130%
2	3.793	117	120	132	rBV	96316	177534	3.49%	0.393%
3	4.028	157	160	164	rVB5	7741	10329	0.20%	0.023%
4	4.116	171	175	179	rVB	14273	15738	0.31%	0.035%
5	7.093	676	681	694	rVB	162410	274001	5.39%	0.606%
6	7.257	703	709	722	rBV	627976	1025735	20.19%	2.269%
7	7.463	734	744	757	rBV	620465	1010852	19.89%	2.236%
8	7.563	758	761	768	rVB9	5029	9579	0.19%	0.021%
9	7.934	817	824	833	rBV	606348	998816	19.66%	2.210%
10	8.010	833	837	841	rVB4	8778	13794	0.27%	0.031%
11	8.640	935	944	960	rBV	515023	868070	17.08%	1.921%
12	9.093	1013	1021	1035	rBV	803686	1375344	27.07%	3.043%
13	9.263	1046	1050	1057	rVB10	2886	7198	0.14%	0.016%
14	9.540	1092	1097	1109	rVB2	17143	33458	0.66%	0.074%
15	9.816	1137	1144	1157	rBV	654132	1099185	21.63%	2.432%
16	10.357	1227	1236	1254	rBV	863686	1524299	30.00%	3.372%
17	10.551	1266	1269	1271	rBV4	5332	6458	0.13%	0.014%
18	10.740	1293	1301	1316	rBV	864153	1472769	28.98%	3.258%
19	10.875	1316	1324	1345	rBV	685929	1331071	26.19%	2.945%
20	11.569	1435	1442	1448	rBV	4492	10365	0.20%	0.023%
21	11.787	1471	1479	1484	rBV	3148	6818	0.13%	0.015%
22	12.175	1537	1545	1553	rVB5	8003	15818	0.31%	0.035%
23	12.328	1567	1571	1576	rBV3	16127	30312	0.60%	0.067%
24	12.369	1576	1578	1587	rVB7	6480	13642	0.27%	0.030%
25	12.981	1678	1682	1689	rVB9	3849	7286	0.14%	0.016%
26	13.122	1702	1706	1711	rVB8	3921	5873	0.12%	0.013%
27	13.192	1714	1718	1723	rVB8	3314	5768	0.11%	0.013%
28	13.404	1749	1754	1761	rVB3	22392	35920	0.71%	0.079%
29	13.545	1773	1778	1787	rVB3	2818	6354	0.13%	0.014%
30	13.975	1844	1851	1864	rBV	2045154	2926437	57.59%	6.474%
31	14.063	1864	1866	1871	rVB5	3942	6083	0.12%	0.013%
32	14.257	1891	1899	1912	rBV	2079125	3177036	62.52%	7.029%
33	14.475	1933	1936	1941	rVB6	6384	10893	0.21%	0.024%
34	14.563	1944	1951	1963	rBV	1339526	2072706	40.79%	4.586%
35	14.763	1979	1985	2005	rBV2	73371	195936	3.86%	0.433%
36	15.204	2054	2060	2064	rVB7	3556	5537	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010092.D
 Acq On : 25 Apr 2022 20:28
 Operator : CG/JU
 Sample : N2475-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 AOBM8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	15.375	2085	2089	2095	rBV6	5983	13189	0.26%	0.029%
38	15.557	2113	2120	2134	rBV	2780635	4227510	83.20%	9.353%
39	15.675	2134	2140	2153	rVV	966041	1420004	27.94%	3.142%
40	15.798	2157	2161	2173	rVB	35695	66403	1.31%	0.147%
41	15.928	2178	2183	2187	rVB8	2963	5624	0.11%	0.012%
42	16.345	2250	2254	2260	rVB3	12111	18665	0.37%	0.041%
43	16.998	2360	2365	2373	rBV9	6491	11339	0.22%	0.025%
44	17.080	2375	2379	2381	rBV5	4577	6910	0.14%	0.015%
45	17.316	2412	2419	2429	rBV	1672841	2449864	48.21%	5.420%
46	17.416	2429	2436	2451	rVV2	2952686	4507653	88.71%	9.973%
47	17.992	2529	2534	2535	rBV5	5217	6017	0.12%	0.013%
48	18.198	2565	2569	2578	rBV7	15216	26499	0.52%	0.059%
49	18.269	2578	2581	2585	rVB2	7077	9645	0.19%	0.021%
50	18.827	2674	2676	2682	rVB7	6799	9310	0.18%	0.021%
51	19.227	2739	2744	2750	rBV	40513	57751	1.14%	0.128%
52	19.292	2751	2755	2759	rBV	37111	55561	1.09%	0.123%
53	19.563	2798	2801	2806	rBV6	10611	16999	0.33%	0.038%
54	19.651	2809	2816	2835	rBV	3626480	5081439	100.00%	11.242%
55	21.110	3060	3064	3072	rBV4	109728	165467	3.26%	0.366%
56	21.398	3108	3113	3120	rBV	1432653	2100975	41.35%	4.648%
57	23.692	3496	3503	3511	rBV2	1585113	3382624	66.57%	7.484%
58	23.851	3523	3530	3545	rVB2	788493	1714690	33.74%	3.794%




Sum of corrected areas: 45199979

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010092.D
Acq On : 25 Apr 2022 20:28
Operator : CG/JU
Sample : N2475-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

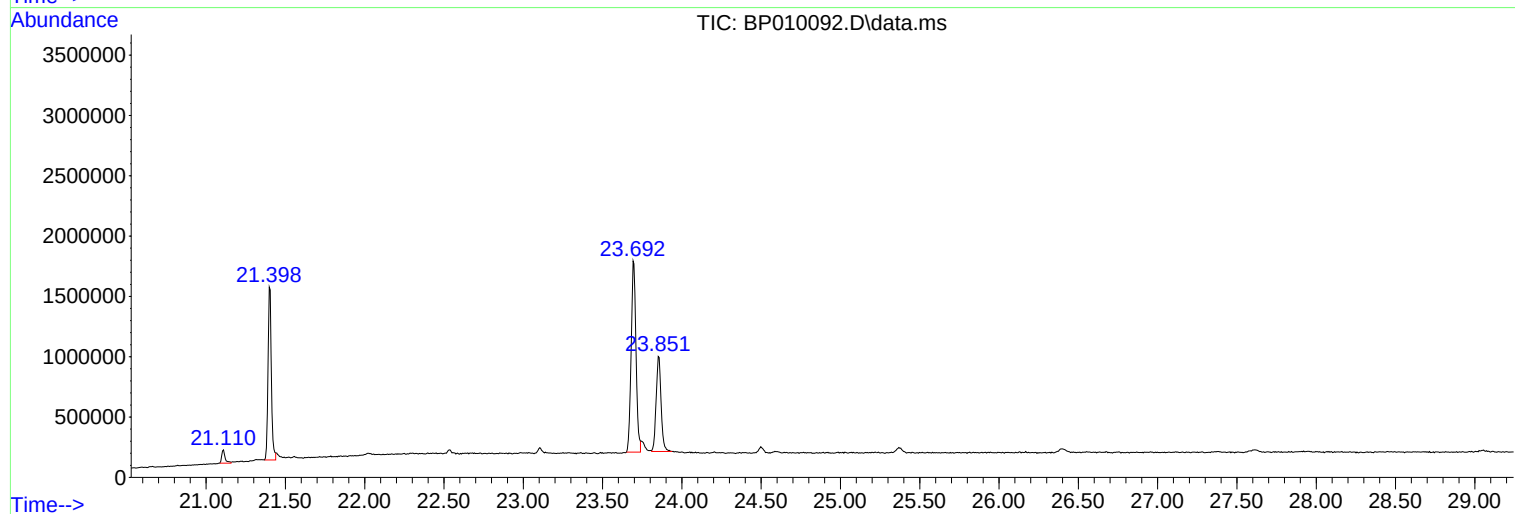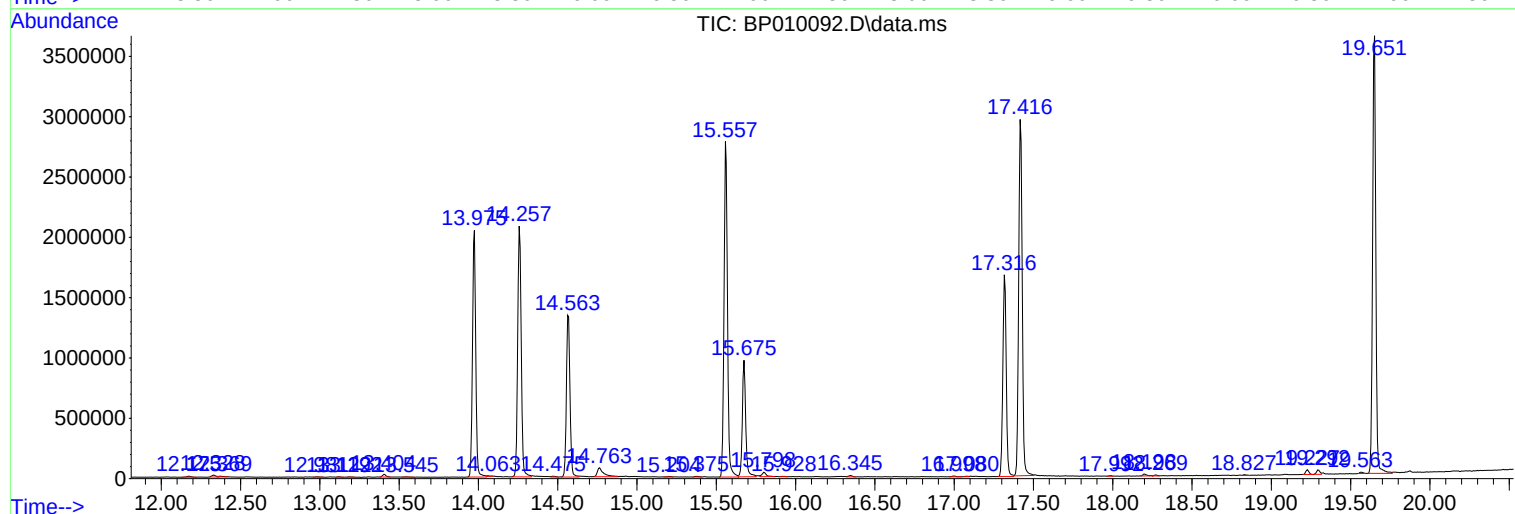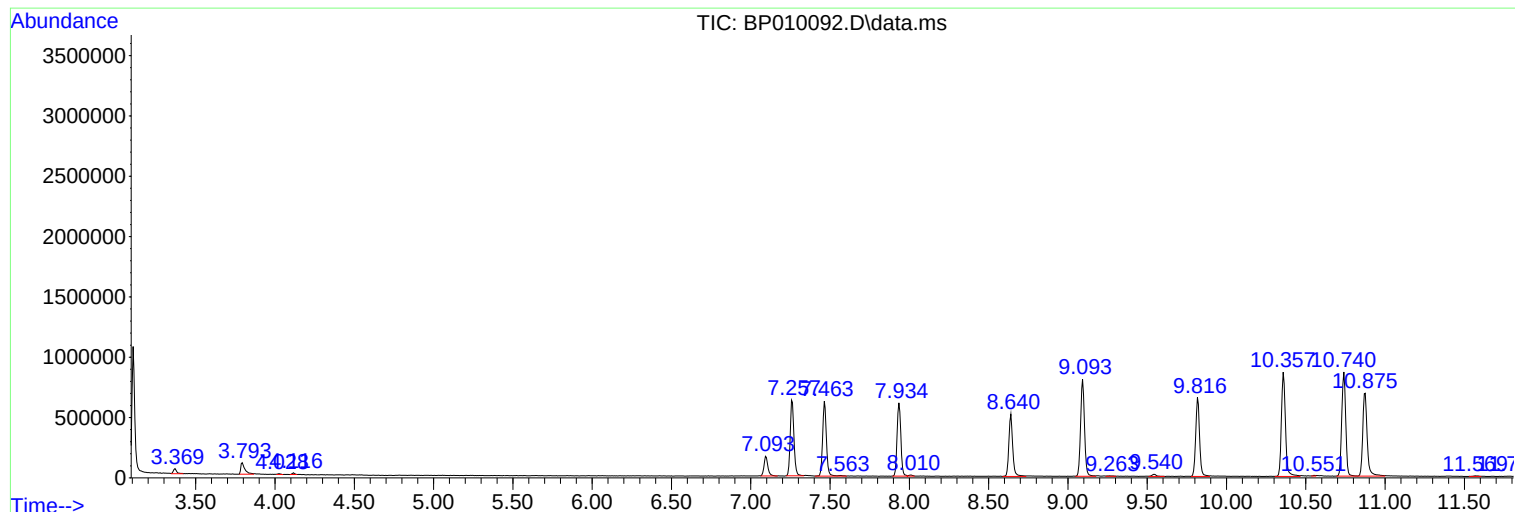

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010092.D
Acq On : 25 Apr 2022 20:28
Operator : CG/JU
Sample : N2475-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010092.D
Acq On : 25 Apr 2022 20:28
Operator : CG/JU
Sample : N2475-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BM8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc