

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010100.D
 Acq On : 26 Apr 2022 00:57
 Operator : CG/JU
 Sample : N2475-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	56	rVB	40019	60990	1.17%	0.138%
2	3.787	116	119	129	rBV	109079	196918	3.79%	0.447%
3	4.017	156	158	164	rVB7	6816	11786	0.23%	0.027%
4	4.117	171	175	181	rVB	26882	39850	0.77%	0.090%
5	7.093	673	681	692	rBV	142626	251509	4.84%	0.570%
6	7.258	702	709	726	rVB	588791	962668	18.52%	2.183%
7	7.463	738	744	757	rBV	571947	925071	17.80%	2.098%
8	7.563	758	761	766	rVB7	4830	7285	0.14%	0.017%
9	7.934	816	824	832	rBV	687358	1109088	21.34%	2.515%
10	8.005	832	836	843	rVB2	14220	26475	0.51%	0.060%
11	8.640	933	944	955	rBV	448207	759254	14.61%	1.722%
12	8.758	960	964	971	rVB3	14519	28087	0.54%	0.064%
13	9.093	1012	1021	1034	rBV	760374	1302751	25.06%	2.954%
14	9.816	1137	1144	1156	rBV	506386	873643	16.81%	1.981%
15	10.357	1228	1236	1253	rBV	762267	1365963	26.28%	3.097%
16	10.740	1293	1301	1311	rBV	968516	1638824	31.53%	3.716%
17	10.869	1316	1323	1337	rBV	765254	1459123	28.07%	3.309%
18	12.081	1527	1529	1536	rVB6	6656	10226	0.20%	0.023%
19	12.328	1562	1571	1582	rVB	16514	32838	0.63%	0.074%
20	12.940	1670	1675	1679	rBV7	2919	5372	0.10%	0.012%
21	12.993	1679	1684	1690	rVB7	5967	10404	0.20%	0.024%
22	13.187	1711	1717	1721	rBV9	3807	6351	0.12%	0.014%
23	13.975	1843	1851	1863	rBV	1844609	2698118	51.90%	6.118%
24	14.257	1890	1899	1922	rBV	1952954	3000800	57.73%	6.804%
25	14.563	1944	1951	1963	rBV	1695502	2579034	49.61%	5.848%
26	14.787	1980	1989	1994	rBV2	60702	145252	2.79%	0.329%
27	15.381	2085	2090	2096	rBV5	7064	13659	0.26%	0.031%
28	15.557	2113	2120	2136	rBV	2517847	3948631	75.96%	8.953%
29	15.681	2136	2141	2154	rVV2	30427	94063	1.81%	0.213%
30	15.798	2156	2161	2167	rVV	34649	59322	1.14%	0.135%
31	15.863	2170	2172	2178	rVV2	6655	9504	0.18%	0.022%
32	16.257	2231	2239	2240	rBV8	4066	7826	0.15%	0.018%
33	16.345	2249	2254	2261	rVB6	10248	19259	0.37%	0.044%
34	16.998	2360	2365	2370	rBV9	6853	11538	0.22%	0.026%
35	17.086	2375	2380	2381	rBV5	3729	6623	0.13%	0.015%
36	17.316	2412	2419	2429	rBV	1842477	2775347	53.39%	6.293%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010100.D
 Acq On : 26 Apr 2022 00:57
 Operator : CG/JU
 Sample : N2475-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	17.416	2430	2436	2449	rVV	3204729	4642213	89.30%	10.526%
38	17.986	2529	2533	2535	rBV6	5071	6560	0.13%	0.015%
39	18.098	2549	2552	2558	rBV8	8212	11809	0.23%	0.027%
40	19.228	2739	2744	2748	rBV2	38722	54173	1.04%	0.123%
41	19.292	2751	2755	2762	rVV	38693	54702	1.05%	0.124%
42	19.645	2809	2815	2832	rBV	3628907	5198195	100.00%	11.787%
43	19.875	2851	2854	2859	rVB3	11797	17422	0.34%	0.040%
44	21.398	3108	3113	3126	rBV	1834859	2520953	48.50%	5.716%
45	23.692	3495	3503	3510	rBV2	1567442	3267452	62.86%	7.409%
46	23.851	3523	3530	3543	rVB	860425	1874997	36.07%	4.252%


Sum of corrected areas: 44101928

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010100.D
Acq On : 26 Apr 2022 00:57
Operator : CG/JU
Sample : N2475-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

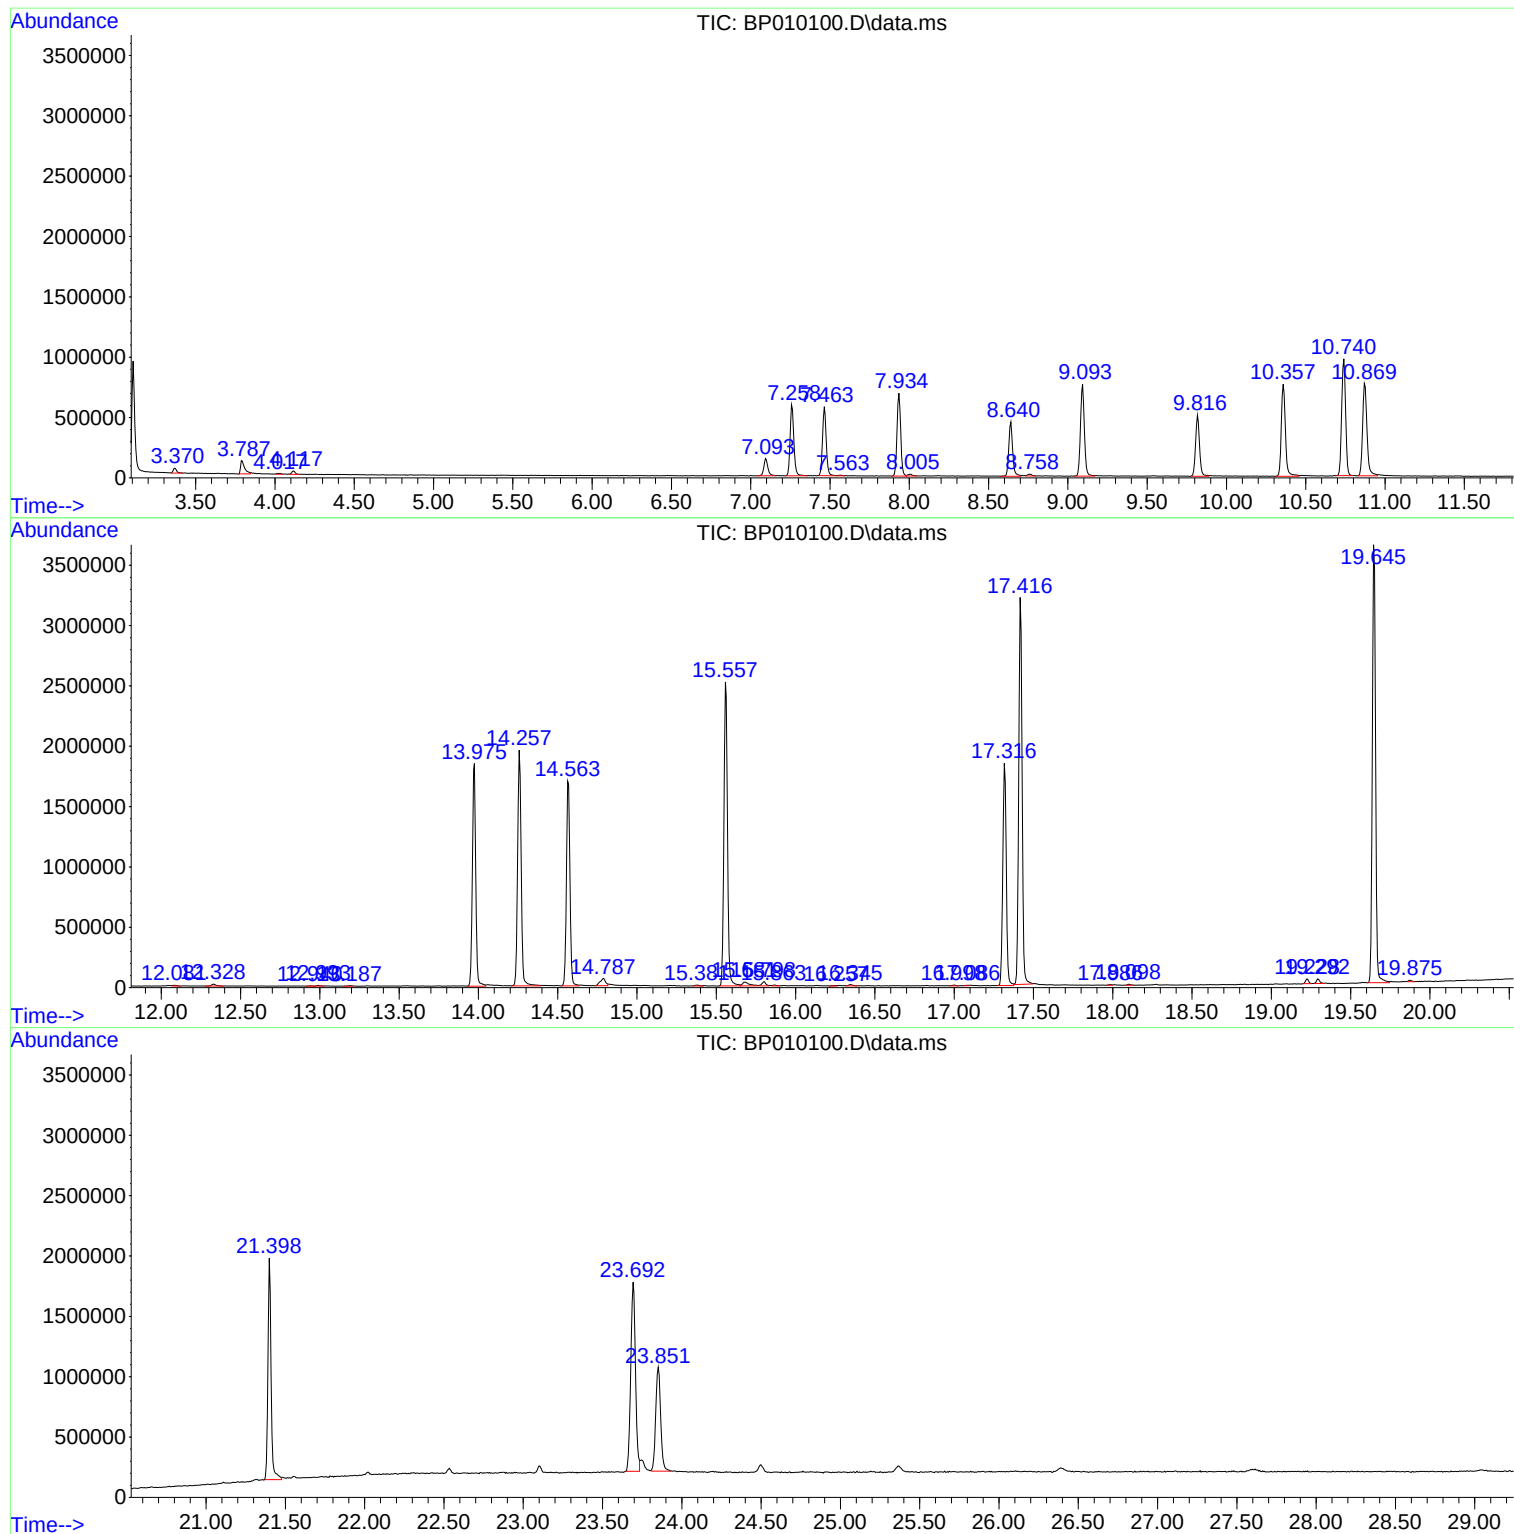

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010100.D
Acq On : 26 Apr 2022 00:57
Operator : CG/JU
Sample : N2475-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010100.D
Acq On : 26 Apr 2022 00:57
Operator : CG/JU
Sample : N2475-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------