

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010102.D
 Acq On : 26 Apr 2022 02:04
 Operator : CG/JU
 Sample : N2475-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	62	rVB	51780	86377	2.03%	0.202%
2	3.787	116	119	134	rBV	168031	266095	6.26%	0.621%
3	4.116	171	175	179	rVB	12920	18631	0.44%	0.043%
4	4.334	210	212	218	rVB5	5710	8011	0.19%	0.019%
5	6.475	571	576	581	rVB8	2283	5216	0.12%	0.012%
6	7.093	674	681	694	rBV	196769	324053	7.62%	0.756%
7	7.257	703	709	722	rBV	641403	1027657	24.18%	2.398%
8	7.463	737	744	757	rBV	651120	1058619	24.91%	2.471%
9	7.934	816	824	835	rBV	685560	1120258	26.36%	2.615%
10	8.287	881	884	891	rVB9	4425	7598	0.18%	0.018%
11	8.357	891	896	899	rBV3	5553	8866	0.21%	0.021%
12	8.640	936	944	960	rBV	539996	924861	21.76%	2.158%
13	9.093	1010	1021	1034	rBV	821640	1396972	32.87%	3.260%
14	9.228	1039	1044	1047	rBV3	9263	17669	0.42%	0.041%
15	9.540	1091	1097	1105	rVB3	11509	19741	0.46%	0.046%
16	9.816	1135	1144	1159	rBV	642984	1125496	26.48%	2.627%
17	10.357	1229	1236	1260	rBV	905700	1593253	37.49%	3.718%
18	10.604	1274	1278	1282	rVB5	6664	9233	0.22%	0.022%
19	10.740	1289	1301	1312	rBV	949989	1623756	38.20%	3.790%
20	10.869	1316	1323	1344	rBV	723505	1387576	32.65%	3.238%
21	11.134	1365	1368	1371	rBV5	3988	5396	0.13%	0.013%
22	11.557	1436	1440	1443	rBV5	3500	4761	0.11%	0.011%
23	12.039	1515	1522	1525	rBV9	3716	7073	0.17%	0.017%
24	12.169	1540	1544	1551	rVB9	3377	8235	0.19%	0.019%
25	12.322	1563	1570	1576	rBV3	18063	34340	0.81%	0.080%
26	12.551	1602	1609	1612	rBV9	3284	7474	0.18%	0.017%
27	12.763	1640	1645	1649	rBV8	3796	7821	0.18%	0.018%
28	12.934	1670	1674	1679	rVB8	3142	5236	0.12%	0.012%
29	13.192	1712	1718	1722	rVB9	6090	11079	0.26%	0.026%
30	13.410	1750	1755	1761	rBV	68105	97501	2.29%	0.228%
31	13.469	1761	1765	1770	rVV4	8447	14588	0.34%	0.034%
32	13.534	1772	1776	1784	rVB9	5973	12030	0.28%	0.028%
33	13.845	1825	1829	1835	rVB9	2520	5305	0.12%	0.012%
34	13.975	1844	1851	1863	rBV	1906979	2751293	64.73%	6.421%
35	14.257	1888	1899	1910	rBV	2064302	3081471	72.50%	7.192%
36	14.569	1942	1952	1964	rBV	1425011	2179105	51.27%	5.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010102.D
 Acq On : 26 Apr 2022 02:04
 Operator : CG/JU
 Sample : N2475-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0BN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.763	1978	1985	1998	rBV2	82485	202547	4.77%	0.473%
38	14.975	2019	2021	2028	rVB8	4931	7422	0.17%	0.017%
39	15.092	2036	2041	2046	rVB10	3957	6533	0.15%	0.015%
40	15.204	2056	2060	2065	rVB7	4439	6832	0.16%	0.016%
41	15.316	2072	2079	2081	rBV8	3656	6418	0.15%	0.015%
42	15.375	2084	2089	2094	rVV6	10446	18193	0.43%	0.042%
43	15.416	2094	2096	2100	rVB5	3762	4548	0.11%	0.011%
44	15.557	2111	2120	2134	rBV	2521676	3940425	92.71%	9.196%
45	15.675	2134	2140	2155	rVV	728527	1069489	25.16%	2.496%
46	15.798	2157	2161	2169	rVB	36615	58504	1.38%	0.137%
47	15.922	2180	2182	2186	rVB4	3648	5061	0.12%	0.012%
48	15.980	2190	2192	2197	rVB6	3752	4273	0.10%	0.010%
49	16.133	2214	2218	2223	rVB8	3476	5208	0.12%	0.012%
50	16.257	2234	2239	2241	rBV6	3611	5321	0.13%	0.012%
51	16.286	2241	2244	2246	rVV4	5437	7573	0.18%	0.018%
52	16.351	2250	2255	2262	rVB2	14125	25499	0.60%	0.060%
53	16.998	2361	2365	2369	rVB6	5773	8637	0.20%	0.020%
54	17.080	2376	2379	2382	rBV5	4472	7185	0.17%	0.017%
55	17.133	2387	2388	2392	rVB4	5883	5715	0.13%	0.013%
56	17.186	2395	2397	2403	rBV7	4110	6431	0.15%	0.015%
57	17.239	2403	2406	2411	rVB7	5231	7305	0.17%	0.017%
58	17.316	2412	2419	2430	rBV	1595681	2372983	55.83%	5.538%
59	17.416	2430	2436	2451	rVV2	2675199	3958027	93.12%	9.237%
60	17.545	2456	2458	2463	rVB5	6648	8871	0.21%	0.021%
61	17.986	2530	2533	2538	rBV7	9366	11480	0.27%	0.027%
62	18.198	2565	2569	2577	rBV2	40843	63523	1.49%	0.148%
63	18.486	2616	2618	2620	rBV3	5547	5275	0.12%	0.012%
64	18.827	2673	2676	2681	rVB2	30318	37702	0.89%	0.088%
65	19.221	2739	2743	2747	rBV2	37183	54340	1.28%	0.127%
66	19.292	2751	2755	2758	rBV	36737	52135	1.23%	0.122%
67	19.427	2776	2778	2781	rVB4	10871	10560	0.25%	0.025%
68	19.563	2799	2801	2806	rVB4	14249	17984	0.42%	0.042%
69	19.645	2809	2815	2830	rBV	3056509	4250338	100.00%	9.920%
70	19.868	2851	2853	2861	rVB5	27126	28888	0.68%	0.067%
71	21.104	3060	3063	3071	rBV2	73787	95253	2.24%	0.222%
72	21.398	3108	3113	3129	rBV	1212802	1761051	41.43%	4.110%
73	23.692	3495	3503	3511	rBV2	1402215	2892729	68.06%	6.751%
74	23.851	3523	3530	3542	rVB2	719318	1554774	36.58%	3.629%

Sum of corrected areas: 42847678




Instrument :
BNA_P
ClientSampleId :
A0BN4

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010102.D
Acq On : 26 Apr 2022 02:04
Operator : CG/JU
Sample : N2475-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

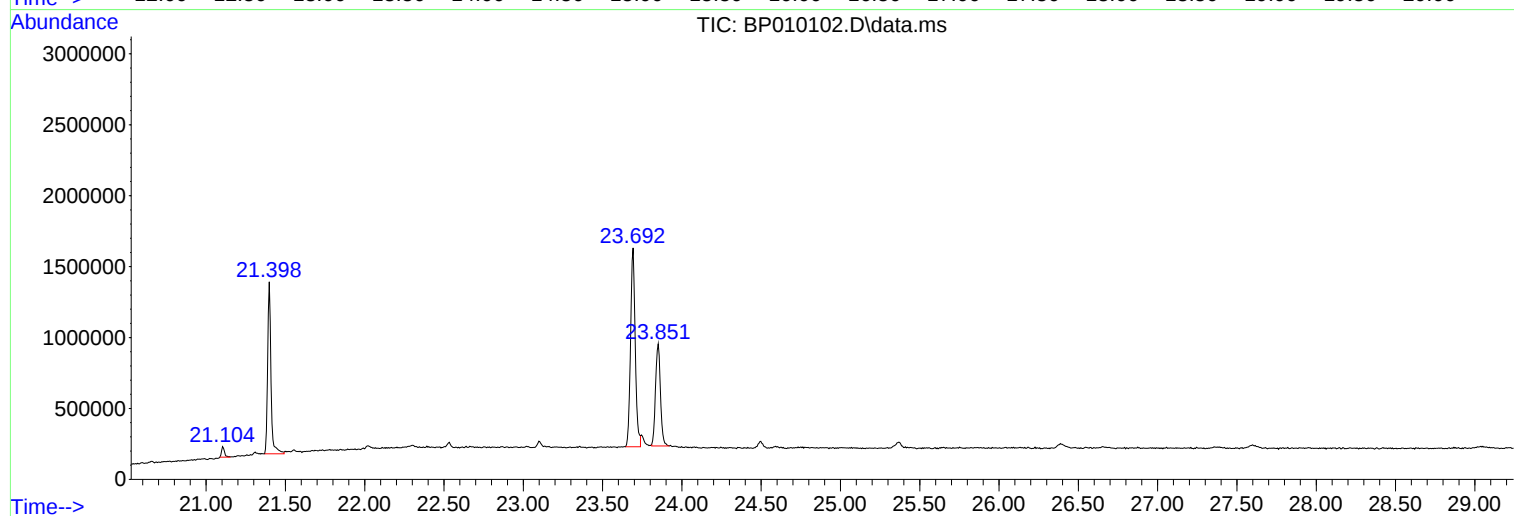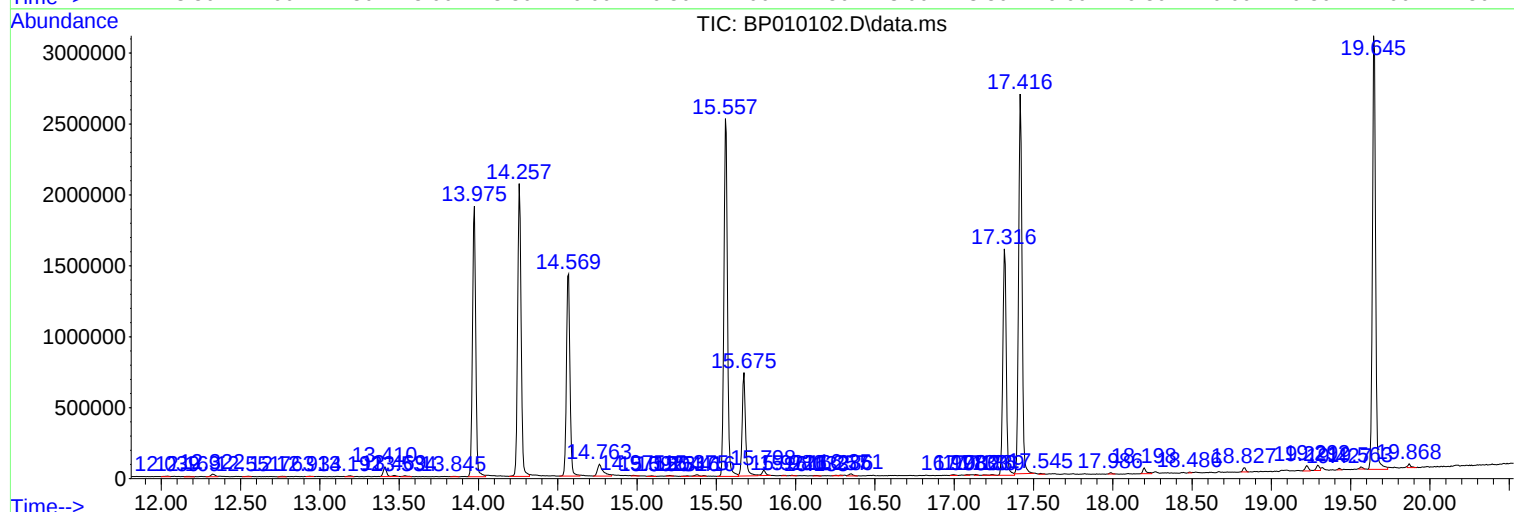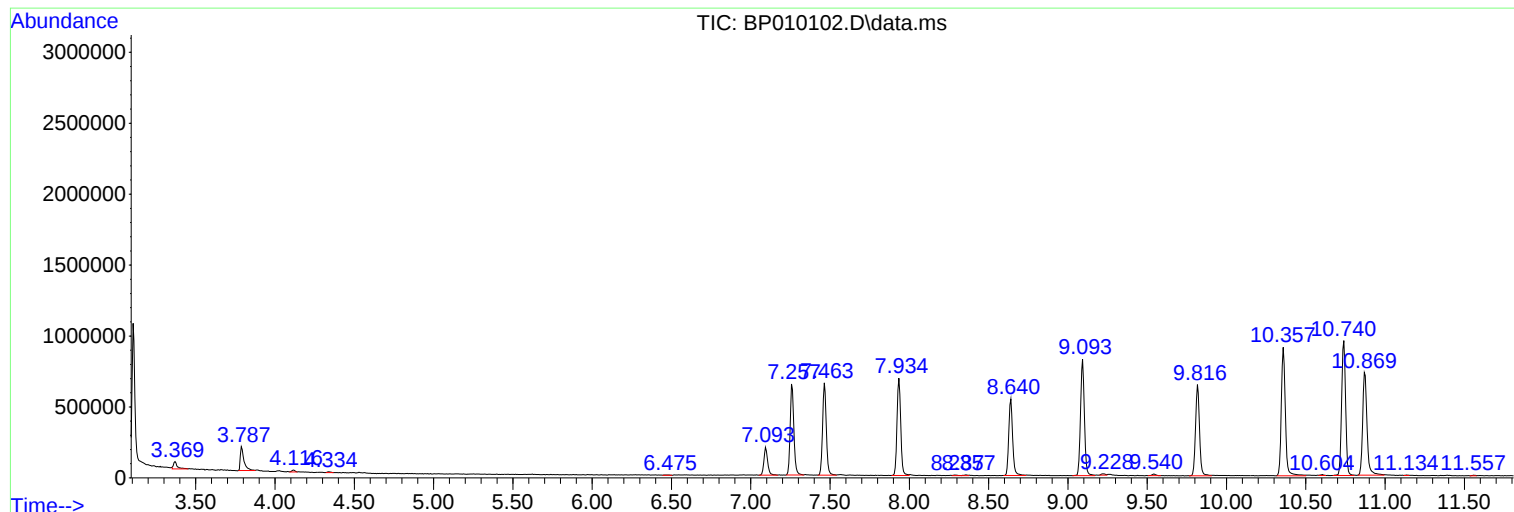

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010102.D
Acq On : 26 Apr 2022 02:04
Operator : CG/JU
Sample : N2475-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010102.D
Acq On : 26 Apr 2022 02:04
Operator : CG/JU
Sample : N2475-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0BN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc