

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010106.D
 Acq On : 26 Apr 2022 09:36
 Operator : CG/JU
 Sample : PB144362BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	60	rVB	56793	79721	1.72%	0.166%
2	3.787	115	119	140	rBV	548360	954756	20.56%	1.992%
3	4.116	172	175	180	rVB2	11896	17054	0.37%	0.036%
4	7.098	675	682	696	rBV	764718	1241343	26.74%	2.590%
5	7.263	704	710	722	rBV	658418	1036314	22.32%	2.162%
6	7.469	738	745	755	rBV	792653	1296695	27.93%	2.705%
7	7.939	818	825	838	rBV	655122	1073945	23.13%	2.241%
8	8.645	934	945	965	rBV	979410	1658312	35.72%	3.460%
9	9.098	1014	1022	1033	rBV	819047	1366522	29.43%	2.851%
10	9.822	1136	1145	1160	rBV	671712	1145673	24.68%	2.390%
11	10.363	1229	1237	1255	rBV	926534	1650217	35.54%	3.443%
12	10.745	1292	1302	1313	rBV	941802	1595171	34.36%	3.328%
13	10.880	1317	1325	1339	rBV	915280	1698926	36.59%	3.545%
14	12.333	1566	1572	1581	rBV2	19440	33363	0.72%	0.070%
15	13.816	1813	1824	1827	rBV2	5904	21607	0.47%	0.045%
16	13.980	1845	1852	1865	rBV	1940904	2700628	58.17%	5.635%
17	14.269	1894	1901	1912	rBV	2089777	3027504	65.21%	6.317%
18	14.574	1946	1953	1966	rVB	1458846	2176353	46.88%	4.541%
19	14.763	1978	1985	2004	rBV	561513	1102678	23.75%	2.301%
20	15.380	2082	2090	2094	rBV9	5782	13198	0.28%	0.028%
21	15.568	2113	2122	2135	rBV	2657514	3894274	83.88%	8.125%
22	15.686	2135	2142	2157	rVV	760673	1164157	25.08%	2.429%
23	15.810	2158	2163	2171	rVB2	31856	54870	1.18%	0.114%
24	15.998	2193	2195	2201	rVB7	6334	9474	0.20%	0.020%
25	16.133	2213	2218	2222	rBV7	3313	5733	0.12%	0.012%
26	16.357	2250	2256	2261	rBV7	10186	19551	0.42%	0.041%
27	16.645	2301	2305	2309	rBV5	7750	10526	0.23%	0.022%
28	16.827	2328	2336	2345	rVB4	14517	26718	0.58%	0.056%
29	17.004	2363	2366	2370	rVB5	5386	7198	0.16%	0.015%
30	17.115	2382	2385	2387	rBV4	4188	5919	0.13%	0.012%
31	17.198	2394	2399	2405	rBV5	9088	16171	0.35%	0.034%
32	17.327	2412	2421	2431	rBV	1733246	2595004	55.89%	5.414%
33	17.427	2431	2438	2453	rVB	2804578	4074821	87.77%	8.502%
34	17.757	2490	2494	2501	rVB10	5257	9345	0.20%	0.019%
35	17.910	2515	2520	2523	rBV	10945	13849	0.30%	0.029%
36	17.945	2523	2526	2533	rVB9	5985	9554	0.21%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
 Data File : BP010106.D
 Acq On : 26 Apr 2022 09:36
 Operator : CG/JU
 Sample : PB144362BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK362

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	18.221	2568	2573	2579	rBV7	7904	15442	0.33%	0.032%
38	18.280	2579	2583	2587	rVV6	10715	16554	0.36%	0.035%
39	18.368	2591	2598	2601	rVV9	3414	6103	0.13%	0.013%
40	18.698	2650	2654	2655	rBV4	6793	8248	0.18%	0.017%
41	18.715	2655	2657	2662	rVB	10371	13223	0.28%	0.028%
42	18.815	2671	2674	2678	rVB5	9867	12200	0.26%	0.025%
43	19.104	2720	2723	2727	rBV6	4453	6554	0.14%	0.014%
44	19.239	2741	2746	2750	rBV5	35847	52878	1.14%	0.110%
45	19.304	2753	2757	2766	rVV	34403	55544	1.20%	0.116%
46	19.586	2802	2805	2808	rVB3	12620	14020	0.30%	0.029%
47	19.662	2811	2818	2837	rBV	3280279	4642677	100.00%	9.687%
48	20.256	2917	2919	2923	rVB2	13239	13855	0.30%	0.029%
49	21.409	3110	3115	3131	rBV	1634632	2434615	52.44%	5.080%
50	21.527	3132	3135	3139	rVB	40874	53077	1.14%	0.111%
51	23.709	3499	3506	3522	rVV2	1394159	3010254	64.84%	6.281%
52	23.868	3526	3533	3549	rVB2	812363	1766574	38.05%	3.686%


Sum of corrected areas: 47928962

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010106.D
Acq On : 26 Apr 2022 09:36
Operator : CG/JU
Sample : PB144362BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

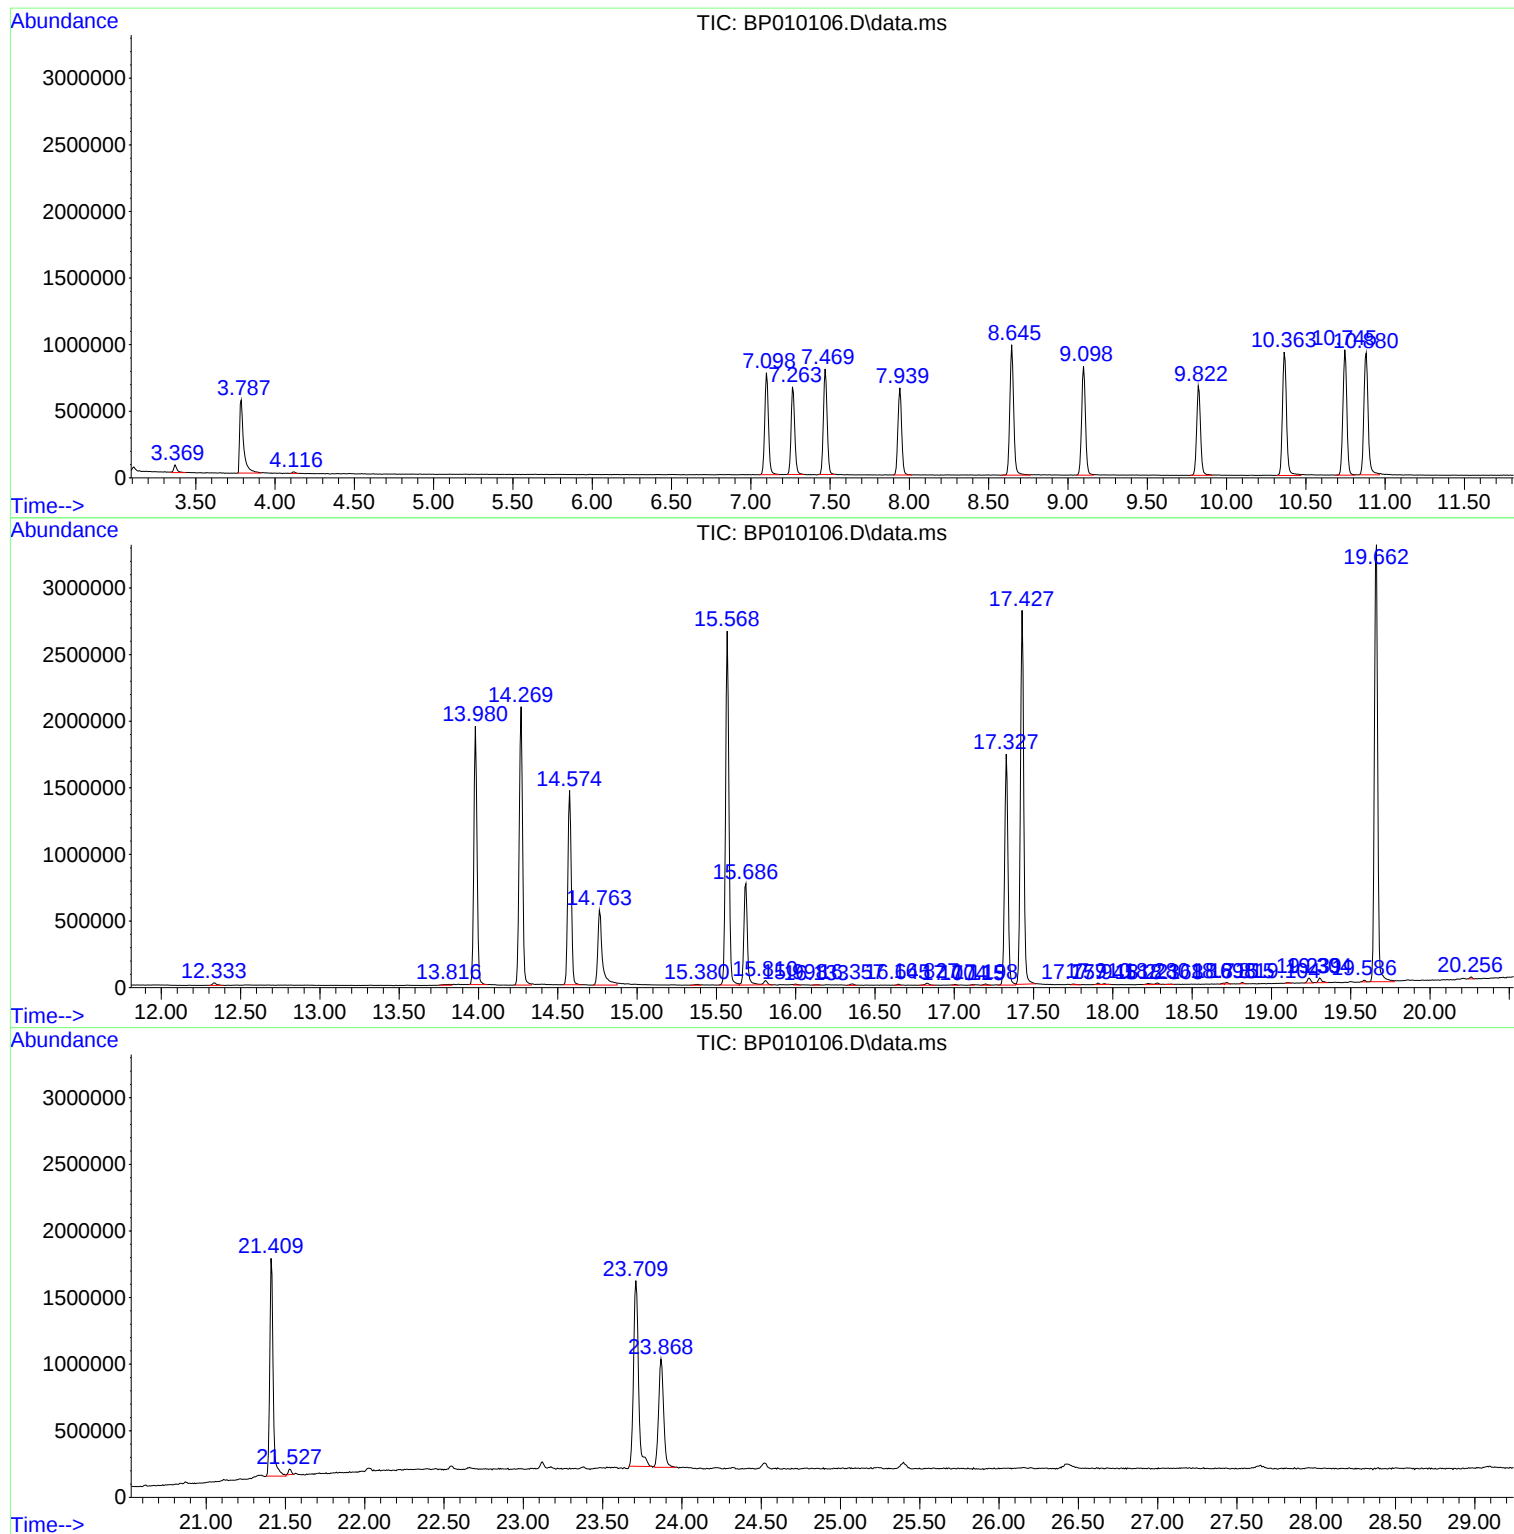

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010106.D
Acq On : 26 Apr 2022 09:36
Operator : CG/JU
Sample : PB144362BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042522\
Data File : BP010106.D
Acq On : 26 Apr 2022 09:36
Operator : CG/JU
Sample : PB144362BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------