

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042523\
 Data File : BP014824.D
 Acq On : 25 Apr 2023 15:06
 Operator : CG/JU
 Sample : SSTD02055
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020641

Quant Time: Apr 26 02:07:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 17:28:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.199	152	285144	20.000	ng/u1	0.00
20) Naphthalene-d8	11.034	136	1299233	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.828	164	846097	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.581	188	1822018	20.000	ng/u1	0.00
79) Chrysene-d12	21.657	240	1623980	20.000	ng/u1	0.00
88) Perylene-d12	24.257	264	1622227	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.505	96	61832	8.526	ng/uL	0.00
4) Pyridine-d5	3.940	84	455100	21.636	ng/u1	0.00
7) Phenol-d5	7.340	99	554670	21.398	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.516	67	345392	22.173	ng/u1	0.00
11) 2-Chlorophenol-d4	7.722	132	416404	21.755	ng/u1	0.00
15) 4-Methylphenol-d8	8.905	113	451739	21.697	ng/u1	0.00
21) Nitrobenzene-d5	9.375	128	208162	21.403	ng/u1	0.00
24) 2-Nitrophenol-d4	10.104	143	216362	21.644	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.640	165	452582	21.782	ng/u1	0.00
31) 4-Chloroaniline-d4	11.163	131	659346	22.114	ng/u1	0.00
46) Dimethylphthalate-d6	14.234	166	1431263	21.800	ng/u1	0.00
49) Acenaphthylene-d8	14.528	160	1653168	21.964	ng/u1	0.00
54) 4-Nitrophenol-d4	15.004	143	255145	21.332	ng/u1	0.00
60) Fluorene-d10	15.822	176	1213621	21.713	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.928	200	204713	20.248	ng/u1	0.00
73) Anthracene-d10	17.681	188	1872688	21.888	ng/u1	0.00
81) Pyrene-d10	19.892	212	2143021	21.705	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.080	264	1819231	21.632	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.540	88	67824	8.666	ng/uL	100
5) Pyridine	3.958	79	469874	21.788	ng/u1	100
6) Benzaldehyde	7.322	77	331644	26.939	ng/u1	100
8) Phenol	7.363	94	584039	21.664	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.611	93	478804	22.157	ng/u1	100
12) 2-Chlorophenol	7.758	128	435540	21.816	ng/u1	100
13) 2-Methylphenol	8.640	108	443137	21.793	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.734	45	600440	22.295	ng/u1	100
16) Acetophenone	9.034	105	765845	23.514	ng/u1	100
17) N-Nitroso-di-n-propyla...	9.016	70	378384	22.701	ng/u1	100
18) 4-Methylphenol	8.969	108	500726	21.997	ng/u1	100
19) Hexachloroethane	9.299	117	173569	21.553	ng/u1	100
22) Nitrobenzene	9.416	77	536246	21.675	ng/u1	100
23) Isophorone	9.946	82	1117419	21.864	ng/u1	100
25) 2-Nitrophenol	10.134	139	245475	21.998	ng/u1	100
26) 2,4-Dimethylphenol	10.187	107	538158	21.733	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.428	93	691907	21.505	ng/u1	100
29) 2,4-Dichlorophenol	10.669	162	452256	21.844	ng/u1	100
30) Naphthalene	11.081	128	1546660	21.522	ng/u1	100
32) 4-Chloroaniline	11.187	127	677939	22.568	ng/u1	100
33) Hexachlorobutadiene	11.369	225	278440	21.145	ng/u1	100
34) Caprolactam	11.951	113	96501	14.114	ng/u1	100
35) 4-Chloro-3-methylphenol	12.293	107	496285	21.647	ng/u1	100
36) 2-Methylnaphthalene	12.675	142	1056916	21.661	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042523\
 Data File : BP014824.D
 Acq On : 25 Apr 2023 15:06
 Operator : CG/JU
 Sample : SSTD02055
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020641


Quant Time: Apr 26 02:07:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 17:28:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.893	142	1058732	21.765	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	13.034	216	569781	21.495	ng/ul	100
40) Hexachlorocyclopentadiene	13.016	237	318268	20.720	ng/ul	100
41) 2,4,6-Trichlorophenol	13.269	196	366204	21.766	ng/ul	100
42) 2,4,5-Trichlorophenol	13.334	196	403306	21.691	ng/ul	100
43) 1,1'-Biphenyl	13.669	154	1458079	21.923	ng/ul	100
44) 2-Chloronaphthalene	13.716	162	1129452	21.692	ng/ul	100
45) 2-Nitroaniline	13.910	65	289334	22.188	ng/ul	100
47) Dimethylphthalate	14.281	163	1422374	21.617	ng/ul	100
48) 2,6-Dinitrotoluene	14.398	165	262755	22.287	ng/ul	100
50) Acenaphthylene	14.557	152	1804309	22.197	ng/ul	100
51) 3-Nitroaniline	14.728	138	286866	22.183	ng/ul	100
52) Acenaphthene	14.892	153	1221292	21.857	ng/ul	100
53) 2,4-Dinitrophenol	14.928	184	126675	18.239	ng/ul	100
55) 4-Nitrophenol	15.022	109	197098	22.024	ng/ul	100
56) Dibenzofuran	15.228	168	1702513	21.636	ng/ul	100
57) 2,4-Dinitrotoluene	15.181	165	381951	21.988	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.445	232	341336	21.770	ng/ul	100
59) Diethylphthalate	15.639	149	1384109	21.722	ng/ul	100
61) Fluorene	15.875	166	1360990	21.926	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.863	204	681073	21.643	ng/ul	100
63) 4-Nitroaniline	15.887	138	277957	23.830	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.945	198	213356	20.996	ng/ul	100
67) N-Nitrosodiphenylamine	16.075	169	1176503	21.956	ng/ul	100
68) 4-Bromophenyl-phenylether	16.763	248	426399	21.628	ng/ul	100
69) Hexachlorobenzene	16.881	284	495566	21.675	ng/ul	100
70) Atrazine	17.028	200	410481	22.414	ng/ul	100
71) Pentachlorophenol	17.222	266	284490	21.211	ng/ul	100
72) Phenanthrene	17.622	178	2186918	21.918	ng/ul	100
74) Anthracene	17.716	178	2223563	22.103	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.640	216	591127	21.794	ng/ul	100
76) Pentachlorobenzene	15.145	250	583599	21.793	ng/ul	100
77) Carbazole	17.975	167	1976231	23.081	ng/ul	100
78) Di-n-butylphthalate	18.510	149	2284568	22.482	ng/ul	100
80) Fluoranthene	19.569	202	2526108	21.710	ng/ul	100
82) Pyrene	19.922	202	2607699	21.669	ng/ul	100
83) Butylbenzylphthalate	20.775	149	894034	22.142	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.557	252	765501	22.589	ng/ul	100
85) Benzo(a)anthracene	21.639	228	2459738	21.772	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.539	149	1350754	22.535	ng/ul	100
87) Chrysene	21.692	228	2311720	21.585	ng/ul	100
89) Di-n-octyl phthalate	22.527	149	2232438	20.700	ng/ul	100
90) Benzo(b)fluoranthene	23.451	252	2342187	21.082	ng/ul	100
91) Benzo(k)fluoranthene	23.504	252	2371061	22.005	ng/ul	100
93) Benzo(a)pyrene	24.139	252	2043043	21.712	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	27.015	276	2329530	21.954	ng/ul	100
95) Dibenzo(a,h)anthracene	27.033	278	1940688	21.930	ng/ul	100
96) Benzo(g,h,i)perylene	27.862	276	1824613	21.704	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 26 02:07:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 25 17:28:12 2023
Response via : Initial Calibration







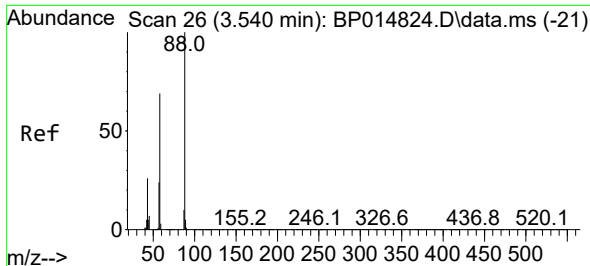

#2
 1,4-Dioxane
 Concen: 8.666 ng/uL
 RT: 3.540 min Scan# 20
 Delta R.T. 0.000 min
 Lab File: BP014824.D
 Acq: 25 Apr 2023 15:06




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020641


Tgt Ion: 88 Resp: 67824
 Ion Ratio Lower Upper
 88 100
 43 26.6 21.3 31.9
 58 69.2 55.4 83.0

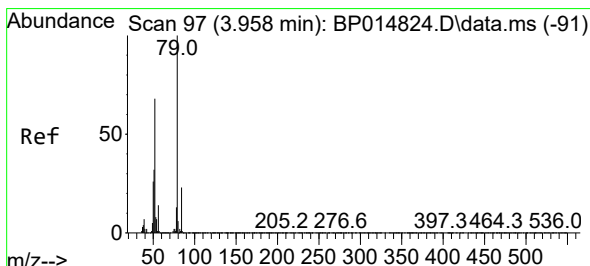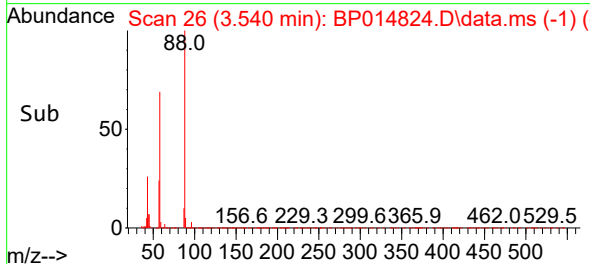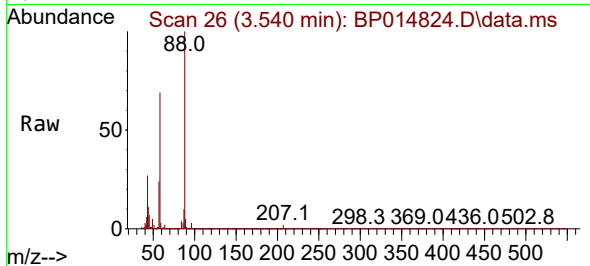

#5
 Pyridine
 Concen: 21.788 ng/uL
 RT: 3.958 min Scan# 97
 Delta R.T. 0.000 min
 Lab File: BP014824.D
 Acq: 25 Apr 2023 15:06

Tgt Ion: 79 Resp: 469874
 Ion Ratio Lower Upper
 79 100
 52 68.4 54.7 82.1
 51 31.9 25.5 38.3


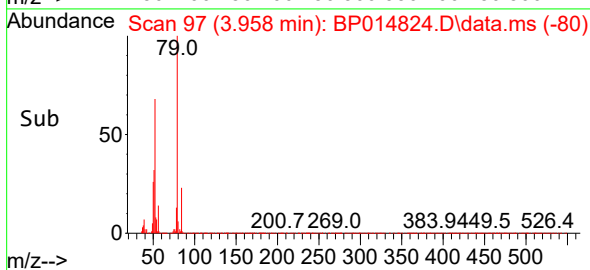

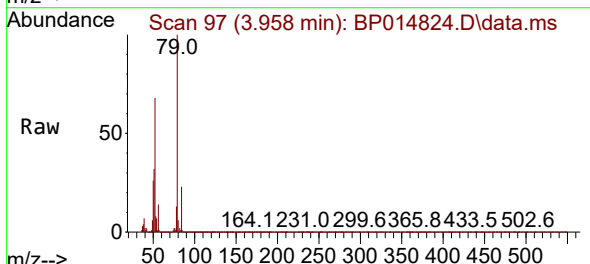




#6
Benzaldehyde
Concen: 26.939 ng/ul
RT: 7.322 min Scan# 609
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion: 77 Resp: 331644
Ion Ratio Lower Upper
77 100
105 99.9 79.9 119.9
106 94.0 75.2 112.8

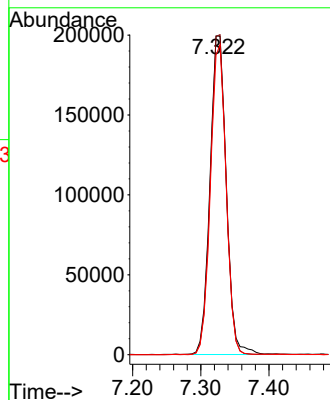

#8
Phenol
Concen: 21.664 ng/ul
RT: 7.363 min Scan# 676
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion: 94 Resp: 584039
Ion Ratio Lower Upper
94 100
65 26.3 21.0 31.6
66 33.8 27.0 40.6



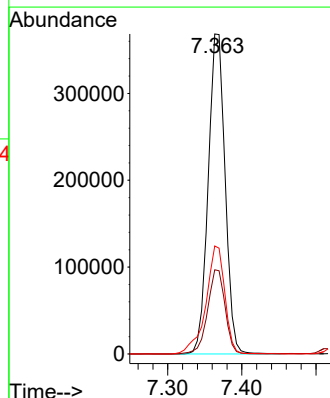





#10
Bis(2-Chloroethyl)ether
Concen: 22.157 ng/ul
RT: 7.611 min Scan# 718
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion: 93 Resp: 478804
Ion Ratio Lower Upper
93 100
63 70.4 56.3 84.5
95 32.4 25.9 38.9



#12
2-Chlorophenol
Concen: 21.816 ng/ul
RT: 7.758 min Scan# 743
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion: 128 Resp: 435540
Ion Ratio Lower Upper
128 100
64 44.5 35.6 53.4
130 31.3 25.0 37.6









#13
2-Methylphenol
Concen: 21.793 ng/ul
RT: 8.640 min Scan# 893
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:108 Resp: 443137
Ion Ratio Lower Upper
108 100
107 88.7 71.0 106.4

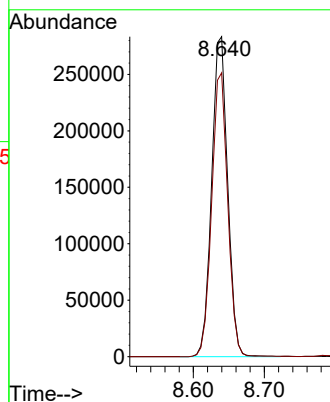

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.295 ng/ul
RT: 8.734 min Scan# 909
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion: 45 Resp: 600440
Ion Ratio Lower Upper
45 100
77 15.6 12.5 18.7
79 11.8 9.4 14.2



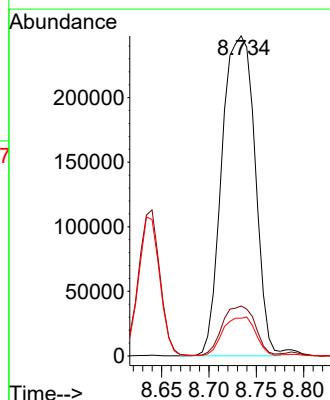





#16
Acetophenone
Concen: 23.514 ng/ul
RT: 9.034 min Scan# 960
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion: 105 Resp: 765845
Ion Ratio Lower Upper
105 100
77 74.8 59.8 89.8
51 24.5 19.6 29.4

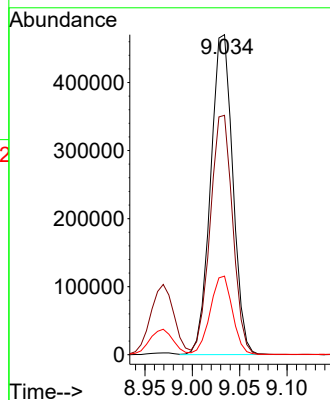

#17
N-Nitroso-di-n-propylamine
Concen: 22.701 ng/ul
RT: 9.016 min Scan# 957
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion: 70 Resp: 378384
Ion Ratio Lower Upper
70 100
42 54.4 43.5 65.3
101 9.9 7.9 11.9
130 20.5 16.4 24.6



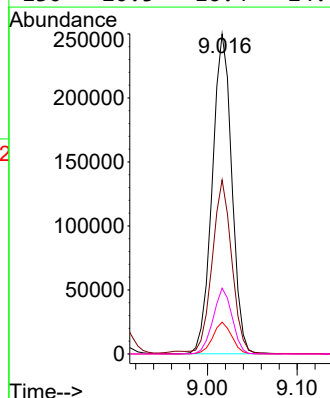





#18
4-Methylphenol
Concen: 21.997 ng/ul
RT: 8.969 min Scan# 949
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:108 Resp: 500726
Ion Ratio Lower Upper
108 100
107 110.7 88.6 132.8



#19
Hexachloroethane
Concen: 21.553 ng/ul
RT: 9.299 min Scan# 1005
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:117 Resp: 173569
Ion Ratio Lower Upper
117 100
201 100.4 80.3 120.5
199 61.3 49.0 73.6









#22
Nitrobenzene
Concen: 21.675 ng/ul
RT: 9.416 min Scan# 1025
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion: 77 Resp: 536246
Ion Ratio Lower Upper
77 100
123 44.7 35.8 53.6
65 12.7 10.2 15.2



#23
Isophorone
Concen: 21.864 ng/ul
RT: 9.946 min Scan# 1115
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion: 82 Resp: 1117419
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.2
138 17.6 14.1 21.1









#25
2-Nitrophenol
Concen: 21.998 ng/ul
RT: 10.134 min Scan# 1147
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:139 Resp: 245475
Ion Ratio Lower Upper
139 100
65 50.9 40.7 61.1
109 29.2 23.4 35.0

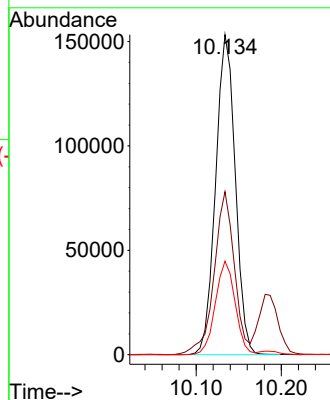

#26
2,4-Dimethylphenol
Concen: 21.733 ng/ul
RT: 10.187 min Scan# 1156
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:107 Resp: 538158
Ion Ratio Lower Upper
107 100
121 51.6 41.3 61.9
122 88.0 70.4 105.6



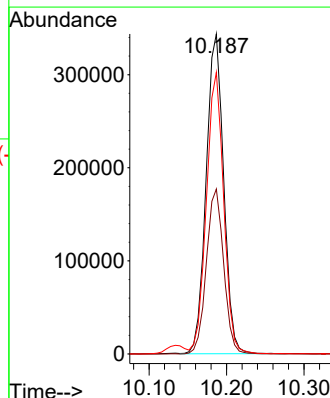





#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.505 ng/ul
 RT: 10.428 min Scan# 1197
 Delta R.T. 0.000 min
 Lab File: BP014824.D
 Acq: 25 Apr 2023 15:06




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020641


Tgt Ion: 93 Resp: 691907
 Ion Ratio Lower Upper
 93 100
 95 31.5 25.2 37.8
 123 10.6 8.5 12.7



#29
 2,4-Dichlorophenol
 Concen: 21.844 ng/ul
 RT: 10.669 min Scan# 1238
 Delta R.T. 0.000 min
 Lab File: BP014824.D
 Acq: 25 Apr 2023 15:06

Tgt Ion: 162 Resp: 452256
 Ion Ratio Lower Upper
 162 100
 164 63.2 50.6 75.8
 98 35.6 28.5 42.7




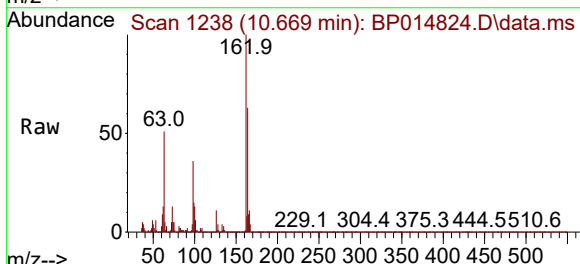




#30
Naphthalene
Concen: 21.522 ng/ul
RT: 11.081 min Scan# 1308
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:128 Resp: 1546660
Ion Ratio Lower Upper
128 100
129 11.4 9.1 13.7
127 13.3 10.6 16.0



#32
4-Chloroaniline
Concen: 22.568 ng/ul
RT: 11.187 min Scan# 1326
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:127 Resp: 677939
Ion Ratio Lower Upper
127 100
129 32.3 25.8 38.8









#33
Hexachlorobutadiene
Concen: 21.145 ng/ul
RT: 11.369 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:225 Resp: 278440
Ion Ratio Lower Upper
225 100
223 62.4 49.9 74.9
227 64.4 51.5 77.3



#34
Caprolactam
Concen: 14.114 ng/ul
RT: 11.951 min Scan# 1456
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:113 Resp: 96501
Ion Ratio Lower Upper
113 100
55 161.3 129.0 193.6
56 124.3 99.4 149.2









#35
4-Chloro-3-methylphenol
Concen: 21.647 ng/ul
RT: 12.293 min Scan# 1514
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:107 Resp: 496285
Ion Ratio Lower Upper
107 100
144 26.7 21.4 32.0
142 81.3 65.0 97.6



#36
2-Methylnaphthalene
Concen: 21.661 ng/ul
RT: 12.675 min Scan# 1579
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:142 Resp: 1056916
Ion Ratio Lower Upper
142 100
141 88.3 70.6 106.0





#37

1-Methylnaphthalene

Concen: 21.765 ng/ul

RT: 12.893 min Scan# 1616

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:142 Resp: 1058732

Ion Ratio Lower Upper

142 100

141 92.1 73.7 110.5

116 3.7 3.0 4.4



#39

1,2,4,5-Tetrachlorobenzene

Concen: 21.495 ng/ul

RT: 13.034 min Scan# 1640

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Tgt Ion:216 Resp: 569781




Ion Ratio Lower Upper


216 100

214 79.1 63.3 94.9

179 20.9 16.7 25.1

108 18.1 14.5 21.7




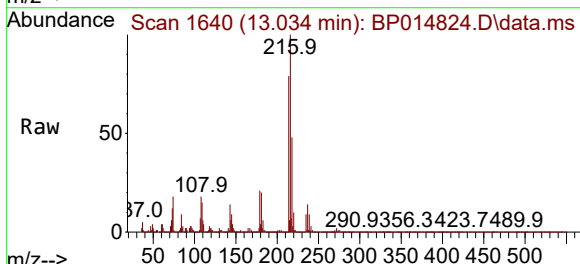




#40
Hexachlorocyclopentadiene
Concen: 20.720 ng/ul
RT: 13.016 min Scan# 1637
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:237 Resp: 318268
Ion Ratio Lower Upper
237 100
235 62.5 50.0 75.0
272 12.6 10.1 15.1



#41
2,4,6-Trichlorophenol
Concen: 21.766 ng/ul
RT: 13.269 min Scan# 1680
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:196 Resp: 366204
Ion Ratio Lower Upper
196 100
198 95.9 76.7 115.1
200 31.6 25.3 37.9





#42

2,4,5-Trichlorophenol

Concen: 21.691 ng/ul

RT: 13.334 min Scan# 1691

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:196 Resp: 403306

Ion Ratio Lower Upper

196 100

198 94.1 75.3 112.9

200 30.3 24.2 36.4

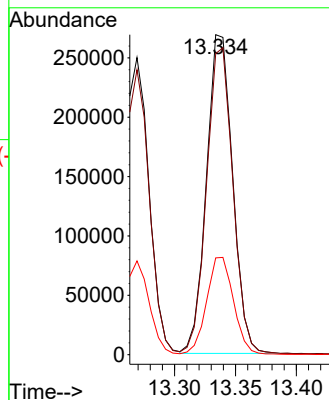

#43

1,1'-Biphenyl

Concen: 21.923 ng/ul

RT: 13.669 min Scan# 1748

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:154 Resp: 1458079


Ion Ratio Lower Upper

154 100

153 39.9 31.9 47.9

76 14.0 11.2 16.8



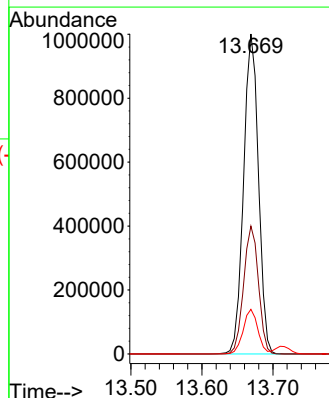





#44
2-Chloronaphthalene
Concen: 21.692 ng/ul
RT: 13.716 min Scan# 1756
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:162 Resp: 1129452
Ion Ratio Lower Upper
162 100
164 32.7 26.2 39.2
127 37.1 29.7 44.5



#45
2-Nitroaniline
Concen: 22.188 ng/ul
RT: 13.910 min Scan# 1789
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion: 65 Resp: 289334
Ion Ratio Lower Upper
65 100
92 73.1 58.5 87.7
138 109.5 87.6 131.4





#47

Dimethylphthalate

Concen: 21.617 ng/ul

RT: 14.281 min Scan# 1852

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:163 Resp: 1422374

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.0 8.0 12.0



#48

2,6-Dinitrotoluene

Concen: 22.287 ng/ul

RT: 14.398 min Scan# 1872

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:165 Resp: 262755


Ion Ratio Lower Upper

165 100

89 59.5 47.6 71.4

121 21.9 17.5 26.3



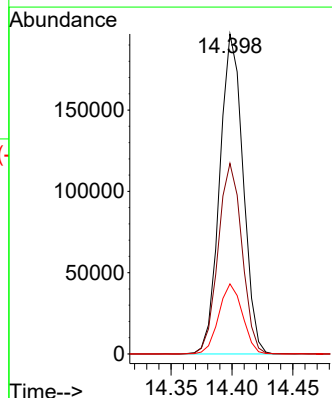
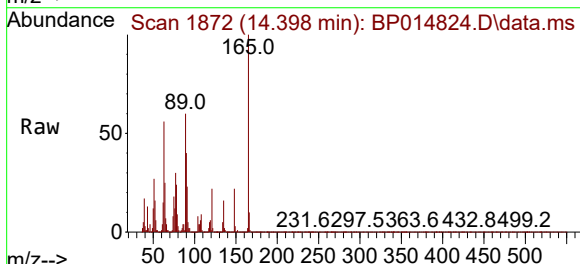




#50
Acenaphthylene
Concen: 22.197 ng/ul
RT: 14.557 min Scan# 1899
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:152 Resp: 1804309
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.6
153 13.0 10.4 15.6

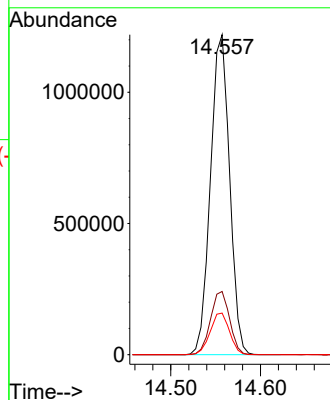

#51
3-Nitroaniline
Concen: 22.183 ng/ul
RT: 14.728 min Scan# 1928
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:138 Resp: 286866
Ion Ratio Lower Upper
138 100
108 10.5 8.4 12.6
92 116.5 93.2 139.8



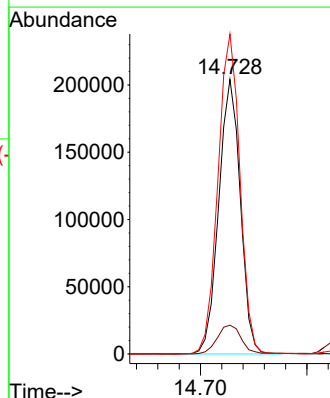
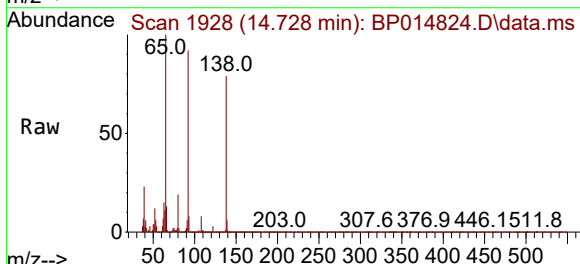




#52
Acenaphthene
Concen: 21.857 ng/ul
RT: 14.892 min Scan# 1956
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:153 Resp: 1221292
Ion Ratio Lower Upper
153 100
152 47.8 38.2 57.4
154 88.7 71.0 106.4

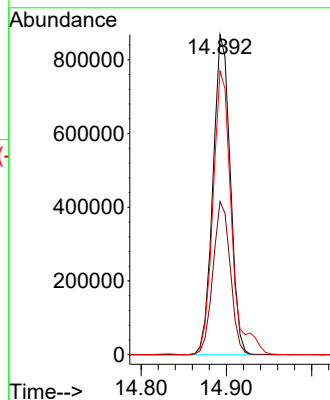

#53
2,4-Dinitrophenol
Concen: 18.239 ng/ul
RT: 14.928 min Scan# 1962
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:184 Resp: 126675
Ion Ratio Lower Upper
184 100
63 67.0 53.6 80.4
154 61.4 49.1 73.7



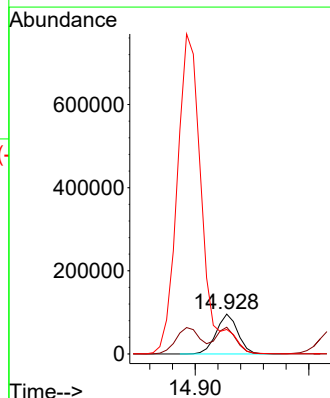
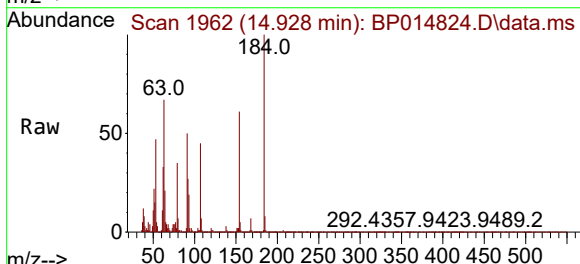




#55
4-Nitrophenol
Concen: 22.024 ng/ul
RT: 15.022 min Scan# 1978
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:109 Resp: 197098
Ion Ratio Lower Upper
109 100
139 141.0 112.8 169.2
65 129.5 103.6 155.4

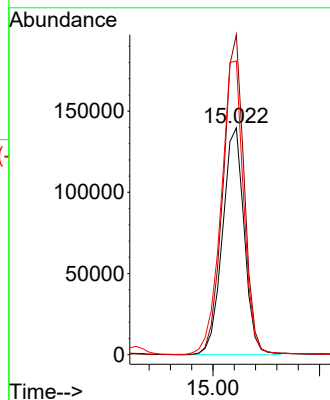

#56
Dibenzofuran
Concen: 21.636 ng/ul
RT: 15.228 min Scan# 2013
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:168 Resp: 1702513
Ion Ratio Lower Upper
168 100
139 35.9 28.7 43.1



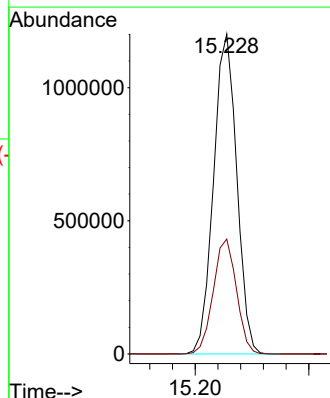
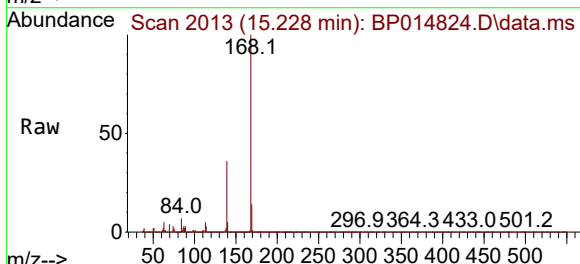




#57
2,4-Dinitrotoluene
Concen: 21.988 ng/ul
RT: 15.181 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:165 Resp: 381951
Ion Ratio Lower Upper
165 100
63 42.2 33.8 50.6
182 2.8 2.2 3.4



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.770 ng/ul
RT: 15.445 min Scan# 2050
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:232 Resp: 341336
Ion Ratio Lower Upper
232 100
131 43.7 35.0 52.4
130 2.2 1.8 2.6
166 31.3 25.0 37.6


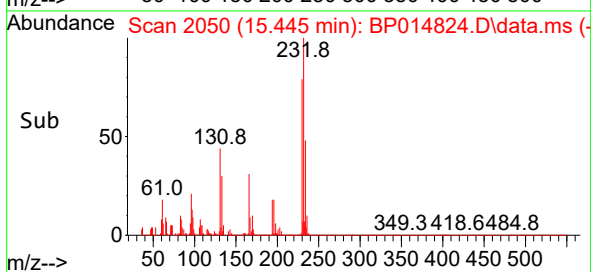






#59
Diethylphthalate
Concen: 21.722 ng/ul
RT: 15.639 min Scan# 2083
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:149 Resp: 1384109
Ion Ratio Lower Upper
149 100
177 22.4 17.9 26.9
150 12.2 9.8 14.6



#61
Fluorene
Concen: 21.926 ng/ul
RT: 15.875 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:166 Resp: 1360990
Ion Ratio Lower Upper
166 100
165 98.9 79.1 118.7
167 13.4 10.7 16.1




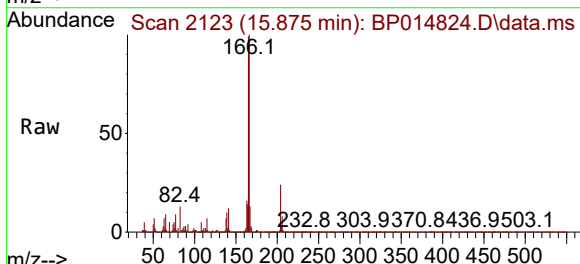




#62
4-Chlorophenyl-phenylether
Concen: 21.643 ng/ul
RT: 15.863 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:204 Resp: 681073
Ion Ratio Lower Upper
204 100
206 32.9 26.3 39.5
141 57.4 45.9 68.9

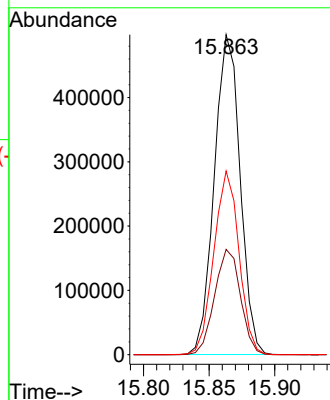

#63
4-Nitroaniline
Concen: 23.830 ng/ul
RT: 15.887 min Scan# 2125
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:138 Resp: 277957
Ion Ratio Lower Upper
138 100
92 48.8 39.0 58.6
108 74.0 59.2 88.8



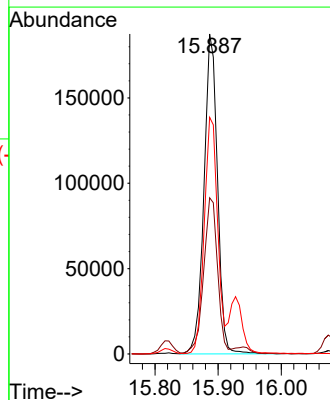
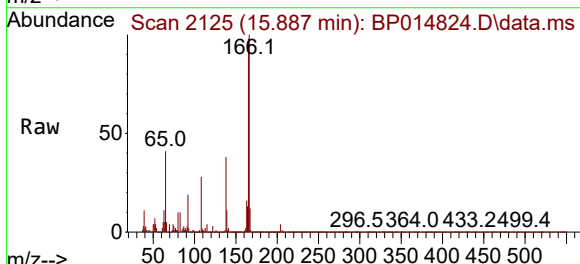




#66
4,6-Dinitro-2-methylphenol
Concen: 20.996 ng/ul
RT: 15.945 min Scan# 2135
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:198 Resp: 213356
Ion Ratio Lower Upper
198 100
182 4.4 3.5 5.3
77 23.4 18.7 28.1



#67
N-Nitrosodiphenylamine
Concen: 21.956 ng/ul
RT: 16.075 min Scan# 2157
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:169 Resp: 1176503
Ion Ratio Lower Upper
169 100
168 67.0 53.6 80.4
167 36.7 29.4 44.0









#68
4-Bromophenyl-phenylether
Concen: 21.628 ng/ul
RT: 16.763 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:248 Resp: 426399
Ion Ratio Lower Upper
248 100
250 98.9 79.1 118.7
141 67.2 53.8 80.6



#69
Hexachlorobenzene
Concen: 21.675 ng/ul
RT: 16.881 min Scan# 2294
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:284 Resp: 495566
Ion Ratio Lower Upper
284 100
142 33.1 26.5 39.7
249 30.5 24.4 36.6

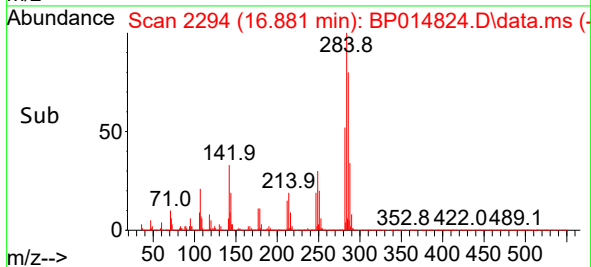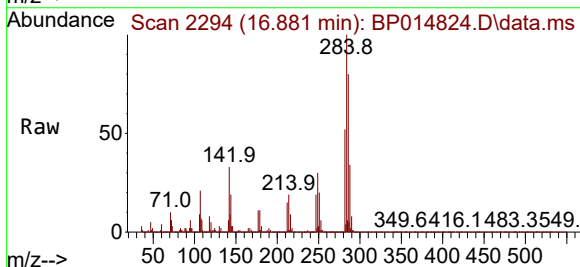



#70

Atrazine

Concen: 22.414 ng/ul

RT: 17.028 min Scan# 2319

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:200 Resp: 410481

Ion Ratio Lower Upper

200 100

173 26.9 21.5 32.3

215 48.0 38.4 57.6



#71

Pentachlorophenol

Concen: 21.211 ng/ul

RT: 17.222 min Scan# 2352

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:266 Resp: 284490


Ion Ratio Lower Upper

266 100

264 61.2 49.0 73.4

268 64.3 51.4 77.2

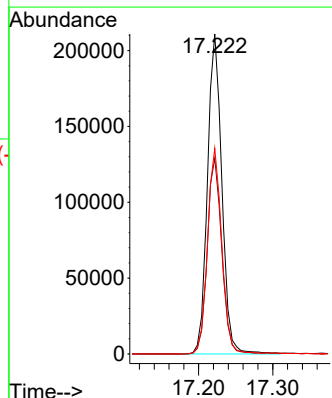



#72

Phenanthrene

Concen: 21.918 ng/ul

RT: 17.622 min Scan# 2420

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:178 Resp: 2186918

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.4

176 19.6 15.7 23.5



#74

Anthracene

Concen: 22.103 ng/ul

RT: 17.716 min Scan# 2436

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:178 Resp: 2223563


Ion Ratio Lower Upper

178 100

179 15.1 12.1 18.1

176 18.6 14.9 22.3









#75
1,2,3,4-Tetrachlorobenzene
Concen: 21.794 ng/uL
RT: 13.640 min Scan# 1743
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:216 Resp: 591127
Ion Ratio Lower Upper
216 100
214 78.6 62.9 94.3
218 49.4 39.5 59.3



#76
Pentachlorobenzene
Concen: 21.793 ng/uL
RT: 15.145 min Scan# 1999
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:250 Resp: 583599
Ion Ratio Lower Upper
250 100
248 63.0 50.4 75.6
252 62.9 50.3 75.5





#77

Carbazole

Concen: 23.081 ng/ul

RT: 17.975 min Scan# 2480

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:167 Resp: 1976231

Ion Ratio Lower Upper

167 100

166 21.5 17.2 25.8

139 12.3 9.8 14.8



#78

Di-n-butylphthalate

Concen: 22.482 ng/ul

RT: 18.510 min Scan# 2571

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:149 Resp: 2284568


Ion Ratio Lower Upper

149 100

150 9.3 7.4 11.2

104 4.9 3.9 5.9

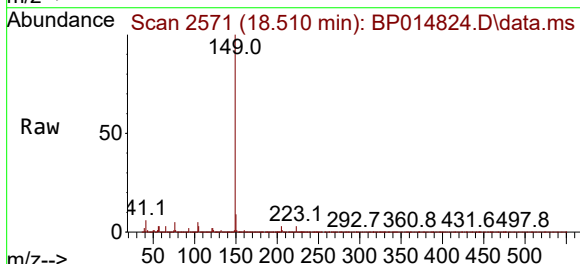



#80

Fluoranthene

Concen: 21.710 ng/ul

RT: 19.569 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:202 Resp: 2526108

Ion Ratio Lower Upper

202 100

101 11.4 9.1 13.7

100 8.7 7.0 10.4



#82

Pyrene

Concen: 21.669 ng/ul

RT: 19.922 min Scan# 2811

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:202 Resp: 2607699


Ion Ratio Lower Upper

202 100

101 13.9 11.1 16.7

100 11.3 9.0 13.6





#83

Butylbenzylphthalate

Concen: 22.142 ng/ul

RT: 20.775 min Scan# 2956

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNP_P

ClientSampleId :

SSTD020641





Tgt Ion:149 Resp: 894034

Ion Ratio Lower Upper

149 100

91 73.1 58.5 87.7

206 20.9 16.7 25.1



#84

3,3'-Dichlorobenzidine

Concen: 22.589 ng/ul

RT: 21.557 min Scan# 3089

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:252 Resp: 765501


Ion Ratio Lower Upper

252 100

254 64.2 51.4 77.0

126 11.5 9.2 13.8





#85

Benzo(a)anthracene

Concen: 21.772 ng/ul

RT: 21.639 min Scan# 3103

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:228 Resp: 2459738

Ion Ratio Lower Upper

228 100

229 19.6 15.7 23.5

226 27.5 22.0 33.0



#86

Bis(2-ethylhexyl)phthalate

Concen: 22.535 ng/ul

RT: 21.539 min Scan# 3086

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:149 Resp: 1350754


Ion Ratio Lower Upper

149 100

167 27.2 21.8 32.6

279 4.2 3.4 5.0





#87

Chrysene

Concen: 21.585 ng/ul

RT: 21.692 min Scan# 3112

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:228 Resp: 2311720

Ion Ratio Lower Upper

228 100

226 30.6 24.5 36.7

229 20.0 16.0 24.0



#89

Di-n-octyl phthalate

Concen: 20.700 ng/ul




RT: 22.527 min Scan# 3254


Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Tgt Ion:149 Resp: 2232438





#90

Benzo(b)fluoranthene

Concen: 21.082 ng/ul

RT: 23.451 min Scan# 3411

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06

Instrument :

BNA_P

ClientSampleId :

SSTD020641





Tgt Ion:252 Resp: 2342187

Ion Ratio Lower Upper

252 100

253 21.5 17.2 25.8

125 9.8 7.8 11.8



#91

Benzo(k)fluoranthene

Concen: 22.005 ng/ul

RT: 23.504 min Scan# 3420

Delta R.T. 0.000 min

Lab File: BP014824.D

Acq: 25 Apr 2023 15:06




Tgt Ion:252 Resp: 2371061


Ion Ratio Lower Upper

252 100

253 21.9 17.5 26.3

125 9.9 7.9 11.9









#93
Benzo(a)pyrene
Concen: 21.712 ng/ul
RT: 24.139 min Scan# 3528
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06




Instrument :
BNA_P
ClientSampleId :
SSTD020641


Tgt Ion:252 Resp: 2043043
Ion Ratio Lower Upper
252 100
253 21.9 17.5 26.3
125 10.7 8.6 12.8



#94
Indeno(1,2,3-cd)pyrene
Concen: 21.954 ng/ul
RT: 27.015 min Scan# 4017
Delta R.T. 0.000 min
Lab File: BP014824.D
Acq: 25 Apr 2023 15:06

Tgt Ion:276 Resp: 2329530
Ion Ratio Lower Upper
276 100
138 22.1 17.7 26.5
277 24.5 19.6 29.4






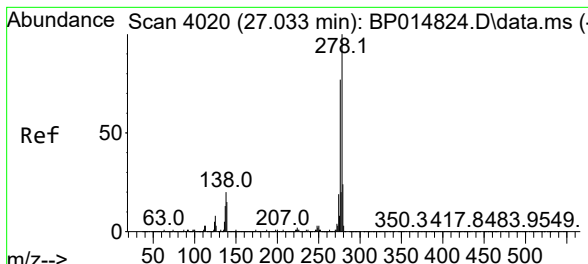


#95
 Dibenzo(a,h)anthracene
 Concen: 21.930 ng/ul
 RT: 27.033 min Scan# 4020
 Delta R.T. 0.000 min
 Lab File: BP014824.D
 Acq: 25 Apr 2023 15:06

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020641

Tgt Ion: 278 Resp: 1940688

Ion	Ratio	Lower	Upper
278	100		
139	15.0	12.0	18.0
279	23.6	18.9	28.3

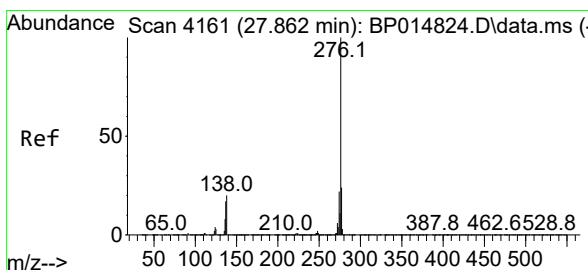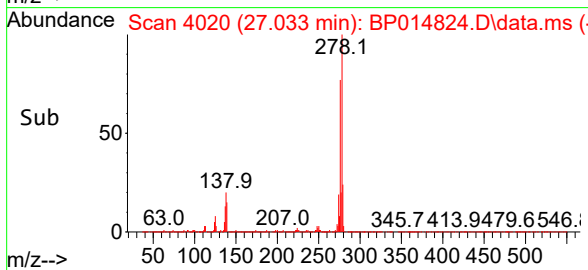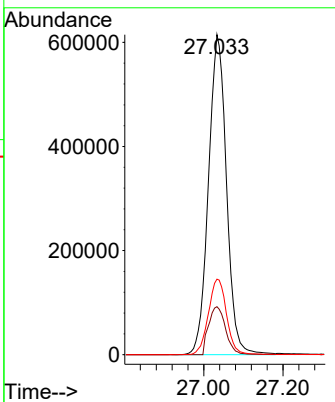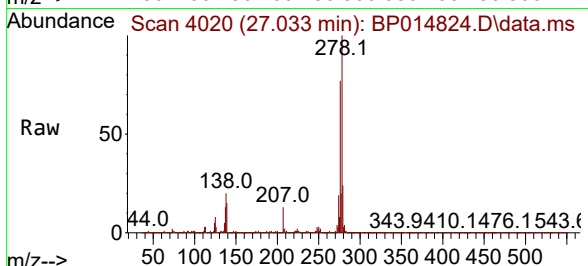

#96
 Benzo(g,h,i)perylene
 Concen: 21.704 ng/ul
 RT: 27.862 min Scan# 4161
 Delta R.T. 0.000 min
 Lab File: BP014824.D
 Acq: 25 Apr 2023 15:06

Tgt Ion: 276 Resp: 1824613

Ion	Ratio	Lower	Upper
276	100		
138	20.2	16.2	24.2
277	23.6	18.9	28.3

