

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042723\
 Data File : BP014867.D
 Acq On : 27 Apr 2023 11:27
 Operator : CG/JU
 Sample : PB152374BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.499	15	19	30	rVB	68624	105001	1.65%	0.152%
2	3.940	90	94	113	rBV	934977	1517080	23.89%	2.190%
3	4.293	149	154	161	rVB2	16520	25249	0.40%	0.036%
4	7.340	665	672	681	rBV	1206674	1903753	29.98%	2.748%
5	7.517	695	702	711	rVB	1049243	1580227	24.88%	2.281%
6	7.722	730	737	746	rBV	1206886	1931784	30.42%	2.788%
7	8.205	811	819	828	rVB	963459	1543097	24.30%	2.227%
8	8.905	930	938	951	rBV	1576774	2481823	39.08%	3.582%
9	9.375	1008	1018	1028	rBV	1184606	1924287	30.30%	2.778%
10	10.105	1131	1142	1151	rBV	960523	1592817	25.08%	2.299%
11	10.646	1226	1234	1245	rBV	1568774	2592357	40.82%	3.742%
12	11.040	1293	1301	1308	rVB	1410341	2391166	37.65%	3.452%
13	11.169	1315	1323	1336	rBV	1614261	2668825	42.02%	3.852%
14	12.610	1561	1568	1574	rBV	32501	53803	0.85%	0.078%
15	13.628	1735	1741	1747	rBV8	5009	11049	0.17%	0.016%
16	13.722	1752	1757	1762	rVV4	9616	16377	0.26%	0.024%
17	13.816	1765	1773	1779	rVB5	4681	10064	0.16%	0.015%
18	14.234	1836	1844	1857	rBV	2753279	3695975	58.20%	5.335%
19	14.534	1887	1895	1906	rBV	3294642	4848730	76.35%	6.999%
20	14.840	1939	1947	1954	rBV	2184598	3283505	51.70%	4.740%
21	14.904	1954	1958	1964	rVB9	3794	7501	0.12%	0.011%
22	15.010	1968	1976	1993	rBV	1192765	1793797	28.25%	2.589%
23	15.240	2011	2015	2018	rVB5	8071	10803	0.17%	0.016%
24	15.828	2107	2115	2122	rBV	4016808	5762225	90.73%	8.318%
25	15.934	2127	2133	2145	rVV	770479	1024238	16.13%	1.478%
26	16.069	2151	2156	2160	rVB	16393	24056	0.38%	0.035%
27	16.610	2241	2248	2250	rBV8	5379	8750	0.14%	0.013%
28	17.263	2355	2359	2364	rBV7	7070	10213	0.16%	0.015%
29	17.587	2407	2414	2424	rBV	2720786	3759091	59.19%	5.426%
30	17.687	2424	2431	2443	rVV	4413468	6060264	95.43%	8.748%
31	17.816	2448	2453	2458	rBV2	28144	44487	0.70%	0.064%
32	17.951	2473	2476	2481	rBV3	4892	7771	0.12%	0.011%
33	18.434	2556	2558	2563	rVB6	6112	6756	0.11%	0.010%
34	19.475	2731	2735	2740	rBV	57257	71278	1.12%	0.103%
35	19.539	2742	2746	2750	rBV	52665	73913	1.16%	0.107%
36	19.898	2801	2807	2816	rBV	4761215	6350626	100.00%	9.167%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042723\
Data File : BP014867.D
Acq On : 27 Apr 2023 11:27
Operator : CG/JU
Sample : PB152374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK374

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Title : SVOA CALIBRATION

37	21.657	3101	3106	3116	rBV2	2159339	2871127	45.21%	4.144%
38	24.092	3513	3520	3534	rVB2	2099867	4594207	72.34%	6.632%
39	24.269	3543	3550	3561	rVB2	1183491	2619105	41.24%	3.781%




Sum of corrected areas: 69277177

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042723\
Data File : BP014867.D
Acq On : 27 Apr 2023 11:27
Operator : CG/JU
Sample : PB152374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

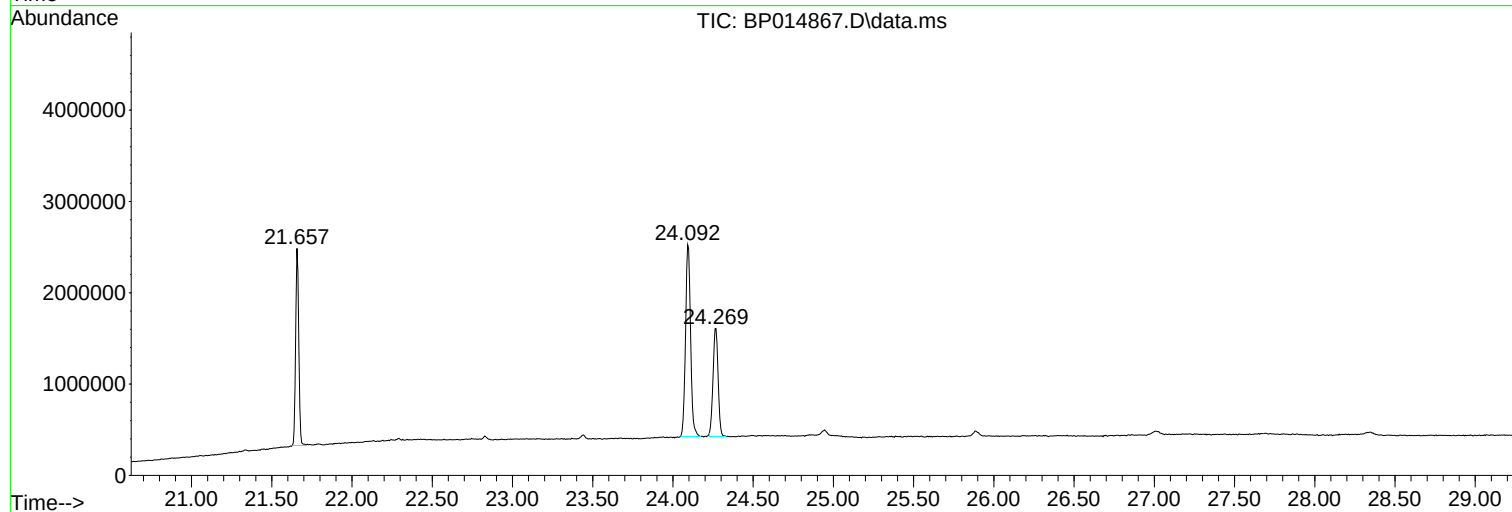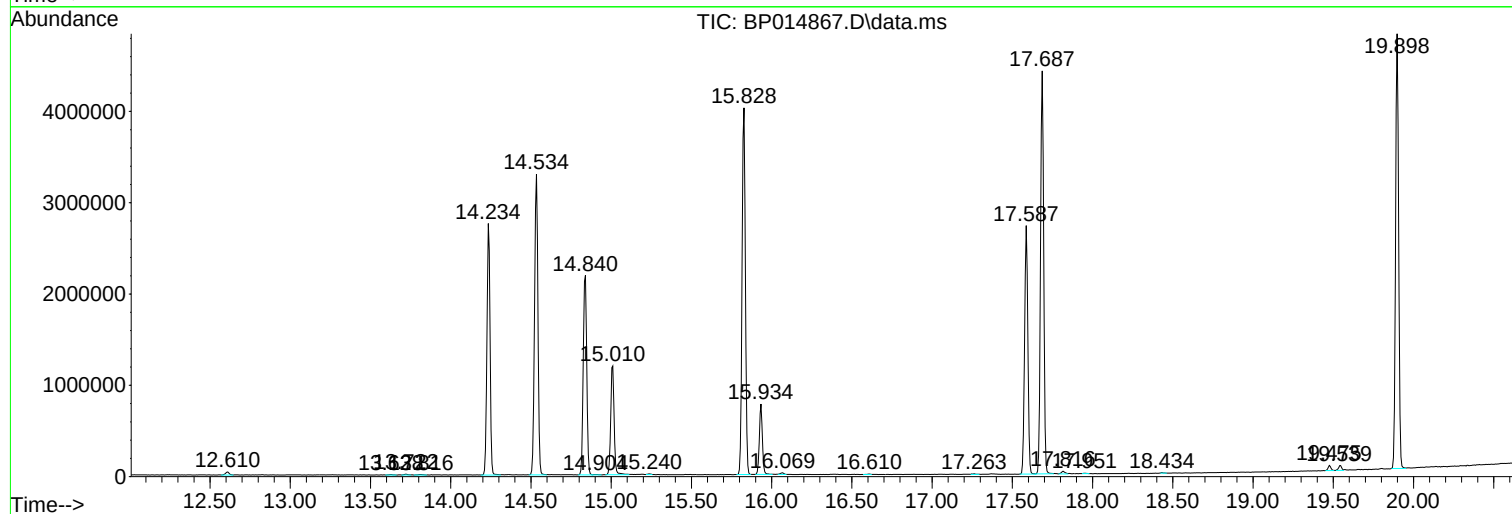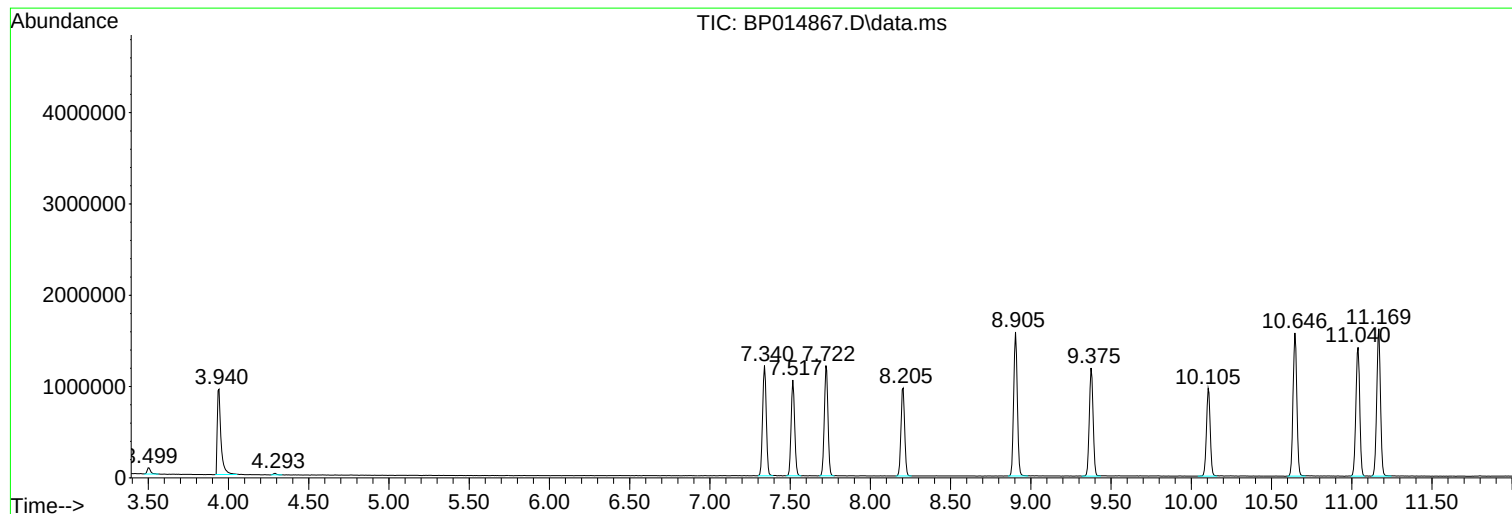

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042723\
Data File : BP014867.D
Acq On : 27 Apr 2023 11:27
Operator : CG/JU
Sample : PB152374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042723\
Data File : BP014867.D
Acq On : 27 Apr 2023 11:27
Operator : CG/JU
Sample : PB152374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------