




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:14:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

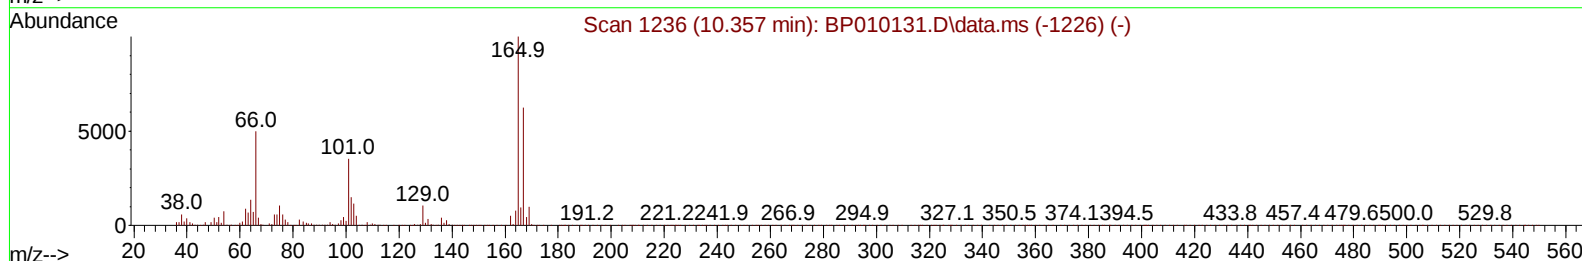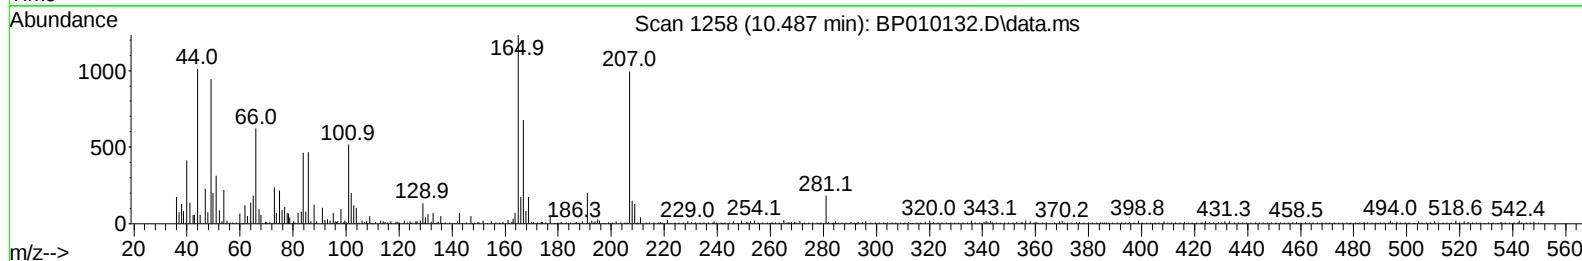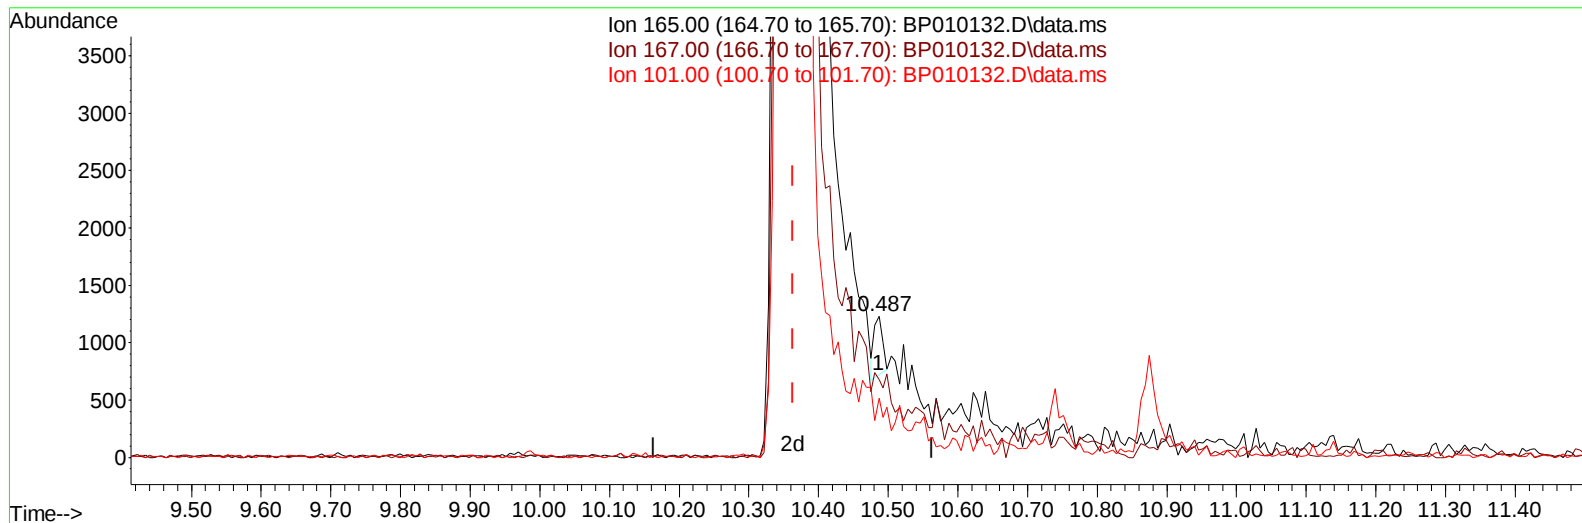

TIC: BP010132.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.487min (+ 0.124) 0.03 ng/u1

response 451

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	54.87
101.00	49.80	41.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:14:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

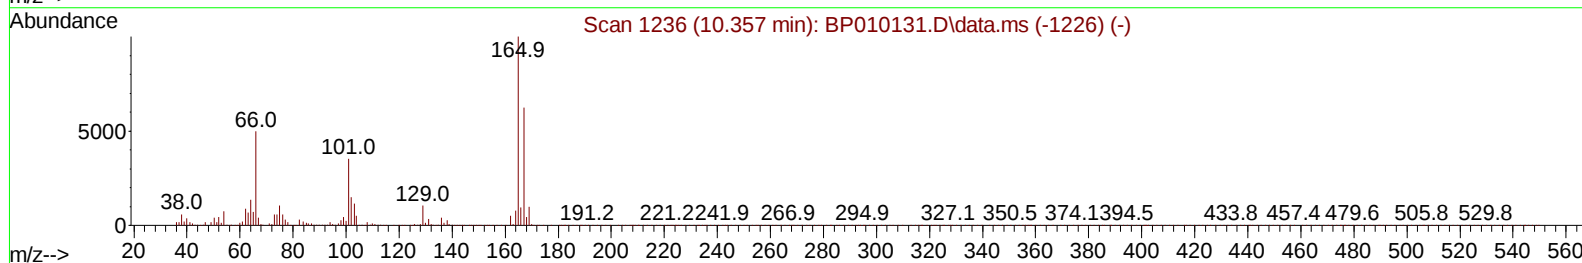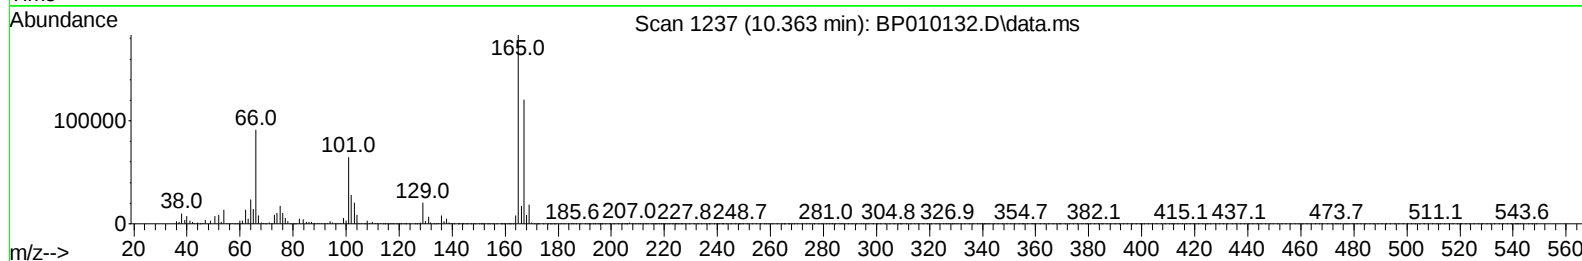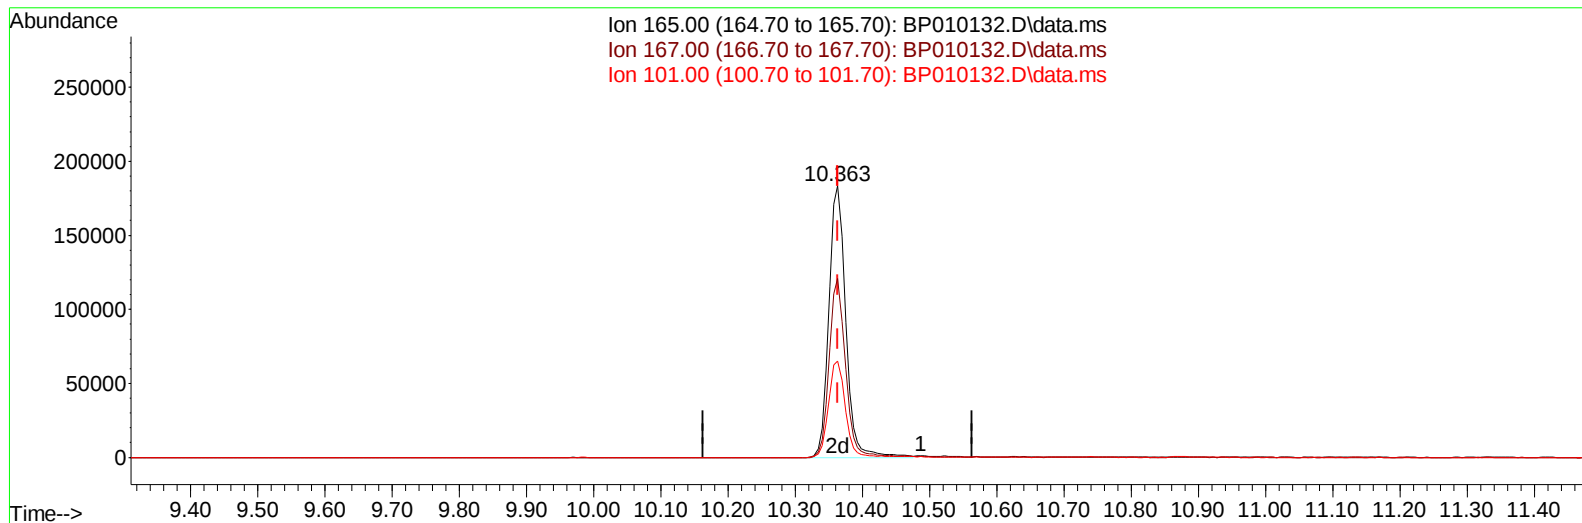

TIC: BP010132.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.363min (+ 0.000) 24.00 ng/ul m

response 320014

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	65.82
101.00	49.80	35.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010132.D
 Acq On : 28 Apr 2022 10:01
 Operator : CG/JU
 Sample : PB144417BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK417

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 29 01:14:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	181657	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136	788684	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.569	164	539199	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1103223	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.410	240	816218	20.000	ng/ul	# 0.00
88) Perylene-d12	23.868	264	609082	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	22981	5.517	ng/uL	0.00
4) Pyridine-d5	3.781	84	285800	24.387	ng/ul	0.00
7) Phenol-d5	7.099	99	392321	23.743	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	267948	27.025	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	321748	26.293	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	334843	24.459	ng/ul	-0.01
21) Nitrobenzene-d5	9.099	128	171022	27.264	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	188786	27.557	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	320014m	23.995	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	466230	24.381	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	1164304	27.759	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1295002	25.511	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	137089	17.754	ng/ul	0.00
60) Fluorene-d10	15.563	176	960311	26.616	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	147893	21.201	ng/ul	0.00
73) Anthracene-d10	17.428	188	1543019	28.910	ng/ul	0.00
81) Pyrene-d10	19.657	212	1698019	36.581	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264	965316	30.231	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 29 01:14:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

