




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010137.D
 Acq On : 28 Apr 2022 12:49
 Operator : CG/JU
 Sample : N2469-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFG8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 14:09:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

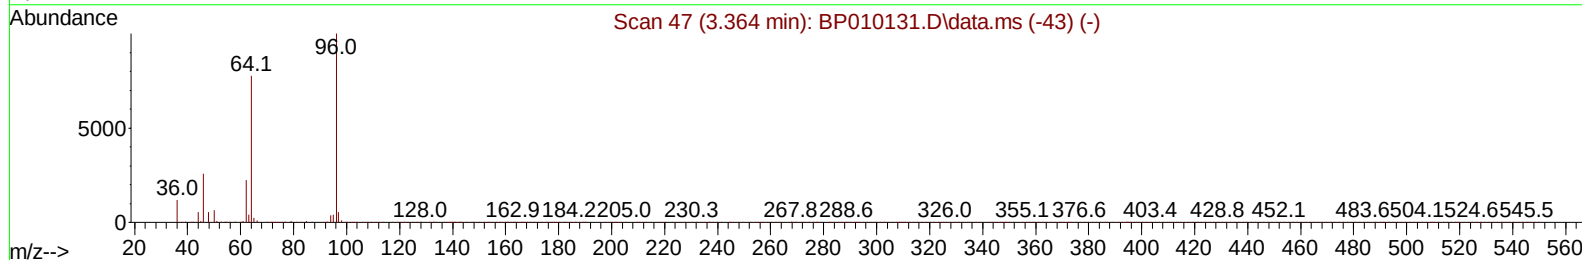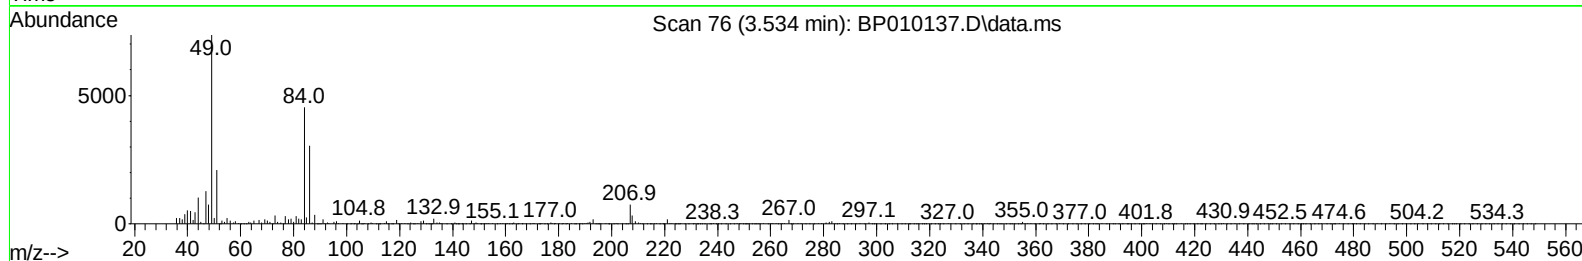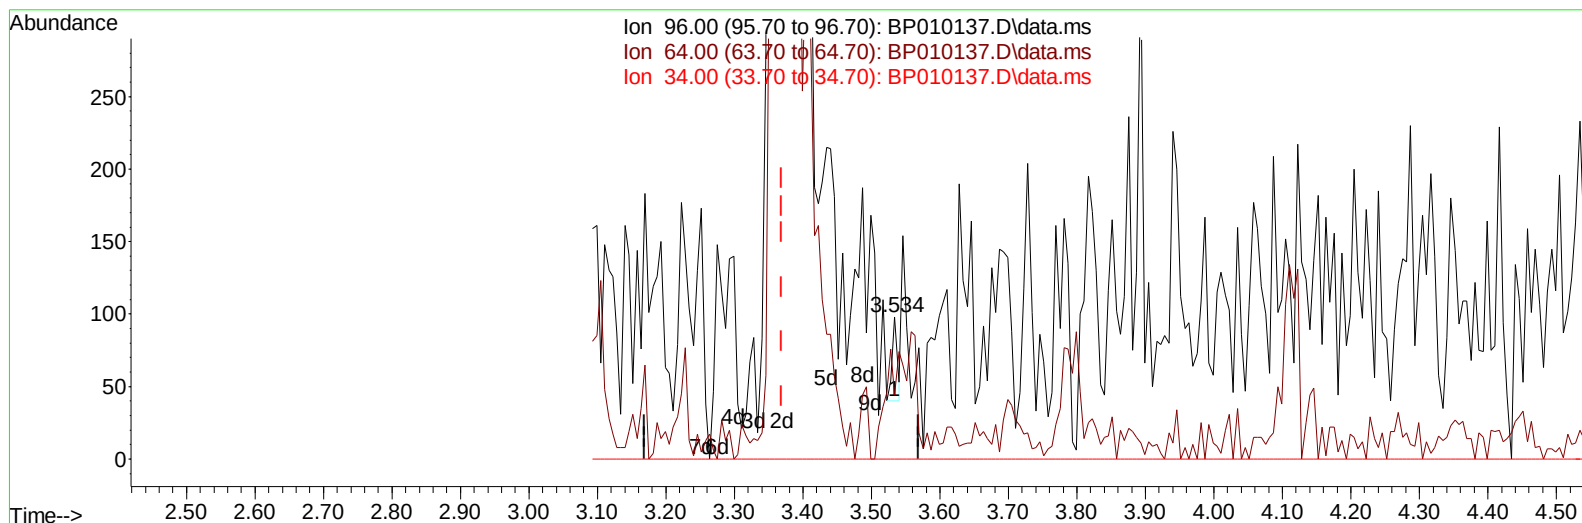

TIC: BP010137.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.534min (+ 0.165) 0.01 ng/uL

response 30

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	44.90
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010137.D
 Acq On : 28 Apr 2022 12:49
 Operator : CG/JU
 Sample : N2469-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFG8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 14:09:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

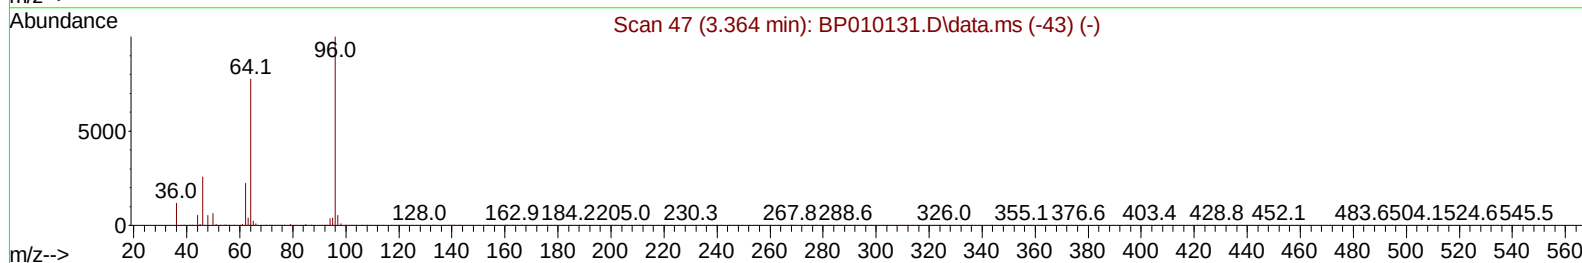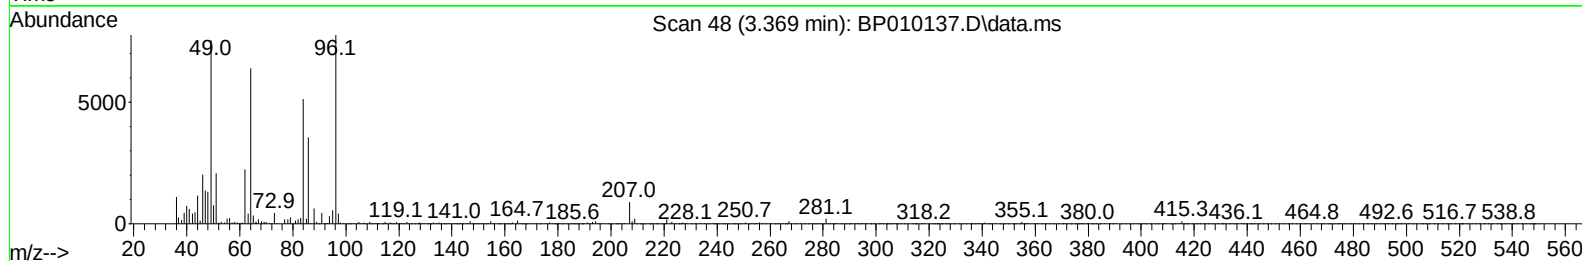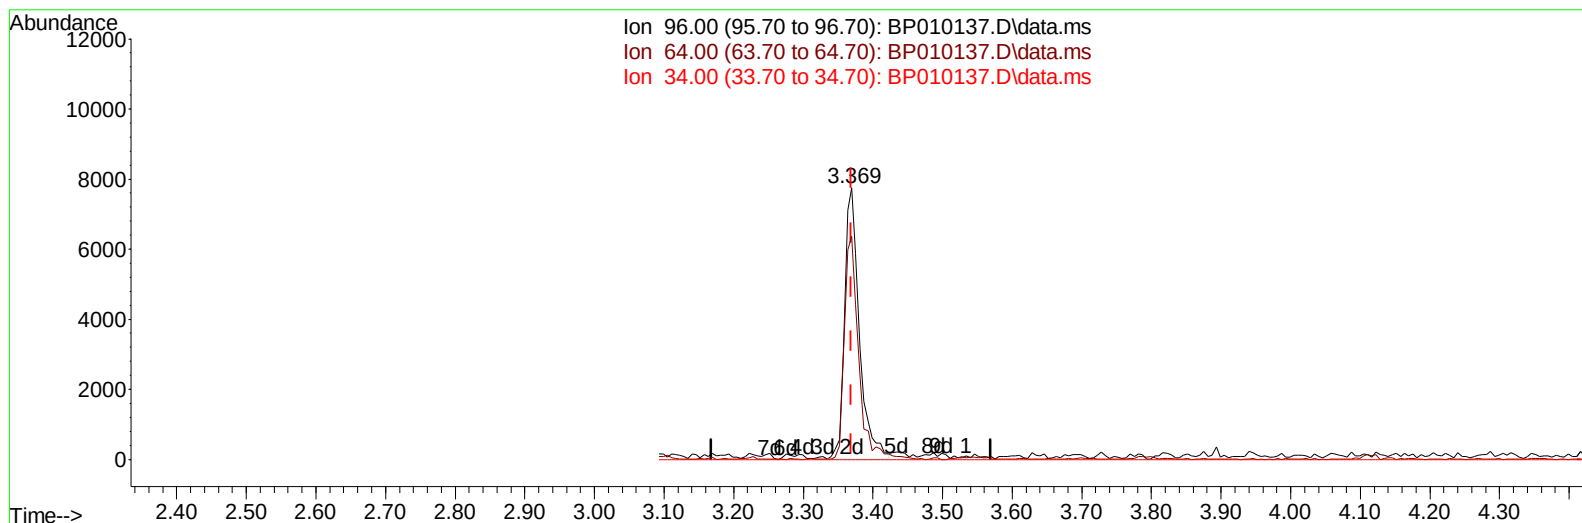

TIC: BP010137.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 2.69 ng/uL m

response 11432

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	82.28#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010137.D
Acq On : 28 Apr 2022 12:49
Operator : CG/JU
Sample : N2469-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFG8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 14:09:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

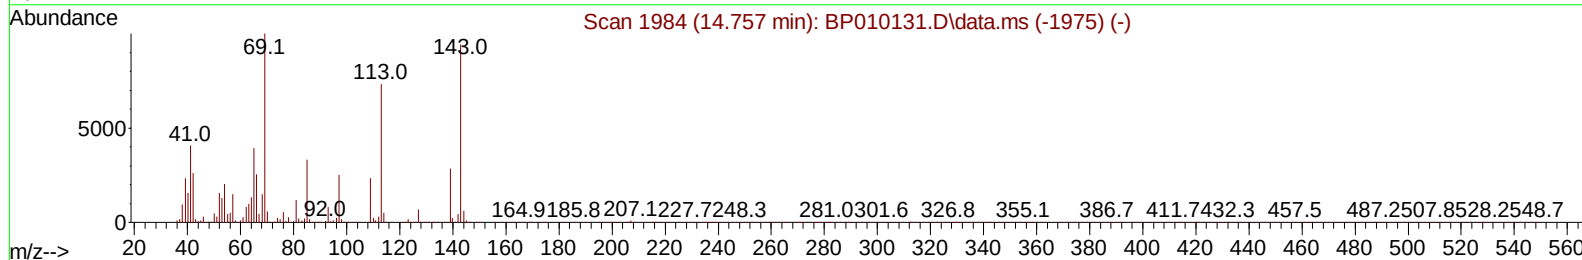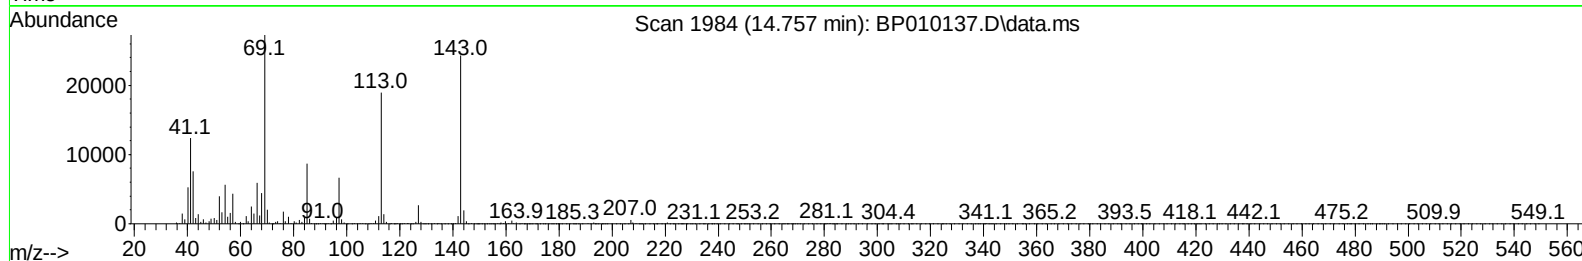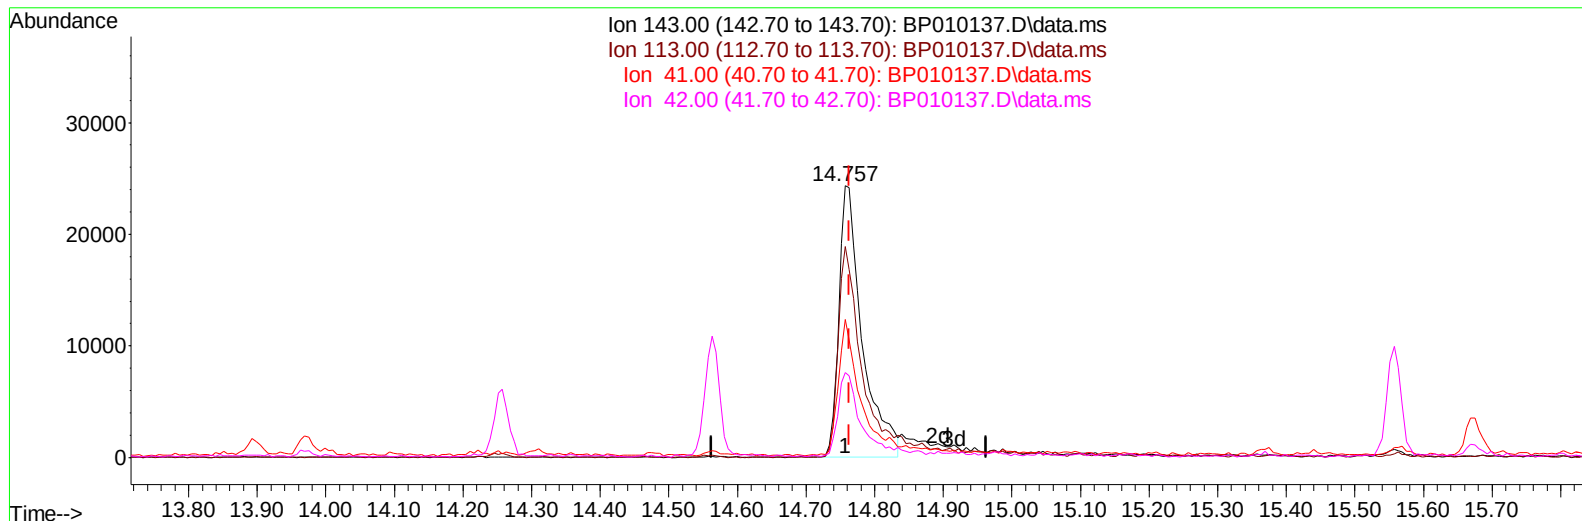

TIC: BP010137.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 7.67 ng/ul

response 57700

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	77.74#
41.00	23.20	50.75#
42.00	18.00	31.16#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010137.D
 Acq On : 28 Apr 2022 12:49
 Operator : CG/JU
 Sample : N2469-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFG8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 14:09:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

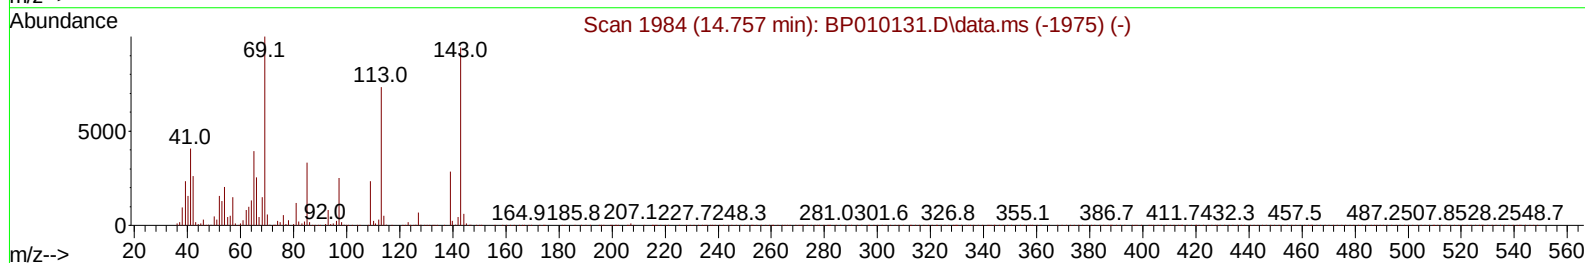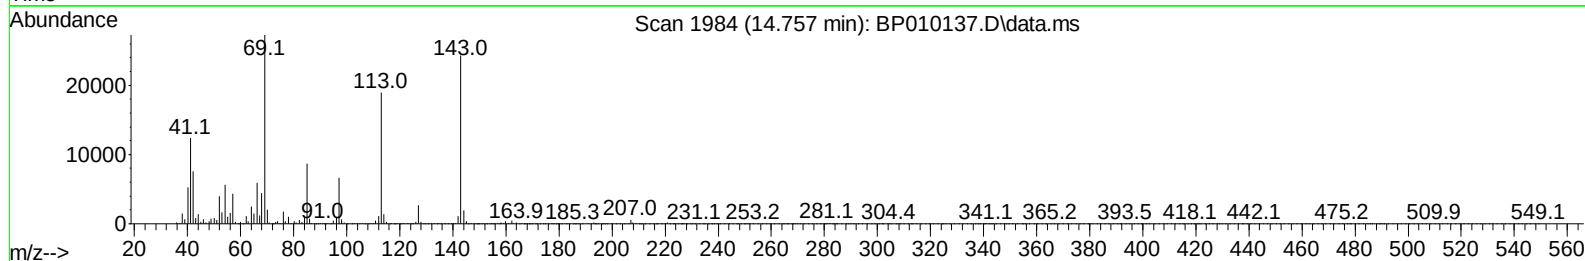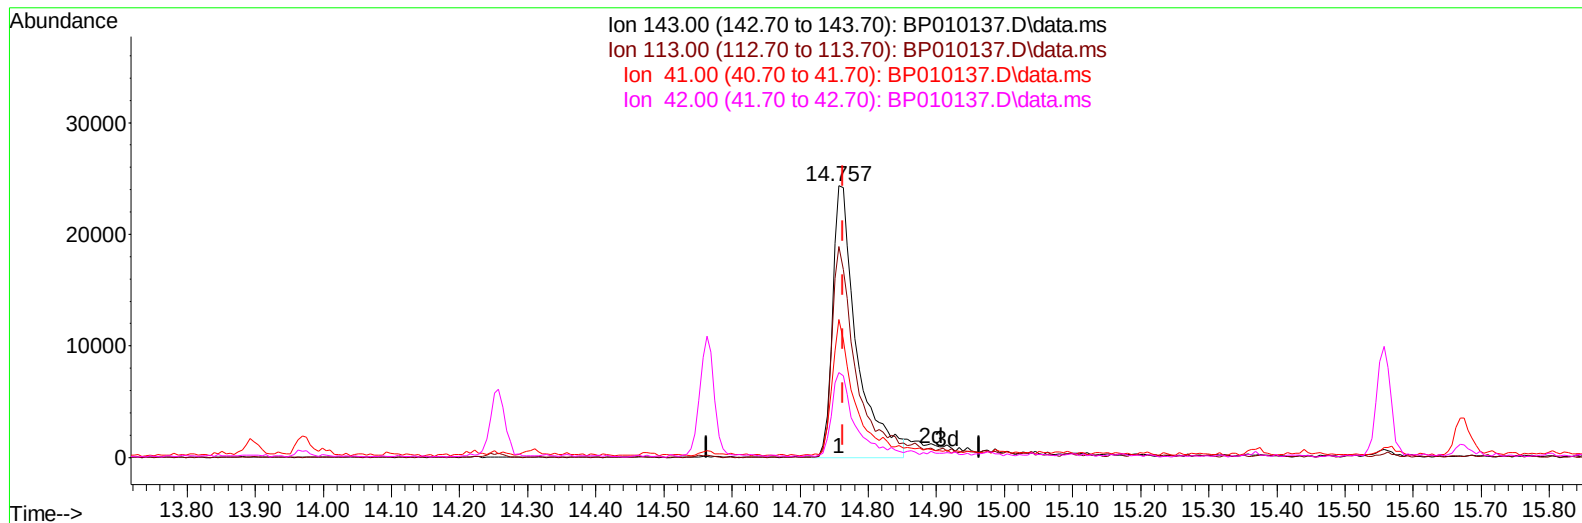

TIC: BP010137.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.006) 7.94 ng/ul m

response 59743

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	77.74#
41.00	23.20	50.75#
42.00	18.00	31.16#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010137.D
Acq On : 28 Apr 2022 12:49
Operator : CG/JU
Sample : N2469-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFG8

Manual IntegrationsAPPROVED

Quant Time: May 06 04:41:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

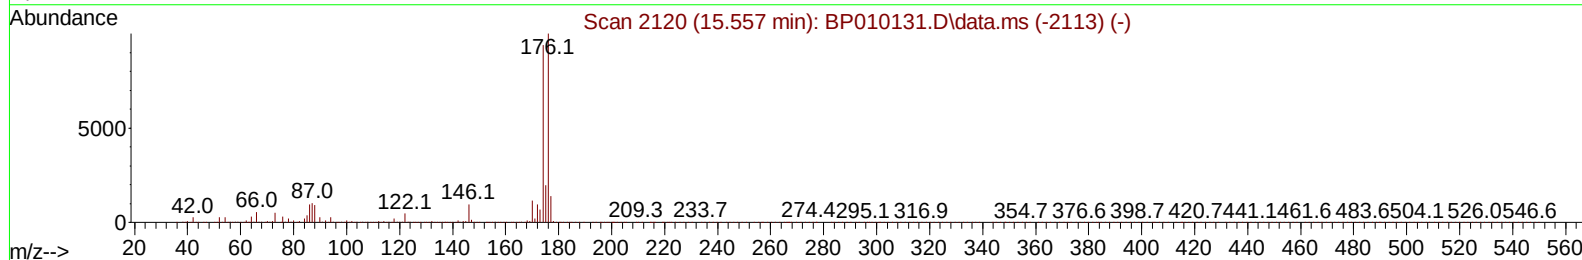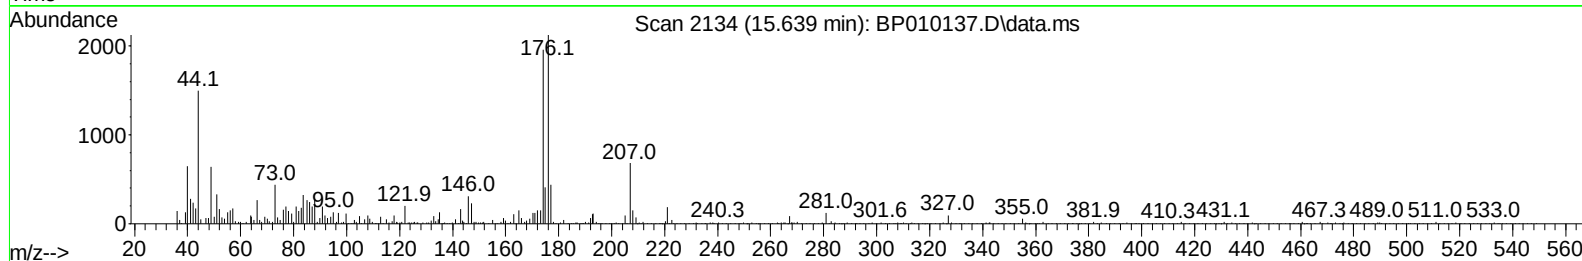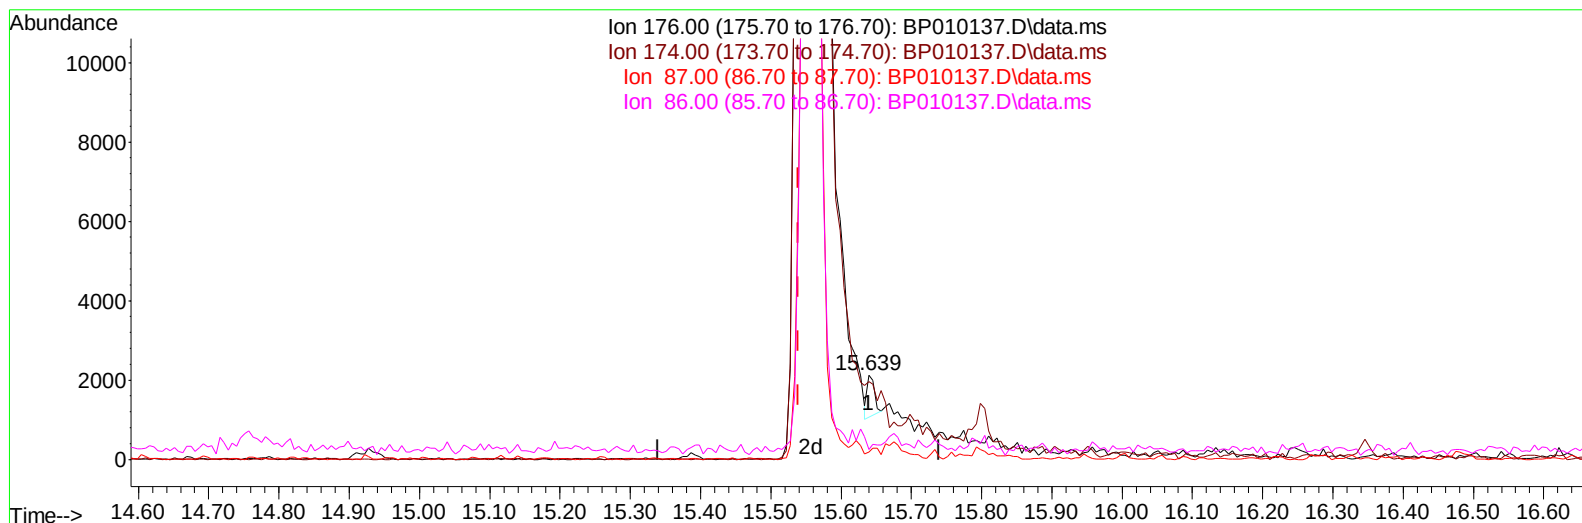

TIC: BP010137.D\data.ms

(60) Fluorene-d10 (S)

15.639min (+ 0.100) 0.02 ng/ul

response 760

Ion	Exp%	Act%
176.00	100.00	100.00
174.00	97.00	92.37
87.00	8.20	9.04
86.00	10.00	11.68




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010137.D
Acq On : 28 Apr 2022 12:49
Operator : CG/JU
Sample : N2469-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFG8

Manual IntegrationsAPPROVED

Quant Time: Apr 28 14:09:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

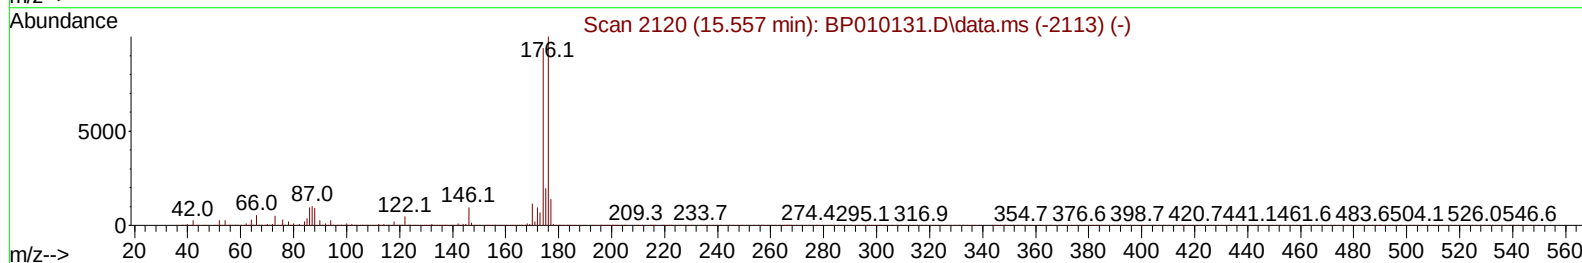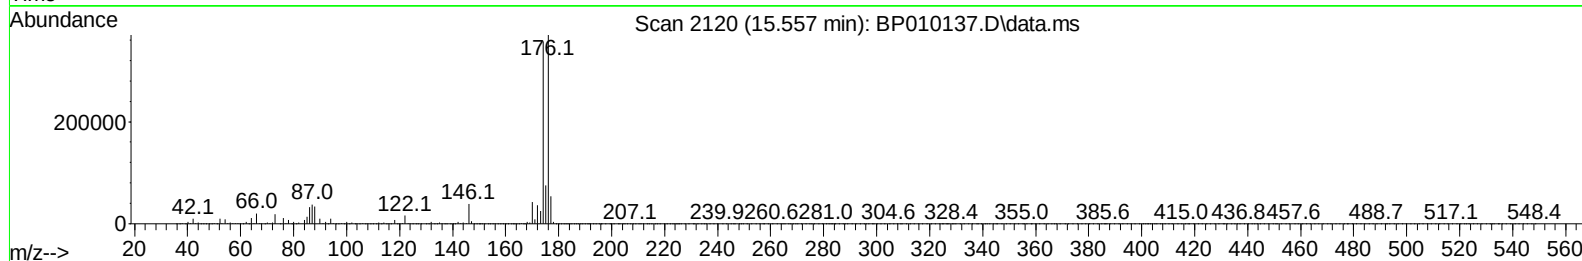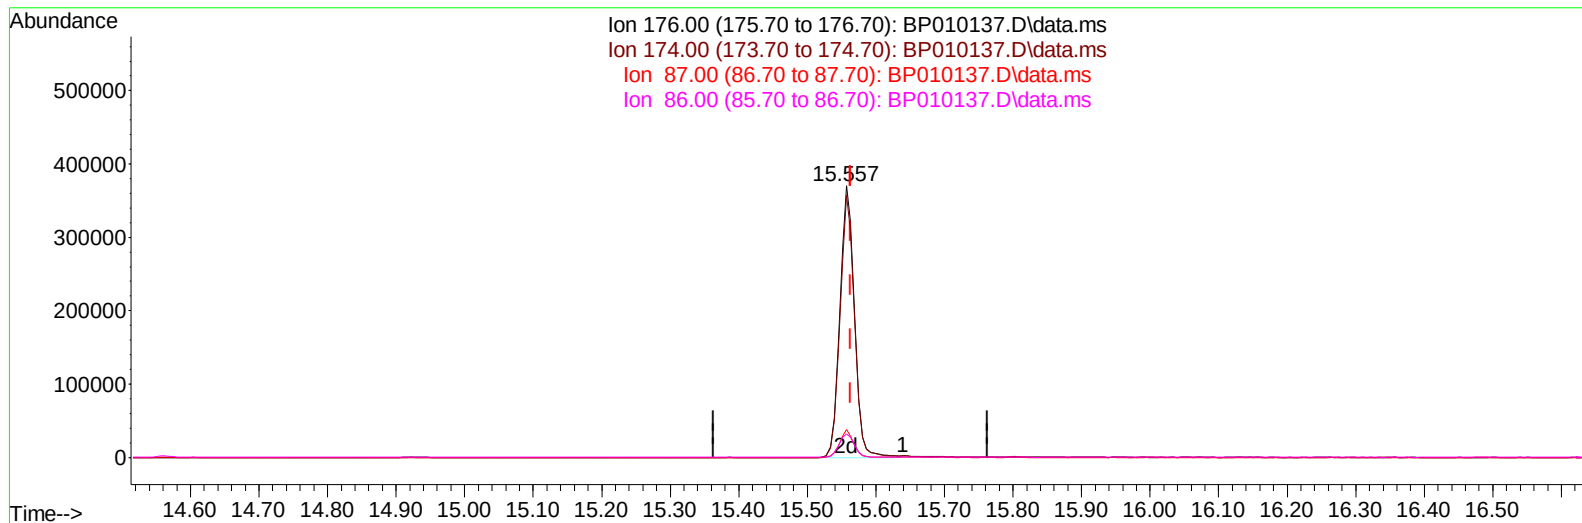

TIC: BP010137.D\data.ms

(60) Fluorene-d10 (S)

15.557min (-0.006) 15.45 ng/ul m

response 543044

Ion	Exp%	Act%
176.00	100.00	100.00
174.00	97.00	96.49
87.00	8.20	10.19#
86.00	10.00	8.69

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010137.D
 Acq On : 28 Apr 2022 12:49
 Operator : CG/JU
 Sample : N2469-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFG8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 14:09:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	185299	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.734	136	800673	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.563	164	525274	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188	1038129	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240	660129	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264	568322	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	11432m	2.690	ng/uL	0.00
4) Pyridine-d5	3.793	84	51610	4.317	ng/ul	0.00
7) Phenol-d5	7.093	99	223081	13.236	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	162256	16.043	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132	192661	15.435	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	186612	13.363	ng/ul	-0.02
21) Nitrobenzene-d5	9.087	128	99262	15.587	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.816	143	110633	15.907	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	184133	13.600	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	240680	12.398	ng/ul	-0.01
46) Dimethylphthalate-d6	13.969	166	648751	15.877	ng/ul	-0.01
49) Acenaphthylene-d8	14.257	160	734157	14.846	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	59743m	7.942	ng/ul	0.00
60) Fluorene-d10	15.557	176	543044m	15.450	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	55630	8.475	ng/ul	0.00
73) Anthracene-d10	17.416	188	810931	16.146	ng/ul	0.00
81) Pyrene-d10	19.645	212	905295	24.114	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.698	264	539478	18.107	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010137.D
Acq On : 28 Apr 2022 12:49
Operator : CG/JU
Sample : N2469-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFG8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 28 14:09:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

