




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010138.D
 Acq On : 28 Apr 2022 13:22
 Operator : CG/JU
 Sample : N2469-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH3

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:05:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

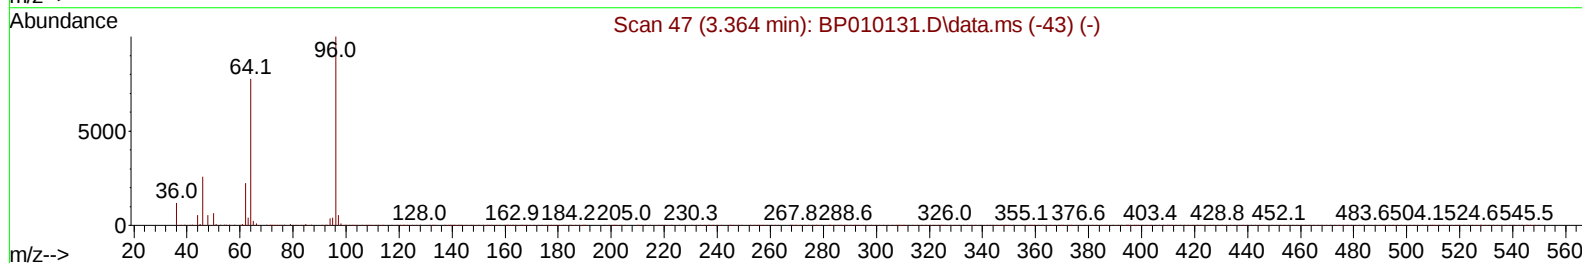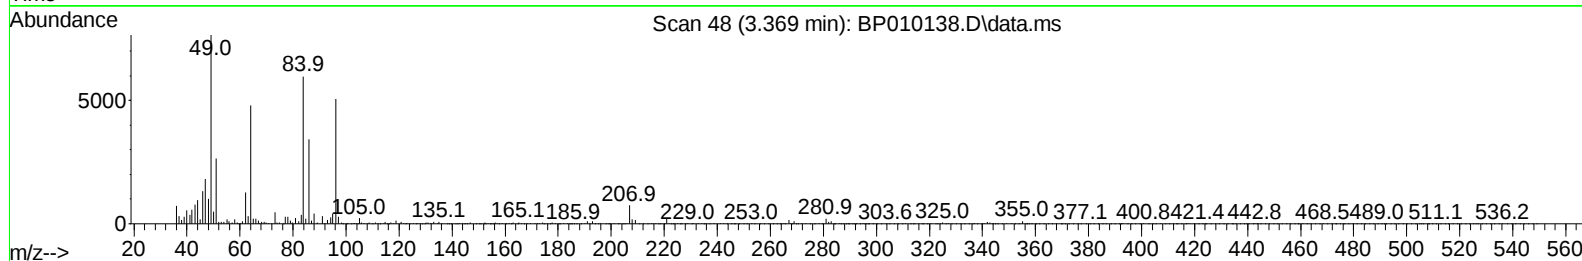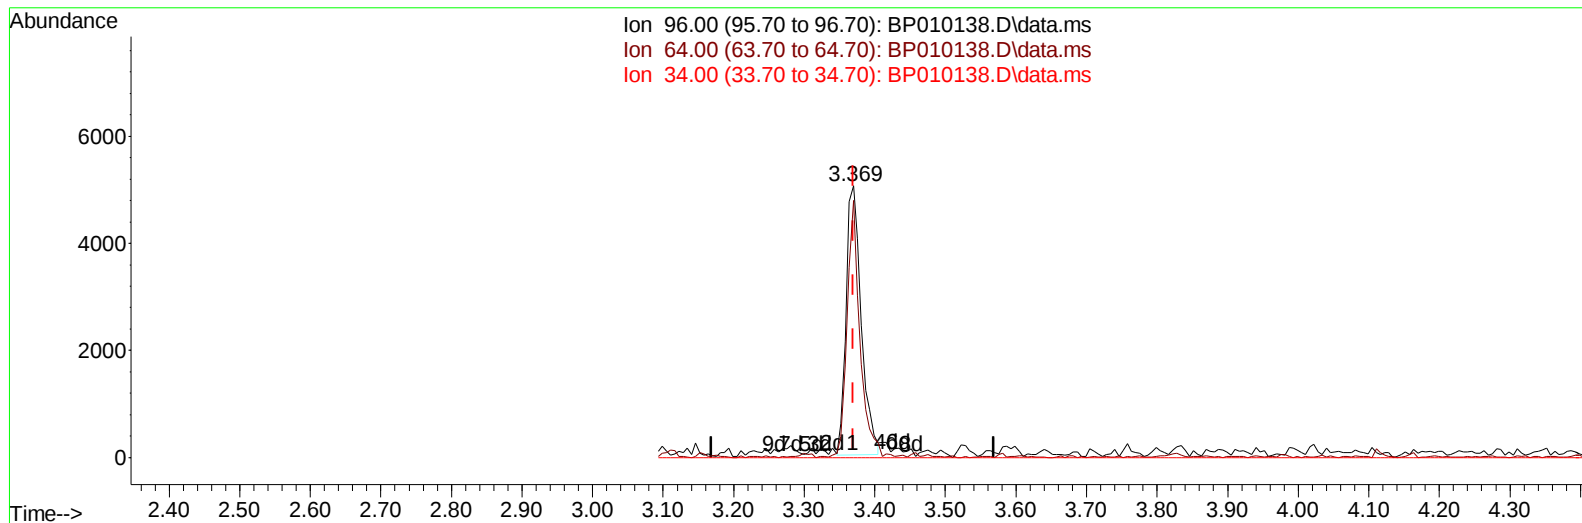

TIC: BP010138.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 1.71 ng/uL

response 7594

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	94.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010138.D
 Acq On : 28 Apr 2022 13:22
 Operator : CG/JU
 Sample : N2469-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH3

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:05:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

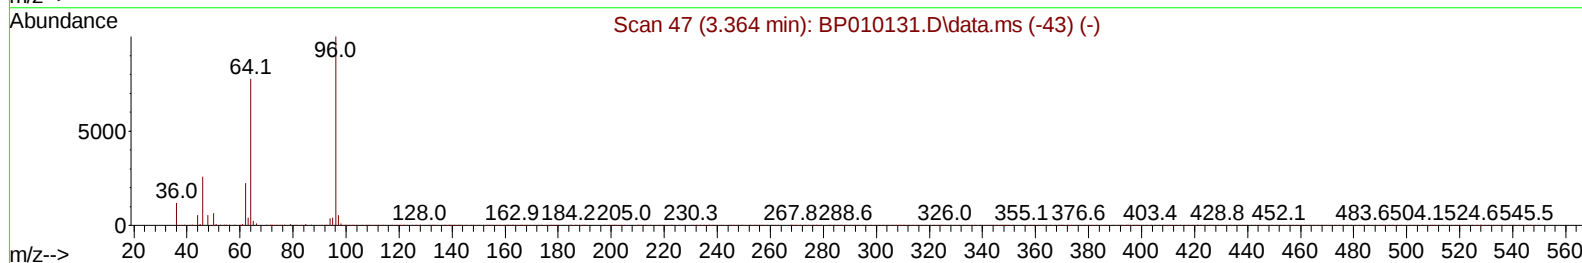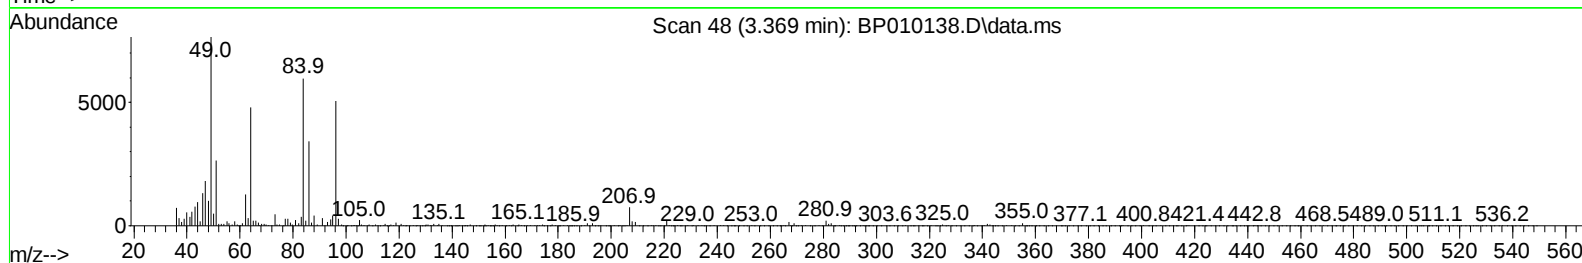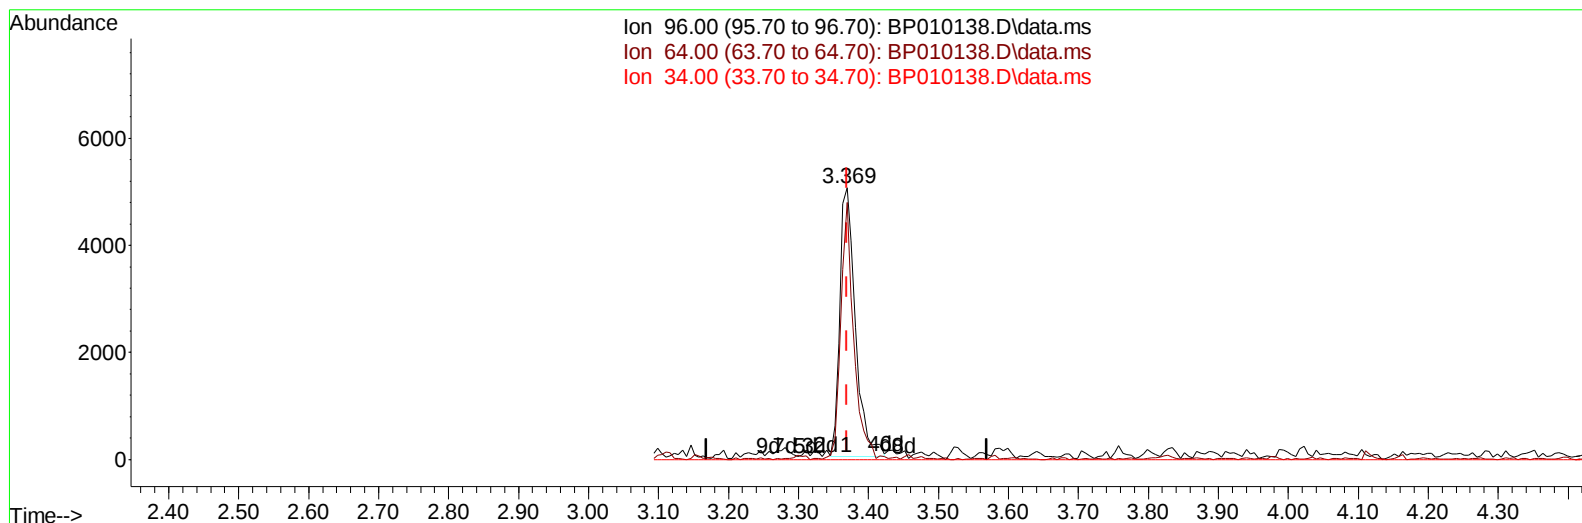

TIC: BP010138.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.369min (+ 0.000) 1.75 ng/uL m

response 7740

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	94.60#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010138.D
Acq On : 28 Apr 2022 13:22
Operator : CG/JU
Sample : N2469-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH3

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:05:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

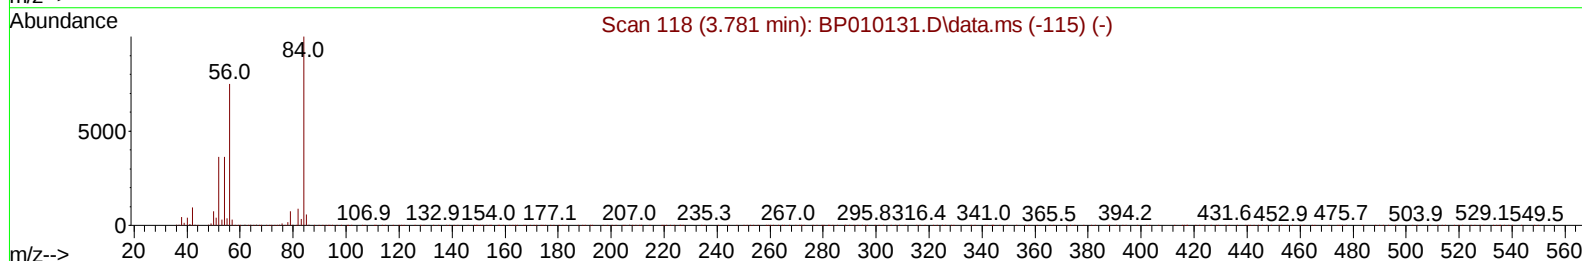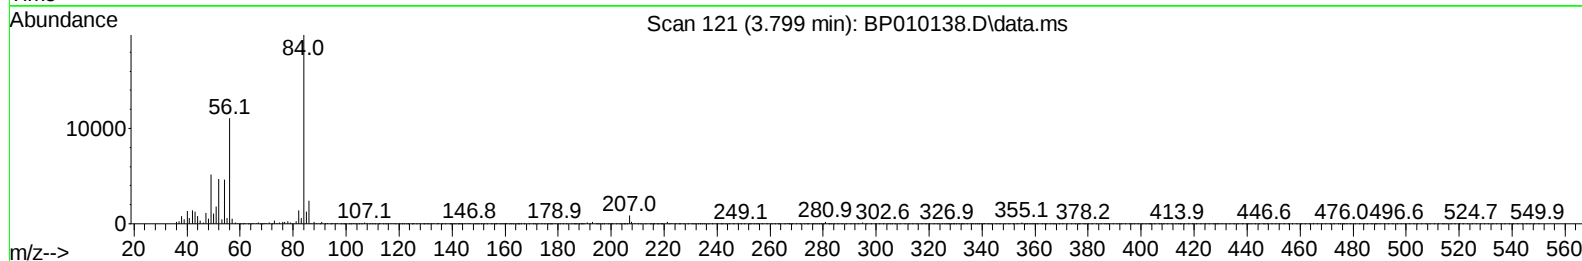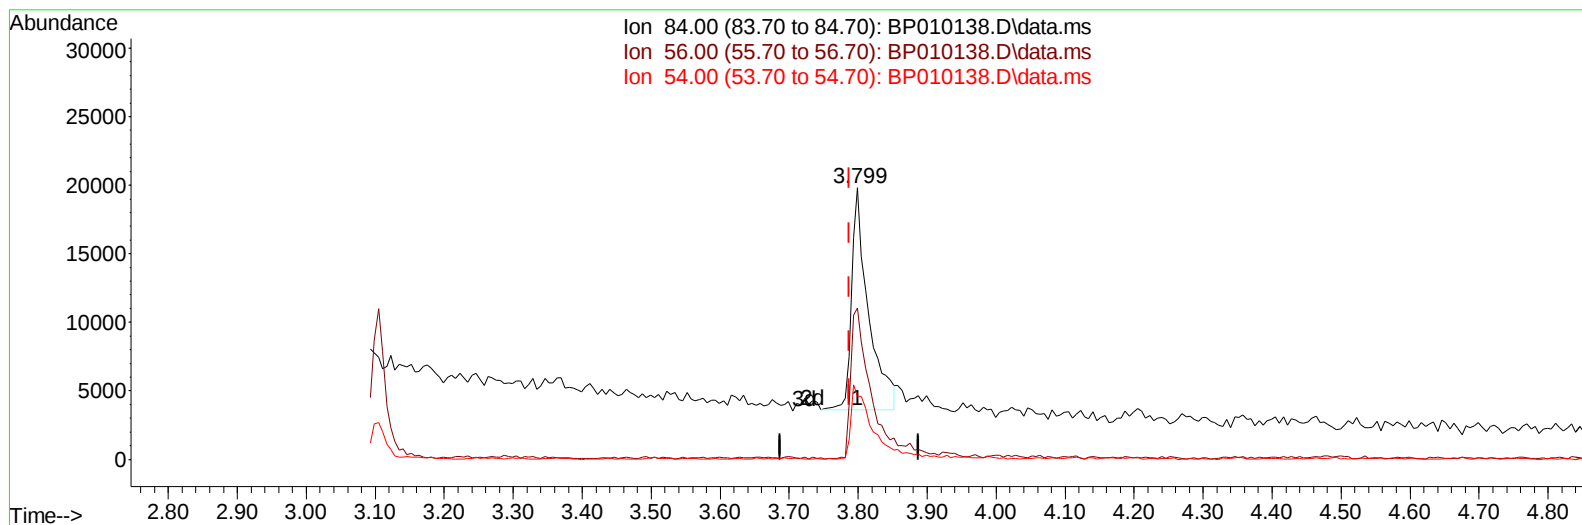

TIC: BP010138.D\data.ms

(4) Pyridine-d5 (S)

3.799min (+ 0.012) 2.21 ng/u1

response 27562

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	55.87#
54.00	24.80	23.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010138.D
Acq On : 28 Apr 2022 13:22
Operator : CG/JU
Sample : N2469-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH3

Manual IntegrationsAPPROVED

Quant Time: Apr 29 01:05:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

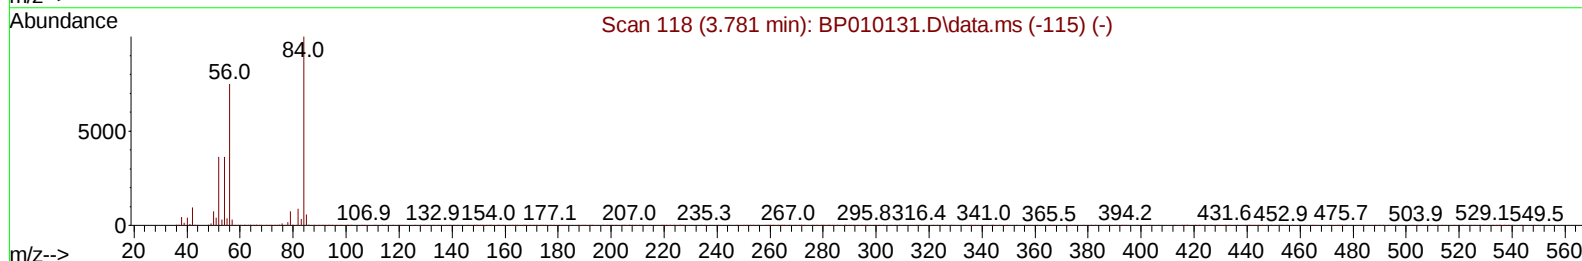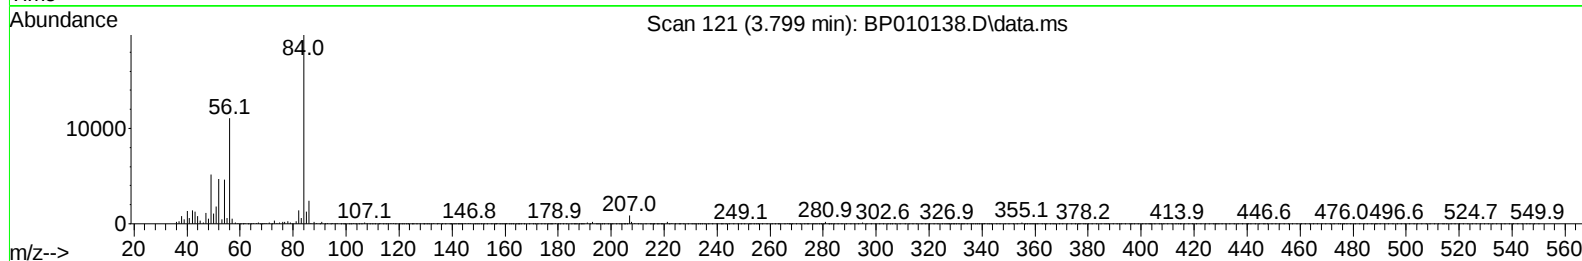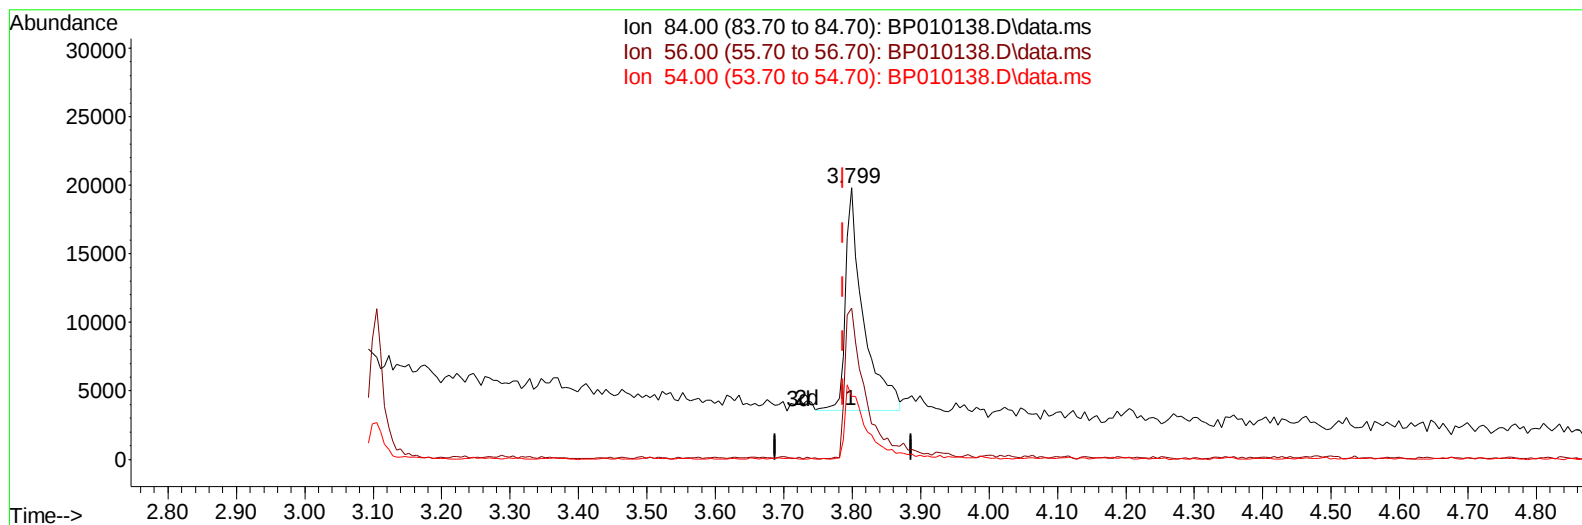

TIC: BP010138.D\data.ms

(4) Pyridine-d5 (S)

3.799min (+ 0.012) 2.35 ng/ul m

response 29313

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	55.87#
54.00	24.80	23.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010138.D
 Acq On : 28 Apr 2022 13:22
 Operator : CG/JU
 Sample : N2469-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFH3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/29/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 29 01:05:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.934	152		193293	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.734	136		834144	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.563	164		549630	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.316	188		1091554	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.404	240		738253	20.000	ng/ul	# 0.00
88) Perylene-d12	23.857	264		592328	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.369	96		7740m	1.746	ng/uL	0.00
4) Pyridine-d5	3.799	84		29313m	2.351	ng/ul	0.01
7) Phenol-d5	7.093	99		159995	9.100	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.257	67		110202	10.446	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.463	132		132914	10.208	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113		128173	8.799	ng/ul	-0.02
21) Nitrobenzene-d5	9.087	128		67895	10.234	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.816	143		73502	10.144	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165		128773	9.129	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131		148576	7.346	ng/ul	-0.01
46) Dimethylphthalate-d6	13.969	166		454642	10.634	ng/ul	-0.01
49) Acenaphthylene-d8	14.257	160		502692	9.715	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143		43744	5.558	ng/ul	0.00
60) Fluorene-d10	15.557	176		382929	10.412	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200		36158	5.239	ng/ul	0.00
73) Anthracene-d10	17.416	188		569749	10.789	ng/ul	0.00
81) Pyrene-d10	19.645	212		663513	15.804	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.698	264		374054	12.046	ng/ul	0.00
Target Compounds							
						Qvalue	
16) Acetophenone	8.752	105		40424	1.779	ng/ul#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010138.D
Acq On : 28 Apr 2022 13:22
Operator : CG/JU
Sample : N2469-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFH3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/29/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 29 01:05:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

