

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
 Data File : BP010132.D
 Acq On : 28 Apr 2022 10:01
 Operator : CG/JU
 Sample : PB144417BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK417

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	56	rVB	47435	67591	1.56%	0.151%
2	3.781	115	118	135	rBV	506856	867108	20.03%	1.935%
3	4.117	171	175	179	rVB3	15688	20930	0.48%	0.047%
4	7.099	674	682	696	rBV	718992	1171468	27.06%	2.614%
5	7.263	703	710	724	rBV	594852	956215	22.08%	2.133%
6	7.469	738	745	757	rBV	741668	1209584	27.94%	2.699%
7	7.940	816	825	836	rBV	656408	1115389	25.76%	2.488%
8	8.640	935	944	958	rBV	896500	1538119	35.52%	3.432%
9	9.093	1014	1021	1033	rBV	751023	1282383	29.62%	2.861%
10	9.822	1137	1145	1162	rBV	606878	1070132	24.72%	2.387%
11	10.363	1228	1237	1256	rBV	864656	1548737	35.77%	3.455%
12	10.487	1256	1258	1262	rVB5	2929	4386	0.10%	0.010%
13	10.740	1294	1301	1312	rBV	963020	1670115	38.57%	3.726%
14	10.875	1316	1324	1349	rVV	832326	1598694	36.92%	3.567%
15	12.334	1566	1572	1583	rBV3	13728	28977	0.67%	0.065%
16	13.551	1774	1779	1784	rBV9	2367	4394	0.10%	0.010%
17	13.863	1825	1832	1836	rBV9	2690	5375	0.12%	0.012%
18	13.975	1843	1851	1863	rBV	1736804	2549073	58.87%	5.687%
19	14.075	1865	1868	1873	rVB5	4926	8573	0.20%	0.019%
20	14.263	1892	1900	1913	rBV	1909615	2844378	65.69%	6.346%
21	14.569	1945	1952	1968	rBV	1512784	2323751	53.67%	5.184%
22	14.763	1978	1985	2004	rBV	479576	984875	22.75%	2.197%
23	15.216	2056	2062	2071	rVB	3112	8461	0.20%	0.019%
24	15.563	2114	2121	2135	rBV	2382379	3577294	82.62%	7.981%
25	15.681	2135	2141	2156	rVV	712267	1066503	24.63%	2.379%
26	15.804	2158	2162	2171	rVB3	30760	52961	1.22%	0.118%
27	16.245	2235	2237	2242	rBV6	2793	4785	0.11%	0.011%
28	16.345	2250	2254	2262	rBV4	9706	15889	0.37%	0.035%
29	16.998	2363	2365	2373	rVB9	4084	6707	0.15%	0.015%
30	17.116	2380	2385	2390	rBV6	4162	8360	0.19%	0.019%
31	17.328	2412	2421	2431	rBV	1786634	2674002	61.76%	5.966%
32	17.428	2431	2438	2453	rVB	2558905	3930132	90.77%	8.768%
33	19.233	2741	2745	2750	rBV4	28928	42634	0.98%	0.095%
34	19.304	2752	2757	2763	rBV	28607	46208	1.07%	0.103%
35	19.657	2810	2817	2832	rBV	3161010	4329755	100.00%	9.660%
36	21.410	3110	3115	3129	rBV	1487039	2138730	49.40%	4.772%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	23.710	3499	3506	3513	rBV	1197174	2454288	56.68%	5.476%
38	23.868	3526	3533	3546	rVB2	758291	1595913	36.86%	3.560%




Sum of corrected areas: 44822869

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

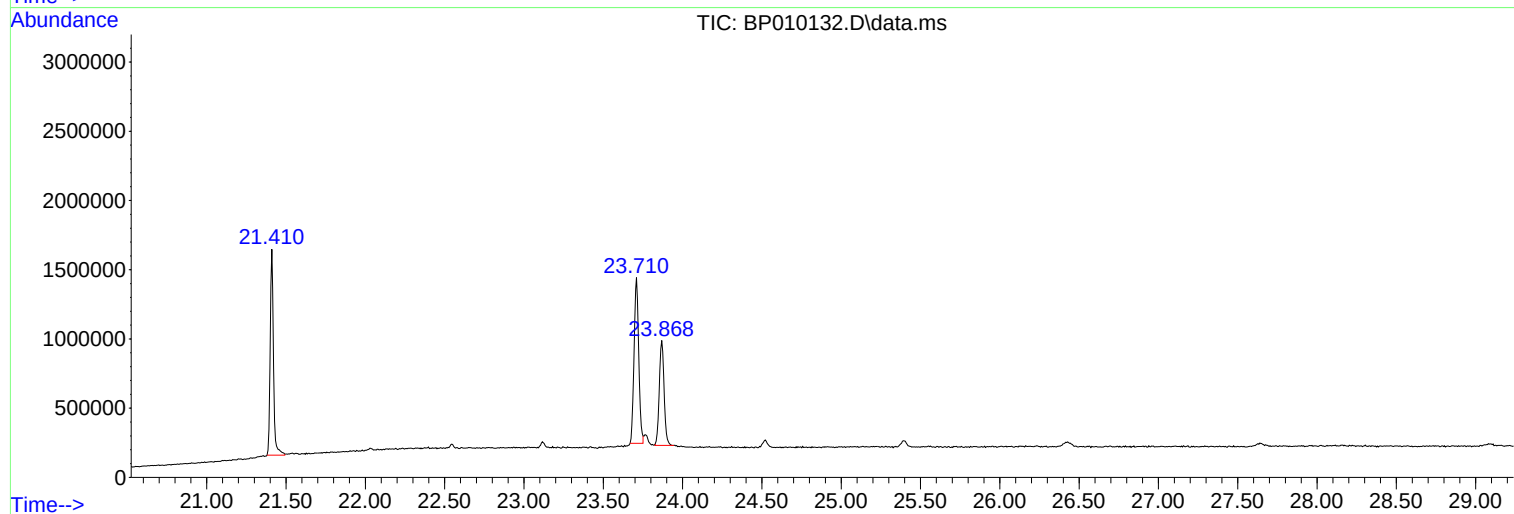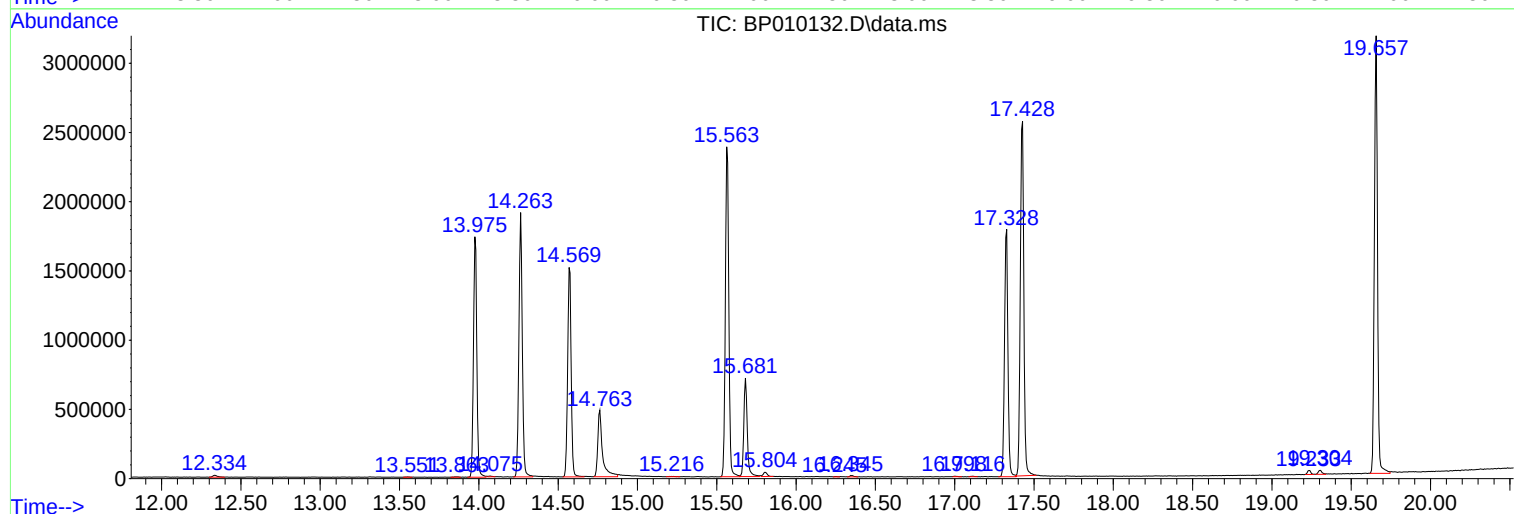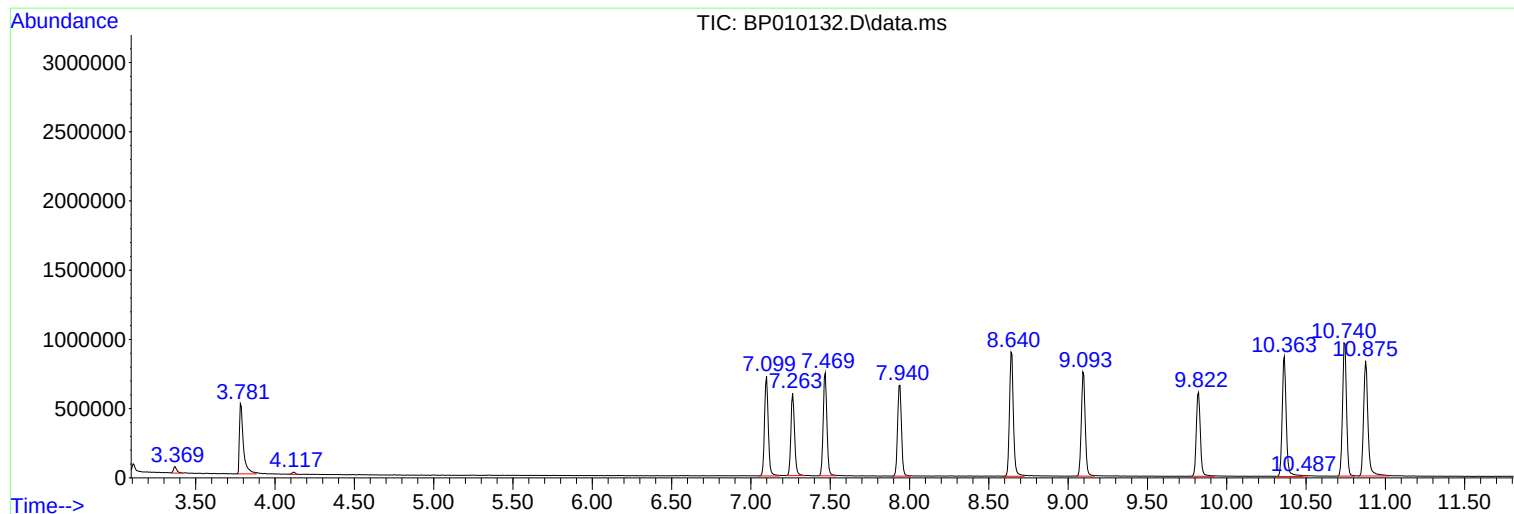

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042822\
Data File : BP010132.D
Acq On : 28 Apr 2022 10:01
Operator : CG/JU
Sample : PB144417BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------