

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014873.D
 Acq On : 28 Apr 2023 13:22
 Operator : CG/JU
 Sample : SSTD01060
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010647

Quant Time: Apr 28 23:56:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 17:04:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.175	152	216716	20.000	ng/ul	0.00
20) Naphthalene-d8	11.016	136	846486	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.822	164	481876	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.581	188	963245	20.000	ng/ul	0.00
79) Chrysene-d12	21.663	240	868386	20.000	ng/ul	0.00
88) Perylene-d12	24.268	264	954692	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.470	96	23899	3.974	ng/uL	0.00
4) Pyridine-d5	3.911	84	131749	9.115	ng/ul	0.00
7) Phenol-d5	7.316	99	145345	8.569	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.493	67	103116	9.693	ng/ul	0.00
11) 2-Chlorophenol-d4	7.699	132	121528	9.463	ng/ul	0.00
15) 4-Methylphenol-d8	8.881	113	111151	8.600	ng/ul	0.00
21) Nitrobenzene-d5	9.352	128	54991	9.048	ng/ul	0.00
24) 2-Nitrophenol-d4	10.081	143	47188	8.458	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.622	165	107293	8.893	ng/ul	0.00
31) 4-Chloroaniline-d4	11.146	131	149859	8.650	ng/ul	0.00
46) Dimethylphthalate-d6	14.222	166	337137	9.762	ng/ul	0.00
49) Acenaphthylene-d8	14.516	160	398885	9.670	ng/ul	0.00
54) 4-Nitrophenol-d4	14.998	143	19483	3.777	ng/ul	0.00
60) Fluorene-d10	15.810	176	297326	9.877	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.922	200	15936	3.926	ng/ul	0.00
73) Anthracene-d10	17.675	188	435586	9.902	ng/ul	0.00
81) Pyrene-d10	19.892	212	469384	9.732	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.092	264	458961	9.733	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.505	88	25139	3.926	ng/uL	97
5) Pyridine	3.928	79	140565	9.272	ng/ul	96
6) Benzaldehyde	7.305	77	36209	7.611	ng/ul	99
8) Phenol	7.340	94	150836	8.575	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.587	93	141168	9.365	ng/ul	99
12) 2-Chlorophenol	7.734	128	130041	9.436	ng/ul	98
13) 2-Methylphenol	8.616	108	121370	8.906	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.710	45	191209	10.083	ng/ul	99
16) Acetophenone	9.010	105	196344	9.353	ng/ul	96
17) N-Nitroso-di-n-propyla...	8.987	70	95984	9.631	ng/ul	97
18) 4-Methylphenol	8.946	108	124728	8.673	ng/ul	94
19) Hexachloroethane	9.275	117	64142	9.880	ng/ul	91
22) Nitrobenzene	9.393	77	147349	9.557	ng/ul	99
23) Isophorone	9.922	82	256335	9.229	ng/ul	98
25) 2-Nitrophenol	10.116	139	50309	8.135	ng/ul	98
26) 2,4-Dimethylphenol	10.169	107	142007	9.496	ng/ul	98
27) Bis(2-Chloroethoxy)met...	10.404	93	184448	9.630	ng/ul	99
29) 2,4-Dichlorophenol	10.651	162	111802	9.269	ng/ul	98
30) Naphthalene	11.063	128	458416	9.849	ng/ul	100
32) 4-Chloroaniline	11.169	127	161744	8.948	ng/ul	94
33) Hexachlorobutadiene	11.351	225	91920	9.999	ng/ul	96
34) Caprolactam	11.928	113	13619	4.493	ng/ul	91
35) 4-Chloro-3-methylphenol	12.281	107	111320	9.067	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014873.D
 Acq On : 28 Apr 2023 13:22
 Operator : CG/JU
 Sample : SST001060
 Misc :
 ALS Vial : 3 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SST0010647

Quant Time: Apr 28 23:56:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 17:04:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.663	142	287288	9.781	ng/ul	99
37) 1-Methylnaphthalene	12.881	142	288807	9.794	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	13.022	216	160370	9.959	ng/ul	98
40) Hexachlorocyclopentadiene	13.004	237	83578	8.268	ng/ul	98
41) 2,4,6-Trichlorophenol	13.257	196	70694	8.640	ng/ul	99
42) 2,4,5-Trichlorophenol	13.328	196	79258	8.330	ng/ul	97
43) 1,1'-Biphenyl	13.657	154	387629	10.026	ng/ul	98
44) 2-Chloronaphthalene	13.704	162	304834	10.011	ng/ul	99
45) 2-Nitroaniline	13.904	65	55766	8.383	ng/ul	98
47) Dimethylphthalate	14.269	163	349191	9.781	ng/ul	100
48) 2,6-Dinitrotoluene	14.387	165	55438	8.620	ng/ul	90
50) Acenaphthylene	14.545	152	454247	9.851	ng/ul	99
51) 3-Nitroaniline	14.781	138	2827	0.539	ng/ul	90
52) Acenaphthene	14.887	153	316942	9.972	ng/ul	100
53) 2,4-Dinitrophenol	14.922	184	2117	0.892	ng/ul#	63
55) 4-Nitrophenol	15.016	109	20095	5.171	ng/ul	96
56) Dibenzofuran	15.216	168	435040	9.930	ng/ul	98
57) 2,4-Dinitrotoluene	15.175	165	72299	8.156	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.439	232	62185	8.259	ng/ul	96
59) Diethylphthalate	15.628	149	336694	9.671	ng/ul	98
61) Fluorene	15.869	166	354034	10.108	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.857	204	178256	10.070	ng/ul	99
63) 4-Nitroaniline	15.875	138	14726	3.594	ng/ul#	73
66) 4,6-Dinitro-2-methylph...	15.939	198	17313	4.102	ng/ul#	97
67) N-Nitrosodiphenylamine	16.069	169	283646	9.981	ng/ul	98
68) 4-Bromophenyl-phenylether	16.757	248	103964	9.920	ng/ul	98
69) Hexachlorobenzene	16.875	284	123108	9.965	ng/ul	98
70) Atrazine	17.022	200	91786	8.921	ng/ul	98
71) Pentachlorophenol	17.222	266	24454	4.468	ng/ul	94
72) Phenanthrene	17.622	178	529874	10.002	ng/ul	99
74) Anthracene	17.710	178	535395	10.089	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.628	216	161958	10.208	ng/uL	98
76) Pentachlorobenzene	15.139	250	156969	10.307	ng/uL	98
77) Carbazole	17.975	167	422908	9.343	ng/ul	100
78) Di-n-butylphthalate	18.510	149	532083	9.475	ng/ul	100
80) Fluoranthene	19.569	202	573030	9.819	ng/ul	99
82) Pyrene	19.922	202	623925	10.060	ng/ul	99
83) Butylbenzylphthalate	20.780	149	216079	9.258	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.569	252	156310	8.293	ng/ul	97
85) Benzo(a)anthracene	21.645	228	570265	9.791	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.545	149	329731	9.319	ng/ul	99
87) Chrysene	21.698	228	584938	10.090	ng/ul	100
89) Di-n-octyl phthalate	22.539	149	567722	9.169	ng/ul	100
90) Benzo(b)fluoranthene	23.463	252	563538	9.486	ng/ul	98
91) Benzo(k)fluoranthene	23.515	252	620151	10.062	ng/ul	99
93) Benzo(a)pyrene	24.151	252	526490	9.745	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	27.033	276	698379	9.734	ng/ul	98
95) Dibenzo(a,h)anthracene	27.057	278	585220	9.862	ng/ul	99
96) Benzo(g,h,i)perylene	27.886	276	577272	9.749	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_P
ClientSampleId :
SSTD010647

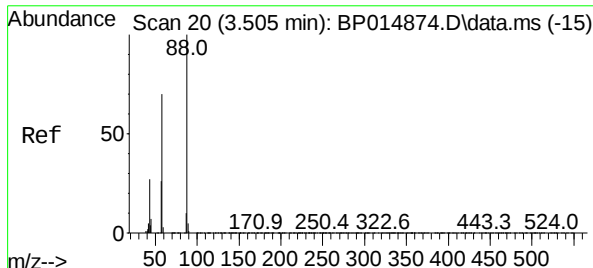

1,4-Dioxane

Concen: 3.926 ng/uL

RT: 3.505 min Scan# 2

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647





Tgt Ion: 88 Resp: 25139

Ion Ratio Lower Upper

88 100

43 28.1 22.2 33.4

58 71.8 55.1 82.7

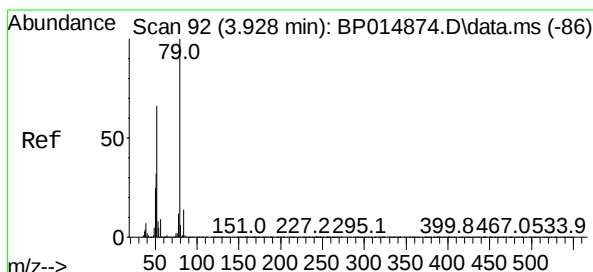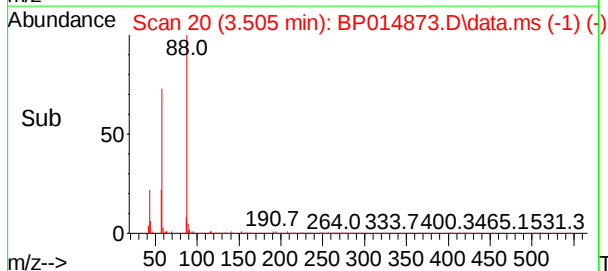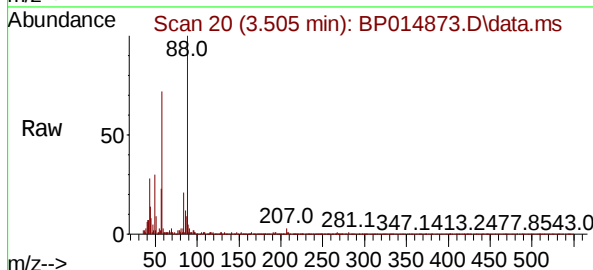

Pyridine

Concen: 9.272 ng/uL

RT: 3.928 min Scan# 92

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion: 79 Resp: 140565


Ion Ratio Lower Upper

79 100

52 70.3 53.2 79.8

51 34.1 26.5 39.7

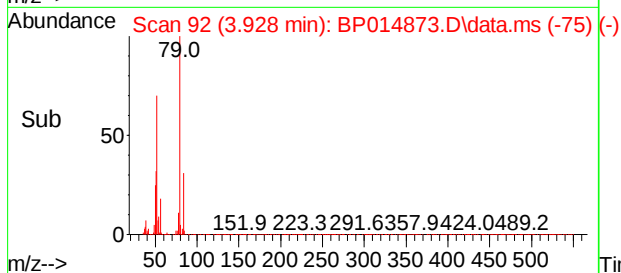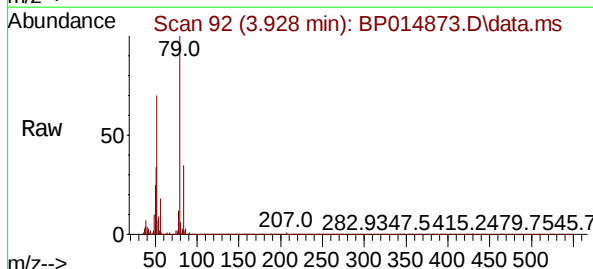

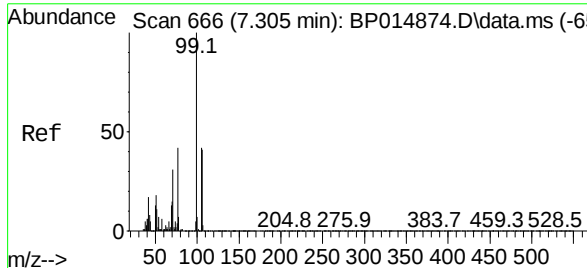

Benzaldehyde

Concen: 7.611 ng/u1

RT: 7.305 min Scan# 666

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647





Tgt Ion: 77 Resp: 36209

Ion Ratio Lower Upper

77 100

105 100.2 79.4 119.0

106 97.1 77.6 116.4

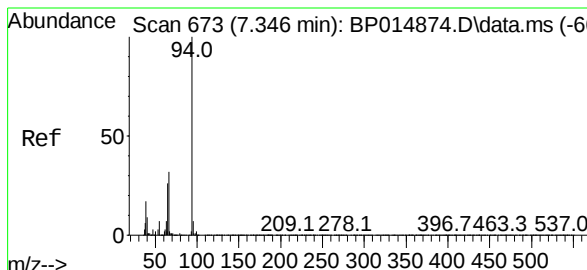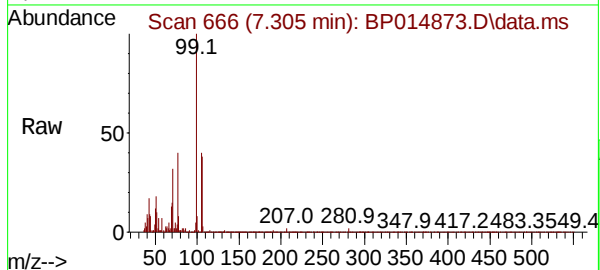

Phenol

Concen: 8.575 ng/u1

RT: 7.340 min Scan# 672

Delta R.T. -0.006 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion: 94 Resp: 150836


Ion Ratio Lower Upper

94 100

65 26.4 21.1 31.7

66 33.6 26.3 39.5


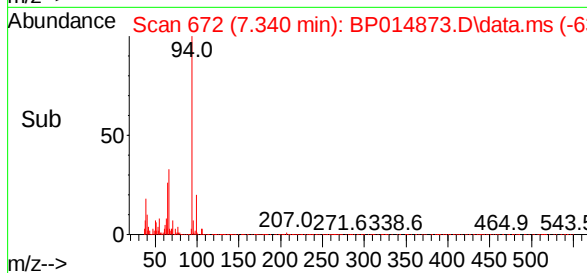

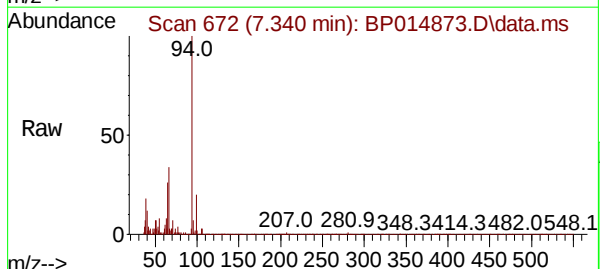


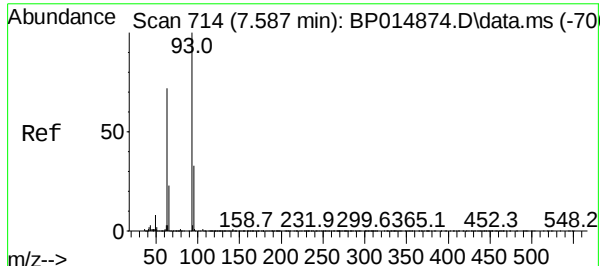

Bis(2-Chloroethyl)ether
 Concen: 9.365 ng/ul
 RT: 7.587 min Scan#
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	93	Resp:	141168
Ion	Ratio	Lower	Upper
93	100		
63	71.5	57.9	86.9
95	33.9	26.4	39.6

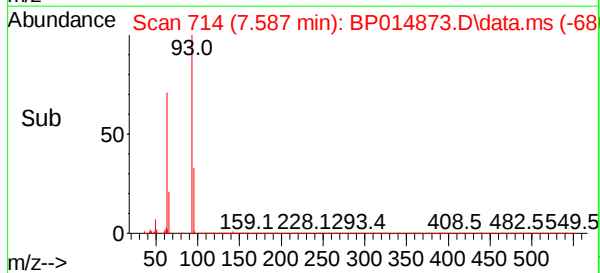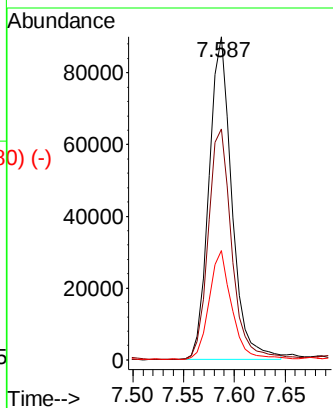

2-Chlorophenol
 Concen: 9.436 ng/ul
 RT: 7.734 min Scan# 739
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	128	Resp:	130041
Ion	Ratio	Lower	Upper
128	100		
64	44.1	35.5	53.3
130	31.3	26.8	40.2

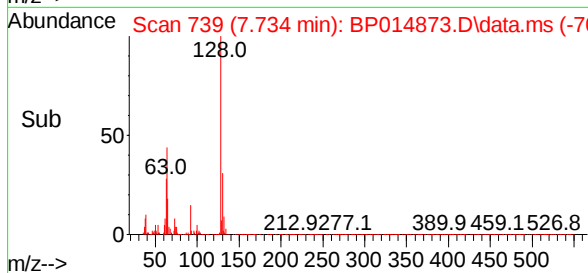

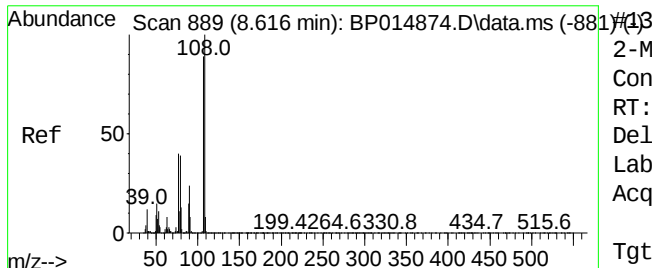

2-Methylphenol

Concen: 8.906 ng/ul

RT: 8.616 min Scan# 889

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :





SSTD010647

Tgt Ion:108 Resp: 121370

Ion Ratio Lower Upper

108 100

107 86.1 71.3 106.9

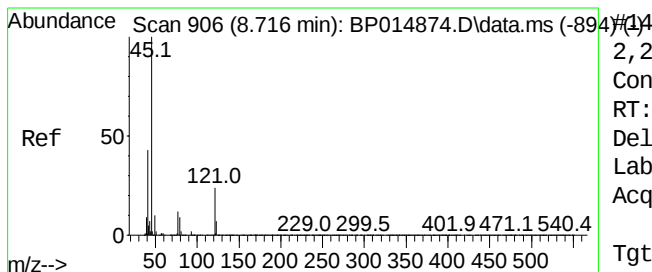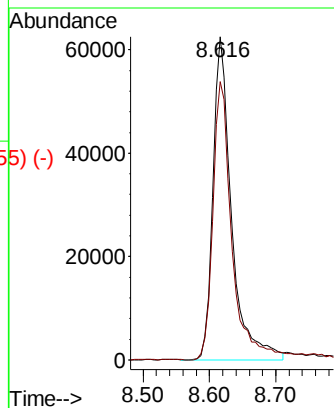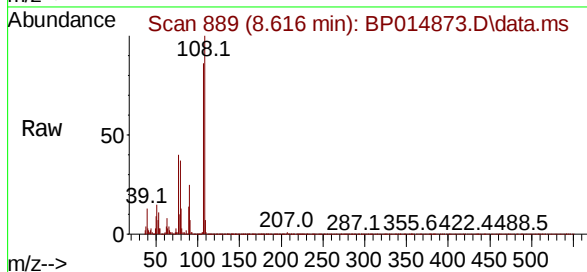

2,2'-oxybis(1-Chloropropane)

Concen: 10.083 ng/ul

RT: 8.710 min Scan# 905

Delta R.T. -0.006 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion: 45 Resp: 191209


Ion Ratio Lower Upper

45 100

77 16.1 12.7 19.1

79 13.3 10.3 15.5



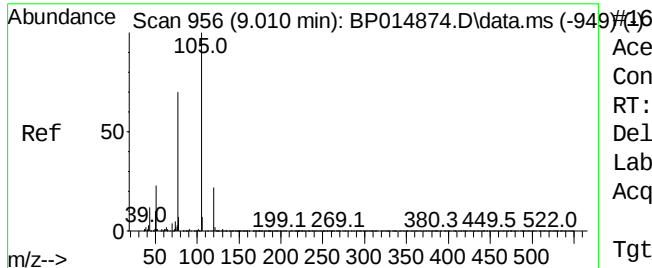

Acetophenone

Concen: 9.353 ng/ul

RT: 9.010 min Scan#

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647





Tgt Ion:105 Resp: 196344

Ion Ratio Lower Upper

105 100

77 79.1 59.8 89.6

51 24.9 19.4 29.2

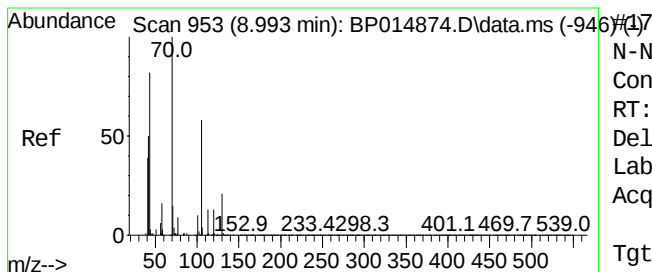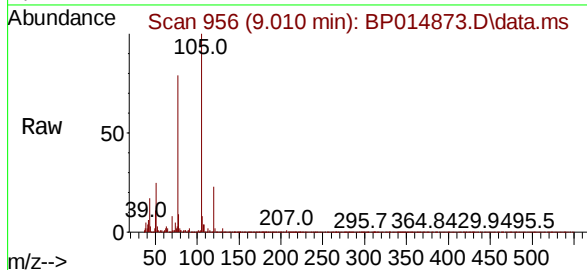

N-Nitroso-di-n-propylamine

Concen: 9.631 ng/ul

RT: 8.987 min Scan# 952

Delta R.T. -0.006 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Tgt Ion: 70 Resp: 95984




Ion Ratio Lower Upper


70 100

42 53.7 40.9 61.3

101 9.6 8.2 12.4

130 21.5 16.6 24.8

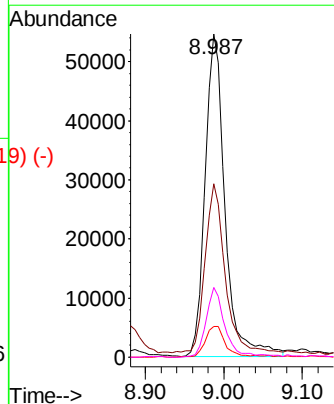

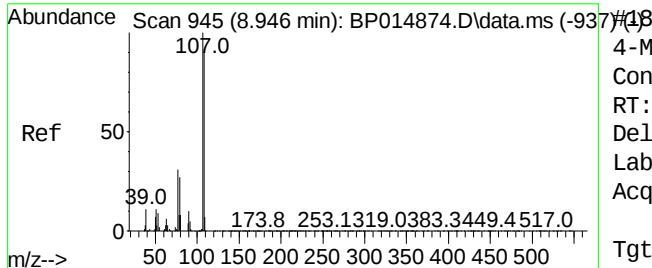

4-Methylphenol

Concen: 8.673 ng/u1

RT: 8.946 min Scan# 945

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :





SSTD010647

Tgt Ion:108 Resp: 124728

Ion Ratio Lower Upper

108 100

107 105.4 89.2 133.8

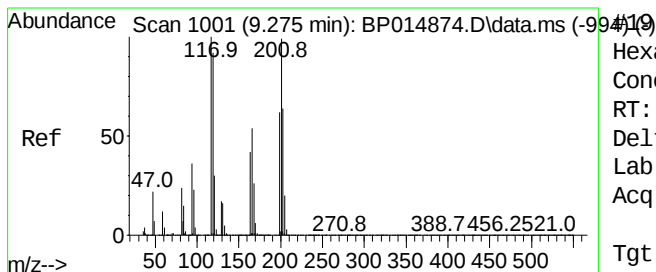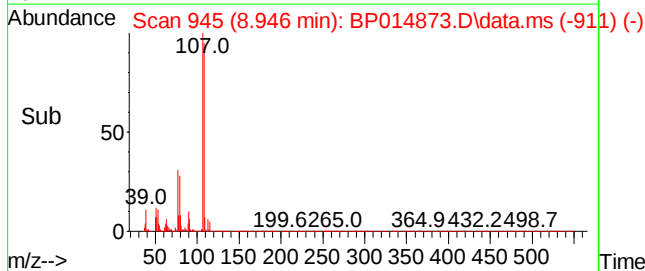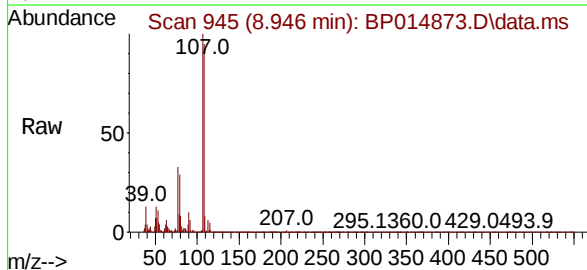

Hexachloroethane

Concen: 9.880 ng/u1

RT: 9.275 min Scan# 1001

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion:117 Resp: 64142

Ion Ratio Lower Upper

117 100

201 108.8 78.9 118.3

199 66.3 49.4 74.0

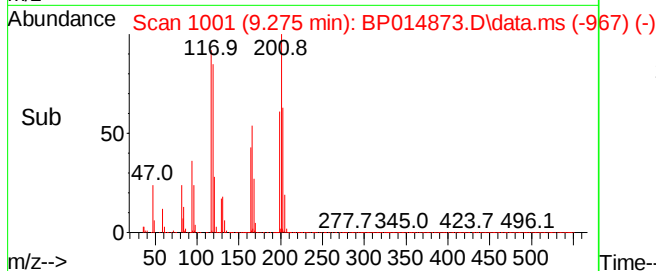

Abundance Scan 1021 (9.393 min): BP014874.D\data.ms (-1021-)

Nitrobenzene

Concen: 9.557 ng/ul

RT: 9.393 min Scan# 1021

Delta R.T. -0.000 min

Lab File: BP014873.D


Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647

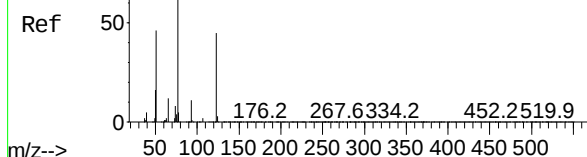




Tgt Ion: 77 Resp: 147349

Ion Ratio Lower Upper

77 100

123 45.0 35.7 53.5

65 12.6 10.0 15.0

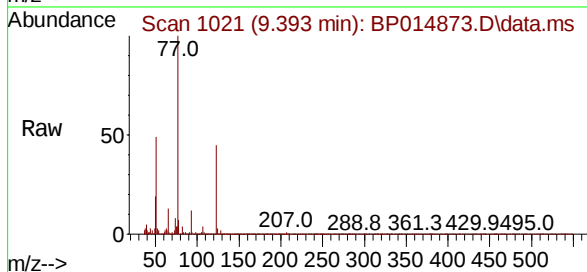

Abundance Scan 1111 (9.922 min): BP014874.D\data.ms (-1111-)

Isophorone

Concen: 9.229 ng/ul

RT: 9.922 min Scan# 1111

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion: 82 Resp: 256335


Ion Ratio Lower Upper

82 100

95 6.7 5.4 8.2

138 17.5 13.3 19.9


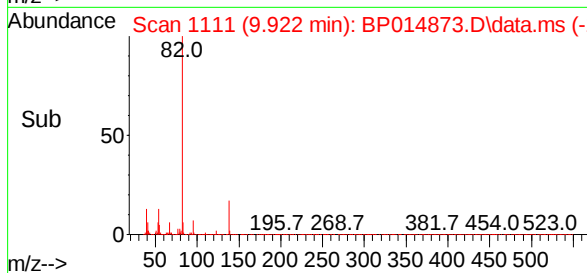






Scan 1144 (10.116 min): BP014874.D\data.ms (-1125) (-)
 2-Nitrophenol
 Concen: 8.135 ng/ul
 RT: 10.116 min Scan# 1144
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument : BNA_P
 ClientSampleId : SST010647


Tgt Ion:	139	Resp:	50309
Ion Ratio	Lower	Upper	
139	100		
65	48.3	37.0	55.4
109	26.7	22.0	33.0

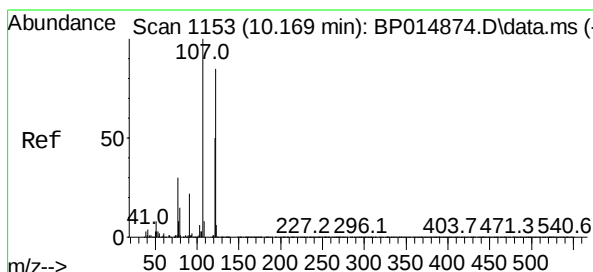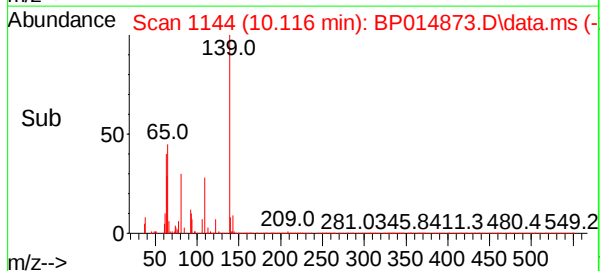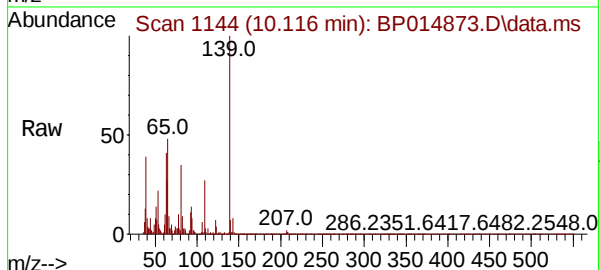

Scan 1153 (10.169 min): BP014874.D\data.ms (-1126) (-)
 2,4-Dimethylphenol
 Concen: 9.496 ng/ul
 RT: 10.169 min Scan# 1153
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	107	Resp:	142007
Ion Ratio	Lower	Upper	
107	100		
121	51.0	40.4	60.6
122	89.7	69.3	103.9



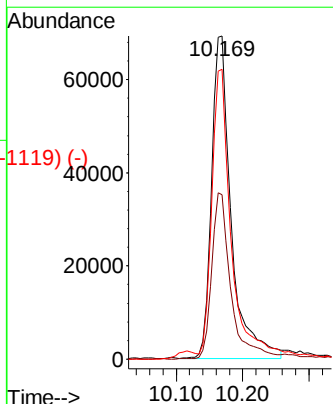



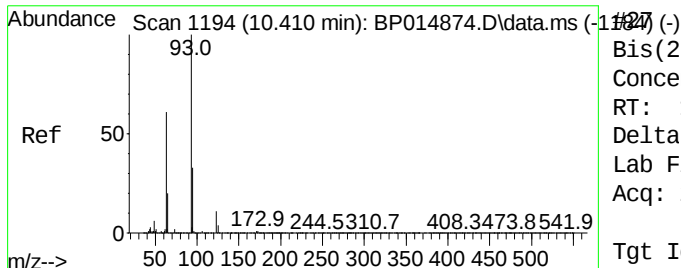

Bis(2-Chloroethoxy)methane
 Concen: 9.630 ng/ul
 RT: 10.404 min Scan# 1194
 Delta R.T. -0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	93	Resp:	184448
Ion	Ratio	Lower	Upper
93	100		
95	32.4	26.1	39.1
123	10.2	8.8	13.2

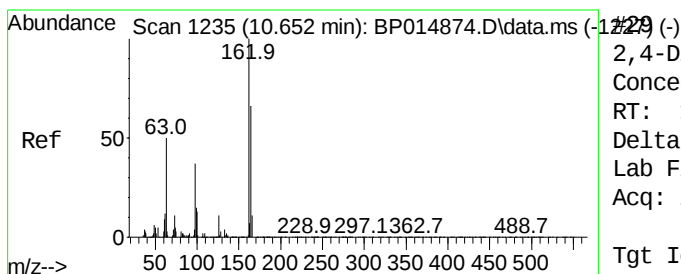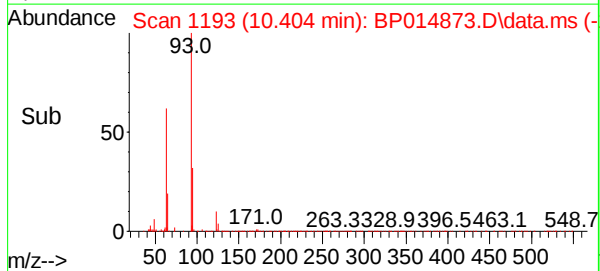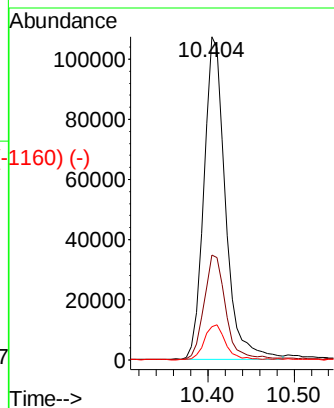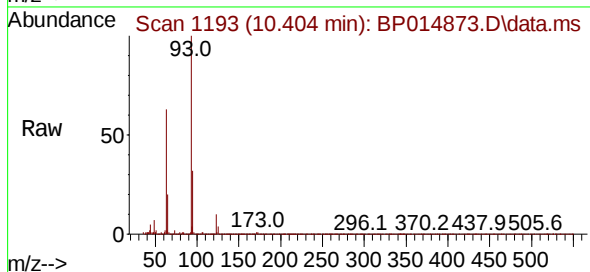

2,4-Dichlorophenol
 Concen: 9.269 ng/ul
 RT: 10.651 min Scan# 1235
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	162	Resp:	111802
Ion	Ratio	Lower	Upper
162	100		
164	67.5	52.7	79.1
98	37.1	29.4	44.2


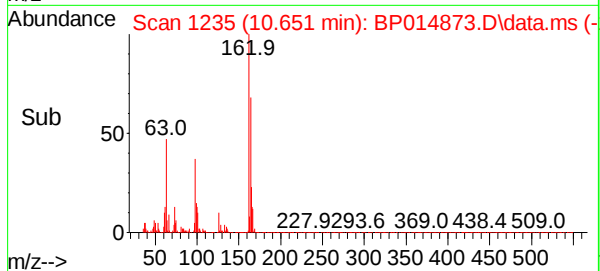

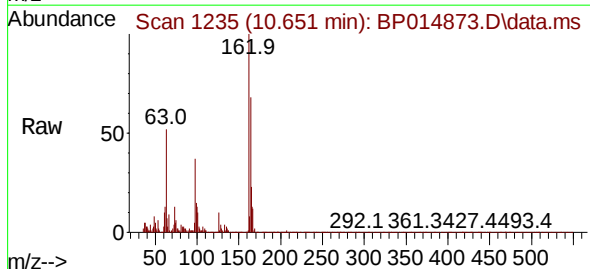




Naphthalene
 Concen: 9.849 ng/ul
 RT: 11.063 min Scan# 1305
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	128	Resp:	458416
Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.9	13.3
127	13.1	10.4	15.6

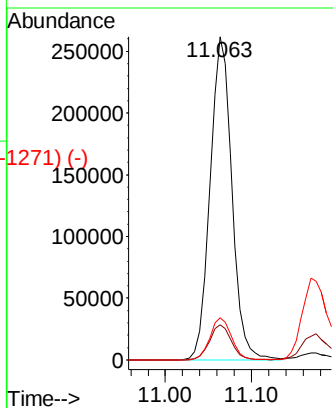

4-Chloroaniline
 Concen: 8.948 ng/ul
 RT: 11.169 min Scan# 1323
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	127	Resp:	161744
Ion	Ratio	Lower	Upper
127	100		
129	29.2	25.9	38.9









Hexachlorobutadiene
 Concen: 9.999 ng/ul
 RT: 11.351 min Scan# 1354
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	225	Resp:	91920
Ion	Ratio	Lower	Upper
225	100		
223	59.4	49.7	74.5
227	61.9	51.8	77.6

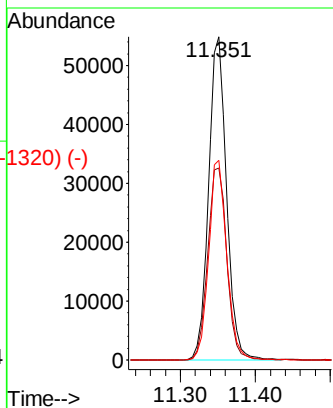

Caprolactam
 Concen: 4.493 ng/ul
 RT: 11.928 min Scan# 1452
 Delta R.T. -0.018 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	113	Resp:	13619
Ion	Ratio	Lower	Upper
113	100		
55	153.4	133.7	200.5
56	114.7	98.7	148.1









Scan 1511 (12.275 min): BP014874.D\data.ms (-1535) (-)
 4-Chloro-3-methylphenol
 Concen: 9.067 ng/ul
 RT: 12.281 min Scan# 1511
 Delta R.T. 0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument : BNA_P
 ClientSampleId : SST010647


Tgt Ion:	107	Resp:	111320
Ion	Ratio	Lower	Upper
107	100		
144	24.7	19.8	29.8
142	79.0	62.4	93.6



Scan 1577 (12.663 min): BP014874.D\data.ms (-1536) (-)
 2-Methylnaphthalene
 Concen: 9.781 ng/ul
 RT: 12.663 min Scan# 1577
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	142	Resp:	287288
Ion	Ratio	Lower	Upper
142	100		
141	89.4	70.5	105.7









1-Methylnaphthalene
 Concen: 9.794 ng/u1
 RT: 12.881 min Scan# 1614
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010647


Tgt Ion:	142	Resp:	288807
Ion	Ratio	Lower	Upper
142	100		
141	92.1	73.3	109.9
116	4.0	3.0	4.4

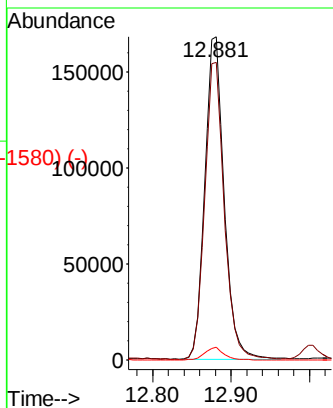

1,2,4,5-Tetrachlorobenzene
 Concen: 9.959 ng/u1
 RT: 13.022 min Scan# 1638
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	216	Resp:	160370
Ion	Ratio	Lower	Upper
216	100		
214	80.7	63.0	94.6
179	19.9	16.2	24.4
108	17.7	13.6	20.4



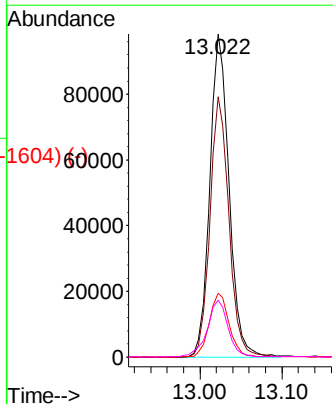



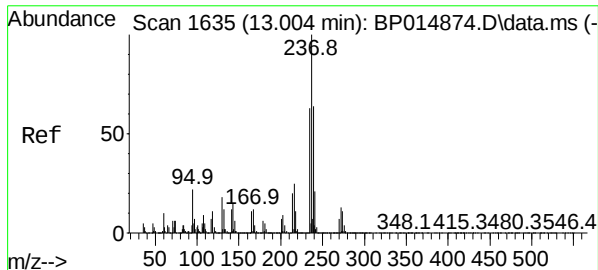

Hexachlorocyclopentadiene
Concen: 8.268 ng/ul
RT: 13.004 min Scan# 1635
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22




Instrument :
BNA_P
ClientSampleId :
SSTD010647


Tgt Ion:	237	Resp:	83578
Ion	Ratio	Lower	Upper
237	100		
235	61.7	50.6	75.8
272	13.9	10.7	16.1

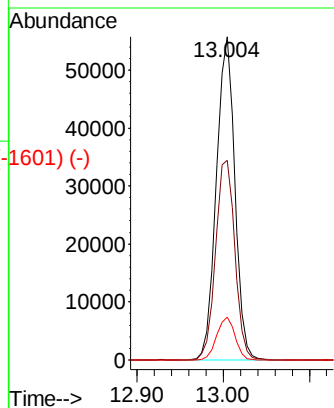

2,4,6-Trichlorophenol
Concen: 8.640 ng/ul
RT: 13.257 min Scan# 1678
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	196	Resp:	70694
Ion	Ratio	Lower	Upper
196	100		
198	98.9	79.1	118.7
200	31.1	26.5	39.7







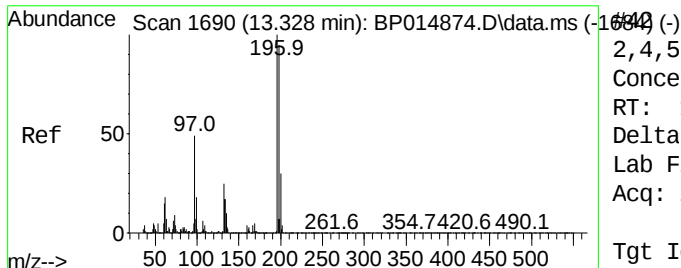

2,4,5-Trichlorophenol
Concen: 8.330 ng/ul
RT: 13.328 min Scan# 1690
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22




Instrument :
BNA_P
ClientSampleId :
SSTD010647

Tgt Ion:	196	Resp:	79258
Ion	Ratio	Lower	Upper
196	100		
198	98.2	76.6	115.0
200	31.8	24.0	36.0

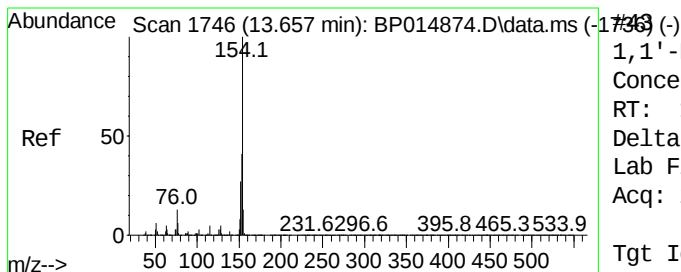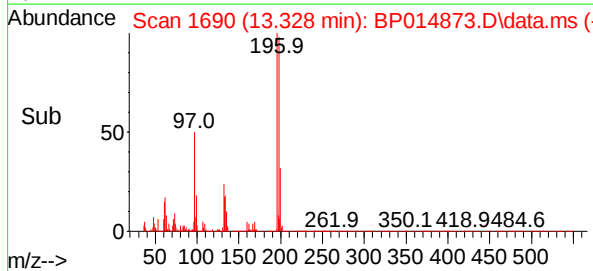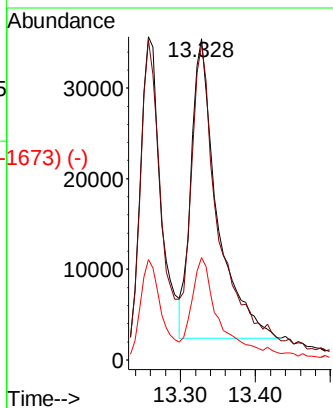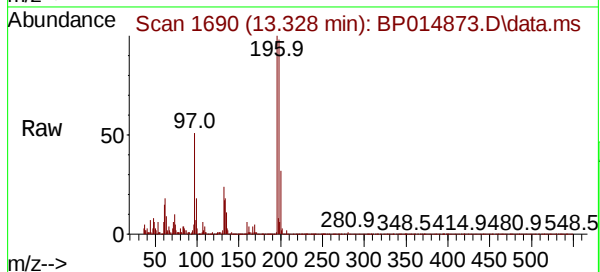

1,1'-Biphenyl
Concen: 10.026 ng/ul
RT: 13.657 min Scan# 1746
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	154	Resp:	387629
Ion	Ratio	Lower	Upper
154	100		
153	38.9	32.5	48.7
76	13.4	10.8	16.2

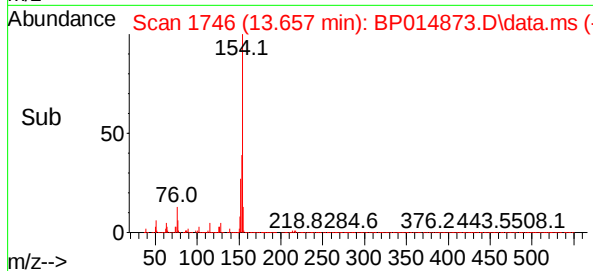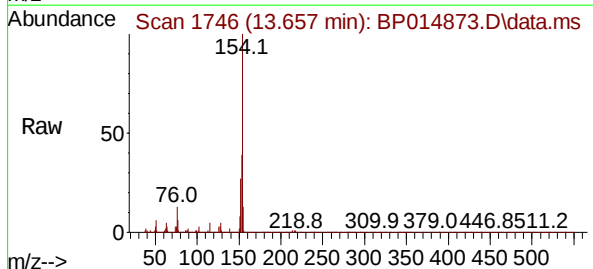

Abundance Scan 1754 (13.704 min): BP014874.D\data.ms (-1746) (-)

2-Chloronaphthalene

Concen: 10.011 ng/ul

RT: 13.704 min Scan# 1754

Delta R.T. -0.000 min

Lab File: BP014873.D


Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647

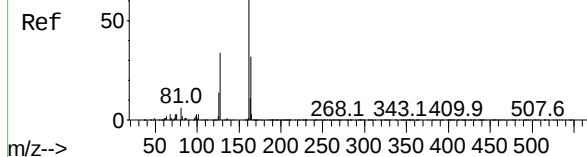




Tgt Ion:162 Resp: 304834

Ion Ratio Lower Upper

162 100

164 31.7 25.6 38.4

127 37.4 30.3 45.5

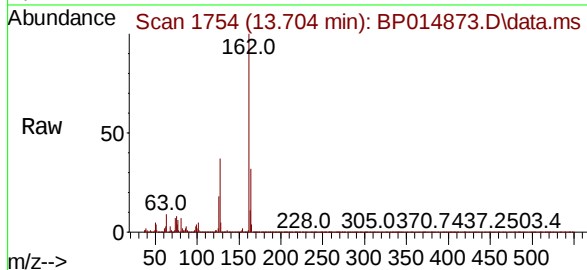

Abundance Scan 1788 (13.904 min): BP014874.D\data.ms (-1745) (-)

2-Nitroaniline


Concen: 8.383 ng/ul

RT: 13.904 min Scan# 1788

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

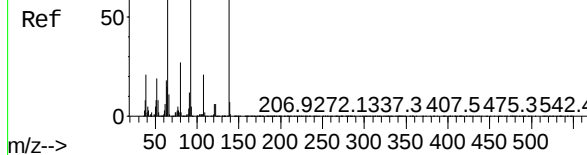




Tgt Ion: 65 Resp: 55766


Ion Ratio Lower Upper

65 100

92 74.2 58.6 87.8

138 109.5 84.8 127.2









Dimethylphthalate
 Concen: 9.781 ng/ul
 RT: 14.269 min Scan# 1850
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	163	Resp:	349191
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.2	4.8
164	10.3	8.3	12.5



2,6-Dinitrotoluene
 Concen: 8.620 ng/ul
 RT: 14.387 min Scan# 1870
 Delta R.T. -0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	165	Resp:	55438
Ion	Ratio	Lower	Upper
165	100		
89	64.4	45.2	67.8
121	23.9	16.3	24.5



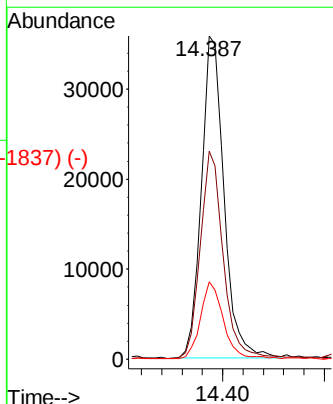





Acenaphthylene
 Concen: 9.851 ng/ul
 RT: 14.545 min Scan# 1897
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	152	Resp:	454247
Ion	Ratio	Lower	Upper
152	100		
151	19.6	16.0	24.0
153	13.3	10.6	15.8



3-Nitroaniline
 Concen: 0.539 ng/ul
 RT: 14.781 min Scan# 1937
 Delta R.T. 0.059 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	138	Resp:	2827
Ion	Ratio	Lower	Upper
138	100		
108	13.4	9.0	13.4
92	106.1	94.2	141.4


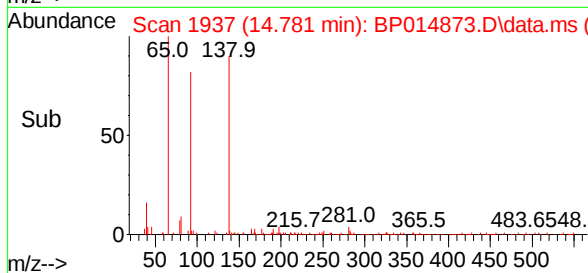




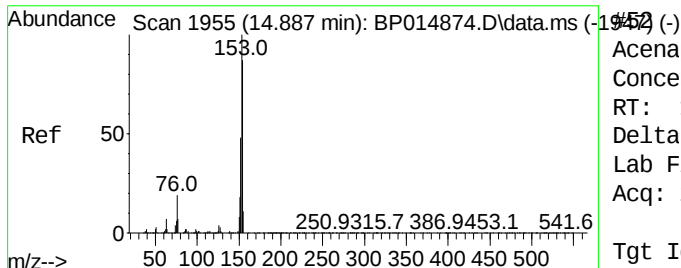

Acenaphthene
 Concen: 9.972 ng/u1
 RT: 14.887 min Scan# 1955
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	153	Resp:	316942
Ion	Ratio	Lower	Upper
153	100		
152	48.2	38.5	57.7
154	86.6	69.4	104.2

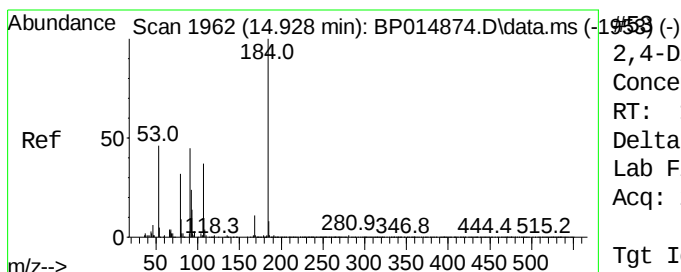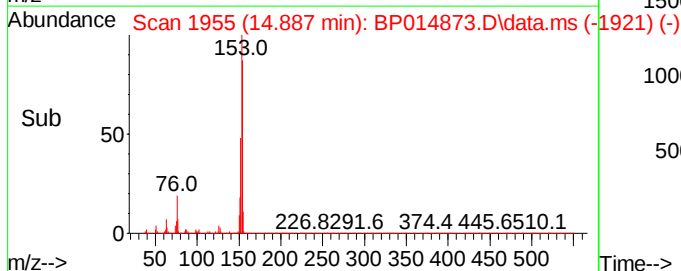

2,4-Dinitrophenol
 Concen: 0.892 ng/u1
 RT: 14.922 min Scan# 1961
 Delta R.T. -0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	184	Resp:	2117
Ion	Ratio	Lower	Upper
184	100		
63	72.4	57.6	86.4
154	130.2	54.6	82.0#


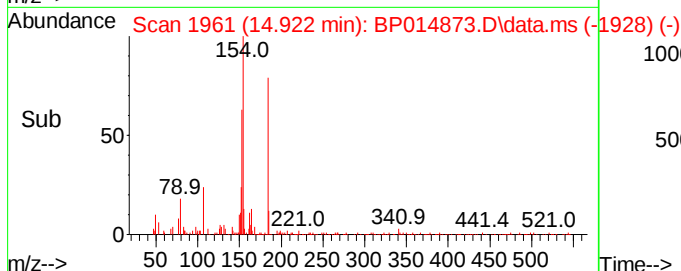
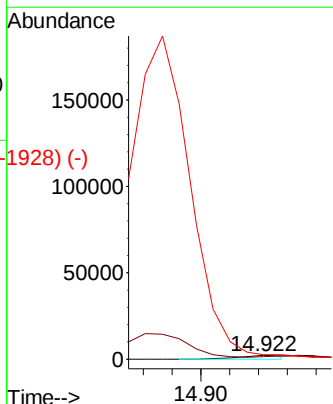
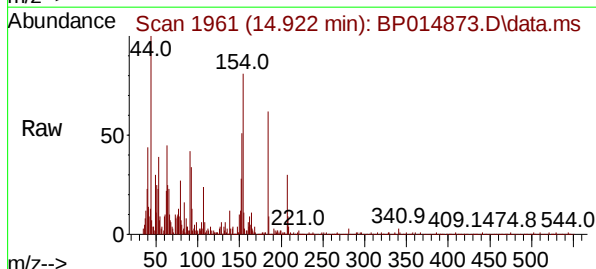




4-Nitrophenol
 Concen: 5.171 ng/ul
 RT: 15.016 min Scan# 1976
 Delta R.T. 0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	109	Resp:	20095
Ion Ratio	Lower	Upper	
109	100		
139	130.0	107.8	161.8
65	130.1	108.6	162.8

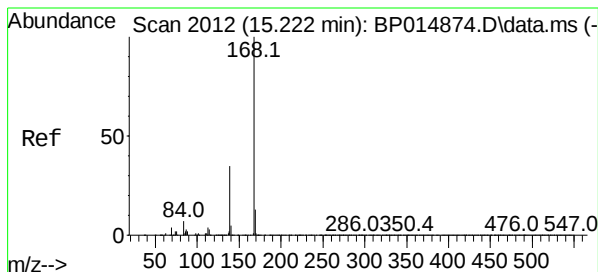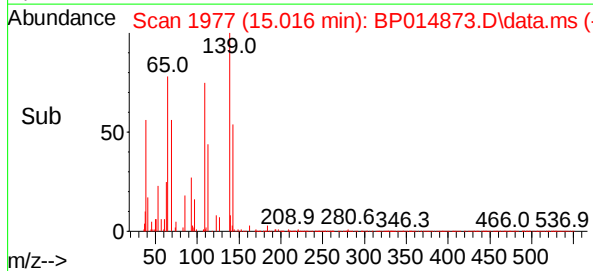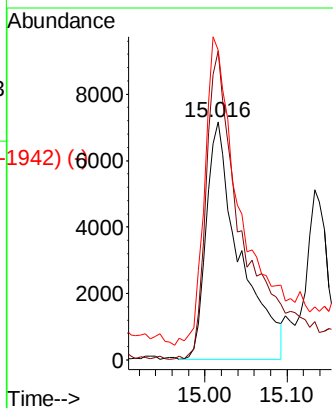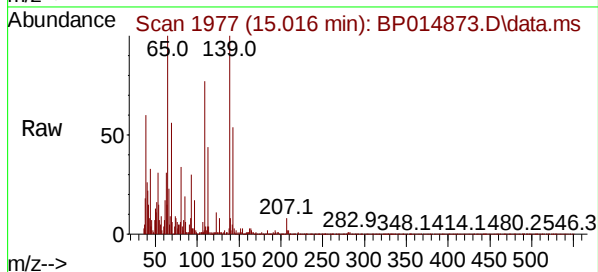

Dibenzofuran
 Concen: 9.930 ng/ul
 RT: 15.216 min Scan# 2011
 Delta R.T. -0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	168	Resp:	435040
Ion Ratio	Lower	Upper	
168	100		
139	35.8	27.8	41.8


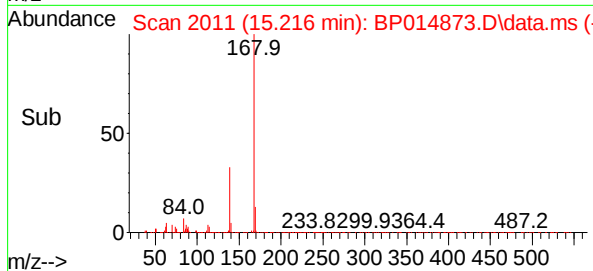






2,4-Dinitrotoluene
 Concen: 8.156 ng/ul
 RT: 15.175 min Scan# 1958
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010647


Tgt Ion:	165	Resp:	72299
Ion Ratio	Lower	Upper	
165	100		
63	42.5	33.9	50.9
182	2.5	2.1	3.1



2,3,4,6-Tetrachlorophenol
 Concen: 8.259 ng/ul
 RT: 15.439 min Scan# 2049
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	232	Resp:	62185
Ion Ratio	Lower	Upper	
232	100		
131	46.0	34.4	51.6
130	2.3	1.8	2.6
166	30.1	25.9	38.9


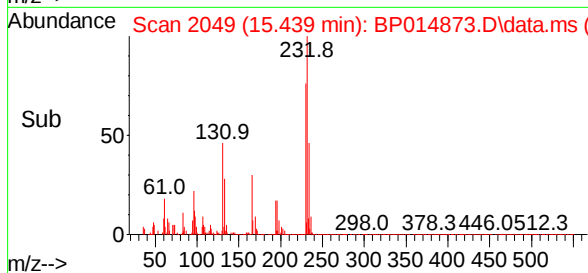
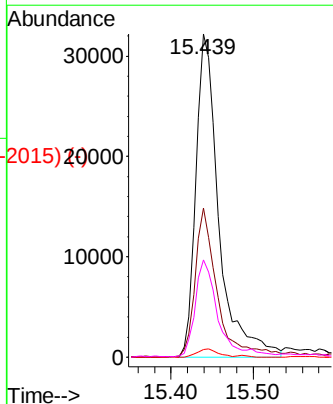





Diethylphthalate
 Concen: 9.671 ng/u1
 RT: 15.628 min Scan# 2081
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647

Tgt Ion:	149	Resp:	336694
Ion	Ratio	Lower	Upper
149	100		
177	21.5	18.0	27.0
150	12.0	9.8	14.8

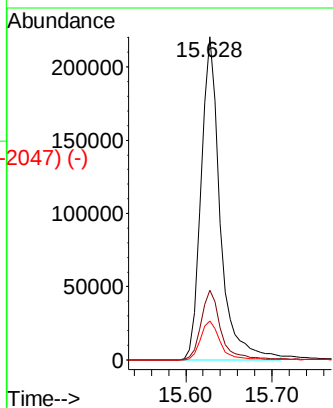

Fluorene
 Concen: 10.108 ng/u1
 RT: 15.869 min Scan# 2122
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	166	Resp:	354034
Ion	Ratio	Lower	Upper
166	100		
165	99.2	79.8	119.6
167	13.4	11.0	16.6



Abundance Scan 2120 (15.857 min): BP014874.D\data.ms (-2160) (-)

4-Chlorophenyl-phenylether

Concen: 10.070 ng/ul

RT: 15.857 min Scan# 2120

Delta R.T. -0.000 min

Lab File: BP014873.D


Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647

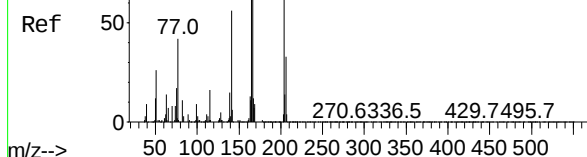



Tgt Ion:204 Resp: 178256

Ion Ratio Lower Upper


204 100

206 32.7 26.1 39.1

141 54.6 44.6 67.0

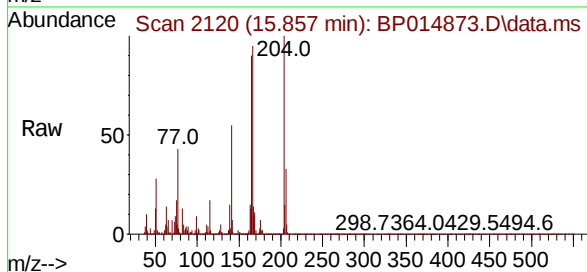

Abundance Scan 2120 (15.857 min): BP014873.D\data.ms (-2086) (-)

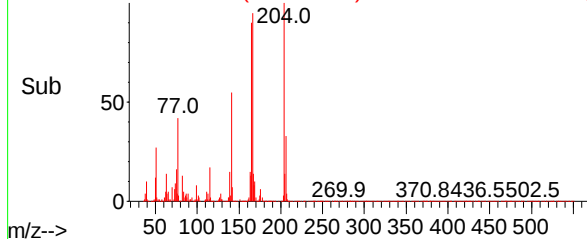

Abundance Scan 2124 (15.881 min): BP014874.D\data.ms (-2163) (-)

4-Nitroaniline

Concen: 3.594 ng/ul

RT: 15.875 min Scan# 2123

Delta R.T. -0.006 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion:138 Resp: 14726

Ion Ratio Lower Upper

138 100

92 38.2 44.2 66.2#


108 49.2 60.1 90.1#

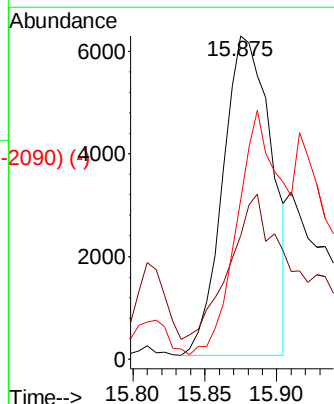

Abundance Scan 2123 (15.875 min): BP014873.D\data.ms (-2090) (-)



Abundance Scan 2134 (15.940 min): BP014874.D\data.ms (-2134) (-)

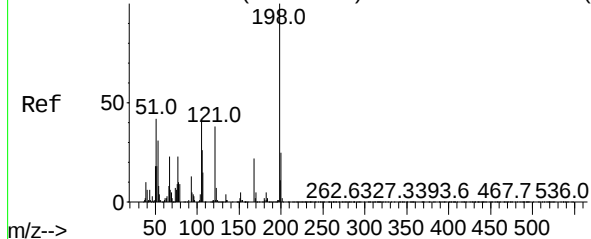

4,6-Dinitro-2-methylphenol

Concen: 4.102 ng/ul

RT: 15.939 min Scan# 2134

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647

Tgt Ion:198 Resp: 17313



Ion Ratio Lower Upper

198 100


182 8.2 4.2 6.2#

77 24.8 20.4 30.6


Abundance Scan 2134 (15.939 min): BP014873.D\data.ms

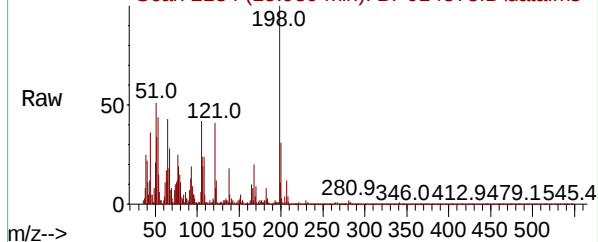

Abundance Scan 2134 (15.939 min): BP014873.D\data.ms (-2100) (-)

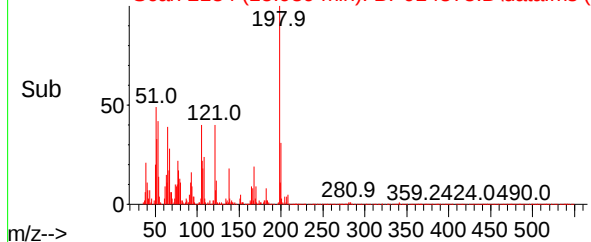

Abundance Scan 2156 (16.069 min): BP014874.D\data.ms (-2156) (-)

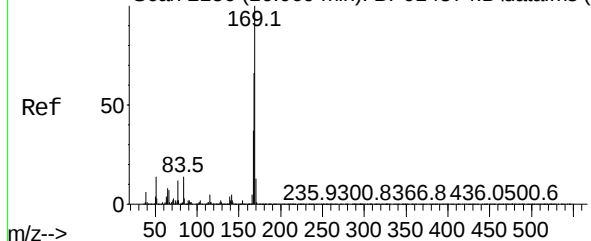

N-Nitrosodiphenylamine

Concen: 9.981 ng/ul

RT: 16.069 min Scan# 2156

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22

Tgt Ion:169 Resp: 283646



Ion Ratio Lower Upper

169 100


168 67.9 53.1 79.7

167 36.5 29.9 44.9

Abundance Scan 2156 (16.069 min): BP014873.D\data.ms

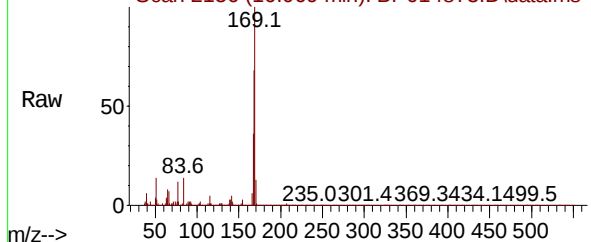

Abundance Scan 2156 (16.069 min): BP014873.D\data.ms (-2122) (-)

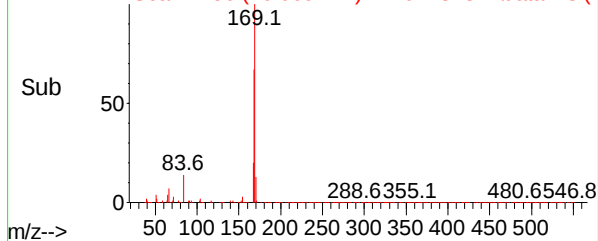

Abundance Scan 2273 (16.757 min): BP014874.D\data.ms (-2268) (-)

4-Bromophenyl-phenylether

Concen: 9.920 ng/ul

RT: 16.757 min Scan# 2273

Delta R.T. -0.000 min

Lab File: BP014873.D


Acq: 28 Apr 2023 13:22

Instrument :

BNA_P

ClientSampleId :

SSTD010647

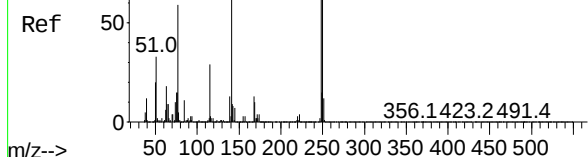




Tgt Ion:248 Resp: 103964

Ion Ratio Lower Upper

248 100

250 98.0 77.3 115.9

141 71.4 55.0 82.6

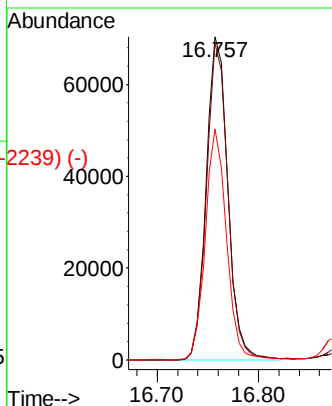

Abundance Scan 2293 (16.875 min): BP014874.D\data.ms (-2269) (-)

Hexachlorobenzene

Concen: 9.965 ng/ul

RT: 16.875 min Scan# 2293

Delta R.T. -0.000 min

Lab File: BP014873.D

Acq: 28 Apr 2023 13:22




Tgt Ion:284 Resp: 123108


Ion Ratio Lower Upper

284 100

142 33.5 27.6 41.4

249 31.3 24.4 36.6



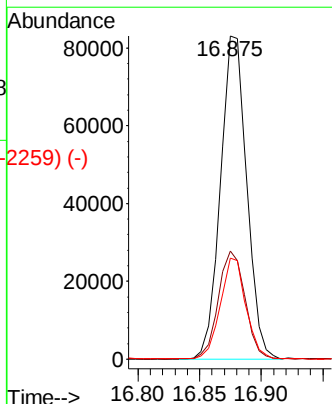



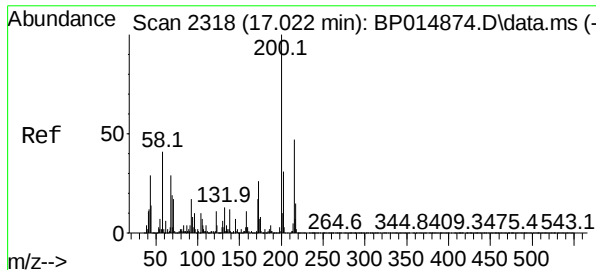

Atrazine
Concen: 8.921 ng/ul
RT: 17.022 min Scan# 2318
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22




Instrument :
BNA_P
ClientSampleId :
SSTD010647

Tgt Ion:	200	Resp:	91786
Ion Ratio	Lower	Upper	
200	100		
173	25.7	21.0	31.4
215	48.9	38.0	57.0

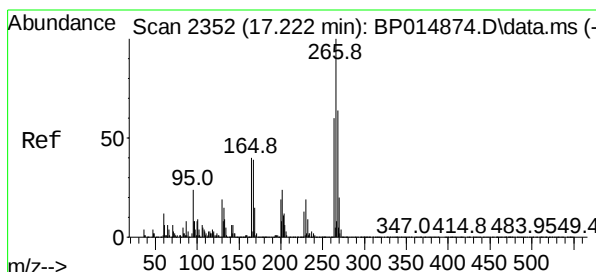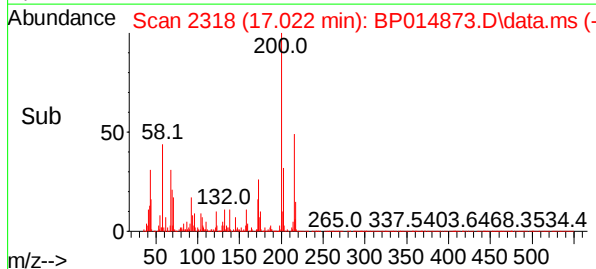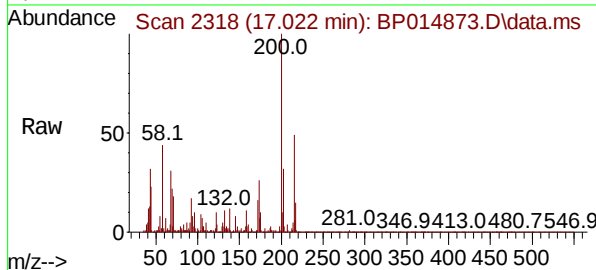


Pentachlorophenol
Concen: 4.468 ng/ul
RT: 17.222 min Scan# 2352
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	266	Resp:	24454
Ion Ratio	Lower	Upper	
266	100		
264	52.1	47.8	71.6
268	62.4	51.1	76.7

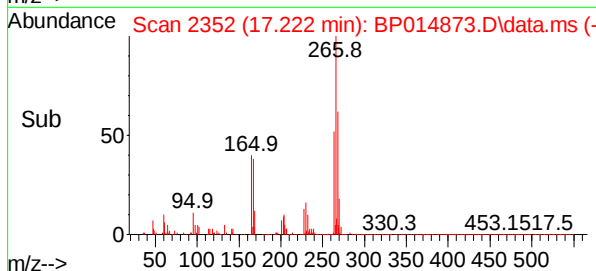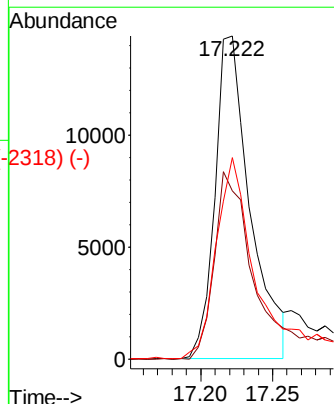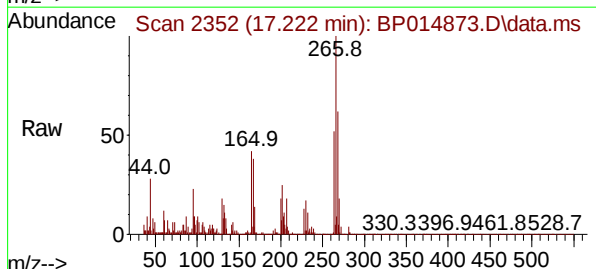




Abundance Scan 2420 (17.622 min): BP014874.D\data.ms (-2473) (-)

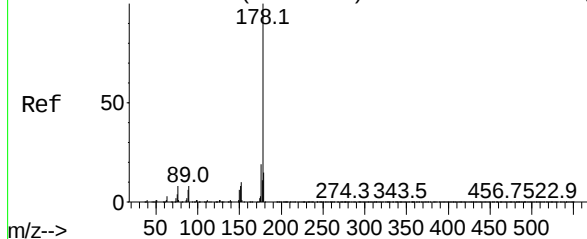


Phenanthrene
Concen: 10.002 ng/u1
RT: 17.622 min Scan# 2420
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Instrument :
BNA_P
ClientSampleId :
SSTD010647

Tgt Ion:	178	Resp:	529874
Ion Ratio	Lower	Upper	
178	100		
179	15.7	12.3	18.5
176	19.7	15.2	22.8



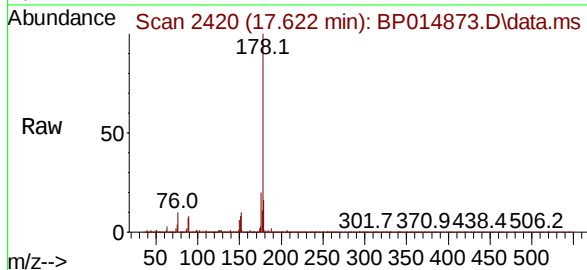



Abundance Scan 2435 (17.710 min): BP014874.D\data.ms (-2479) (-)

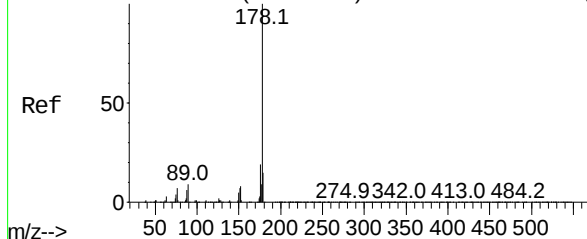

Anthracene
Concen: 10.089 ng/u1
RT: 17.710 min Scan# 2435
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	178	Resp:	535395
Ion Ratio	Lower	Upper	
178	100		
179	15.3	12.3	18.5
176	19.2	15.2	22.8









1,2,3,4-Tetrachlorobenzene
 Concen: 10.208 ng/uL
 RT: 13.628 min Scan# 1735
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010647


Tgt Ion:	216	Resp:	161958
Ion	Ratio	Lower	Upper
216	100		
214	75.8	62.1	93.1
218	47.4	38.6	58.0

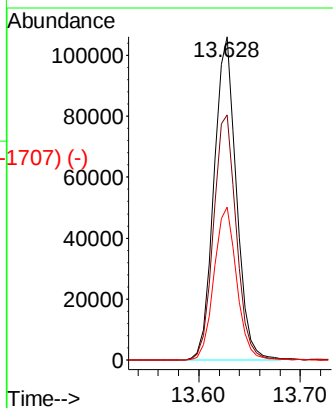

Pentachlorobenzene
 Concen: 10.307 ng/uL
 RT: 15.139 min Scan# 1998
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	250	Resp:	156969
Ion	Ratio	Lower	Upper
250	100		
248	60.0	50.5	75.7
252	66.0	52.3	78.5







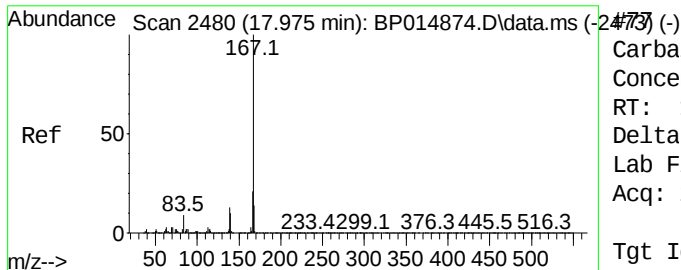

Carbazole
Concen: 9.343 ng/ul
RT: 17.975 min Scan# 2480
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22




Instrument :
BNA_P
ClientSampleId :
SSTD010647


Tgt Ion:	167	Resp:	422908
Ion	Ratio	Lower	Upper
167	100		
166	21.2	17.2	25.8
139	12.6	10.2	15.2

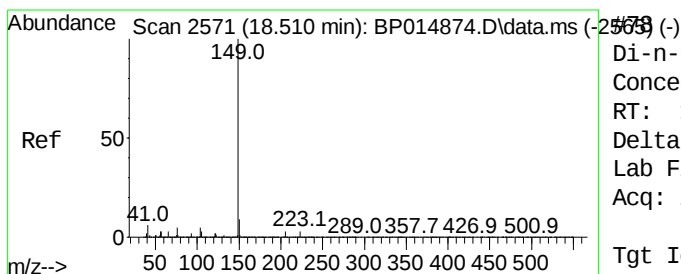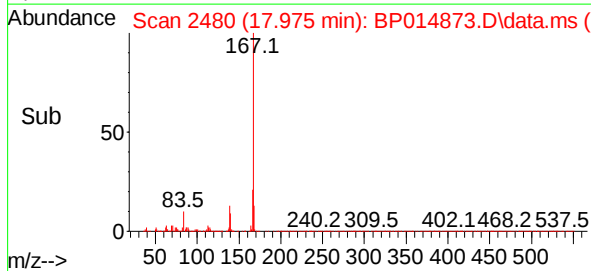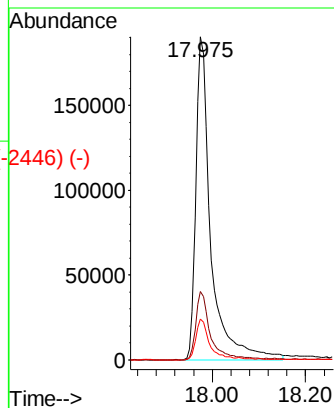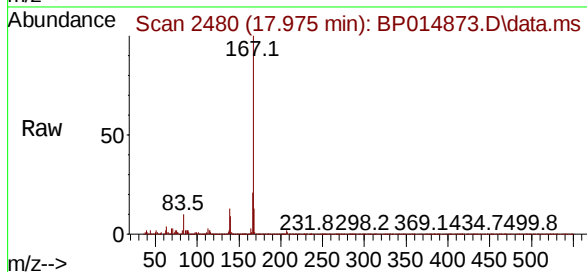

Di-n-butylphthalate
Concen: 9.475 ng/ul
RT: 18.510 min Scan# 2571
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	149	Resp:	532083
Ion	Ratio	Lower	Upper
149	100		
150	9.2	7.4	11.0
104	5.2	4.0	6.0


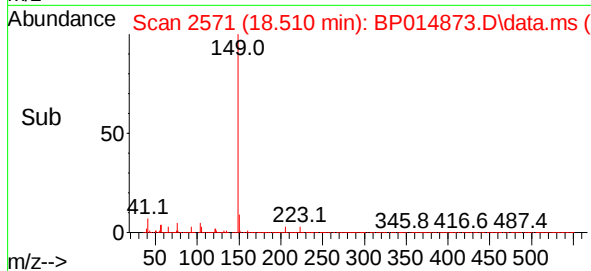




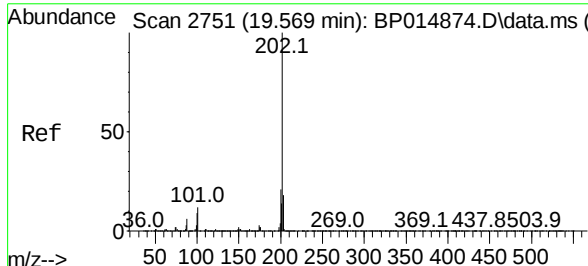

Scan 2751 (19.569 min): BP014874.D\data.ms (-2748) (-)
 Fluoranthene
 Concen: 9.819 ng/ul
 RT: 19.569 min Scan# 2751
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	202	Resp:	573030
Ion	Ratio	Lower	Upper
202	100		
101	11.5	9.4	14.2
100	8.9	7.3	10.9

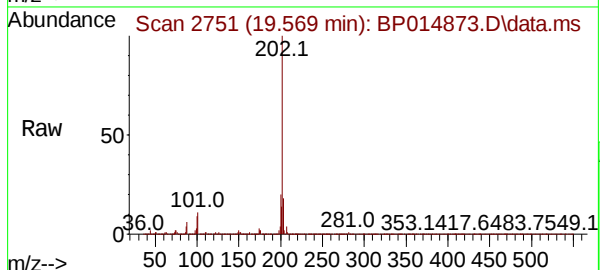

Scan 2811 (19.922 min): BP014874.D\data.ms (-2802) (-)
 Pyrene
 Concen: 10.060 ng/ul
 RT: 19.922 min Scan# 2811
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	202	Resp:	623925
Ion	Ratio	Lower	Upper
202	100		
101	13.3	10.9	16.3
100	10.8	8.6	12.8


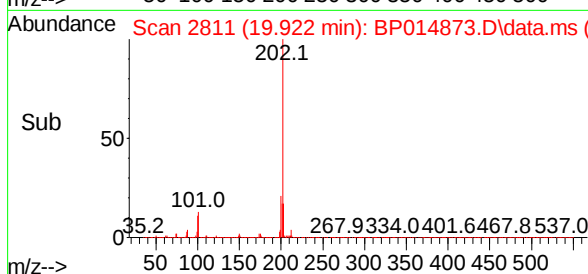




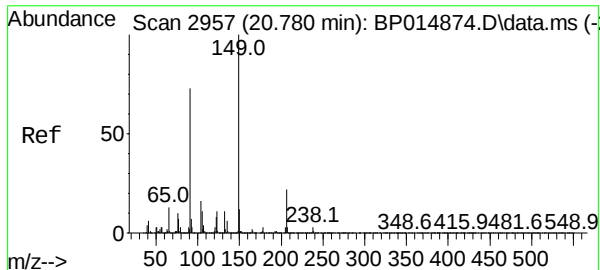

Butylbenzylphthalate
Concen: 9.258 ng/ul
RT: 20.780 min Scan# 2957
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22




Instrument :
BNA_P
ClientSampleId :
SSTD010647


Tgt Ion:	149	Resp:	216079
Ion	Ratio	Lower	Upper
149	100		
91	76.8	58.3	87.5
206	20.8	17.4	26.0

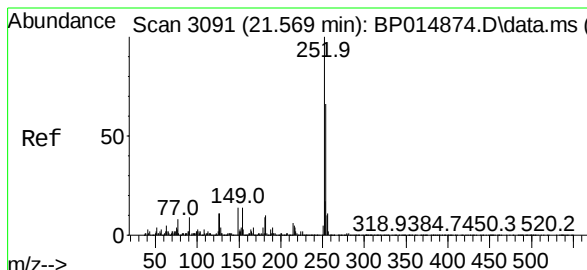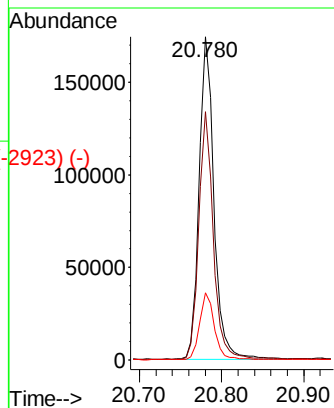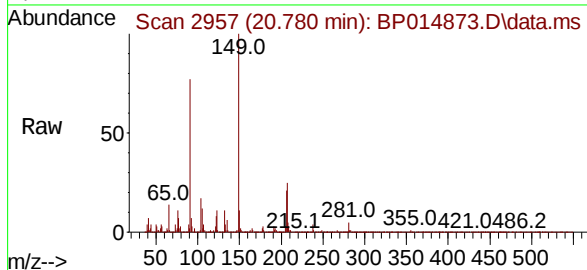

3,3'-Dichlorobenzidine
Concen: 8.293 ng/ul
RT: 21.569 min Scan# 3091
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	252	Resp:	156310
Ion	Ratio	Lower	Upper
252	100		
254	62.8	52.6	78.8
126	11.0	8.9	13.3


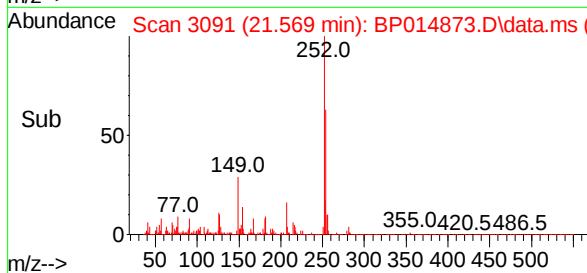






Scan 3104 (21.645 min): BP014874.D\data.ms (-3085) (-)
 Benzo(a)anthracene
 Concen: 9.791 ng/u1
 RT: 21.645 min Scan# 3104
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010647


Tgt Ion:	228	Resp:	570265
Ion	Ratio	Lower	Upper
228	100		
229	19.3	15.8	23.6
226	26.8	21.7	32.5

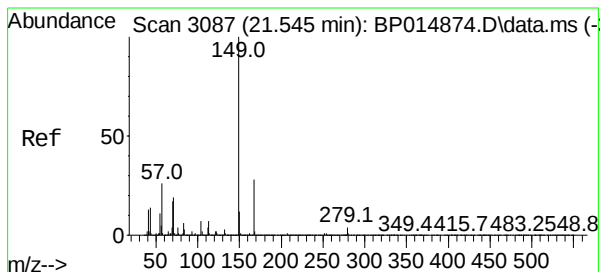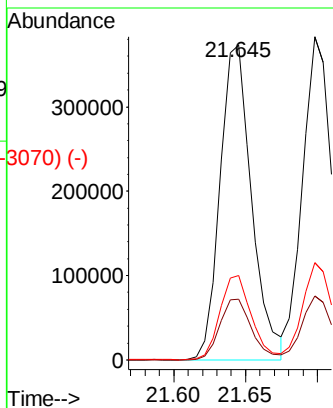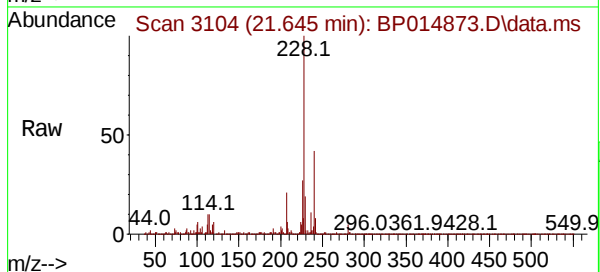

Scan 3087 (21.545 min): BP014874.D\data.ms (-3086) (-)
 Bis(2-ethylhexyl)phthalate
 Concen: 9.319 ng/u1
 RT: 21.545 min Scan# 3087
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	149	Resp:	329731
Ion	Ratio	Lower	Upper
149	100		
167	27.1	22.2	33.2
279	4.2	3.4	5.0


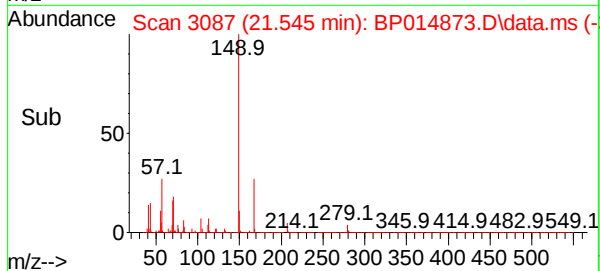

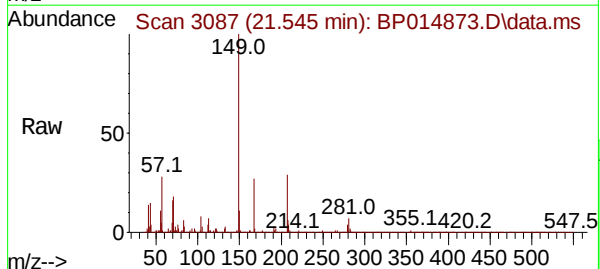


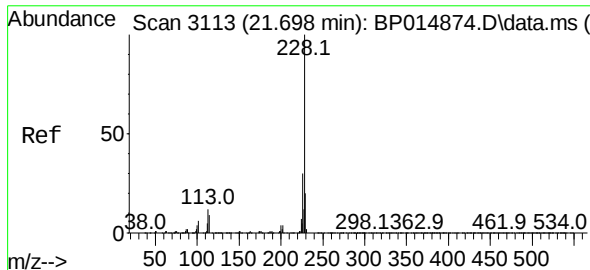

Scan 3113 (21.698 min): BP014874.D\data.ms (-3187) (-)
 Chrysene
 Concen: 10.090 ng/u1
 RT: 21.698 min Scan# 3113
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	228	Resp:	584938
Ion	Ratio	Lower	Upper
228	100		
226	30.1	24.0	36.0
229	19.8	15.6	23.4

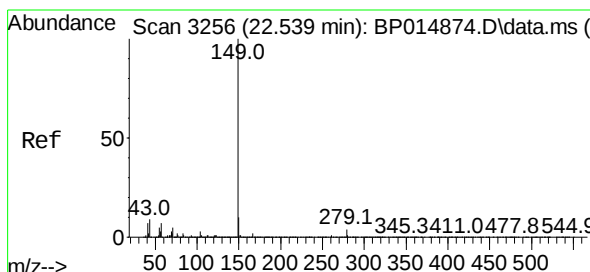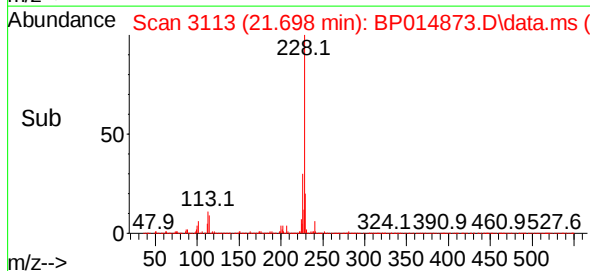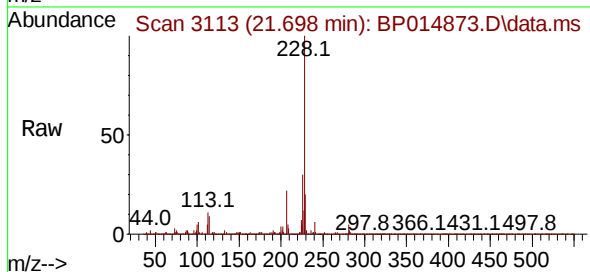

Scan 3256 (22.539 min): BP014874.D\data.ms (-3248) (-)
 Di-n-octyl phthalate
 Concen: 9.169 ng/u1
 RT: 22.539 min Scan# 3256
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:149 Resp: 567722


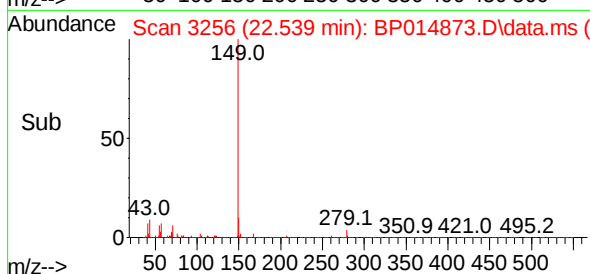

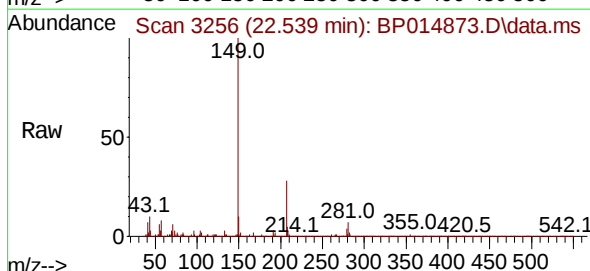


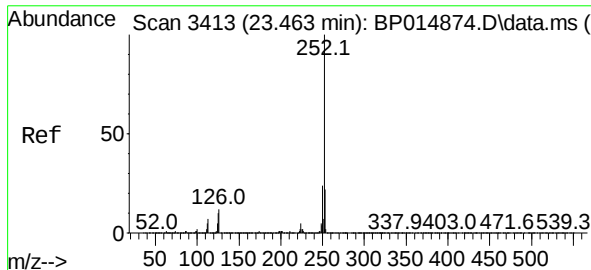

Benzo(b)fluoranthene
Concen: 9.486 ng/u1
RT: 23.463 min Scan# 3413
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22




Instrument :
BNA_P
ClientSampleId :
SSTD010647


Tgt Ion:	252	Resp:	563538
Ion	Ratio	Lower	Upper
252	100		
253	21.1	17.5	26.3
125	9.5	8.1	12.1

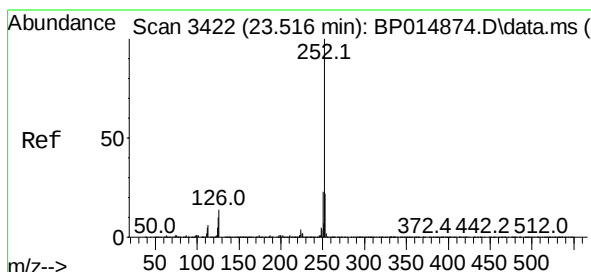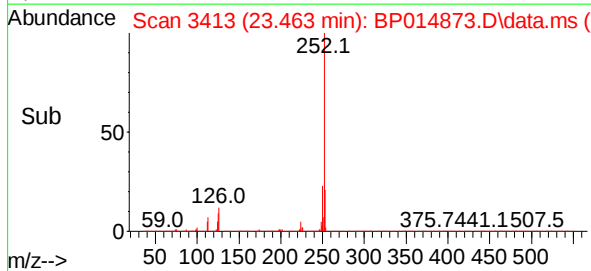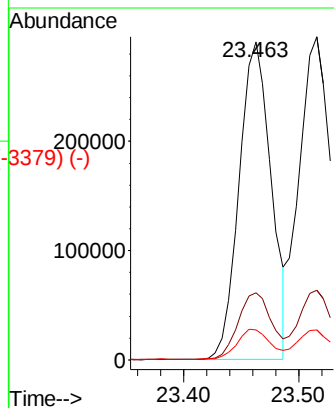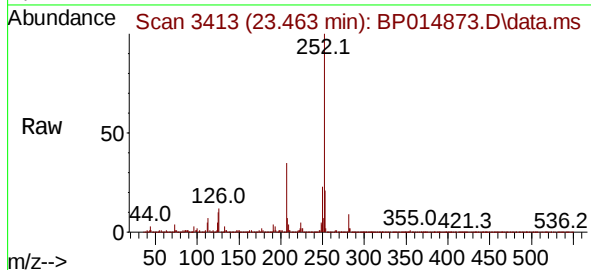

Benzo(k)fluoranthene
Concen: 10.062 ng/u1
RT: 23.515 min Scan# 3422
Delta R.T. -0.000 min
Lab File: BP014873.D
Acq: 28 Apr 2023 13:22

Tgt Ion:	252	Resp:	620151
Ion	Ratio	Lower	Upper
252	100		
253	21.6	17.5	26.3
125	9.3	7.8	11.6


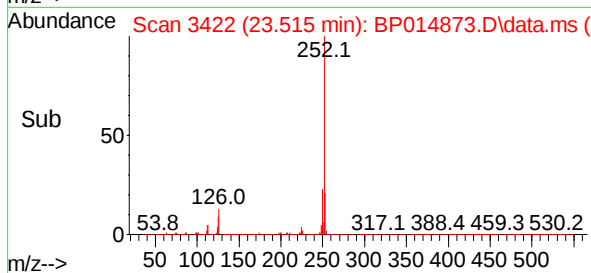

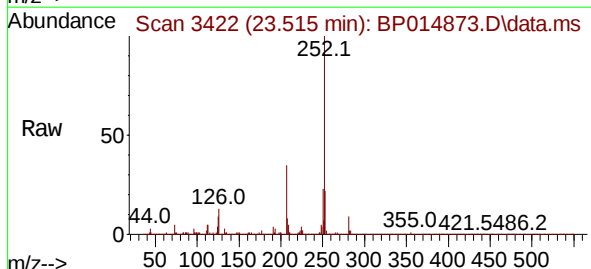




Benzo(a)pyrene
 Concen: 9.745 ng/u1
 RT: 24.151 min Scan# 3530
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22




Instrument :
 BNA_P
 ClientSampleId :
 SST010647


Tgt Ion:	252	Resp:	526490
Ion Ratio	Lower	Upper	
252	100		
253	21.3	17.6	26.4
125	10.6	8.4	12.6



Indeno(1,2,3-cd)pyrene
 Concen: 9.734 ng/u1
 RT: 27.033 min Scan# 4020
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	276	Resp:	698379
Ion Ratio	Lower	Upper	
276	100		
138	20.4	17.4	26.0
277	25.3	19.4	29.2


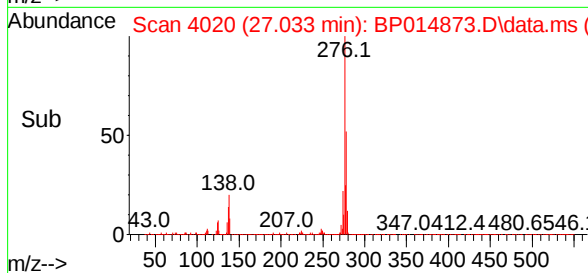






Scan 4024 (27.057 min): BP014874.D\data.ms (-4095) (-)
 Dibenzo(a,h)anthracene
 Concen: 9.862 ng/ul
 RT: 27.057 min Scan# 4165
 Delta R.T. -0.000 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010647

Tgt Ion:	278	Resp:	585220
Ion	Ratio	Lower	Upper
278	100		
139	14.3	12.1	18.1
279	23.1	18.7	28.1



Scan 4166 (27.892 min): BP014874.D\data.ms (-4146) (-)
 Benzo(g,h,i)perylene
 Concen: 9.749 ng/ul
 RT: 27.886 min Scan# 4165
 Delta R.T. -0.006 min
 Lab File: BP014873.D
 Acq: 28 Apr 2023 13:22

Tgt Ion:	276	Resp:	577272
Ion	Ratio	Lower	Upper
276	100		
138	20.7	15.8	23.6
277	23.4	19.0	28.6

