

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014884.D
 Acq On : 28 Apr 2023 20:29
 Operator : CG/JU
 Sample : 02488-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHE74

Quant Time: Apr 29 03:18:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.175	152	196006	20.000	ng/u1	0.00
20) Naphthalene-d8	11.010	136	798305	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.822	164	485992	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.575	188	1028271	20.000	ng/u1	0.00
79) Chrysene-d12	21.657	240	981185	20.000	ng/u1	0.00
88) Perylene-d12	24.262	264	1110854	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.469	96	29683	5.458	ng/uL	0.00
4) Pyridine-d5	3.916	84	137744	10.536	ng/u1	0.01
7) Phenol-d5	7.316	99	129254	8.426	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.487	67	376899	39.172	ng/u1	0.00
11) 2-Chlorophenol-d4	7.699	132	357886	30.811	ng/u1	0.00
15) 4-Methylphenol-d8	8.881	113	232402	19.881	ng/u1	0.00
21) Nitrobenzene-d5	9.351	128	223725	39.032	ng/u1	0.00
24) 2-Nitrophenol-d4	10.081	143	217157	41.271	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.628	165	395431	34.992	ng/u1	0.00
31) 4-Chloroaniline-d4	11.151	131	405483	24.818	ng/u1	0.00
46) Dimethylphthalate-d6	14.222	166	1456902	41.830	ng/u1	0.00
49) Acenaphthylene-d8	14.516	160	1770912	42.566	ng/u1	0.00
54) 4-Nitrophenol-d4	14.992	143	27899	5.383	ng/u1	0.00
60) Fluorene-d10	15.810	176	1313160	43.253	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	141485	32.529	ng/u1	0.00
73) Anthracene-d10	17.675	188	2053053	43.718	ng/u1	0.00
81) Pyrene-d10	19.892	212	2426218	44.521	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.092	264	2483864	45.271	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.505	88	6008	1.037	ng/uL#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014884.D
Acq On : 28 Apr 2023 20:29
Operator : CG/JU
Sample : 02488-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHE74


Quant Time: Apr 29 03:18:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

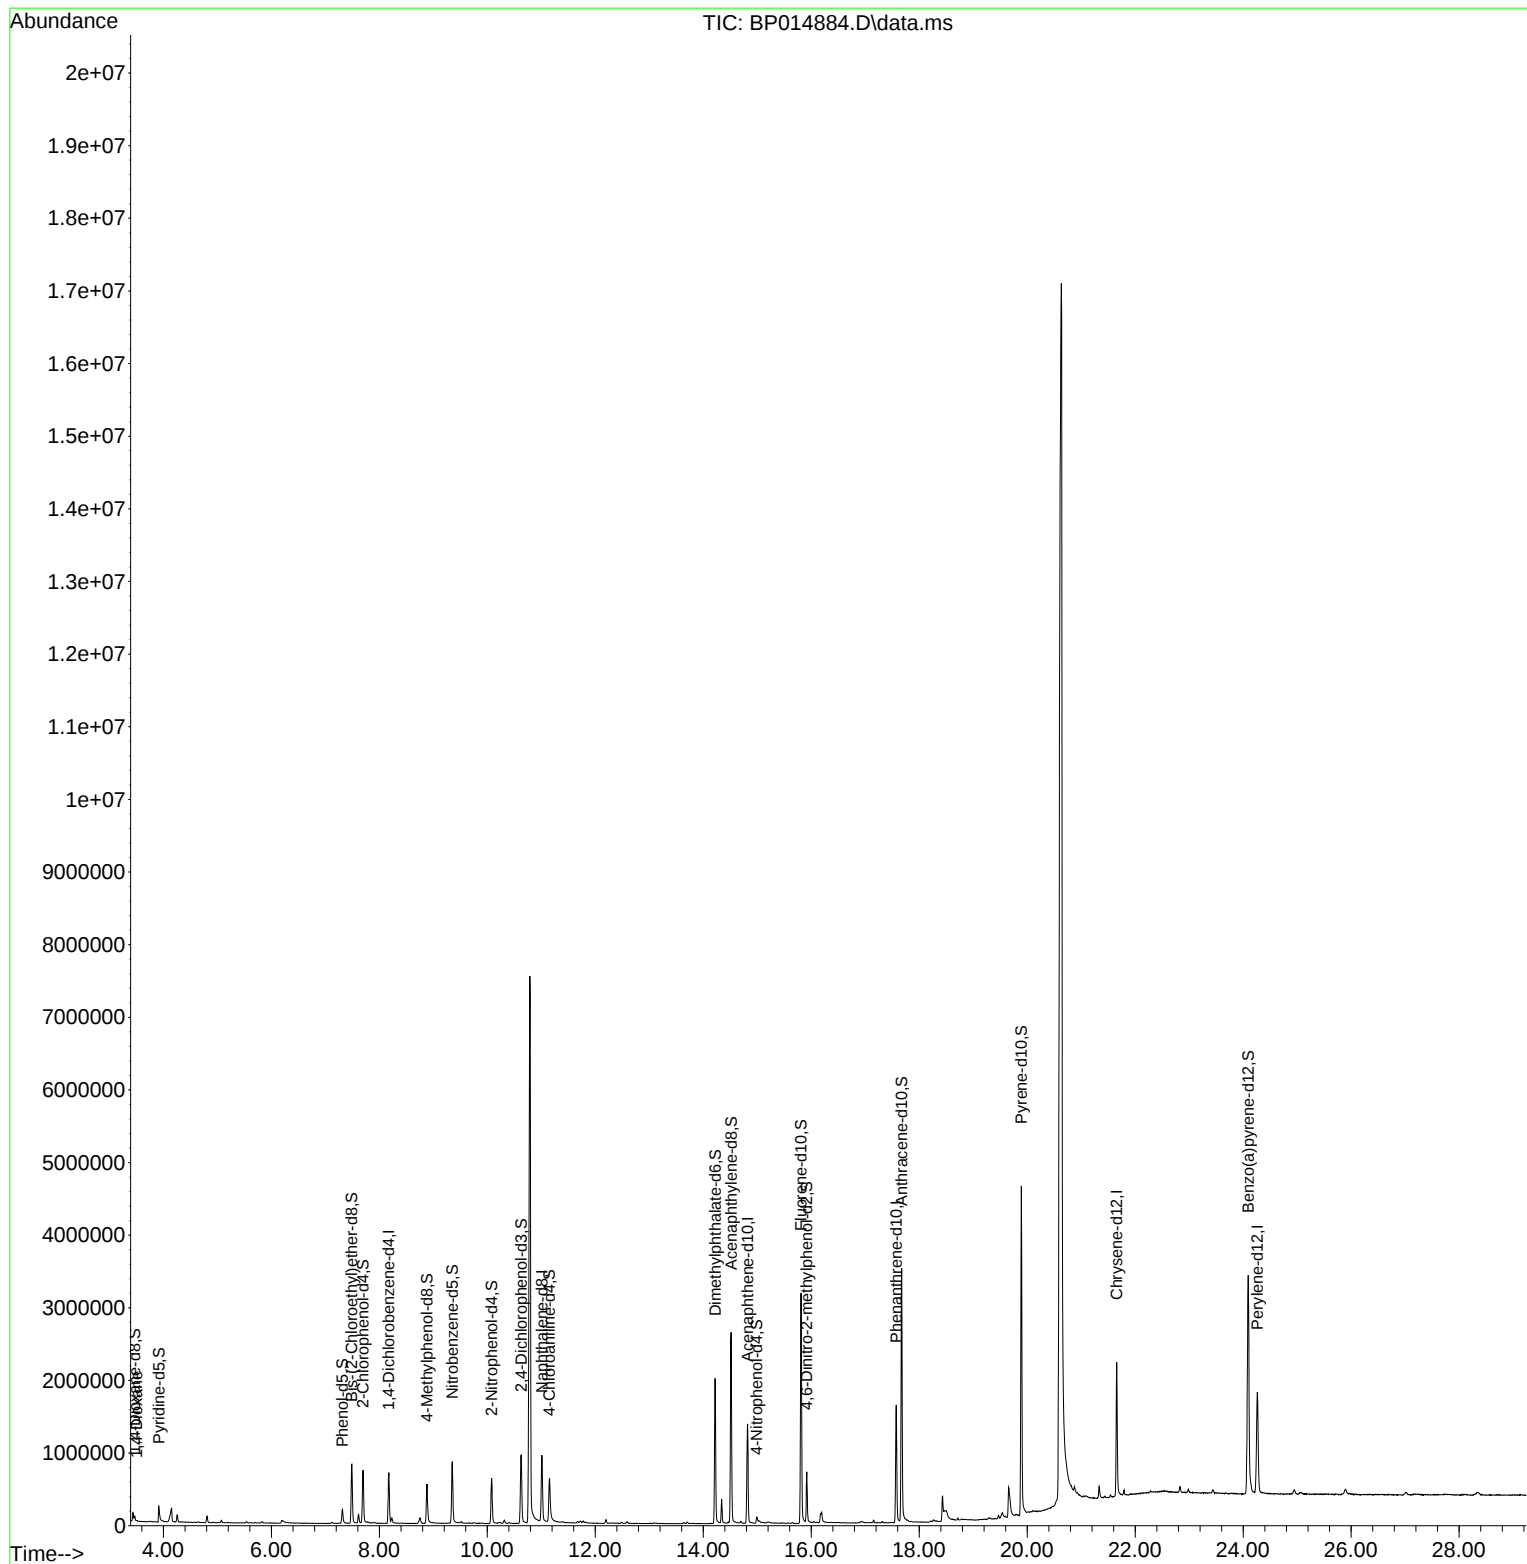

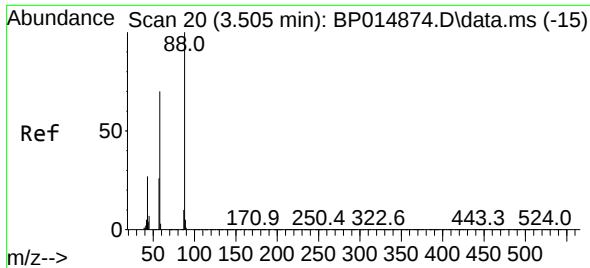

#2
 1,4-Dioxane
 Concen: 1.037 ng/uL
 RT: 3.505 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BP014884.D
 Acq: 28 Apr 2023 20:29

Instrument :
 BNA_P
 ClientSampleId :
 BHE74

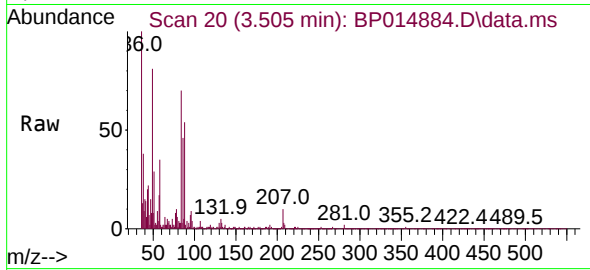

Tgt Ion: 88 Resp: 6008
 Ion Ratio Lower Upper
 88 100
 43 37.3 22.2 33.4#
 58 64.5 55.1 82.7

