

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014898.D
 Acq On : 29 Apr 2023 04:51
 Operator : CG/JU
 Sample : 02528-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA38

Quant Time: Apr 29 05:39:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.175	152	189508	20.000	ng/u1	0.00
20) Naphthalene-d8	11.010	136	776499	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.816	164	458166	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.569	188	931243	20.000	ng/u1	-0.01
79) Chrysene-d12	21.651	240	850631	20.000	ng/u1	-0.01
88) Perylene-d12	24.251	264	962475	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	37335	7.100	ng/uL	0.00
4) Pyridine-d5	3.911	84	195486	15.466	ng/u1	0.00
7) Phenol-d5	7.311	99	264349	17.823	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.487	67	317807	34.163	ng/u1	0.00
11) 2-Chlorophenol-d4	7.693	132	369072	32.864	ng/u1	0.00
15) 4-Methylphenol-d8	8.875	113	276263	24.444	ng/u1	0.00
21) Nitrobenzene-d5	9.346	128	187339	33.602	ng/u1	0.00
24) 2-Nitrophenol-d4	10.075	143	203674	39.796	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.616	165	374986	34.114	ng/u1	0.00
31) 4-Chloroaniline-d4	11.140	131	221366	13.929	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	1333150	40.602	ng/u1	0.00
49) Acenaphthylene-d8	14.510	160	1559180	39.753	ng/u1	0.00
54) 4-Nitrophenol-d4	14.993	143	79173	16.205	ng/u1	0.00
60) Fluorene-d10	15.810	176	1131571	39.535	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	162337	41.212	ng/u1	0.00
73) Anthracene-d10	17.669	188	1712827	40.274	ng/u1	0.00
81) Pyrene-d10	19.886	212	2070016	43.814	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.080	264	2000068	42.073	ng/u1	-0.02


Target Compounds					Qvalue
2) 1,4-Dioxane	3.505	88	220066	39.304	ng/uL 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014898.D
Acq On : 29 Apr 2023 04:51
Operator : CG/JU
Sample : 02528-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA38

Quant Time: Apr 29 05:39:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

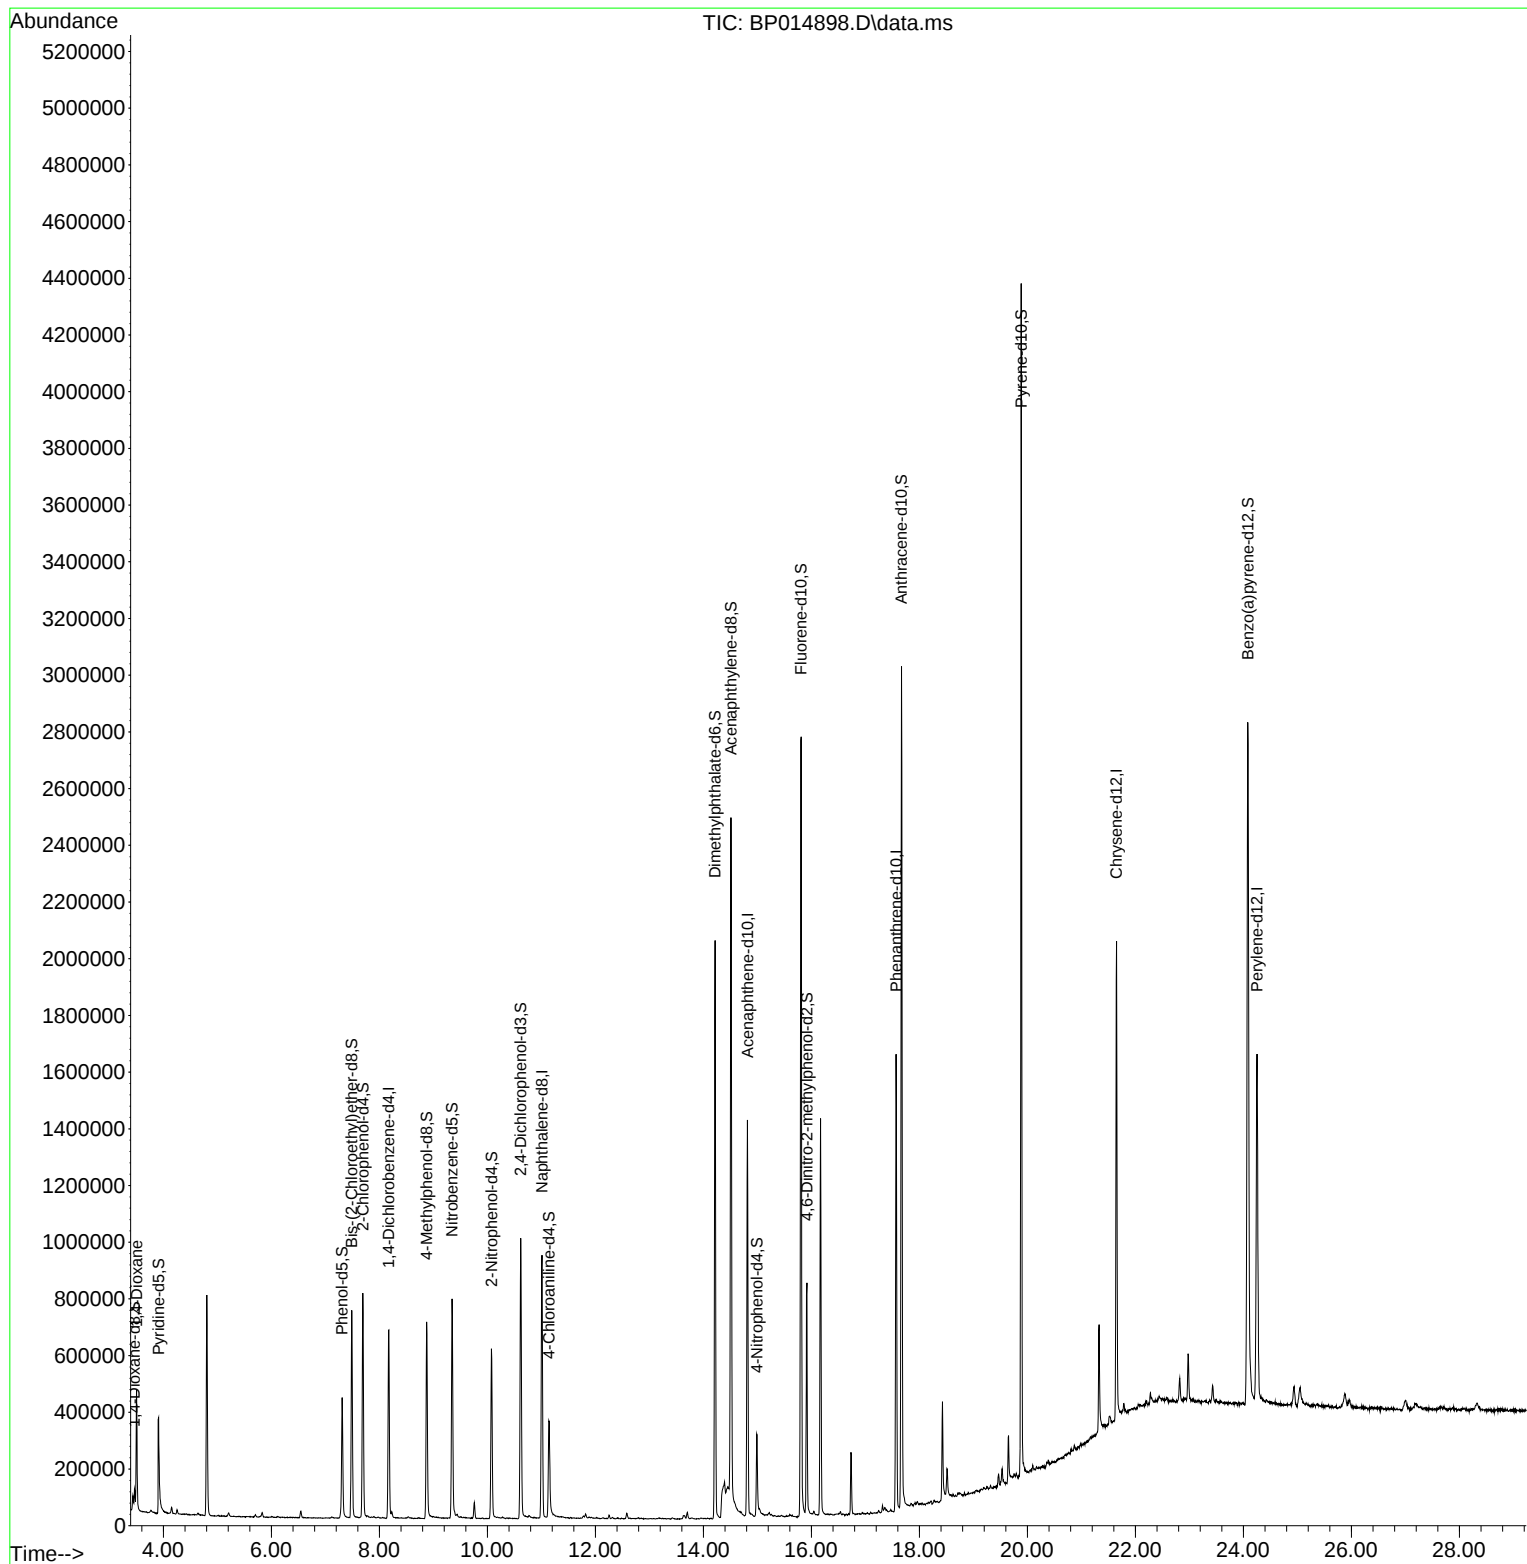

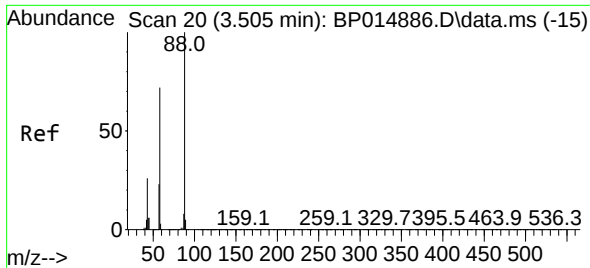

#2
 1,4-Dioxane
 Concen: 39.304 ng/uL
 RT: 3.505 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BP014898.D
 Acq: 29 Apr 2023 04:51

Instrument :
 BNA_P
 ClientSampleId :
 HOA38

Tgt Ion: 88 Resp: 220066
 Ion Ratio Lower Upper
 88 100
 43 25.3 22.2 33.4
 58 68.3 55.1 82.7

