

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014899.D
 Acq On : 29 Apr 2023 05:24
 Operator : CG/JU
 Sample : 02528-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA39

Quant Time: Apr 29 06:02:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:40:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.175	152	203888	20.000	ng/u1	0.00
20) Naphthalene-d8	11.010	136	847535	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.816	164	509378	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.569	188	1071491	20.000	ng/u1	-0.01
79) Chrysene-d12	21.651	240	959460	20.000	ng/u1	-0.01
88) Perylene-d12	24.251	264	1125535	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.464	96	30714	5.429	ng/uL	0.00
4) Pyridine-d5	3.911	84	180699	13.287	ng/u1	0.00
7) Phenol-d5	7.311	99	132112	8.279	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.487	67	350187	34.989	ng/u1	0.00
11) 2-Chlorophenol-d4	7.693	132	349823	28.953	ng/u1	0.00
15) 4-Methylphenol-d8	8.875	113	222568	18.304	ng/u1	0.00
21) Nitrobenzene-d5	9.346	128	207731	34.136	ng/u1	0.00
24) 2-Nitrophenol-d4	10.075	143	214779	38.448	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.616	165	383352	31.952	ng/u1	0.00
31) 4-Chloroaniline-d4	11.140	131	305341	17.603	ng/u1	0.00
46) Dimethylphthalate-d6	14.216	166	1416958	38.816	ng/u1	0.00
49) Acenaphthylene-d8	14.510	160	1573856	36.093	ng/u1	0.00
54) 4-Nitrophenol-d4	14.992	143	32020	5.895	ng/u1	0.00
60) Fluorene-d10	15.810	176	1201283	37.751	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	179127	39.522	ng/u1	0.00
73) Anthracene-d10	17.669	188	1863284	38.077	ng/u1	0.00
81) Pyrene-d10	19.886	212	2224693	41.747	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.080	264	2150472	38.683	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.505	88	440987	73.206	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014899.D
Acq On : 29 Apr 2023 05:24
Operator : CG/JU
Sample : 02528-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA39

Quant Time: Apr 29 06:02:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:40:33 2023
Response via : Initial Calibration

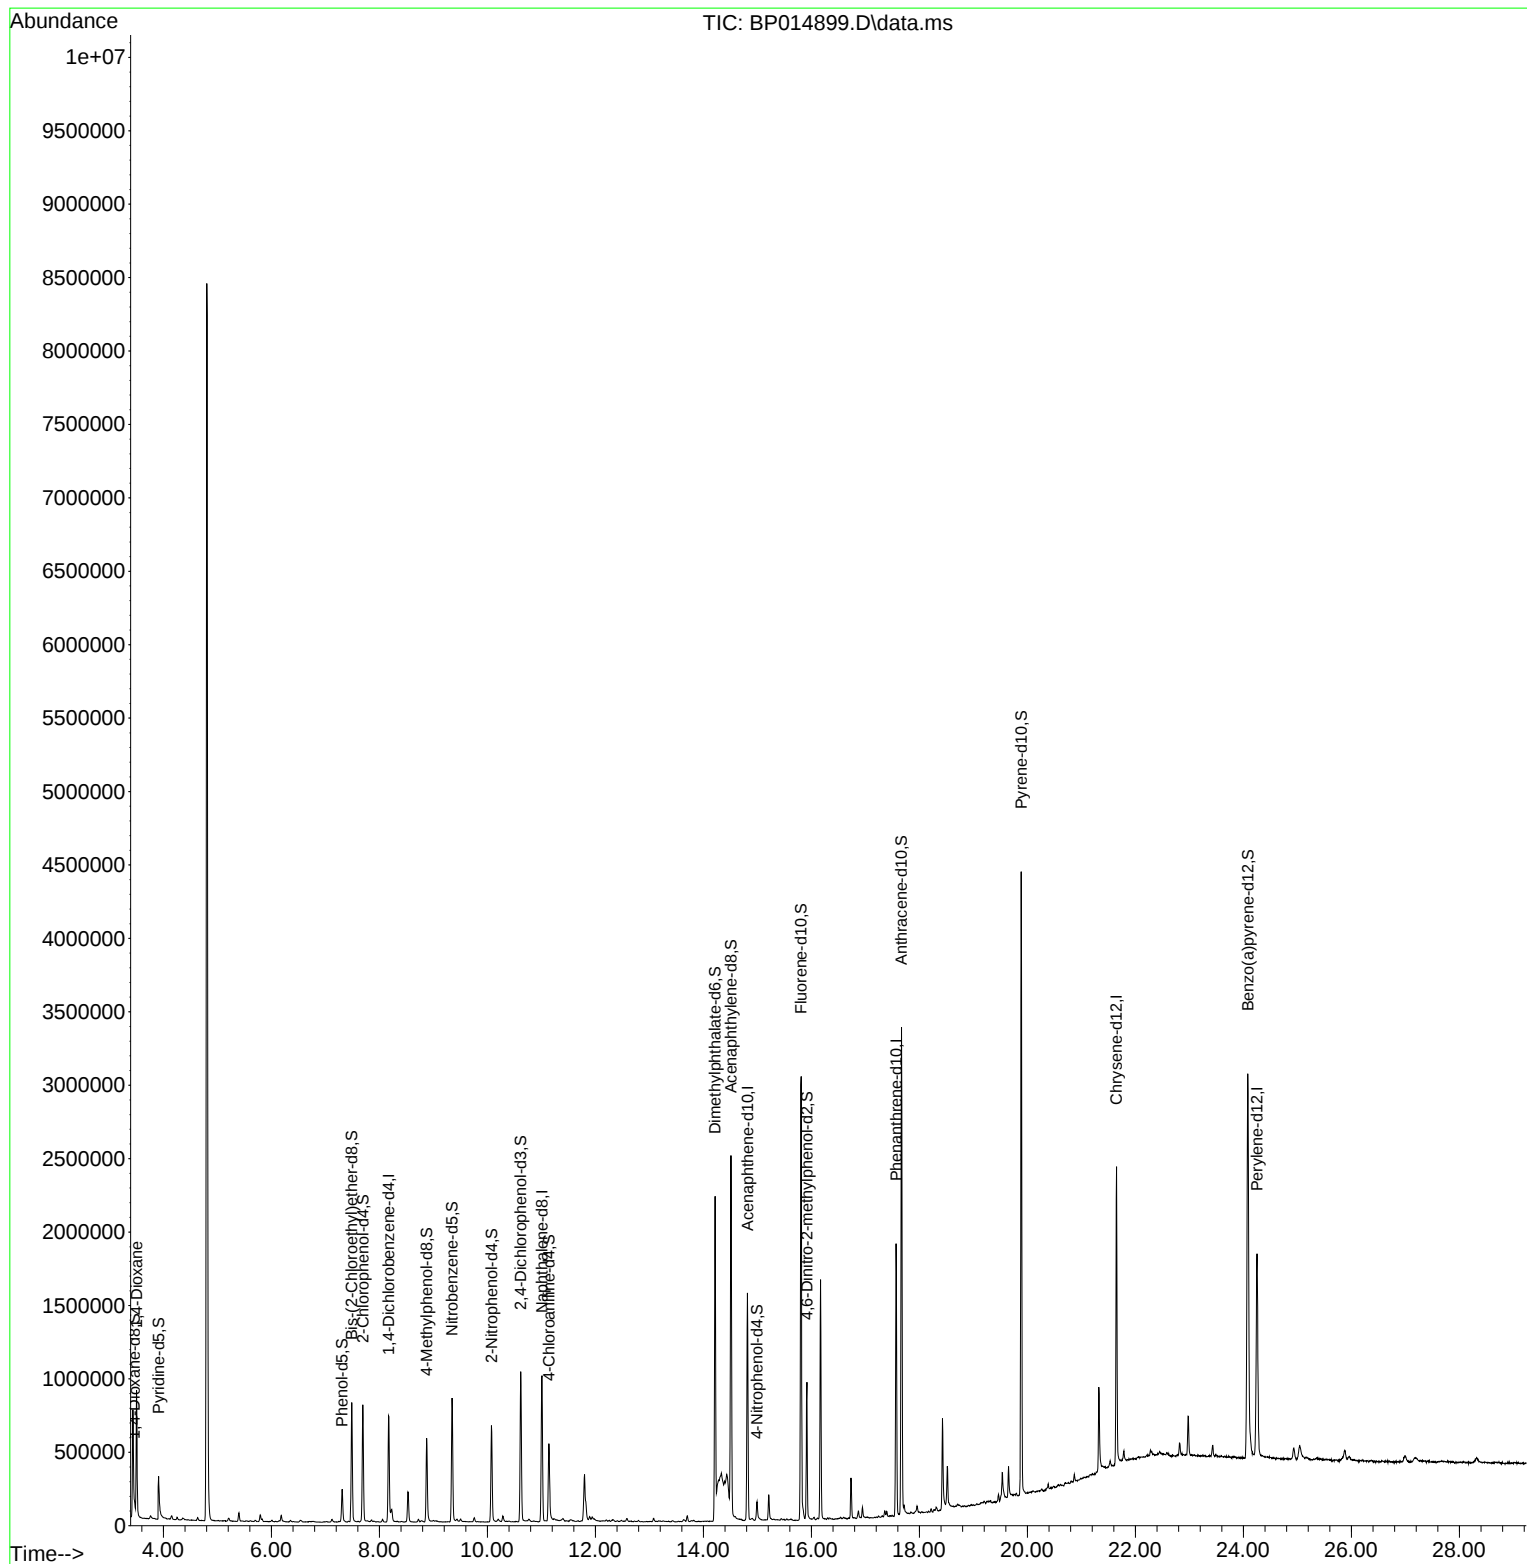

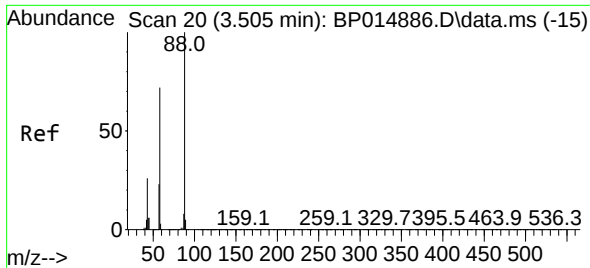

#2
 1,4-Dioxane
 Concen: 73.206 ng/uL
 RT: 3.505 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: BP014899.D
 Acq: 29 Apr 2023 05:24

Instrument :
 BNA_P
 ClientSampleId :
 HOA39

Tgt Ion: 88 Resp: 440987

Ion	Ratio	Lower	Upper
88	100		
43	24.9	22.2	33.4
58	67.6	55.1	82.7

