

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014888.D
 Acq On : 28 Apr 2023 23:16
 Operator : CG/JU
 Sample : PB152453BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK453

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	9	14	22	rVB	71312	97549	1.95%	0.196%
2	3.904	85	88	106	rBV	692227	1100133	22.03%	2.211%
3	4.257	144	148	153	rVB	14454	21904	0.44%	0.044%
4	7.310	661	667	682	rBV	703074	1281541	25.66%	2.575%
5	7.493	691	698	720	rVB	725782	1215825	24.35%	2.443%
6	7.698	726	733	753	rBV	832950	1430177	28.64%	2.874%
7	8.175	805	814	828	rBV	653744	1097345	21.98%	2.205%
8	8.881	926	934	955	rBV	875214	1652991	33.10%	3.322%
9	9.351	1004	1014	1035	rBV	756373	1367716	27.39%	2.748%
10	10.081	1130	1138	1154	rBV	557307	992054	19.87%	1.993%
11	10.622	1222	1230	1242	rBV	843761	1553615	31.11%	3.122%
12	11.010	1287	1296	1311	rBV	847059	1527930	30.60%	3.070%
13	11.145	1311	1319	1338	rBV	700723	1536194	30.76%	3.087%
14	12.586	1559	1564	1575	rBV5	11538	31676	0.63%	0.064%
15	13.704	1749	1754	1763	rVB5	9099	17352	0.35%	0.035%
16	14.216	1834	1841	1860	rBV	1545110	2531712	50.70%	5.087%
17	14.516	1883	1892	1915	rBV	1990971	3317144	66.43%	6.666%
18	14.822	1937	1944	1963	rBV	1209475	2001261	40.08%	4.021%
19	14.992	1967	1973	1995	rBV	272384	687260	13.76%	1.381%
20	15.310	2026	2027	2036	rVB9	5534	8350	0.17%	0.017%
21	15.810	2105	2112	2125	rBV	2421859	3997164	80.05%	8.032%
22	15.916	2125	2130	2148	rVV	487184	821938	16.46%	1.652%
23	16.051	2150	2153	2161	rVB6	13399	25273	0.51%	0.051%
24	17.245	2354	2356	2361	rVB6	3715	5124	0.10%	0.010%
25	17.574	2404	2412	2423	rBV	1461220	2319456	46.45%	4.661%
26	17.674	2423	2429	2454	rVB	2632466	4275297	85.62%	8.591%
27	19.468	2731	2734	2738	rBV4	28273	41577	0.83%	0.084%
28	19.539	2742	2746	2750	rBV2	22407	34082	0.68%	0.068%
29	19.892	2800	2806	2829	rBV	3105260	4993349	100.00%	10.034%
30	21.656	3101	3106	3124	rBV	1196339	2395417	47.97%	4.813%
31	24.086	3512	3519	3540	rBV2	1914334	4827968	96.69%	9.702%
32	24.256	3541	3548	3566	rVB2	1056520	2558488	51.24%	5.141%




Sum of corrected areas: 49764862

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014888.D
Acq On : 28 Apr 2023 23:16
Operator : CG/JU
Sample : PB152453BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

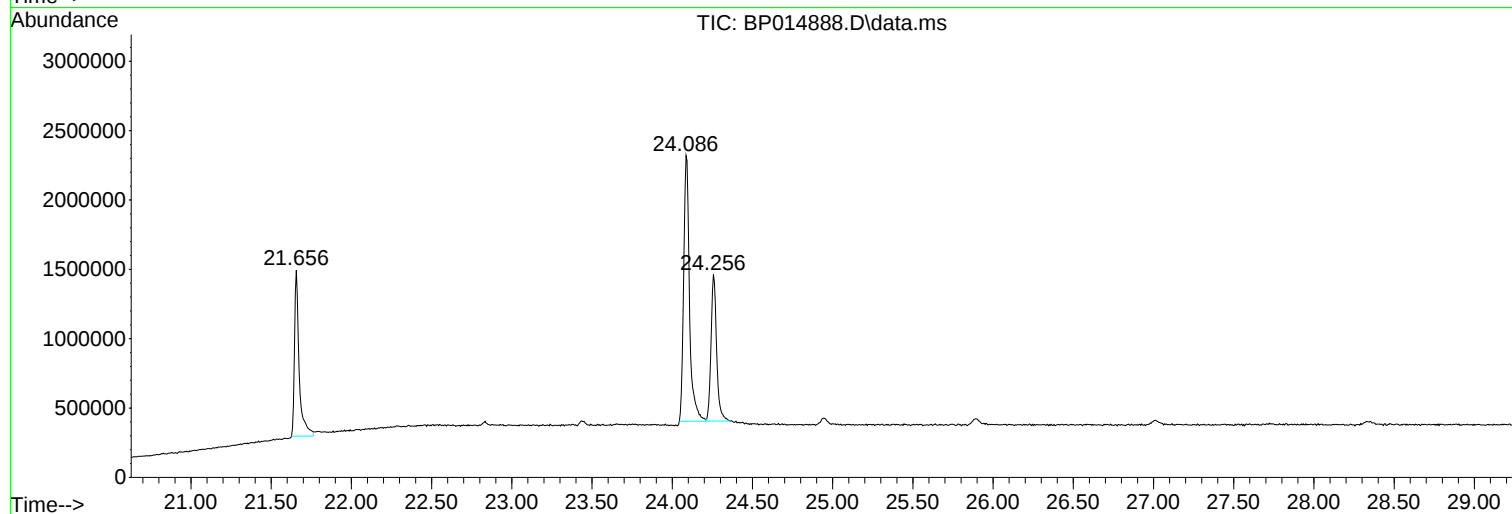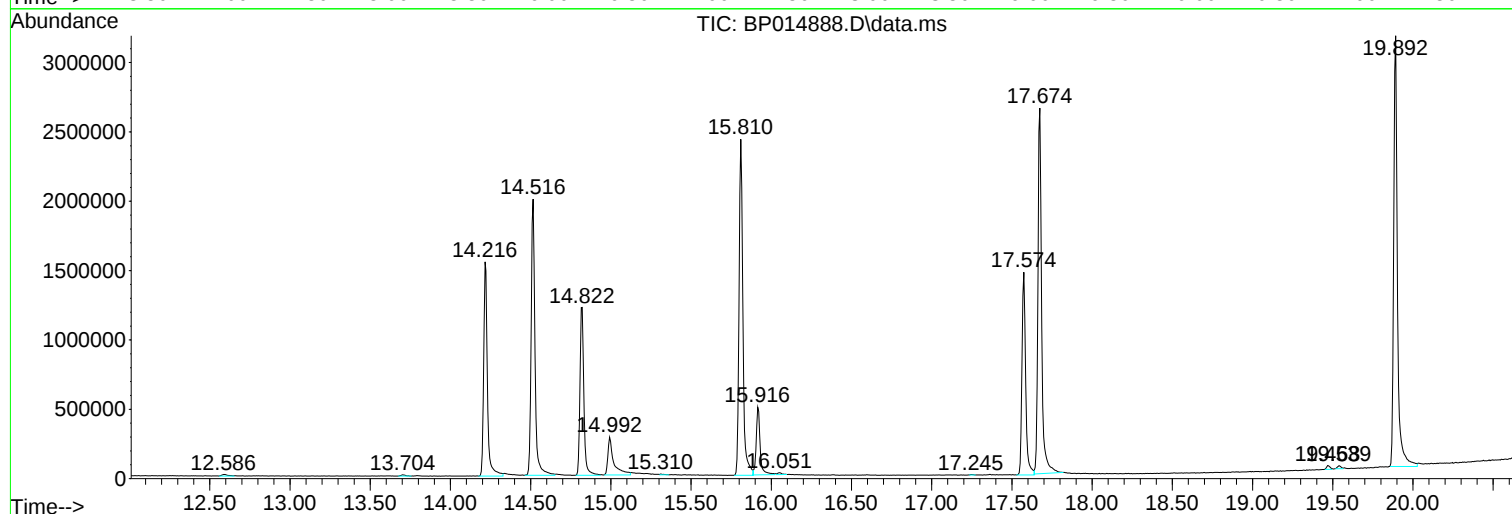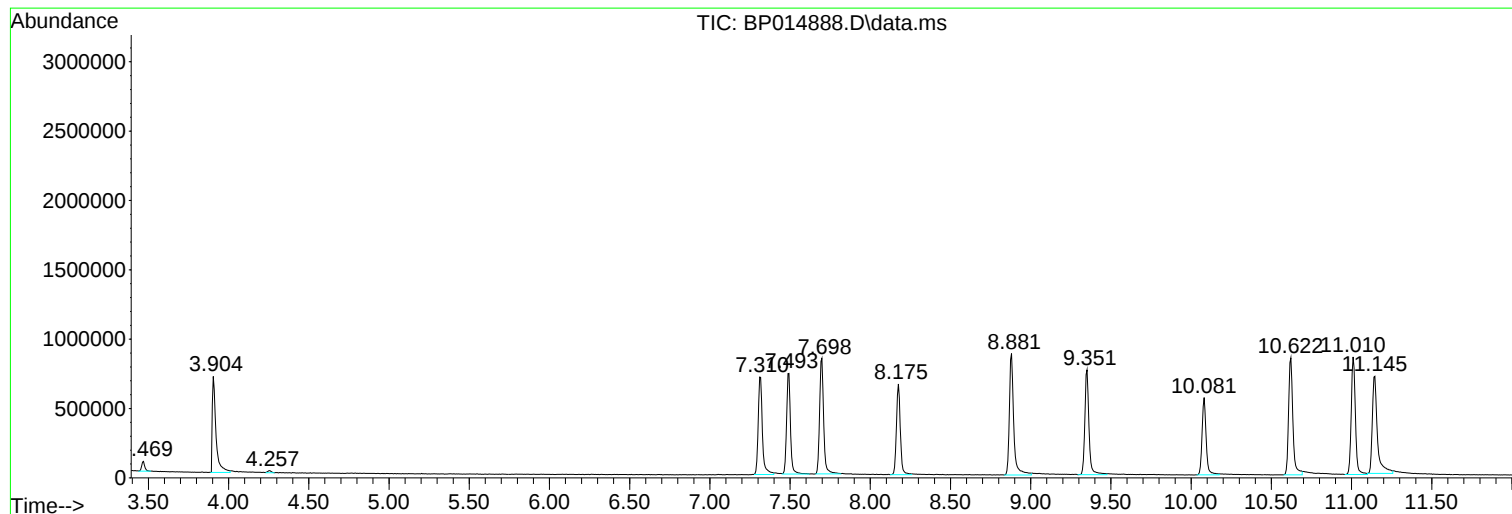

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014888.D
Acq On : 28 Apr 2023 23:16
Operator : CG/JU
Sample : PB152453BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014888.D
Acq On : 28 Apr 2023 23:16
Operator : CG/JU
Sample : PB152453BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------