

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014894.D
 Acq On : 29 Apr 2023 02:37
 Operator : CG/JU
 Sample : 02528-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	11	rBV	98946	132796	5.12%	0.407%
2	3.464	11	13	16	rVV	71796	90657	3.50%	0.278%
3	3.505	16	20	34	rVB	456001	606624	23.40%	1.861%
4	3.911	88	89	102	rBV	140639	231310	8.92%	0.709%
5	4.152	126	130	135	rVB	21346	32412	1.25%	0.099%
6	4.252	144	147	153	rVB	16594	22298	0.86%	0.068%
7	4.640	210	213	220	rVB6	6891	9395	0.36%	0.029%
8	4.805	235	241	255	rBV	1553890	2303957	88.87%	7.066%
9	5.205	305	309	316	rVB3	8567	15254	0.59%	0.047%
10	5.405	337	343	346	rBV6	5043	8302	0.32%	0.025%
11	5.699	387	393	399	rBV	9152	16273	0.63%	0.050%
12	5.764	402	404	407	rBV3	2087	2745	0.11%	0.008%
13	5.828	411	415	419	rVB	14167	18405	0.71%	0.056%
14	6.487	525	527	533	rBV7	1456	2656	0.10%	0.008%
15	6.628	548	551	556	rVB7	2247	3819	0.15%	0.012%
16	6.669	556	558	561	rBV4	2293	2625	0.10%	0.008%
17	7.005	613	615	617	rBV3	2559	2683	0.10%	0.008%
18	7.311	660	667	681	rBV	286598	493227	19.03%	1.513%
19	7.487	691	697	711	rBV	336334	532431	20.54%	1.633%
20	7.693	725	732	744	rBV	325088	557674	21.51%	1.710%
21	7.893	764	766	770	rBV5	3796	4497	0.17%	0.014%
22	7.987	777	782	784	rBV5	3879	5593	0.22%	0.017%
23	8.063	788	795	798	rBV9	3187	6310	0.24%	0.019%
24	8.175	806	814	832	rBV	715059	1213735	46.82%	3.723%
25	8.875	926	933	947	rBV	341967	654902	25.26%	2.009%
26	9.346	1006	1013	1028	rBV	291933	530320	20.46%	1.627%
27	9.757	1080	1083	1088	rVB7	3731	4844	0.19%	0.015%
28	10.081	1130	1138	1147	rBV	190935	345606	13.33%	1.060%
29	10.316	1176	1178	1183	rVB6	2178	2638	0.10%	0.008%
30	10.616	1220	1229	1246	rBV	330709	627230	24.20%	1.924%
31	10.857	1268	1270	1275	rVB6	2526	3882	0.15%	0.012%
32	11.010	1288	1296	1310	rBV	965586	1689524	65.17%	5.182%
33	11.140	1310	1318	1336	rBV	682398	1331183	51.35%	4.083%
34	11.493	1375	1378	1382	rVB6	2596	3809	0.15%	0.012%
35	11.575	1391	1392	1397	rVB5	2820	3227	0.12%	0.010%
36	12.587	1559	1564	1569	rBV8	4987	8781	0.34%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
 Data File : BP014894.D
 Acq On : 29 Apr 2023 02:37
 Operator : CG/JU
 Sample : 02528-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
 Title : SVOA CALIBRATION

37	12.828	1602	1605	1608	rVB5	2060	2808	0.11%	0.009%
38	13.163	1660	1662	1668	rVB7	1652	3136	0.12%	0.010%
39	13.704	1745	1754	1759	rVB2	15849	26798	1.03%	0.082%
40	13.757	1759	1763	1765	rBV5	2741	3090	0.12%	0.009%
41	14.216	1833	1841	1853	rBV	840180	1206836	46.55%	3.702%
42	14.510	1883	1891	1911	rBV	874811	1415527	54.60%	4.342%
43	14.816	1937	1943	1961	rBV	1394005	2179894	84.09%	6.686%
44	14.993	1967	1973	1984	rBV2	73282	177294	6.84%	0.544%
45	15.222	2008	2012	2021	rVB2	7693	12781	0.49%	0.039%
46	15.810	2104	2112	2125	rBV	1075720	1796781	69.31%	5.511%
47	15.916	2125	2130	2140	rVB	210038	320978	12.38%	0.984%
48	16.045	2150	2152	2156	rVB4	5450	6660	0.26%	0.020%
49	16.687	2259	2261	2263	rBV3	2546	2890	0.11%	0.009%
50	17.034	2315	2320	2322	rBV5	2991	4718	0.18%	0.014%
51	17.363	2371	2376	2380	rBV8	4652	9103	0.35%	0.028%
52	17.569	2404	2411	2423	rBV	1558464	2416143	93.20%	7.411%
53	17.669	2423	2428	2440	rVV	1241538	1879566	72.50%	5.765%
54	18.433	2554	2558	2562	rBV7	7400	13322	0.51%	0.041%
55	18.510	2568	2571	2576	rVB6	6140	9149	0.35%	0.028%
56	19.469	2731	2734	2740	rVB3	14695	20140	0.78%	0.062%
57	19.657	2763	2766	2767	rBV3	10249	12315	0.48%	0.038%
58	19.886	2799	2805	2825	rBV	1551915	2362147	91.12%	7.245%
59	21.651	3100	3105	3121	rBV	1419726	2431851	93.81%	7.459%
60	24.080	3511	3518	3536	rBV2	867644	2176017	83.94%	6.674%
61	24.251	3540	3547	3565	rVB2	1086777	2592373	100.00%	7.951%




Sum of corrected areas: 32603941

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014894.D
Acq On : 29 Apr 2023 02:37
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

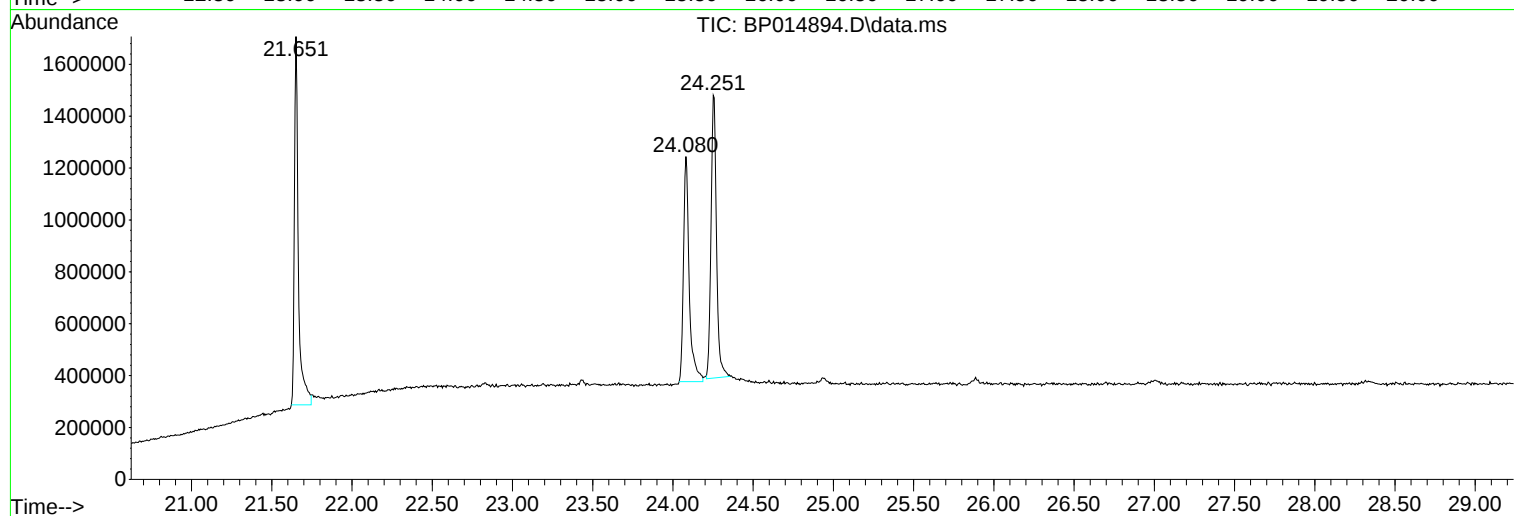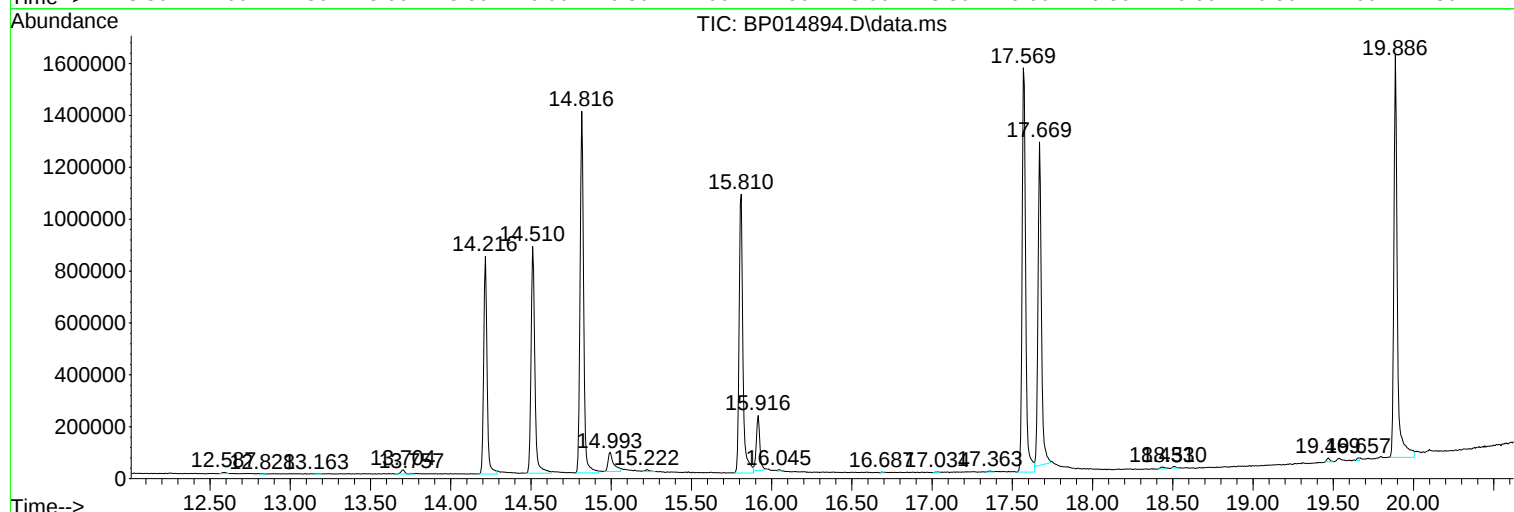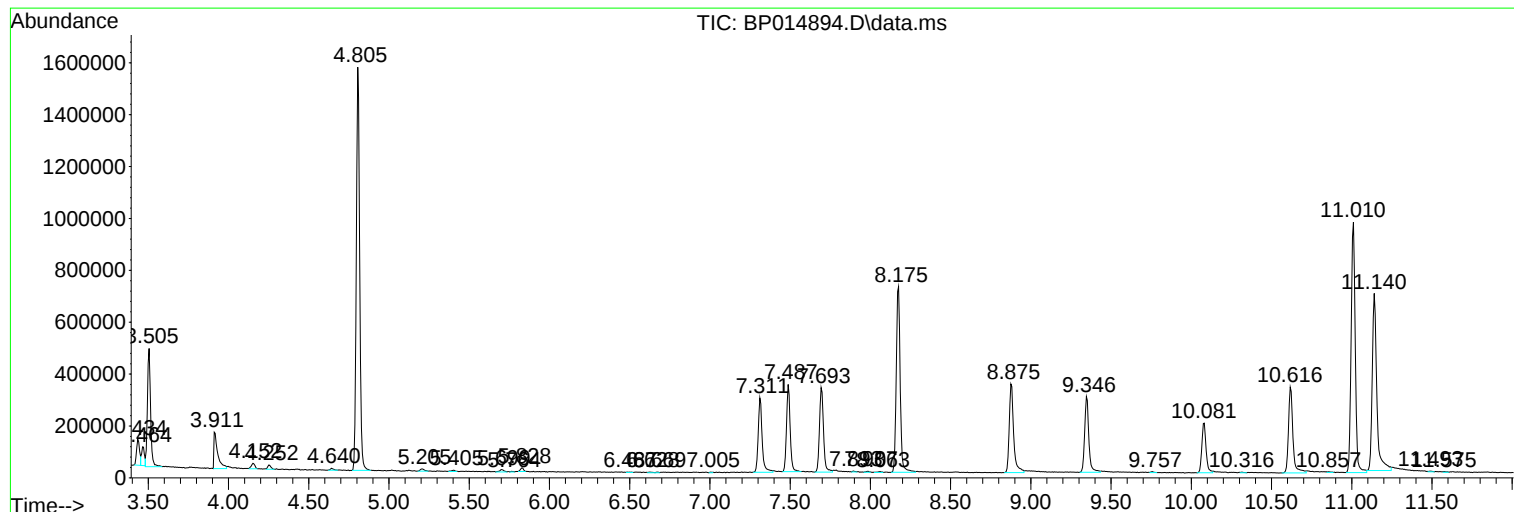

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014894.D
Acq On : 29 Apr 2023 02:37
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042823\
Data File : BP014894.D
Acq On : 29 Apr 2023 02:37
Operator : CG/JU
Sample : 02528-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc