
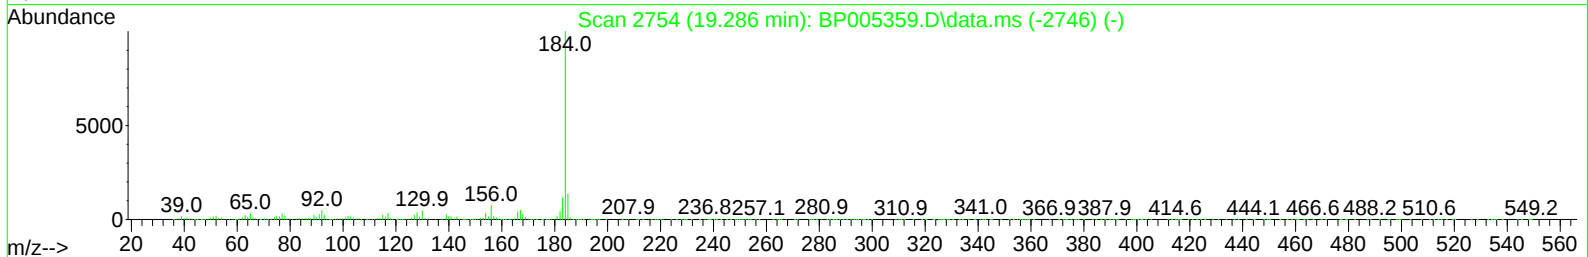
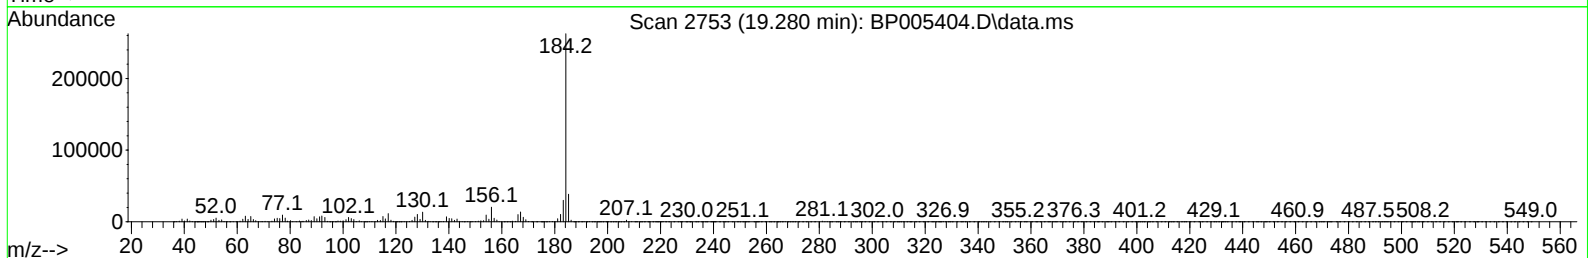


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042921\
 Data File : BP005404.D
 Acq On : 29 Apr 2021 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 12:51:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:38:20 2021
 Response via : Initial Calibration

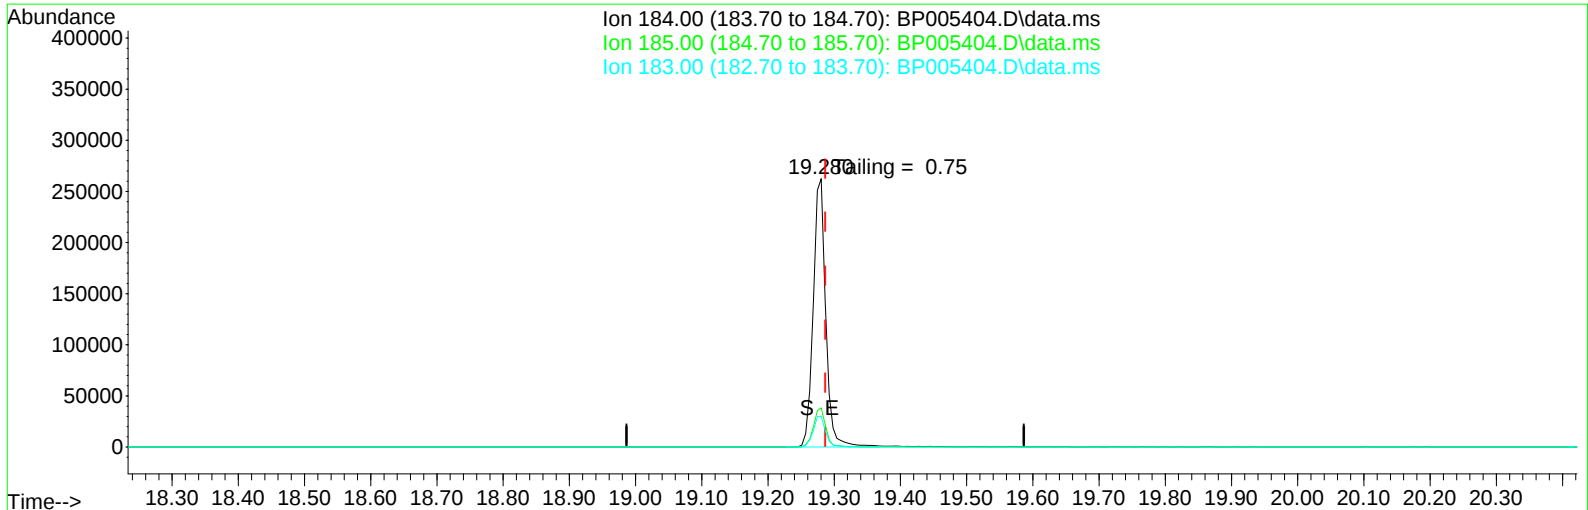




TIC: BP005404.D\data.ms

(77) Benzidine**19.280min (-0.006) 422510.27 ng****response 347151**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.63
183.00	12.30	11.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042921\
 Data File : BP005404.D
 Acq On : 29 Apr 2021 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 12:51:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:38:20 2021
 Response via : Initial Calibration

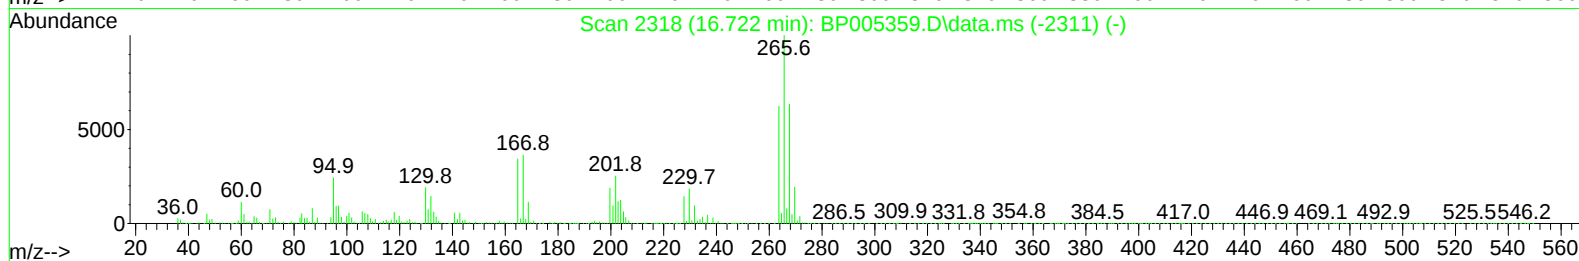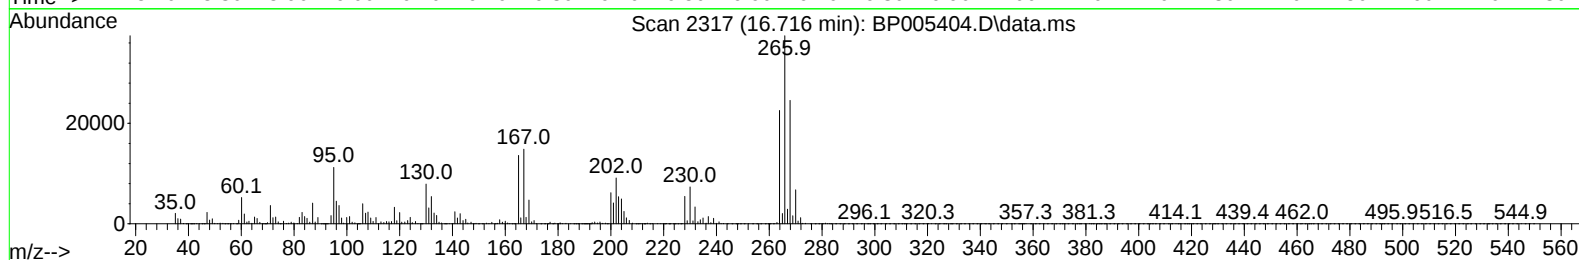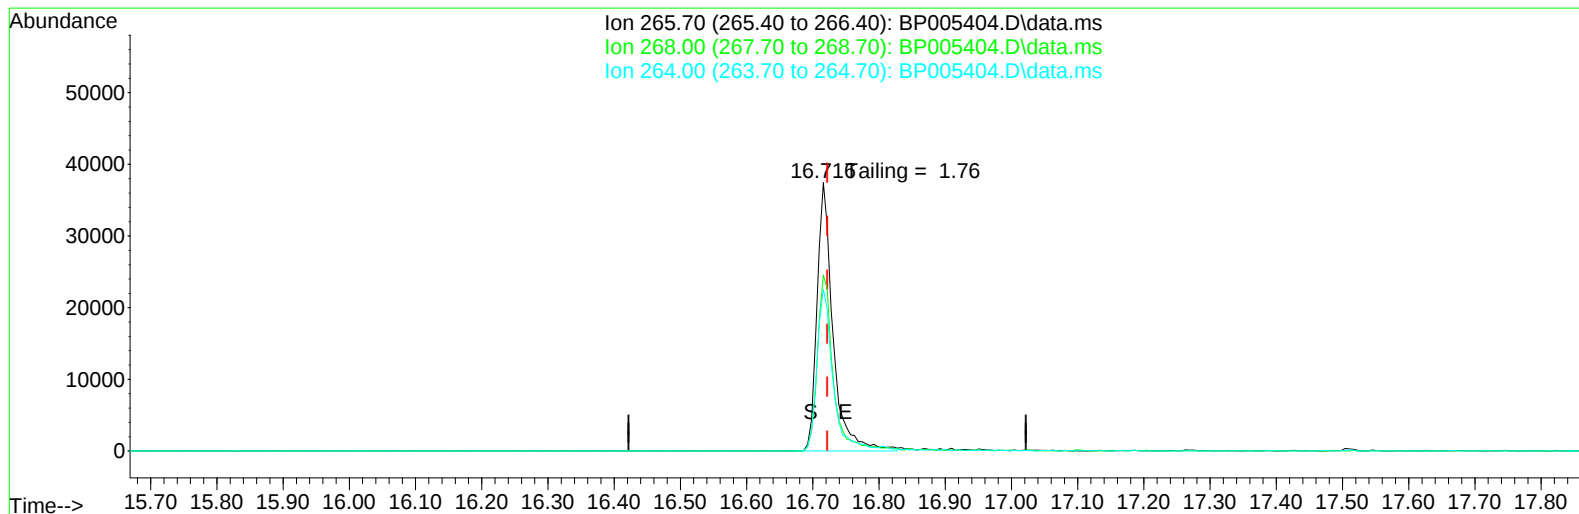

TIC: BP005404.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.006) 816739.29 ng

response 63331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.61
264.00	67.10	60.26
0.00	0.00	0.00