
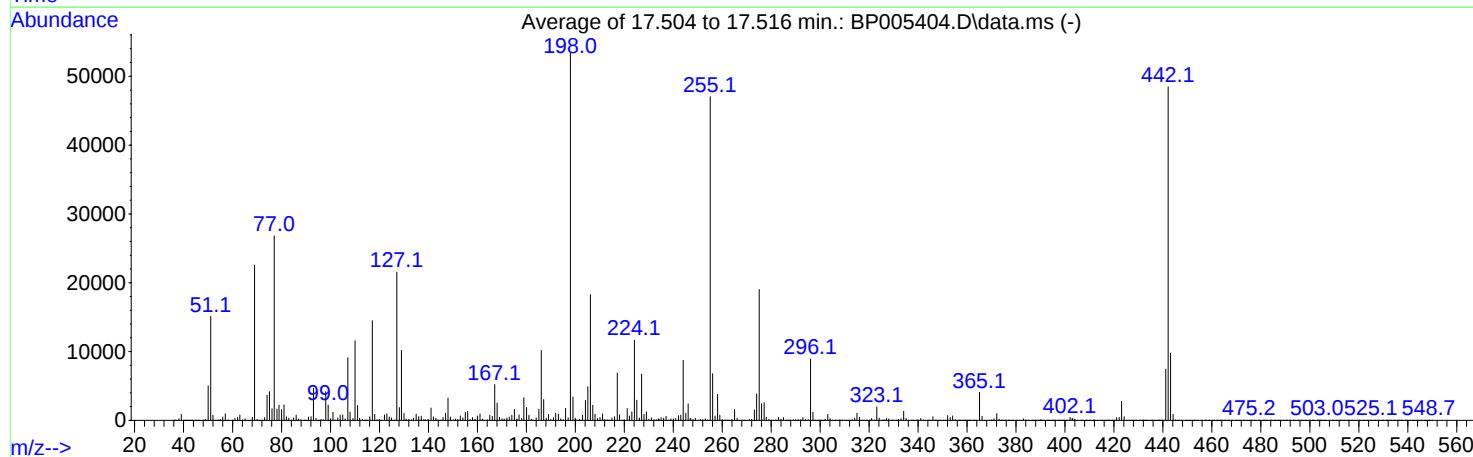


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042921\
 Data File : BP005404.D
 Acq On : 29 Apr 2021 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 30 11:27:53 2021

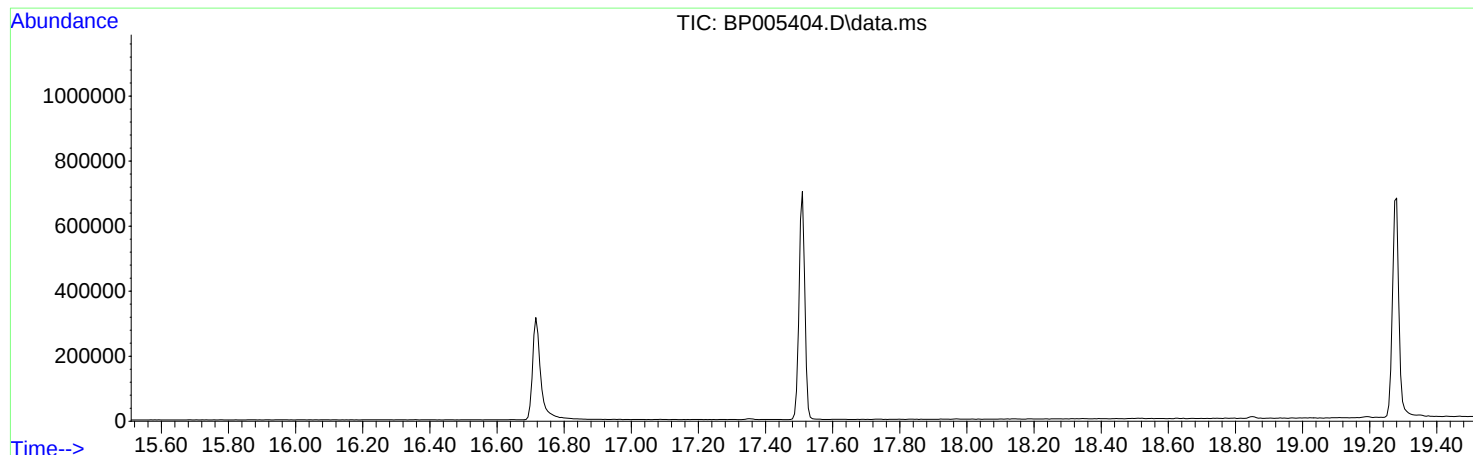




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	15109	PASS
68	69	0.00	2	1.9	433	PASS
69	198	0.00	100	42.2	22566	PASS
70	69	0.00	2	0.6	135	PASS
127	198	10	80	40.3	21524	PASS
197	198	0.00	2	0.7	362	PASS
198	198	100	100	100.0	53453	PASS
199	198	5	9	6.4	3398	PASS
275	198	10	60	35.6	19008	PASS
365	198	1	100	7.6	4058	PASS
441	198	0.01	100	13.9	7430	PASS
442	442	100	100	100.0	48477	PASS
443	442	15	24	20.2	9781	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042921\
 Data File : BP005404.D
 Acq On : 29 Apr 2021 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 29 12:51:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:38:20 2021
 Response via : Initial Calibration

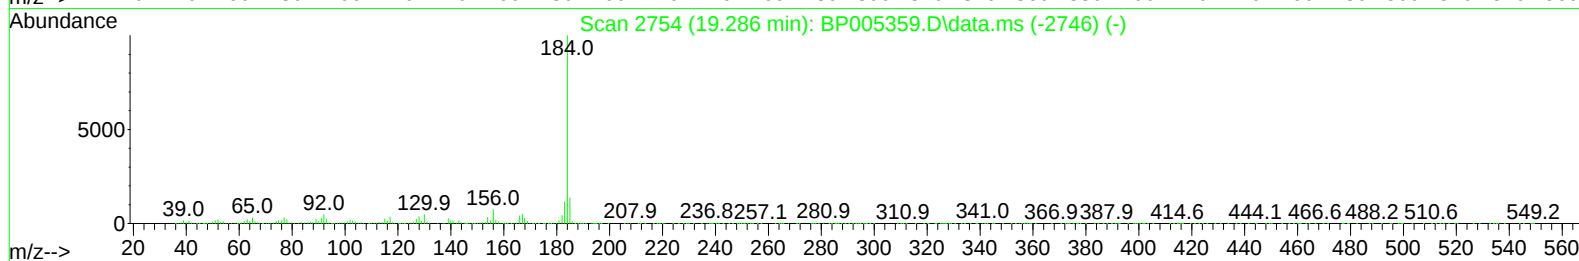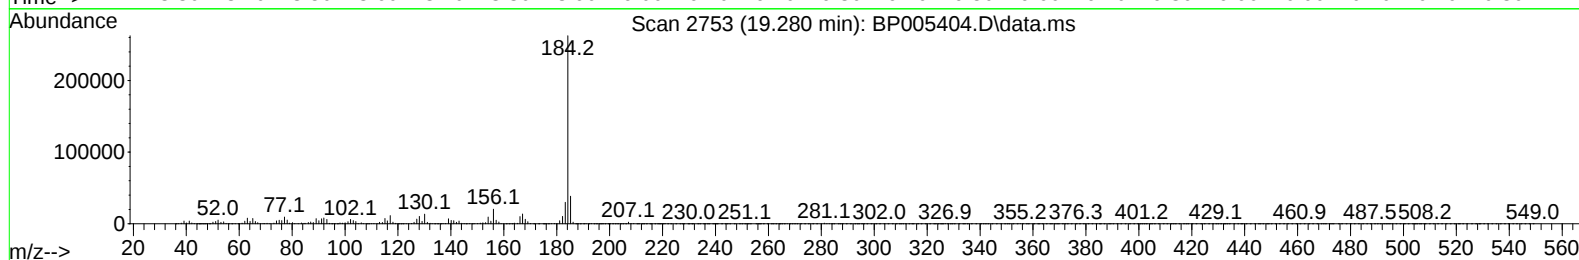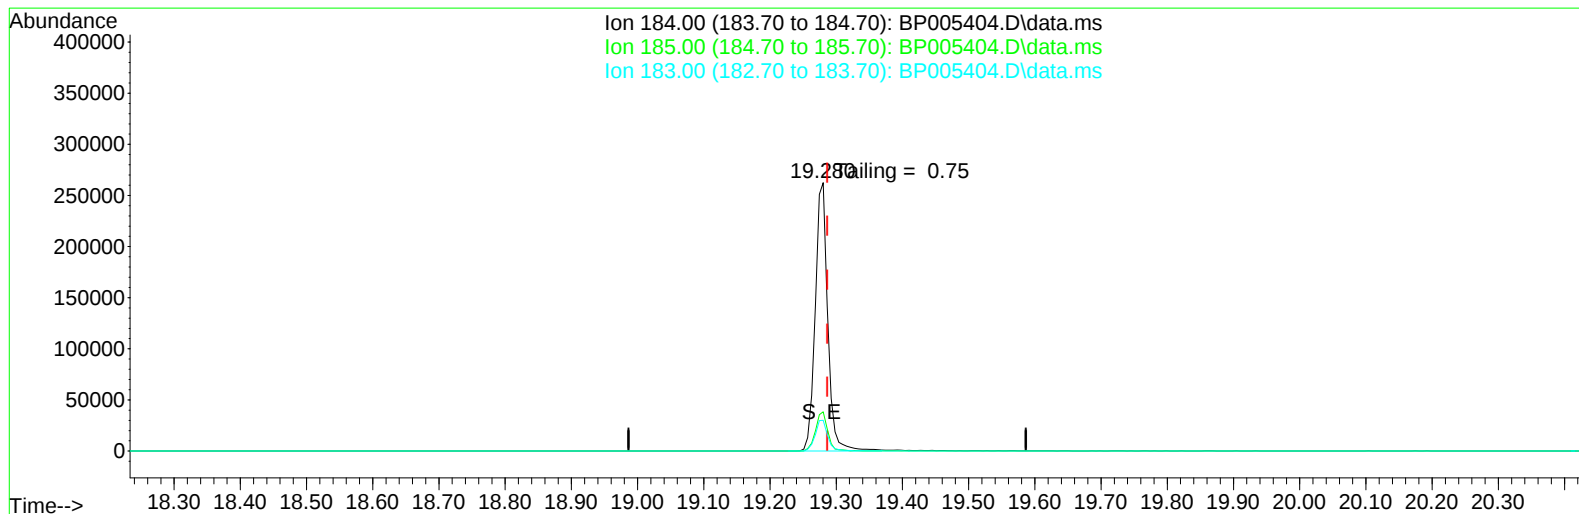

TIC: BP005404.D\data.ms

(77) Benzidine

19.280min (-0.006) 422510.27 ng




response 347151

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.63
183.00	12.30	11.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042921\
 Data File : BP005404.D
 Acq On : 29 Apr 2021 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 29 12:51:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 12:38:20 2021
 Response via : Initial Calibration

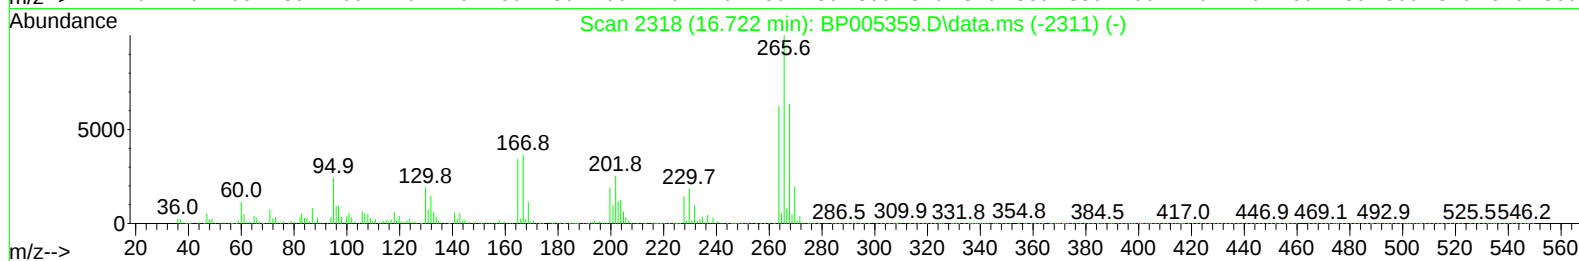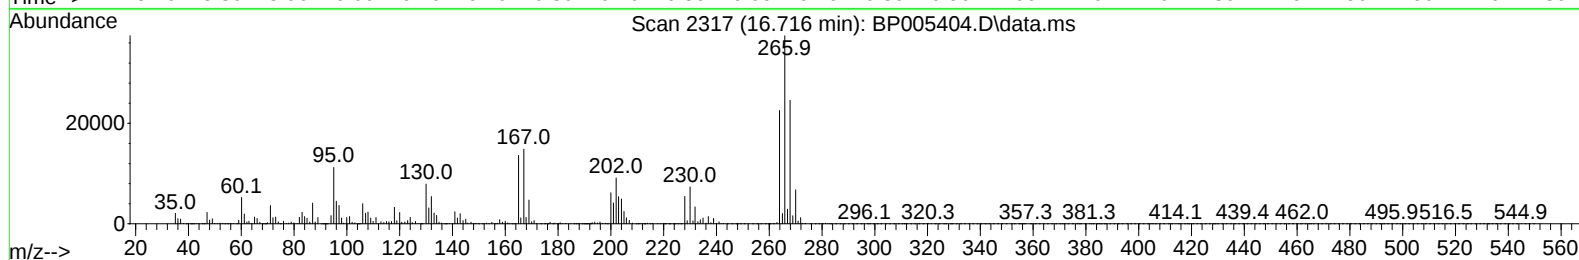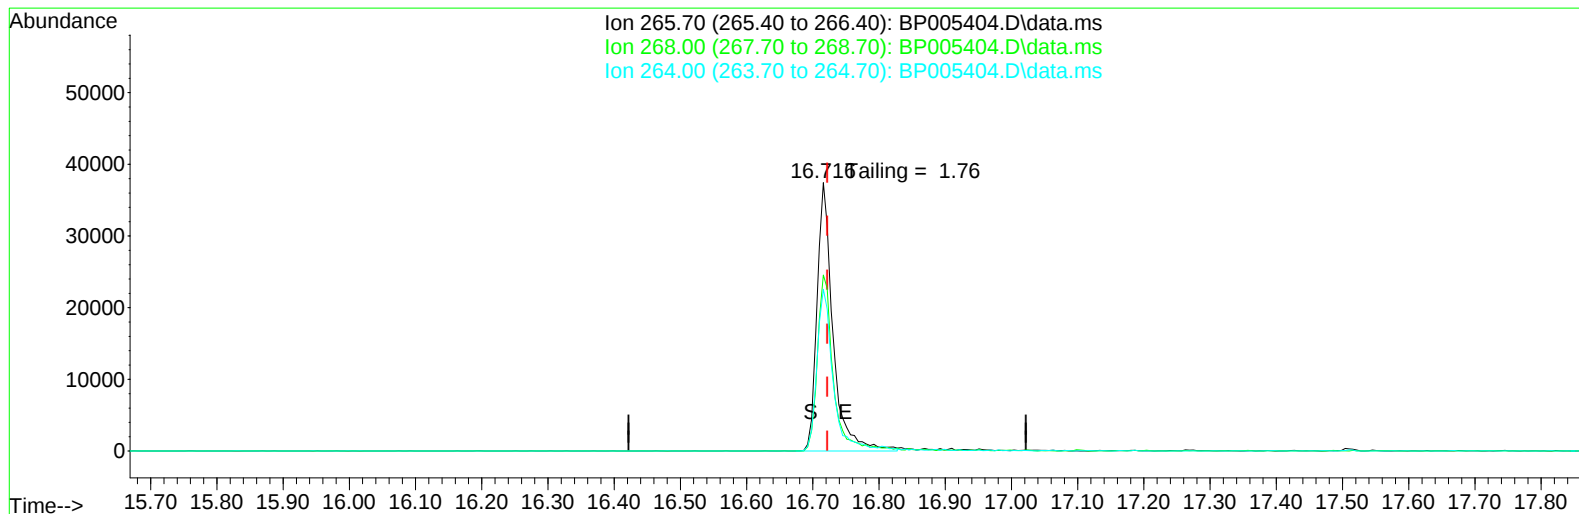

TIC: BP005404.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.006) 816739.29 ng

response 63331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.61
264.00	67.10	60.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/29/2021	BNA_P	BP005404.D
Compound Name	Response	Retention Time
DDT	218811	20.47
DDD	684	20.05
DDE	453	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1137	219948	0.52

Instrument :
BNA_P
ClientSampleId :
DFTPP