
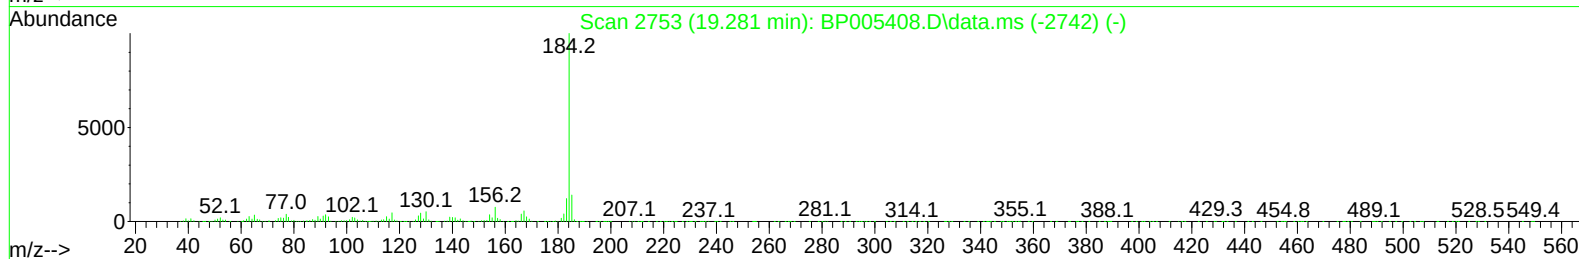
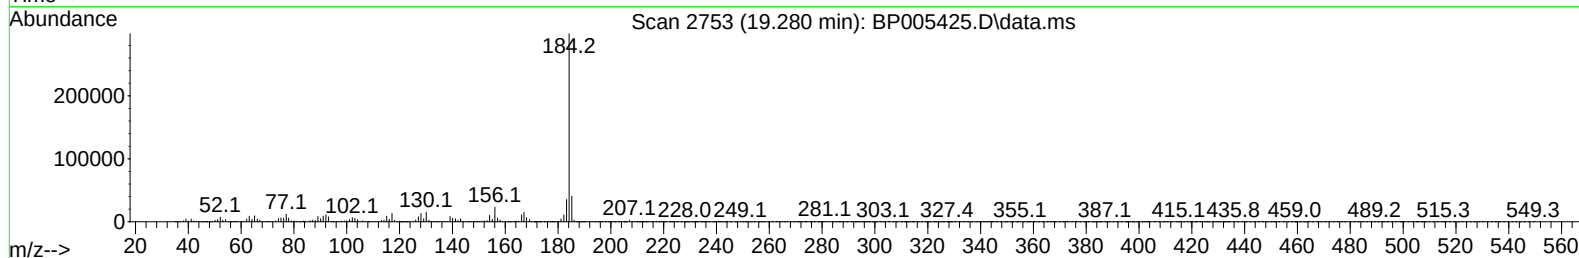


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
Data File : BP005425.D
Acq On : 30 Apr 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 12:58:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 30 11:27:53 2021
Response via : Initial Calibration

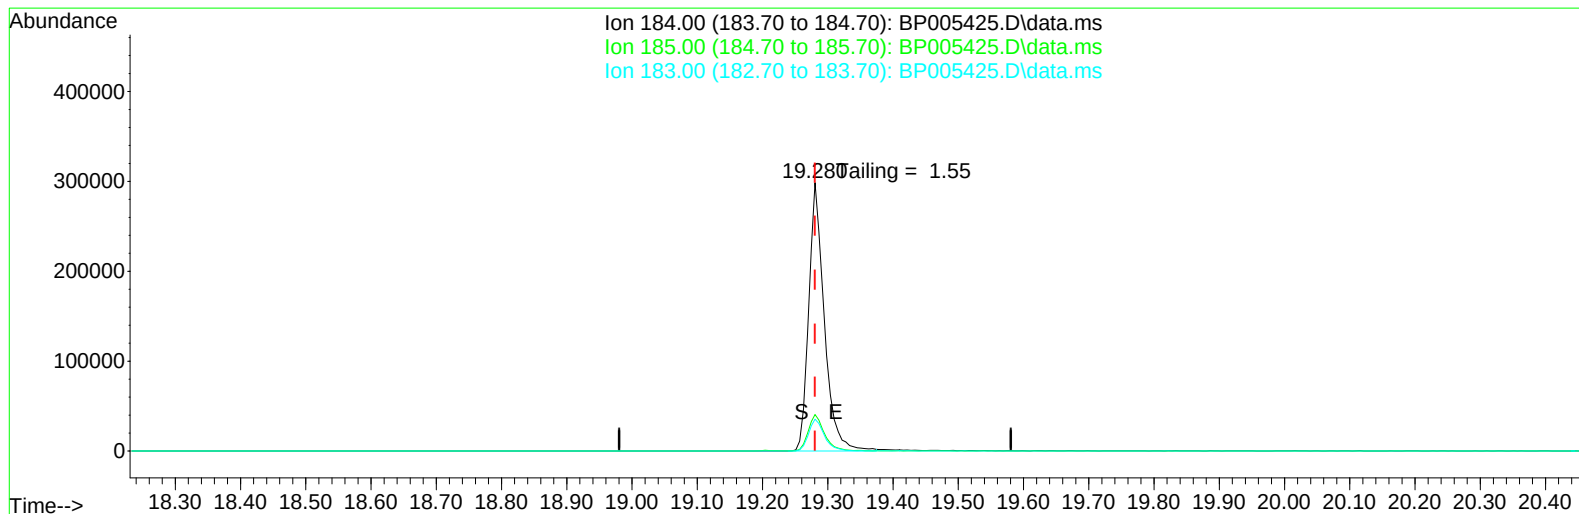




TIC: BP005425.D\data.ms

(77) Benzidine**19.280min (-0.000) 1130429.14 ng****response 502636**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.60
183.00	12.30	11.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
Data File : BP005425.D
Acq On : 30 Apr 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 12:58:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 30 11:27:53 2021
Response via : Initial Calibration

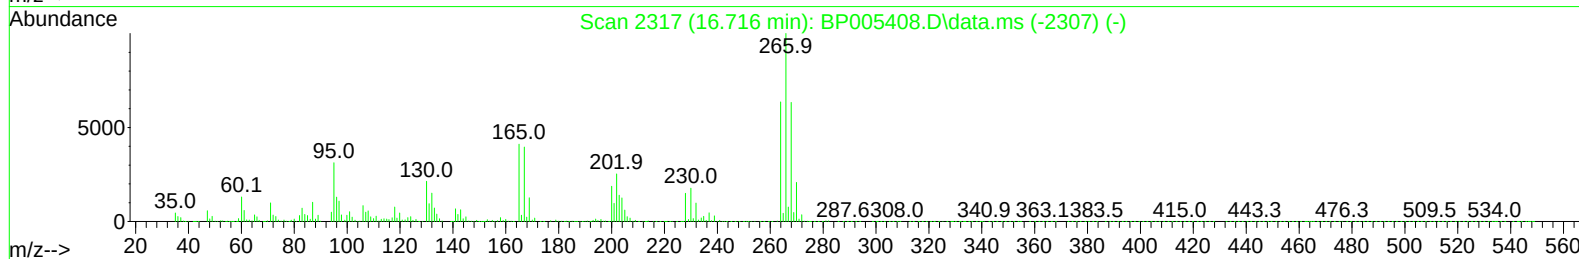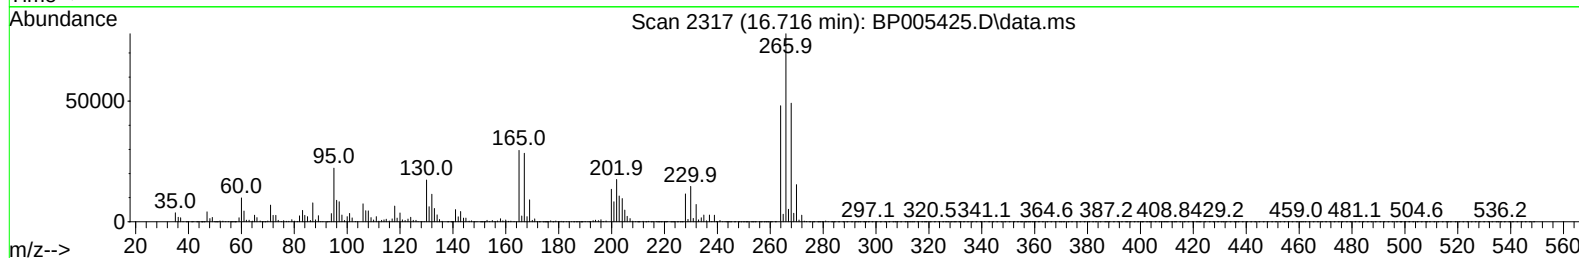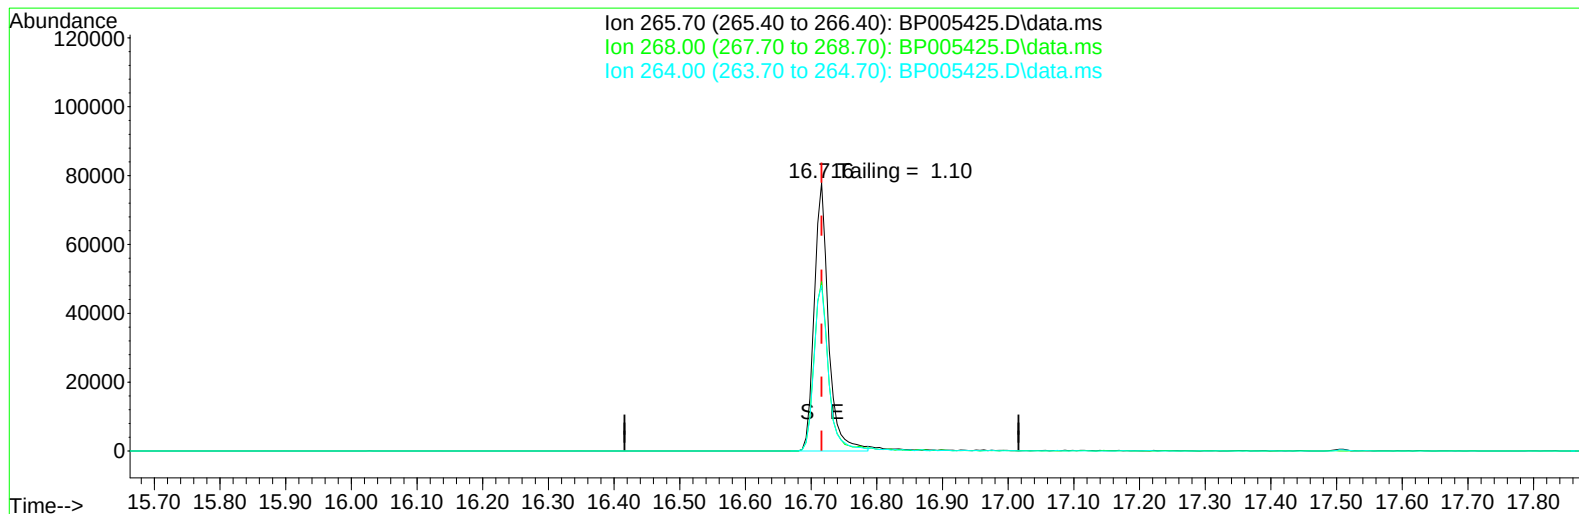

TIC: BP005425.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.000) 1976833.86 ng

response 120330

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.07
264.00	67.10	61.72
0.00	0.00	0.00