

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
 Data File : BP005427.D
 Acq On : 30 Apr 2021 11:05
 Operator : CG/JU
 Sample : PB136031BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136031BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	355	364	379	rBV	1014670	1377680	35.18%	9.919%
2	6.816	626	634	649	rBV	849011	1314639	33.57%	9.465%
3	7.622	764	771	785	rBV	160219	252954	6.46%	1.821%
4	8.787	959	969	982	rBV	502152	827584	21.13%	5.959%
5	10.410	1237	1245	1255	rBV	164114	284448	7.26%	2.048%
6	12.904	1660	1669	1677	rBV	1457876	2031121	51.87%	14.624%
7	14.292	1898	1905	1914	rBV2	252562	380451	9.72%	2.739%
8	15.798	2152	2161	2193	rBV	1244714	1848888	47.21%	13.312%
9	17.057	2368	2375	2386	rBV	335109	488558	12.48%	3.518%
10	19.639	2808	2814	2826	rBV	3556169	3915892	100.00%	28.194%
11	21.162	3068	3073	3080	rBV	476352	596432	15.23%	4.294%
12	23.415	3450	3456	3466	rVB2	281062	570476	14.57%	4.107%




Sum of corrected areas: 13889123

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
Data File : BP005427.D
Acq On : 30 Apr 2021 11:05
Operator : CG/JU
Sample : PB136031BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136031BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

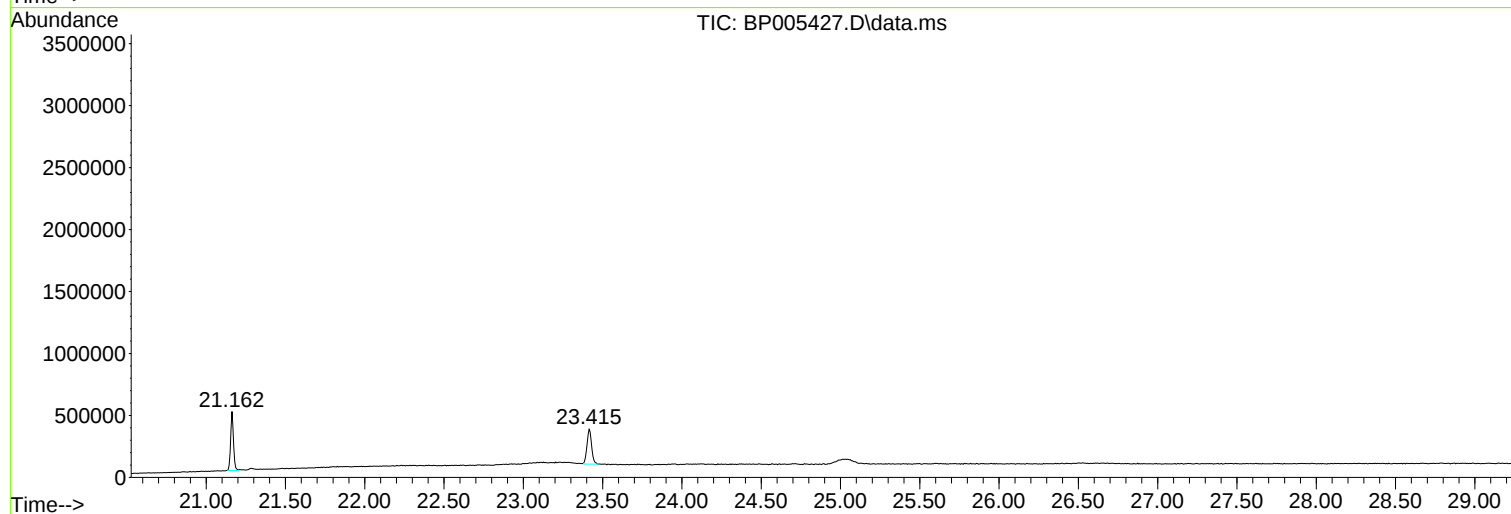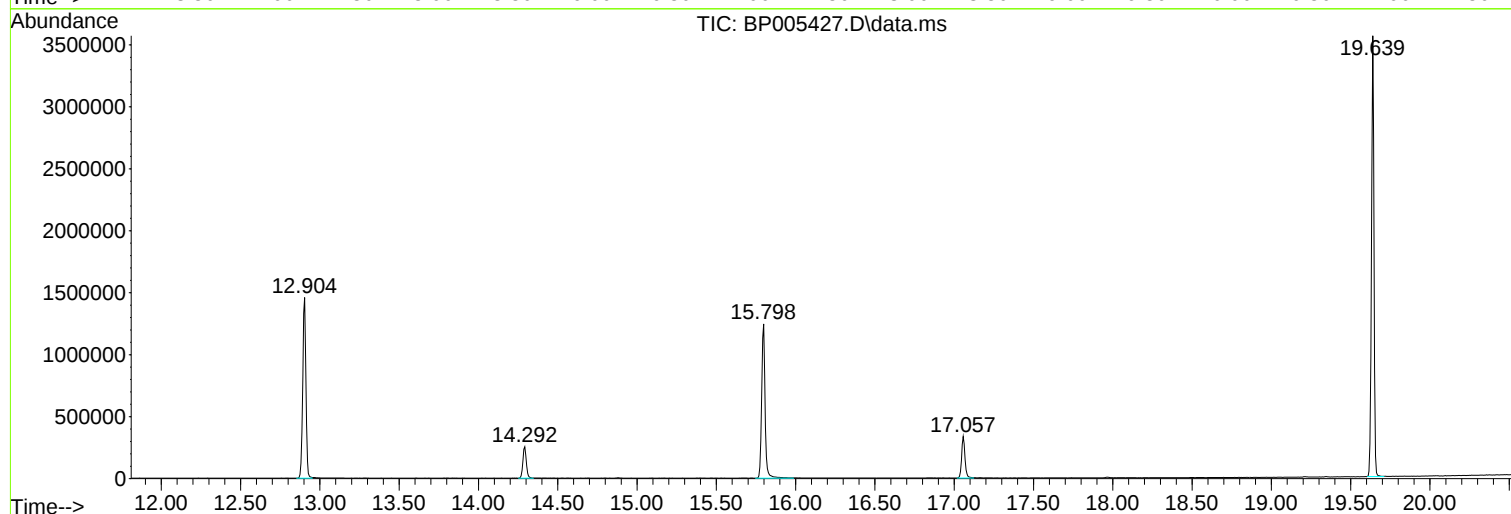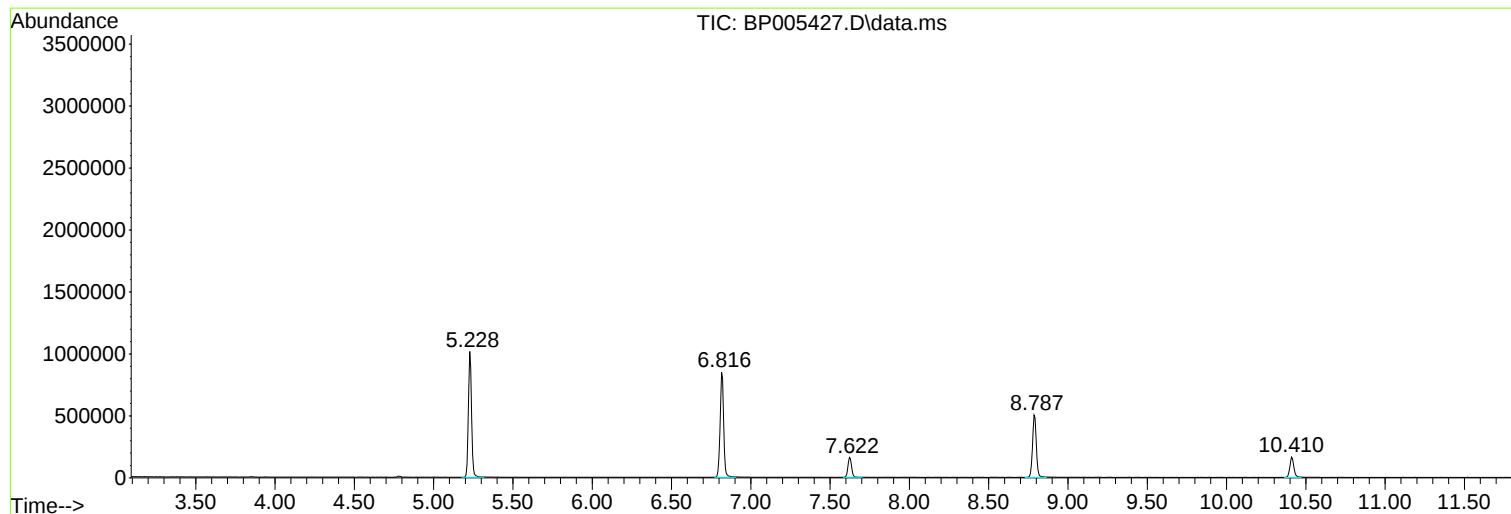

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
Data File : BP005427.D
Acq On : 30 Apr 2021 11:05
Operator : CG/JU
Sample : PB136031BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136031BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
Data File : BP005427.D
Acq On : 30 Apr 2021 11:05
Operator : CG/JU
Sample : PB136031BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136031BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------