
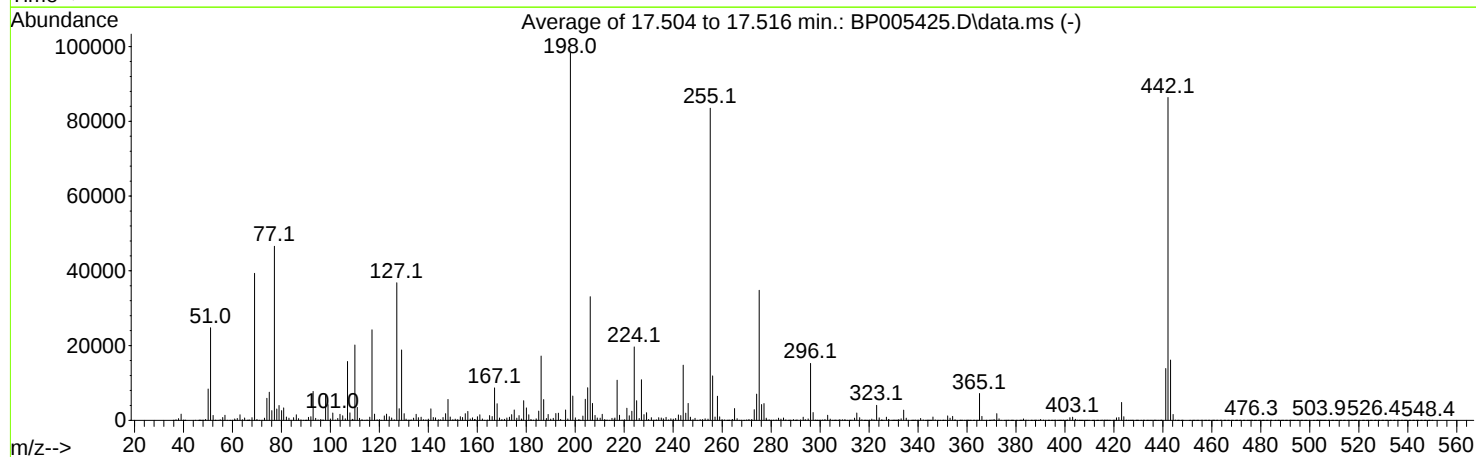


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
 Data File : BP005425.D
 Acq On : 30 Apr 2021 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 30 11:27:53 2021

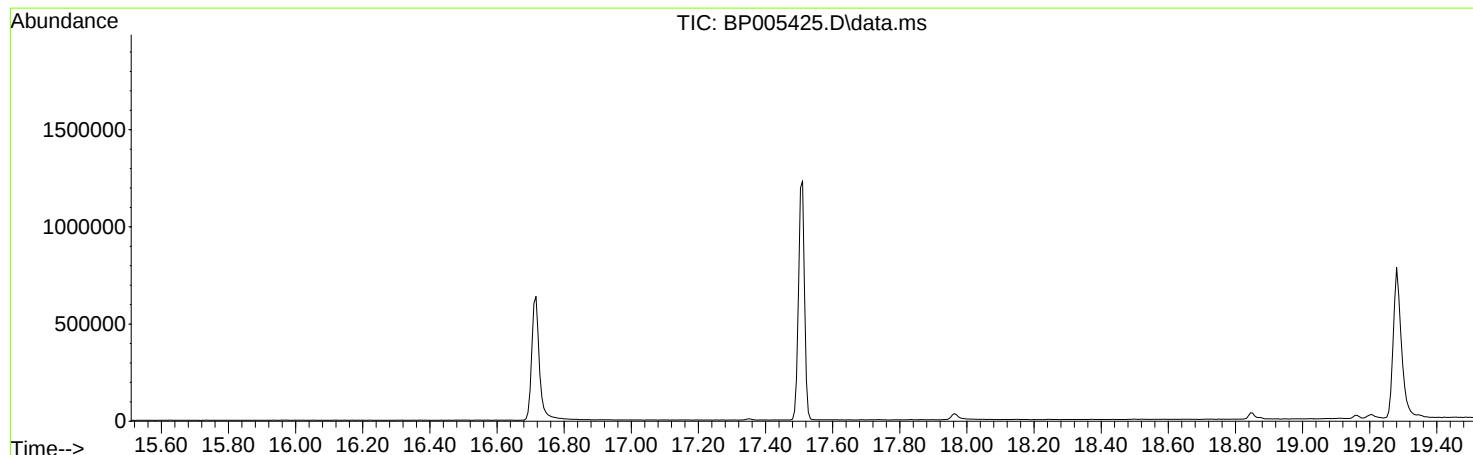

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	24791	PASS
68	69	0.00	2	1.9	743	PASS
69	198	0.00	100	40.0	39340	PASS
70	69	0.00	2	0.6	249	PASS
127	198	10	80	37.4	36795	PASS
197	198	0.00	2	0.4	406	PASS
198	198	100	100	100.0	98403	PASS
199	198	5	9	6.6	6506	PASS
275	198	10	60	35.4	34813	PASS
365	198	1	100	7.3	7188	PASS
441	198	0.01	100	14.1	13848	PASS
442	442	100	100	100.0	86361	PASS
443	442	15	24	18.7	16153	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/30/2021	BNA_P	<u>BP005425.D</u>
Compound Name	Response	Retention Time
DDT	378378	20.47
DDD	5316	20.04
DDE	902	20.04
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6218	384596	1.62

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
Data File : BP005425.D
Acq On : 30 Apr 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 30 12:58:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 30 11:27:53 2021
Response via : Initial Calibration

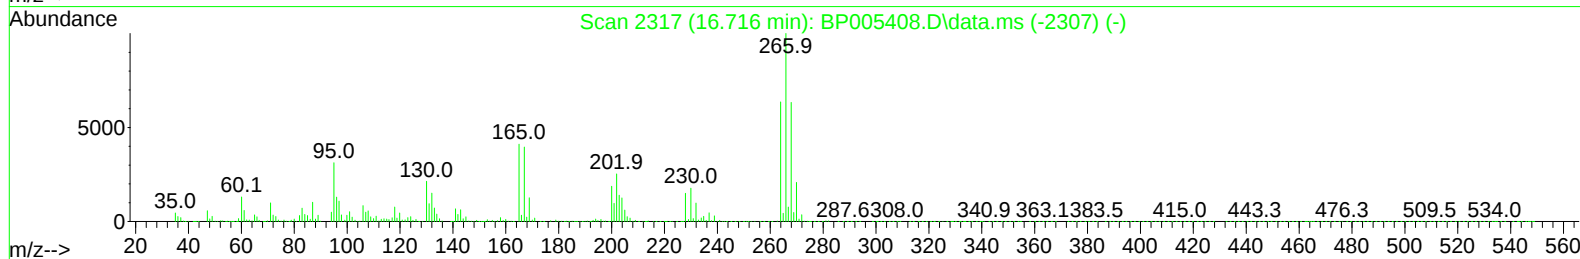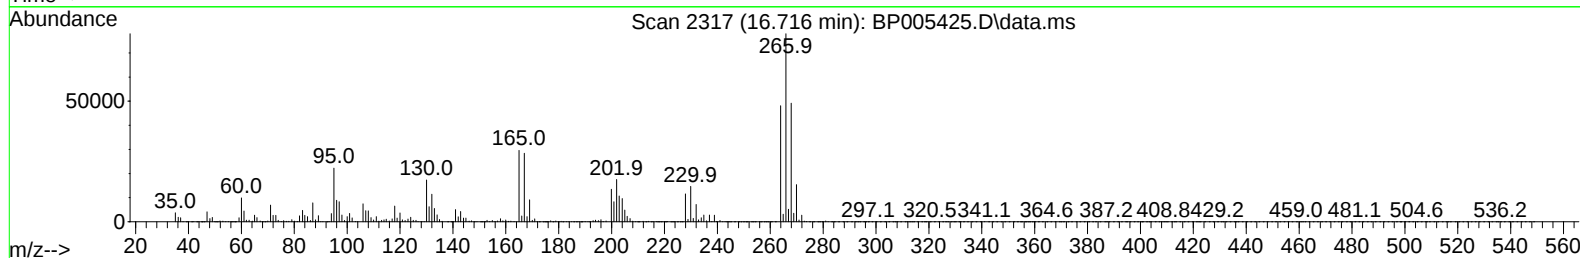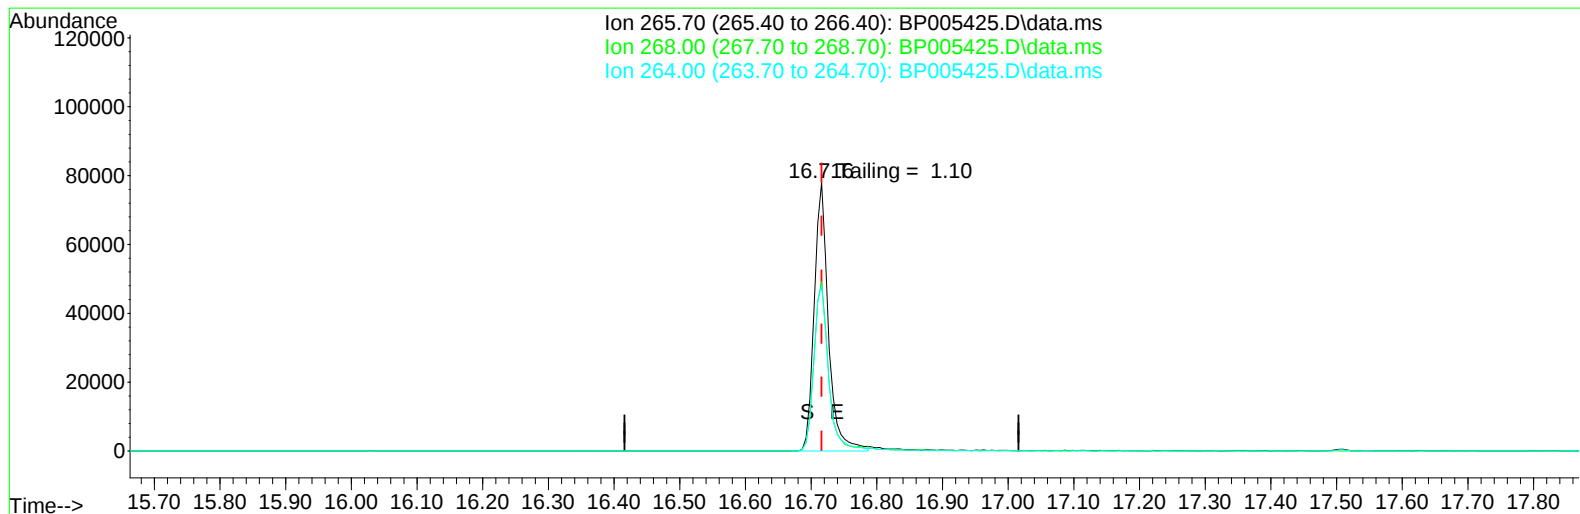

TIC: BP005425.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.000) 1976833.86 ng




response 120330

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.07
264.00	67.10	61.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043021\
 Data File : BP005425.D
 Acq On : 30 Apr 2021 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 30 12:58:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP042921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 30 11:27:53 2021
 Response via : Initial Calibration

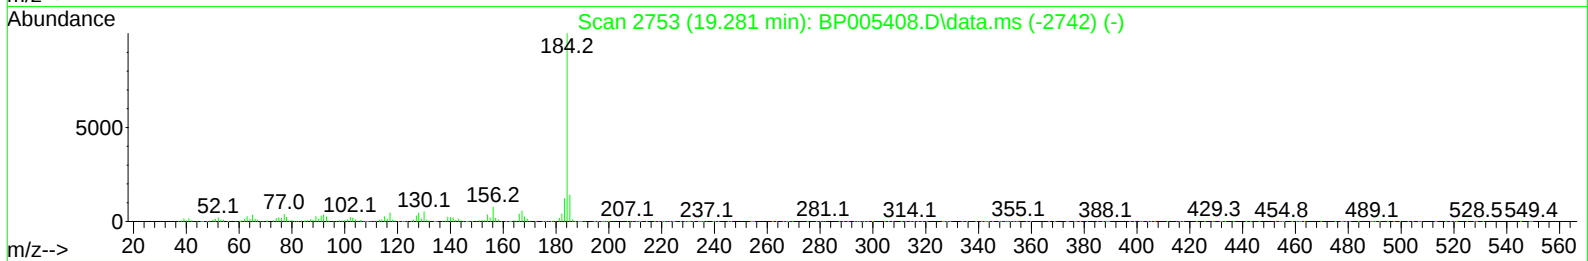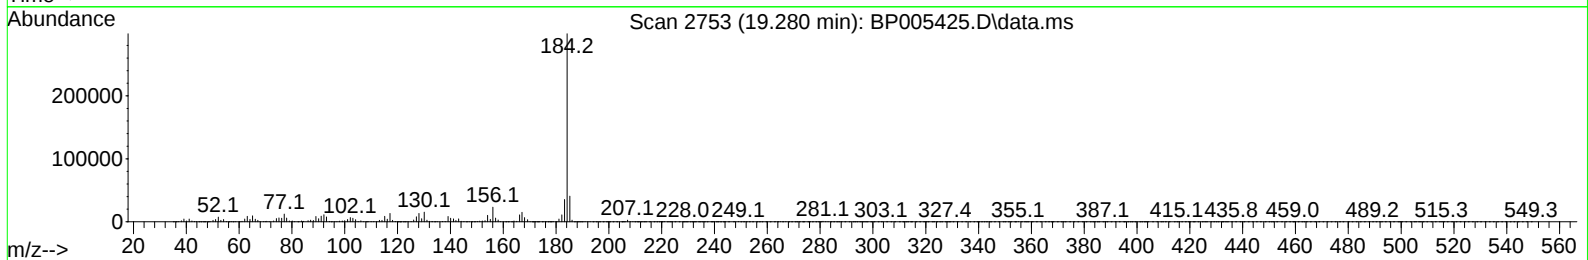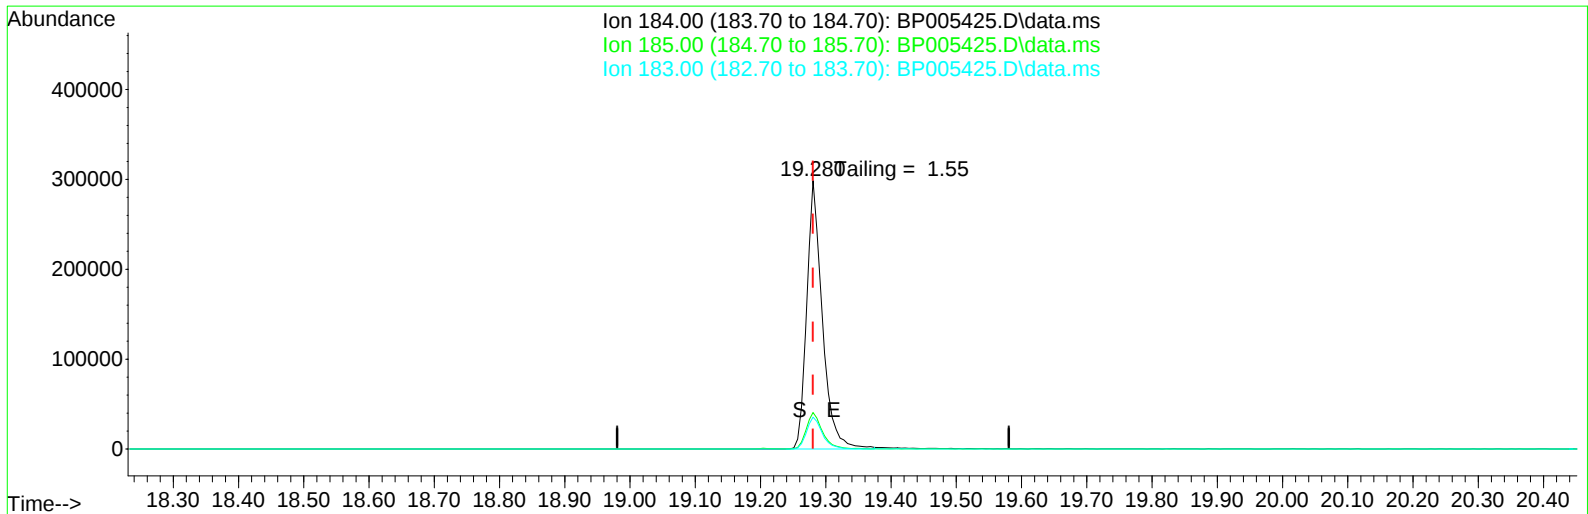

TIC: BP005425.D\data.ms

(77) Benzidine

19.280min (-0.000) 1130429.14 ng

response 502636

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.60
183.00	12.30	11.88
0.00	0.00	0.00