




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Manual IntegrationsAPPROVED

Quant Time: May 03 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

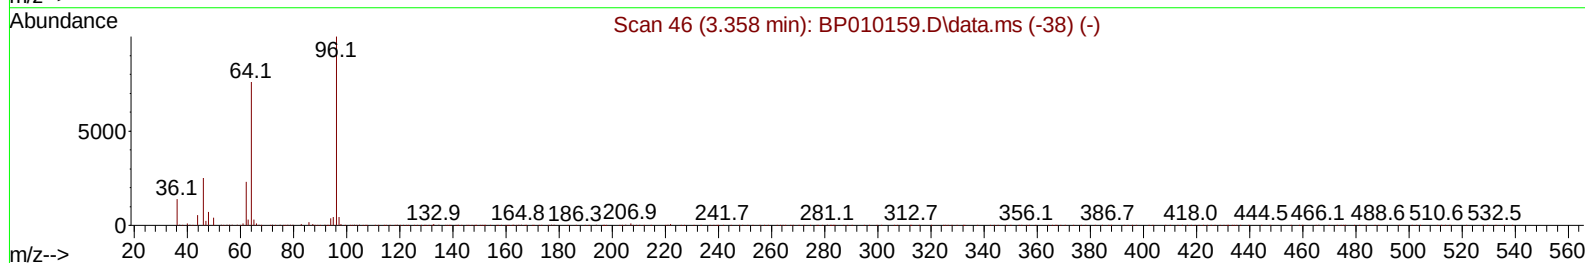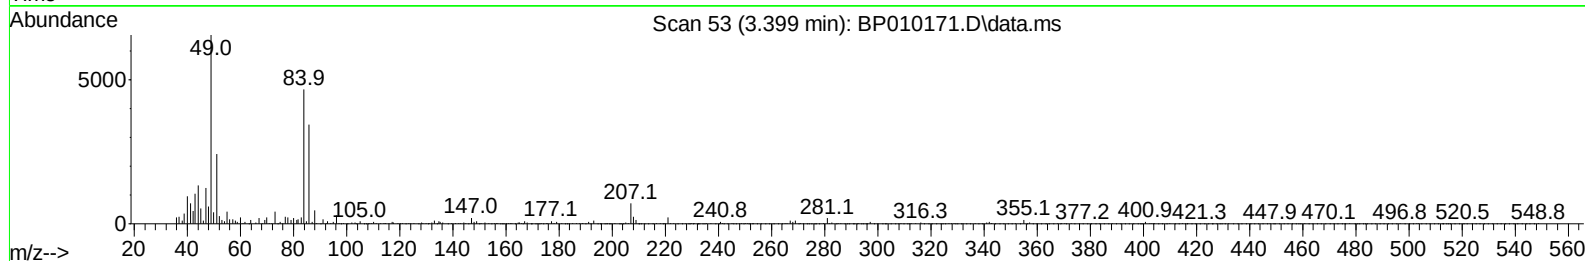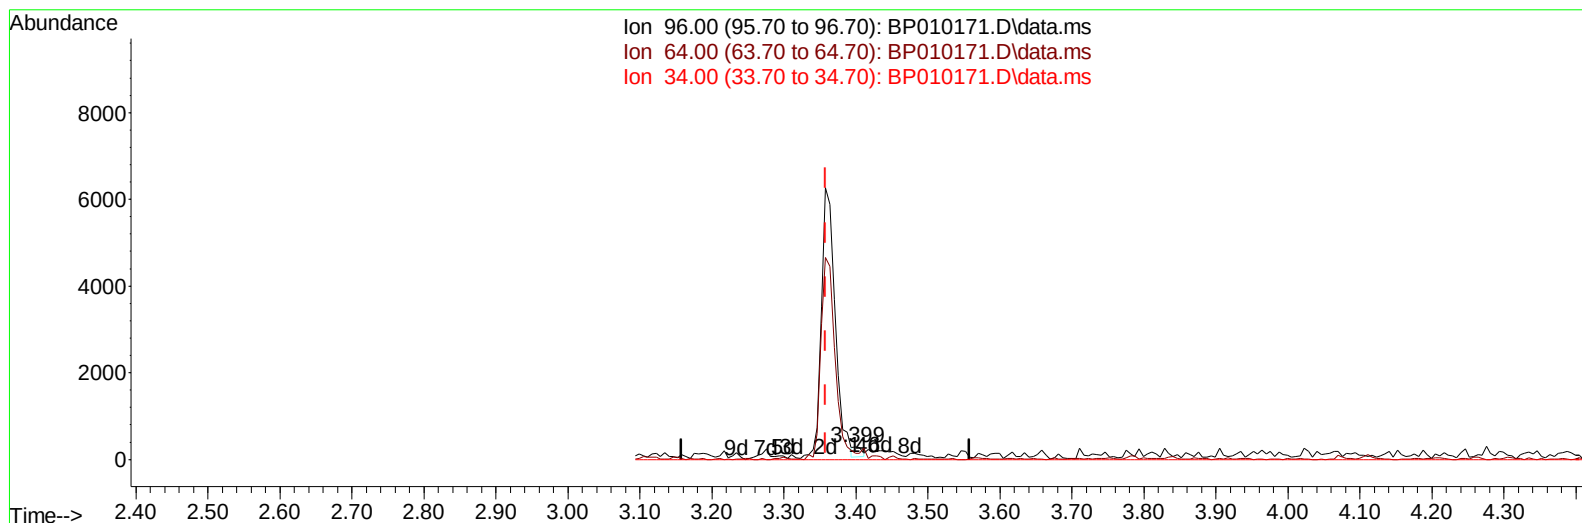

TIC: BP010171.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.399min (+ 0.041) 0.05 ng/uL

response 183

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	50.35
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Manual IntegrationsAPPROVED

Quant Time: May 03 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

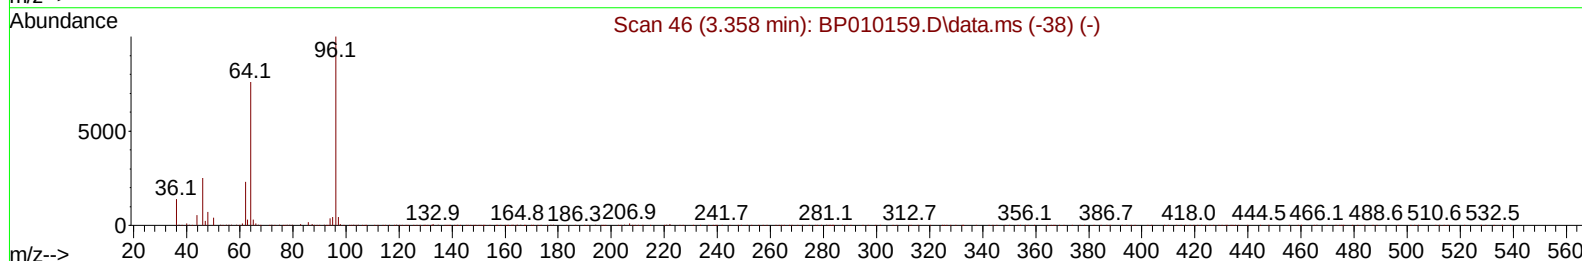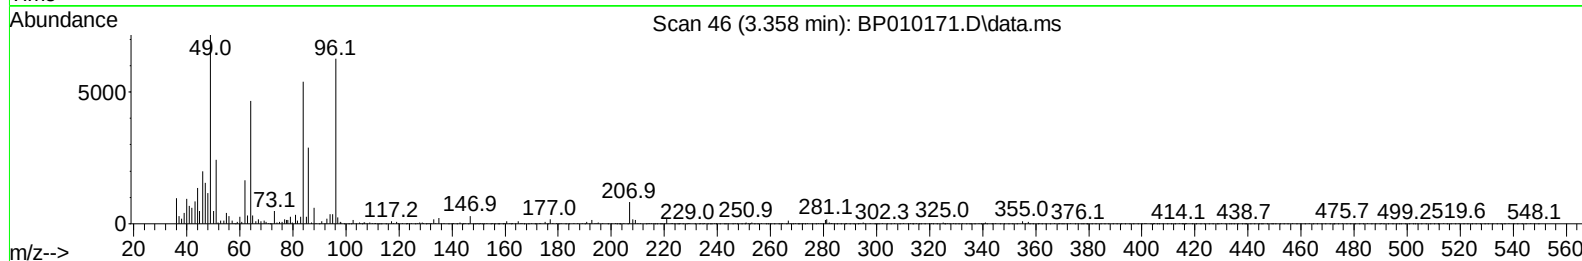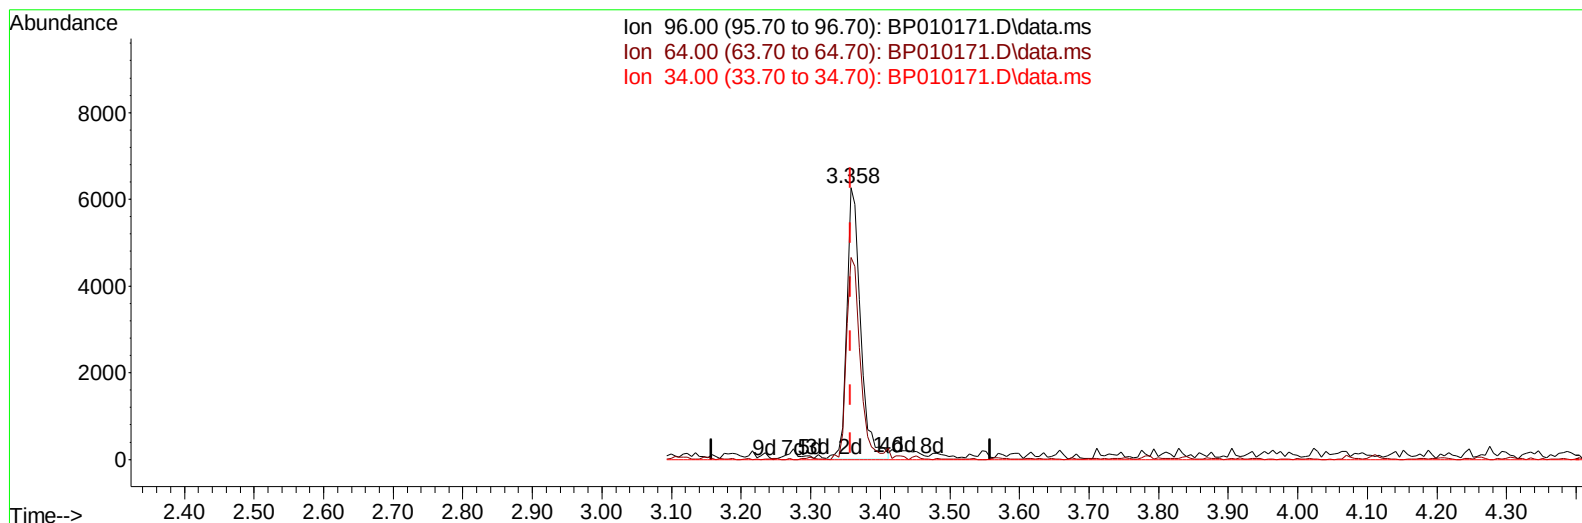

TIC: BP010171.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (+ 0.000) 2.39 ng/uL m

response 8676

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	74.44#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010171.D
Acq On : 02 May 2022 14:10
Operator : CG/JU
Sample : N2562-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW470

Manual IntegrationsAPPROVED

Quant Time: May 03 01:07:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

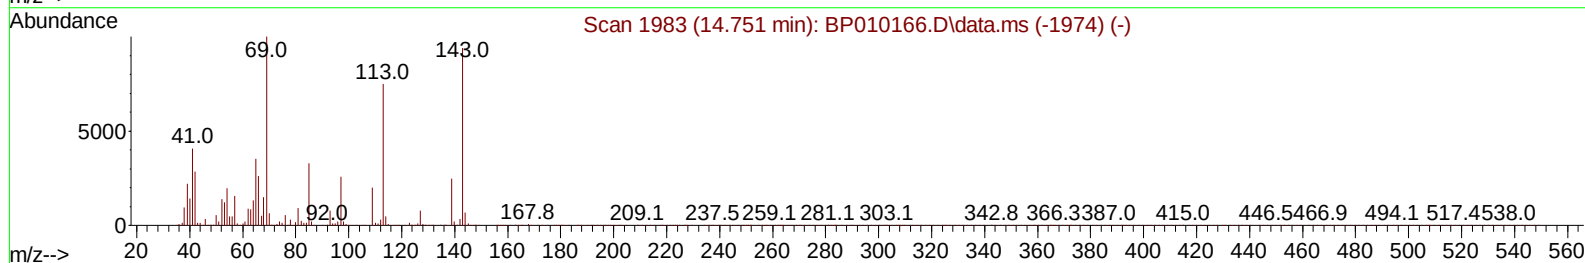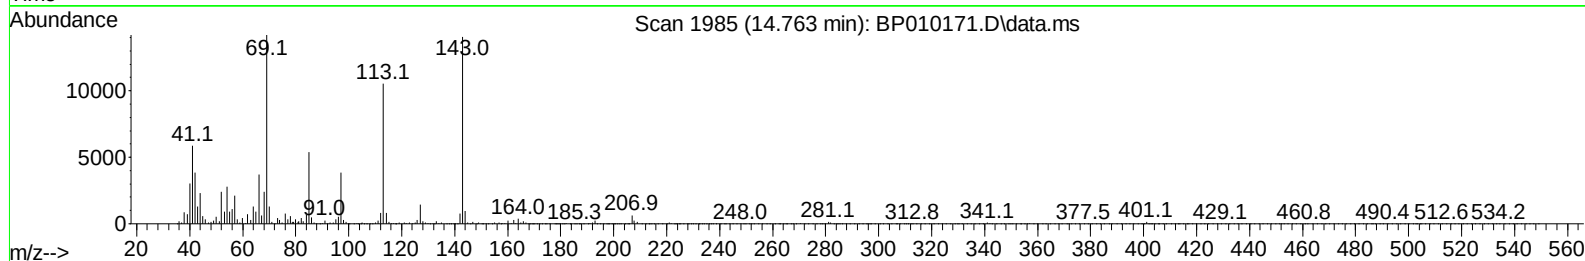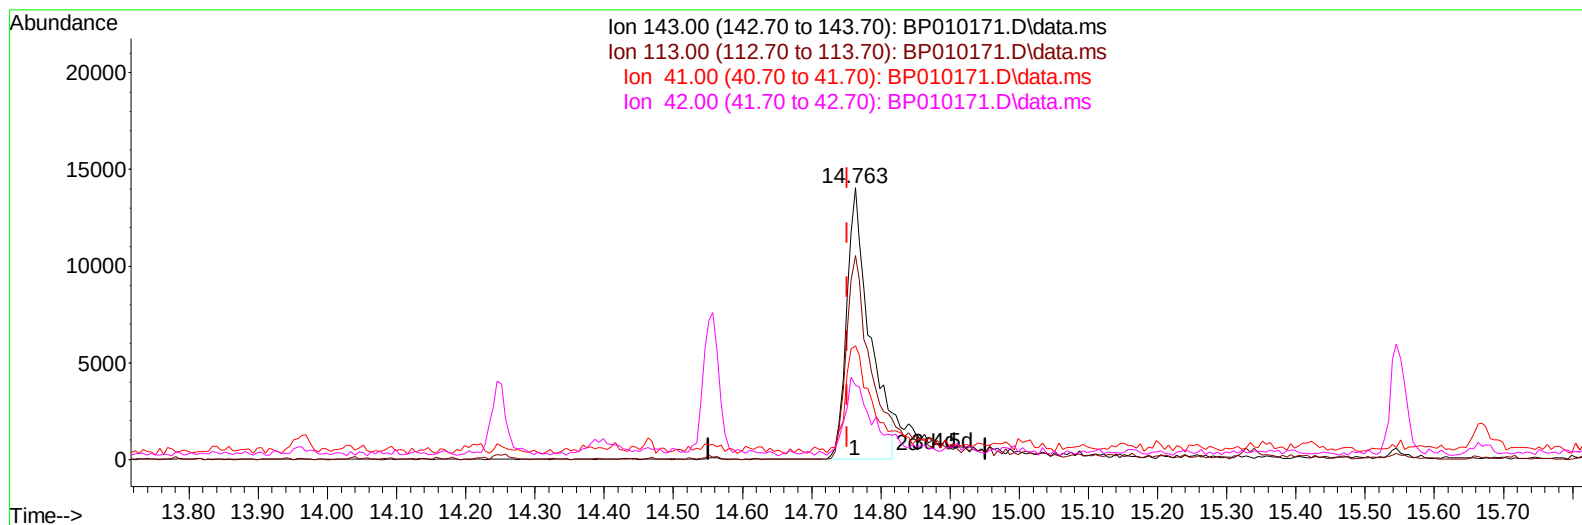

TIC: BP010171.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.012) 5.94 ng/ul

response 32138

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.11#
41.00	23.20	41.95#
42.00	18.00	27.34#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010171.D
Acq On : 02 May 2022 14:10
Operator : CG/JU
Sample : N2562-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW470

Manual IntegrationsAPPROVED

Quant Time: May 03 01:07:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

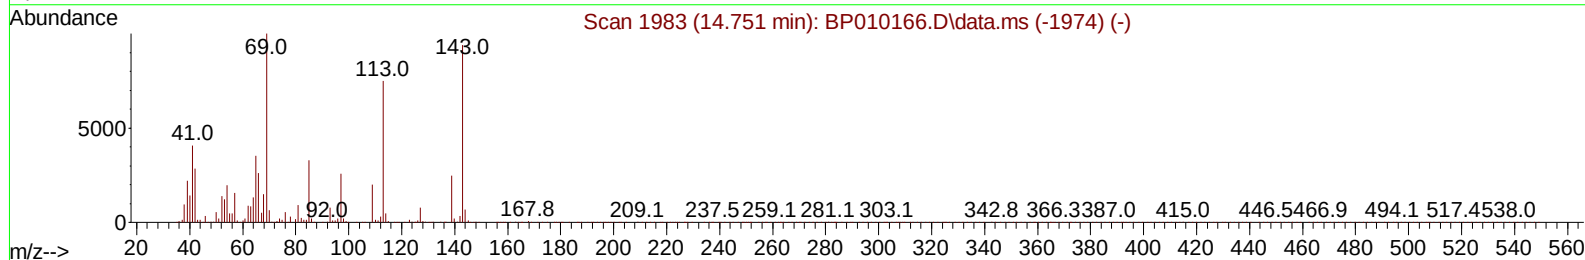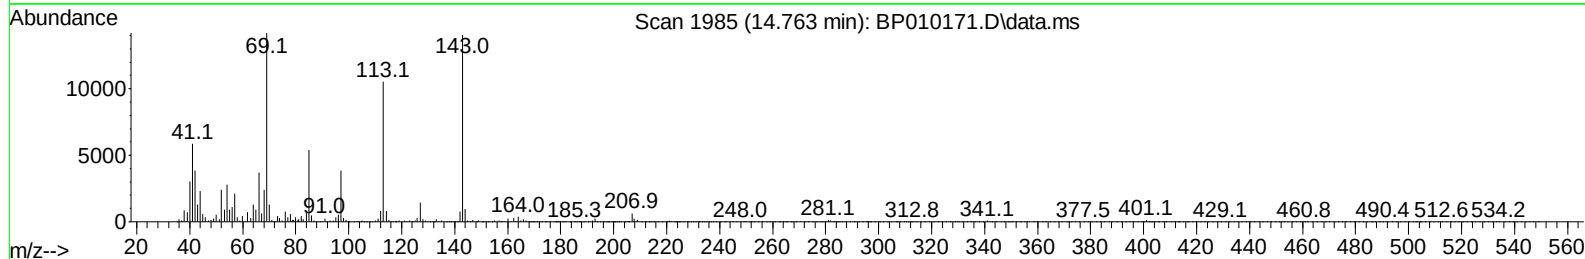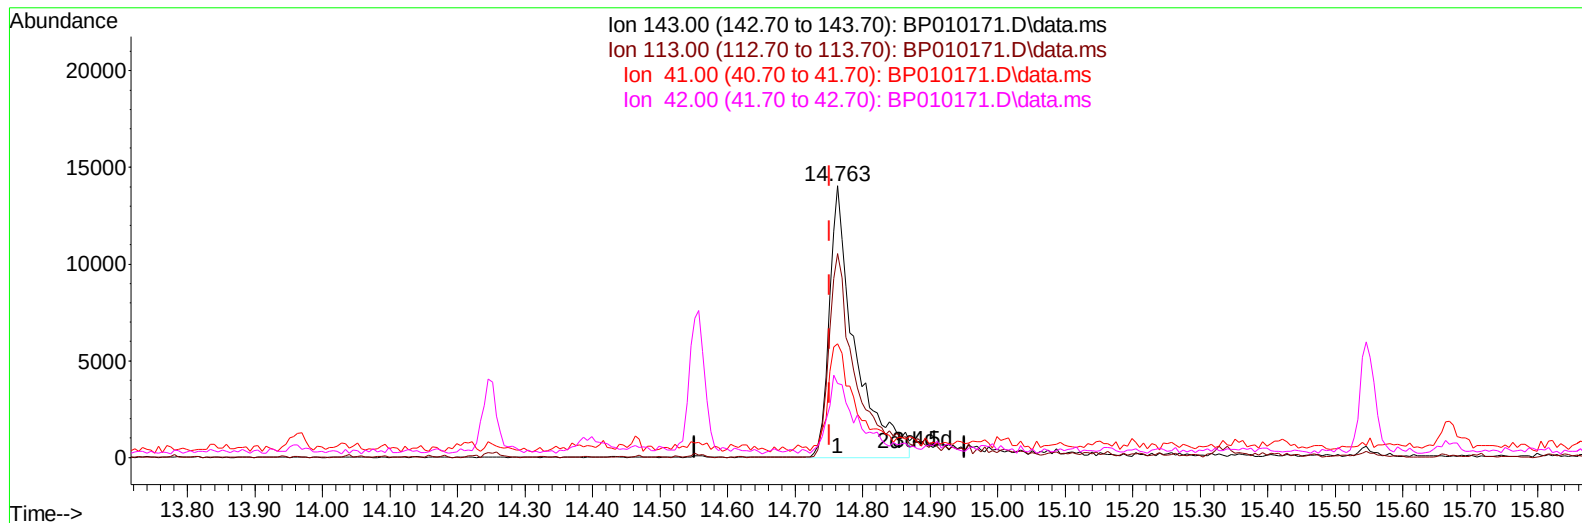

TIC: BP010171.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.012) 6.83 ng/ul m

response 36961

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.11#
41.00	23.20	41.95#
42.00	18.00	27.34#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Manual IntegrationsAPPROVED

Quant Time: May 03 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

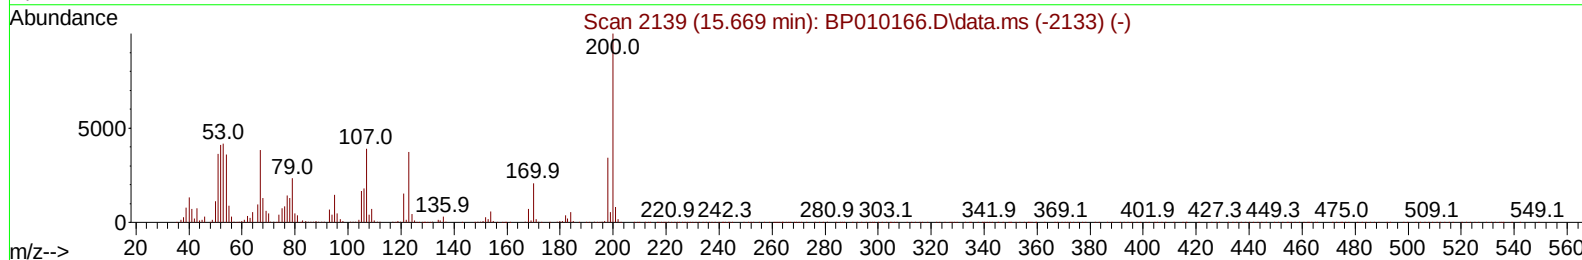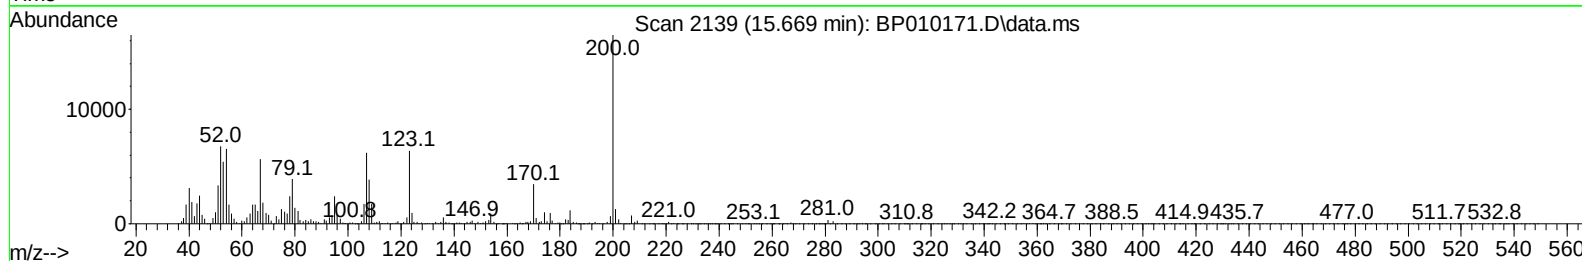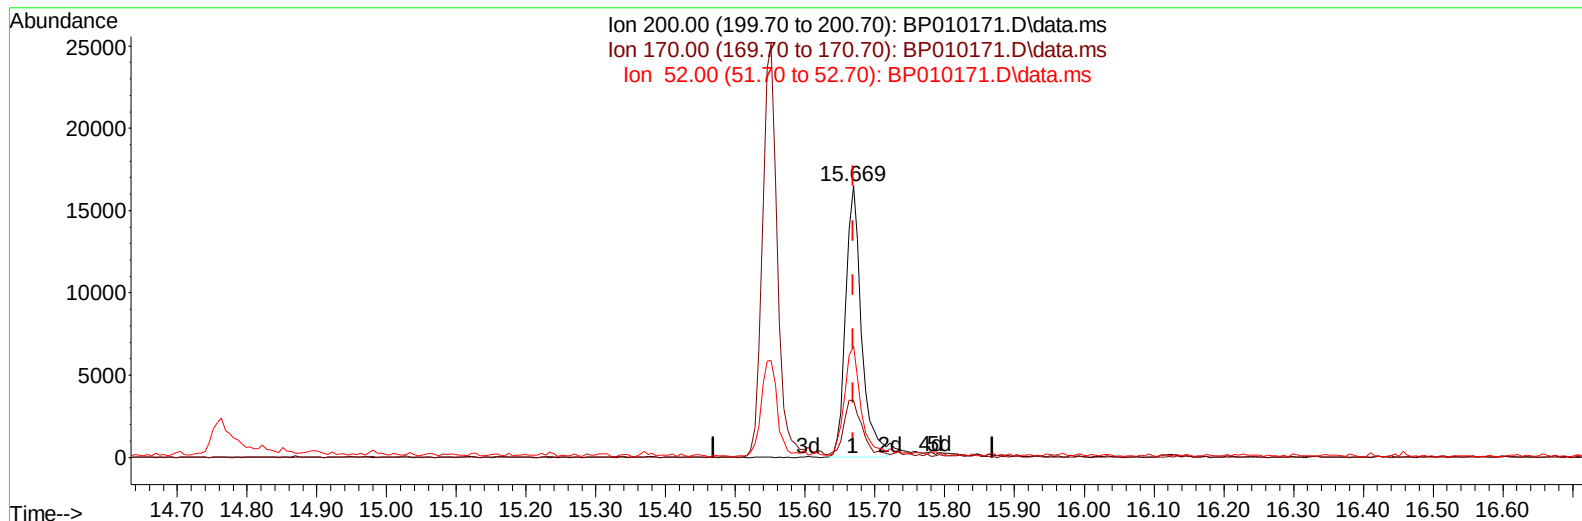

TIC: BP010171.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.669min (+ 0.000) 5.93 ng/ul

response 26175

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	20.96
52.00	21.20	40.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Manual IntegrationsAPPROVED

Quant Time: May 03 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

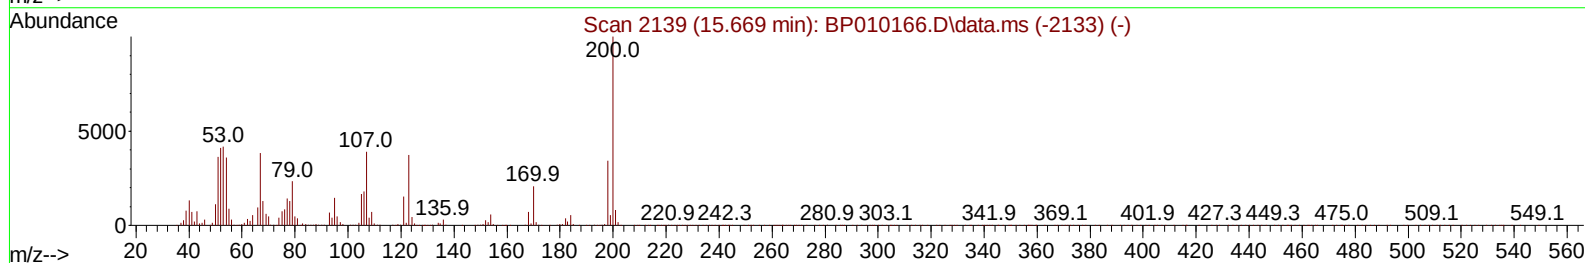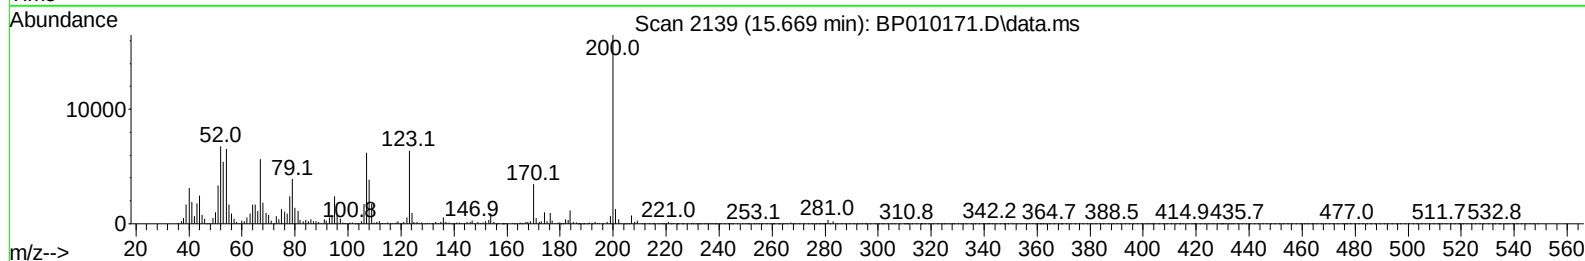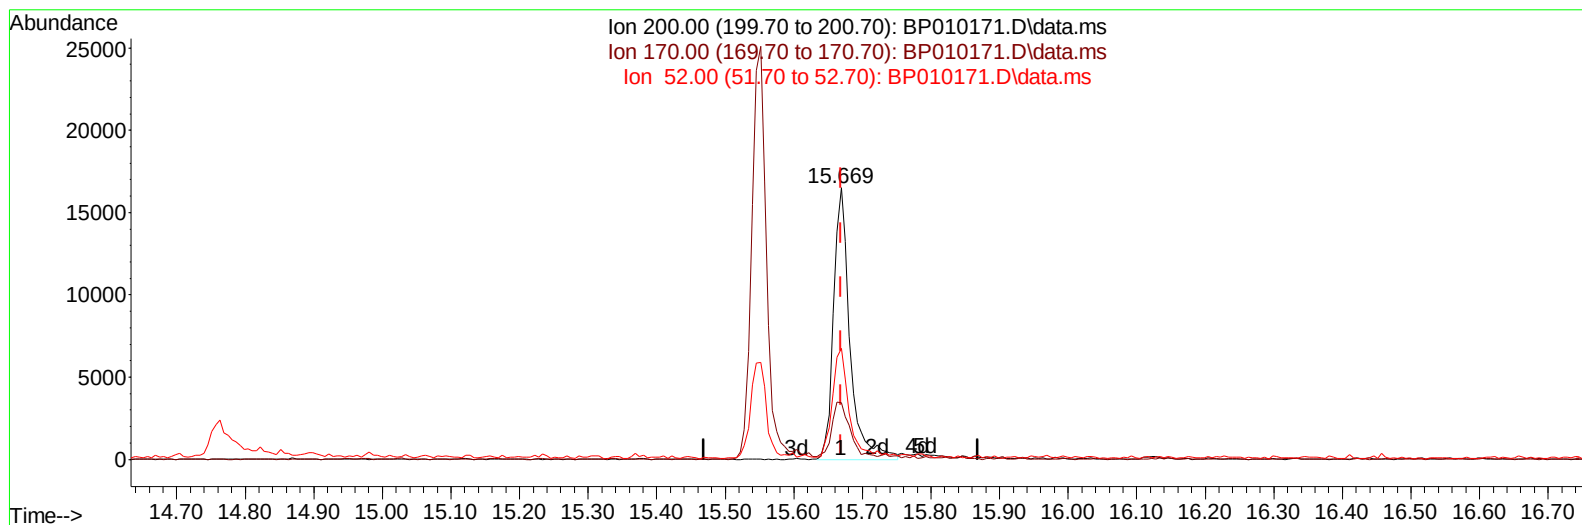

TIC: BP010171.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.669min (+ 0.000) 6.18 ng/ul m

response 27306

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	20.96
52.00	21.20	40.91#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	158592	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	640213	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	377612	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	698585	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	597333	20.000	ng/ul	# 0.00
88) Perylene-d12	23.833	264	599319	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	8676m	2.386	ng/uL	0.00
4) Pyridine-d5	3.787	84	37091	3.625	ng/ul	0.01
7) Phenol-d5	7.087	99	153932	10.671	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.252	67	112060	12.946	ng/ul	0.00
11) 2-Chlorophenol-d4	7.458	132	130179	12.185	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	108399	9.070	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	65541	12.872	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	72344	13.009	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	113980	10.528	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131	154552	9.956	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	388288	13.219	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	439677	12.368	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	36961m	6.835	ng/ul	0.01
60) Fluorene-d10	15.551	176	323294	12.795	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	27306m	6.182	ng/ul	0.00
73) Anthracene-d10	17.404	188	461553	13.657	ng/ul	0.00
81) Pyrene-d10	19.639	212	537353	15.818	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	473538	15.071	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010171.D
Acq On : 02 May 2022 14:10
Operator : CG/JU
Sample : N2562-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW470

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:07:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

