




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010174.D
 Acq On : 02 May 2022 15:51
 Operator : CG/JU
 Sample : N2562-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW480

Manual IntegrationsAPPROVED

Quant Time: May 03 01:36:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

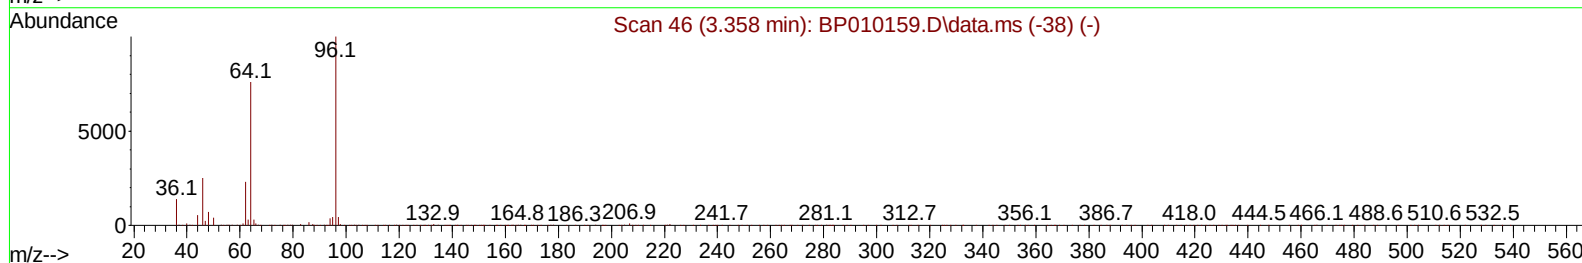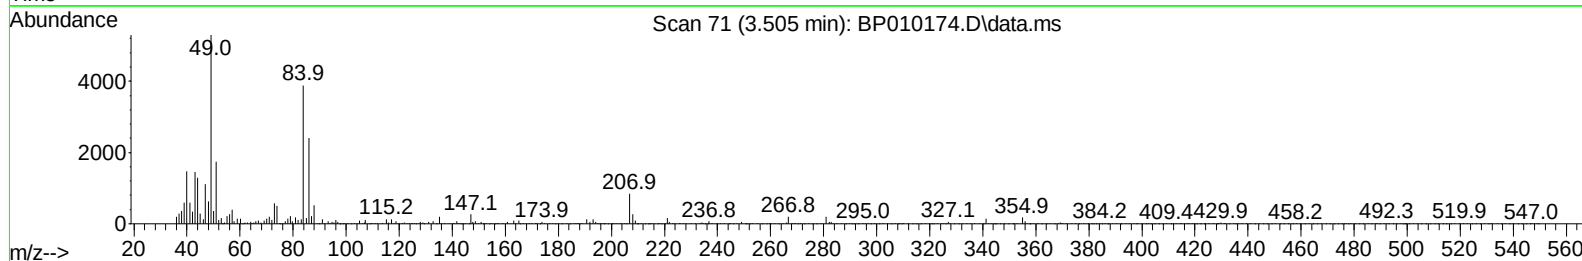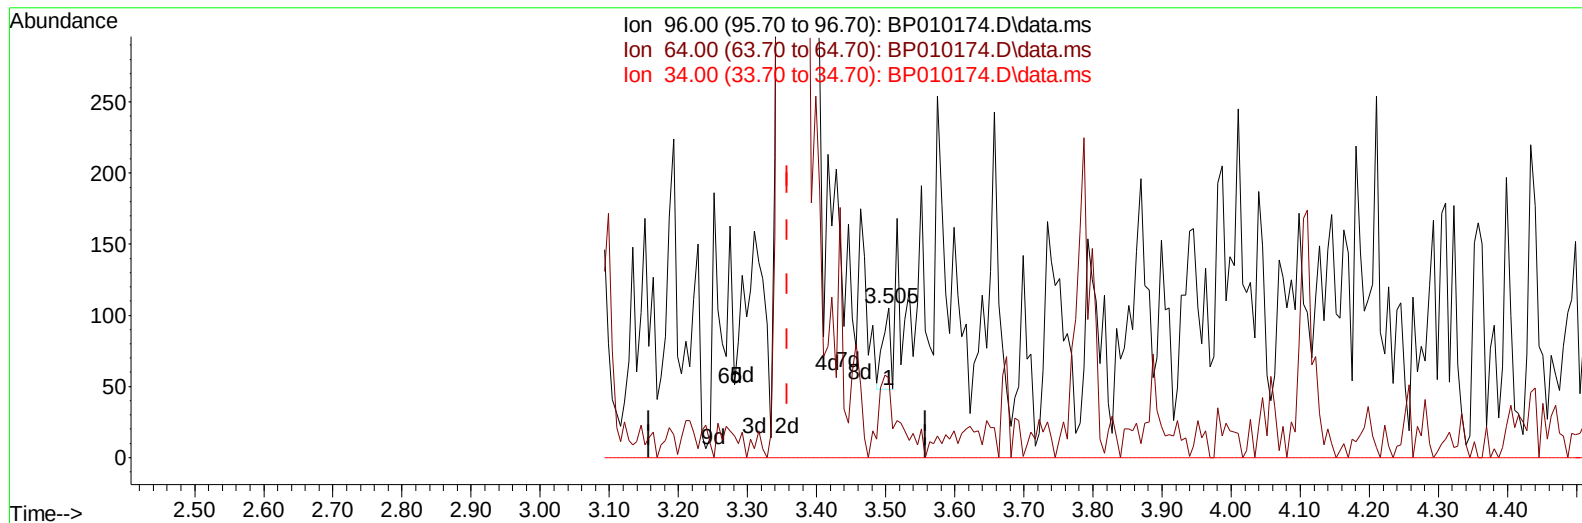

TIC: BP010174.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.505min (+ 0.147) 0.01 ng/uL

response 44

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	53.33
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010174.D
 Acq On : 02 May 2022 15:51
 Operator : CG/JU
 Sample : N2562-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW480

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:36:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	185948	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	813841	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	538783	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1062736	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.392	240	744657	20.000	ng/ul	# 0.00
88) Perylene-d12	23.833	264	641777	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	12660m	2.969	ng/uL	0.00
4) Pyridine-d5	3.781	84	77514	6.462	ng/ul	0.00
7) Phenol-d5	7.087	99	244967	14.483	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.251	67	176084	17.350	ng/ul	0.00
11) 2-Chlorophenol-d4	7.457	132	203597	16.254	ng/ul	0.00
15) 4-Methylphenol-d8	8.634	113	200439	14.303	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	110611	17.088	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	119889	16.959	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.351	165	200614	14.577	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131	259973	13.175	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	734670	17.529	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	803654	15.844	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	67183	8.707	ng/ul	0.00
60) Fluorene-d10	15.551	176	625027	17.337	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	57181	8.509	ng/ul	0.00
73) Anthracene-d10	17.404	188	914599	17.789	ng/ul	0.00
81) Pyrene-d10	19.639	212	982761	23.206	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	642716	19.103	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010174.D
Acq On : 02 May 2022 15:51
Operator : CG/JU
Sample : N2562-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW480

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:36:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

